


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE011819\
 Data File : BE098662.D
 Acq On : 18 Jan 2019 7:58
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE011519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 15 14:30:55 2019

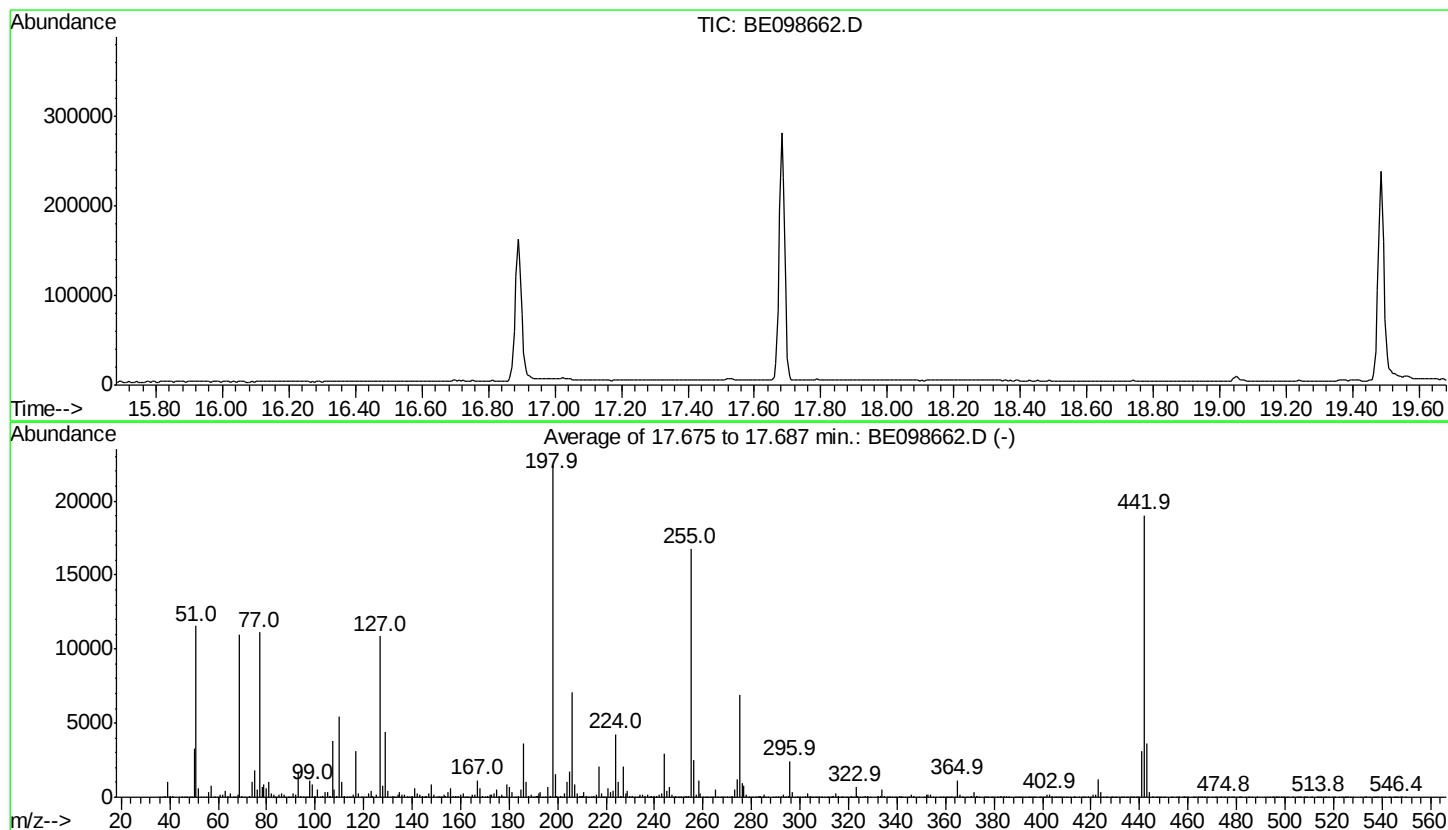

AutoFind: Scans 2568, 2569, 2570; Background Corrected with Scan 2561

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.7	11570	PASS
68	69	0.00	2	1.4	148	PASS
69	198	0.00	100	48.9	10958	PASS
70	69	0.00	2	0.6	67	PASS
127	198	10	80	48.5	10869	PASS
197	198	0.00	2	0.5	119	PASS
198	198	100	100	100.0	22388	PASS
199	198	5	9	6.8	1529	PASS
275	198	10	60	30.7	6880	PASS
365	198	1	100	5.0	1125	PASS
441	198	0.01	100	13.8	3091	PASS
442	198	50	100	84.9	19017	PASS
443	442	15	24	19.1	3632	PASS