


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE012220\
 Data File : BE101113.D
 Acq On : 22 Jan 2020 12:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE010820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 08 18:36:25 2020

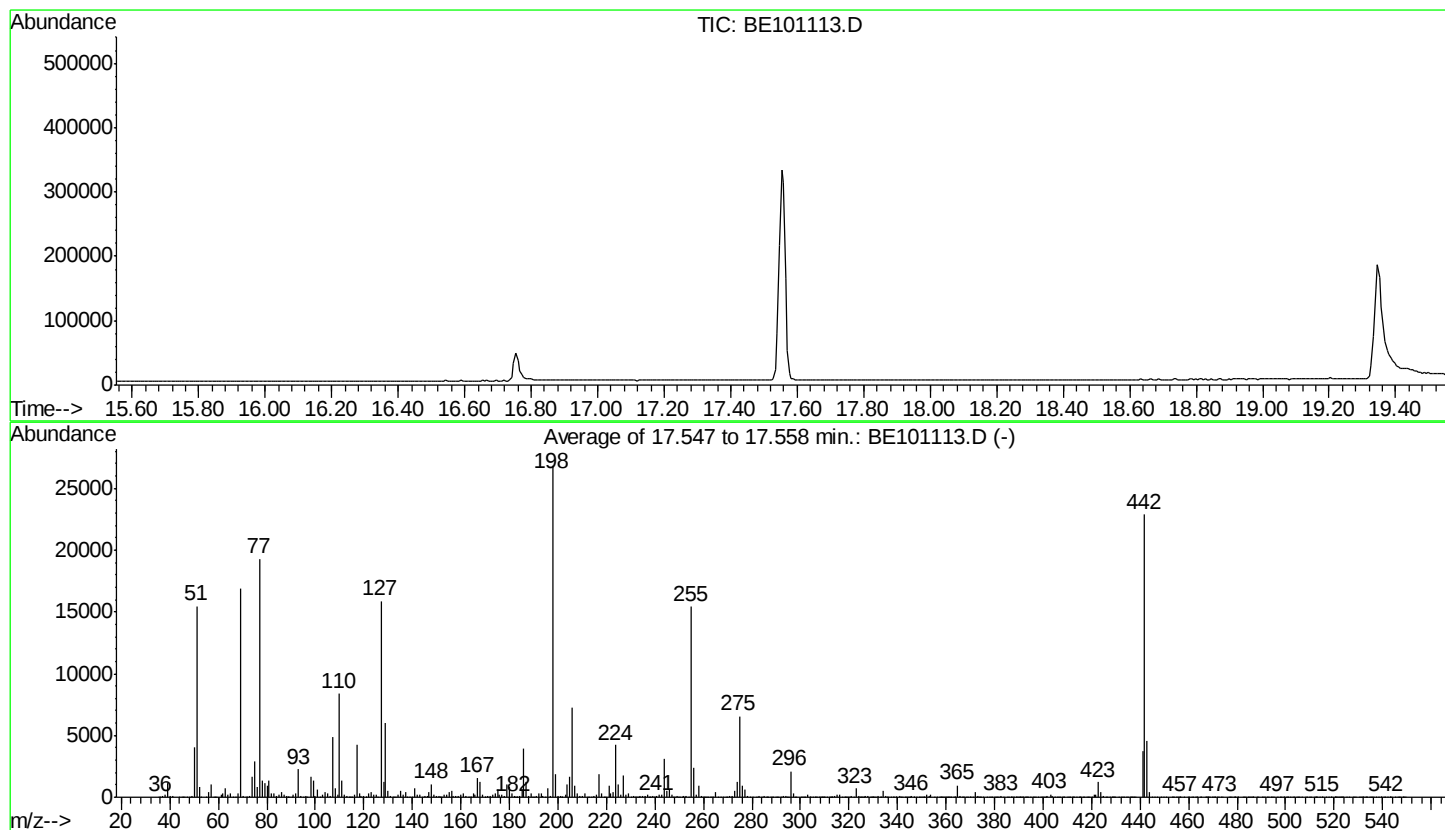

AutoFind: Scans 2546, 2547, 2548; Background Corrected with Scan 2539

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.6	15475	PASS
68	69	0.00	2	1.6	271	PASS
69	198	0.00	100	62.9	16885	PASS
70	69	0.00	2	0.3	58	PASS
127	198	10	80	59.1	15863	PASS
197	198	0.00	2	0.4	115	PASS
198	198	100	100	100.0	26844	PASS
199	198	5	9	7.0	1886	PASS
275	198	10	60	24.4	6545	PASS
365	198	1	100	3.6	953	PASS
441	198	0.01	100	13.7	3690	PASS
442	198	50	100	85.2	22881	PASS
443	442	15	24	19.9	4551	PASS