


n-Nitrosodimethylamine

Response Ratio

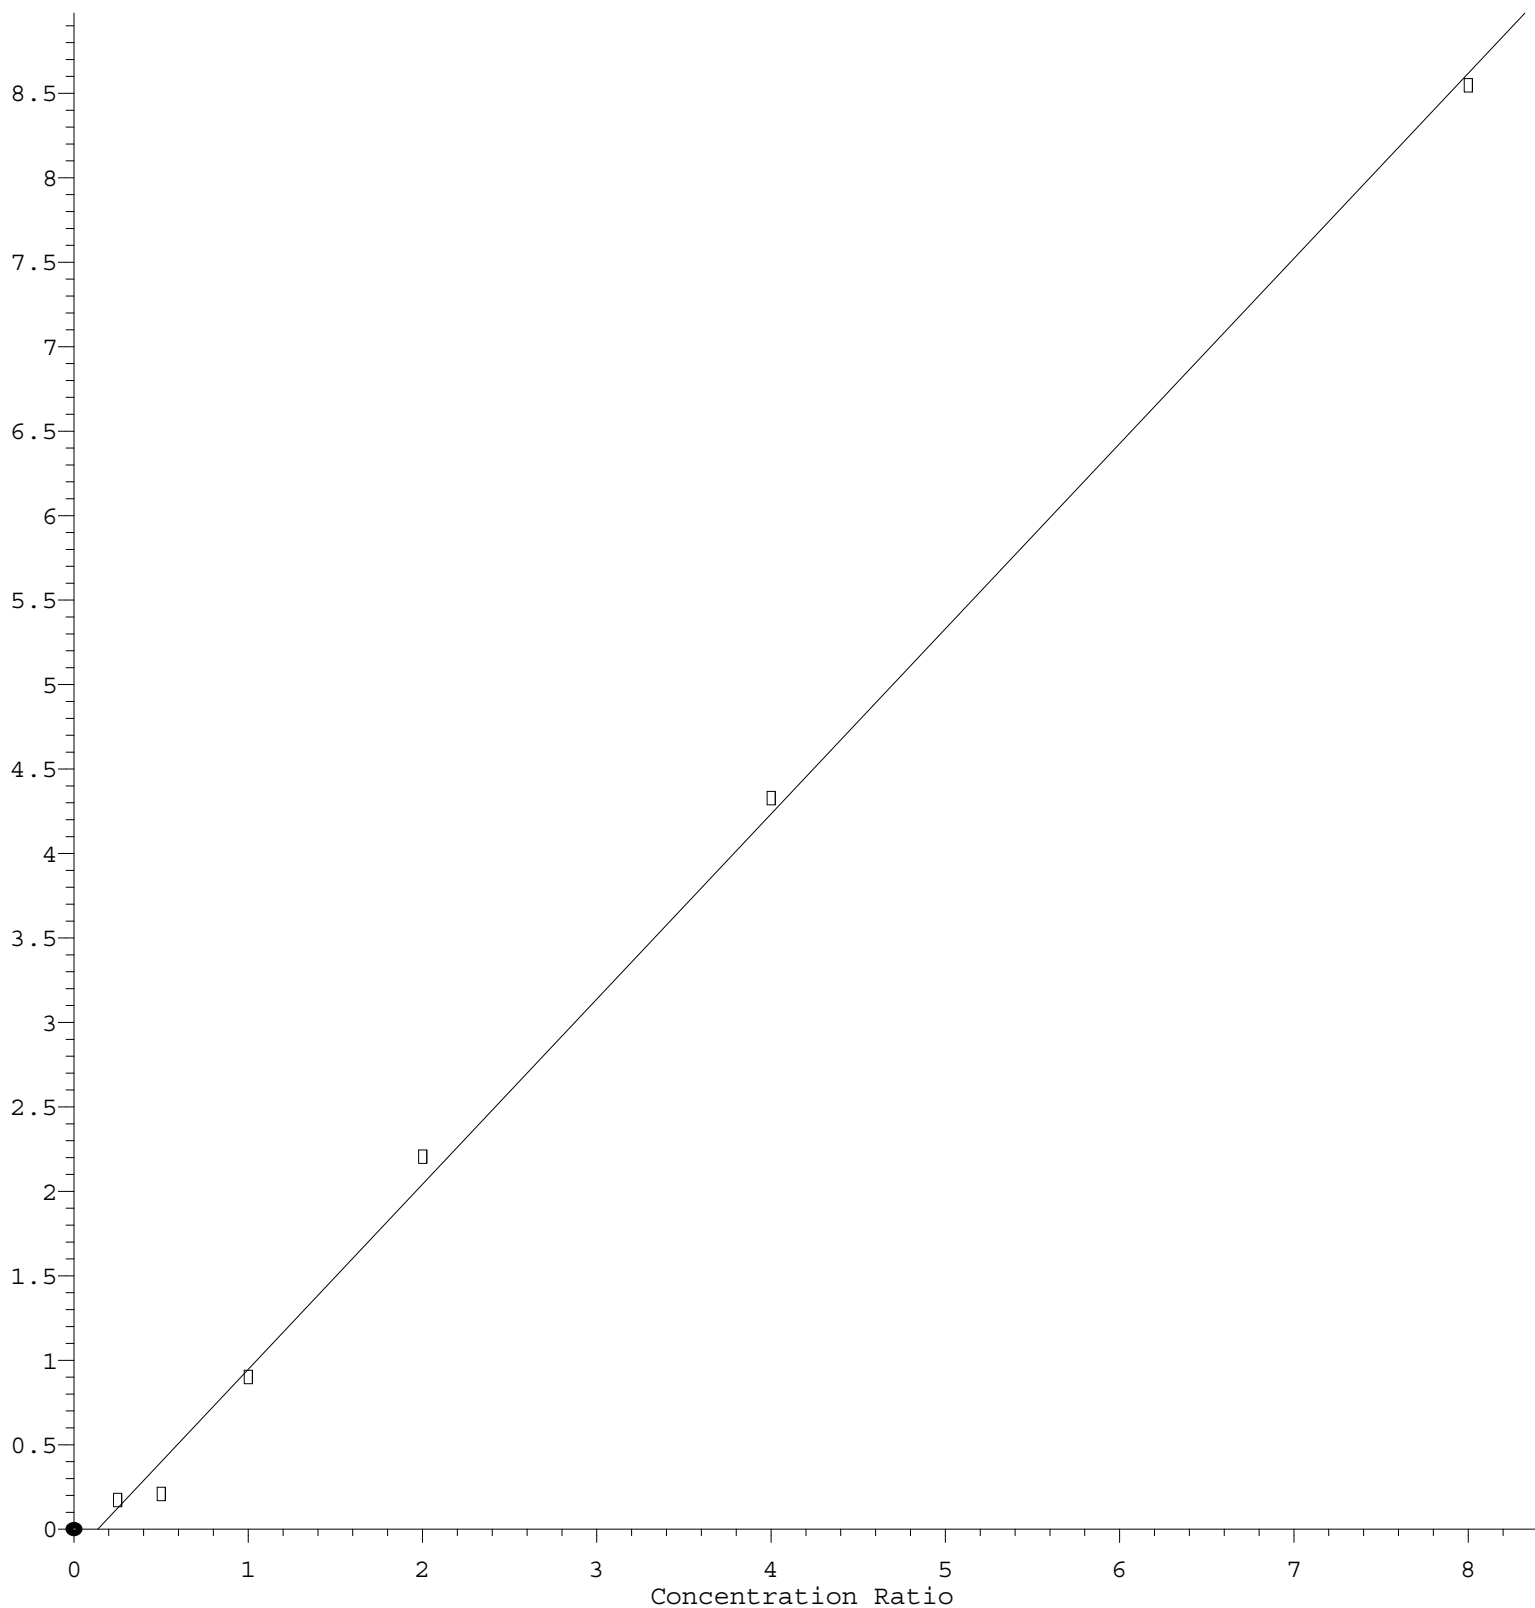

$$\text{Response} = 1.096e+000 * \text{Amt} - 1.506e-001$$


Coef of Det (r^2) = 0.998472 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE012419.M

Calibration Table Last Updated: Thu Jan 24 14:44:44 2019

Nitrobenzene-d5

Response Ratio

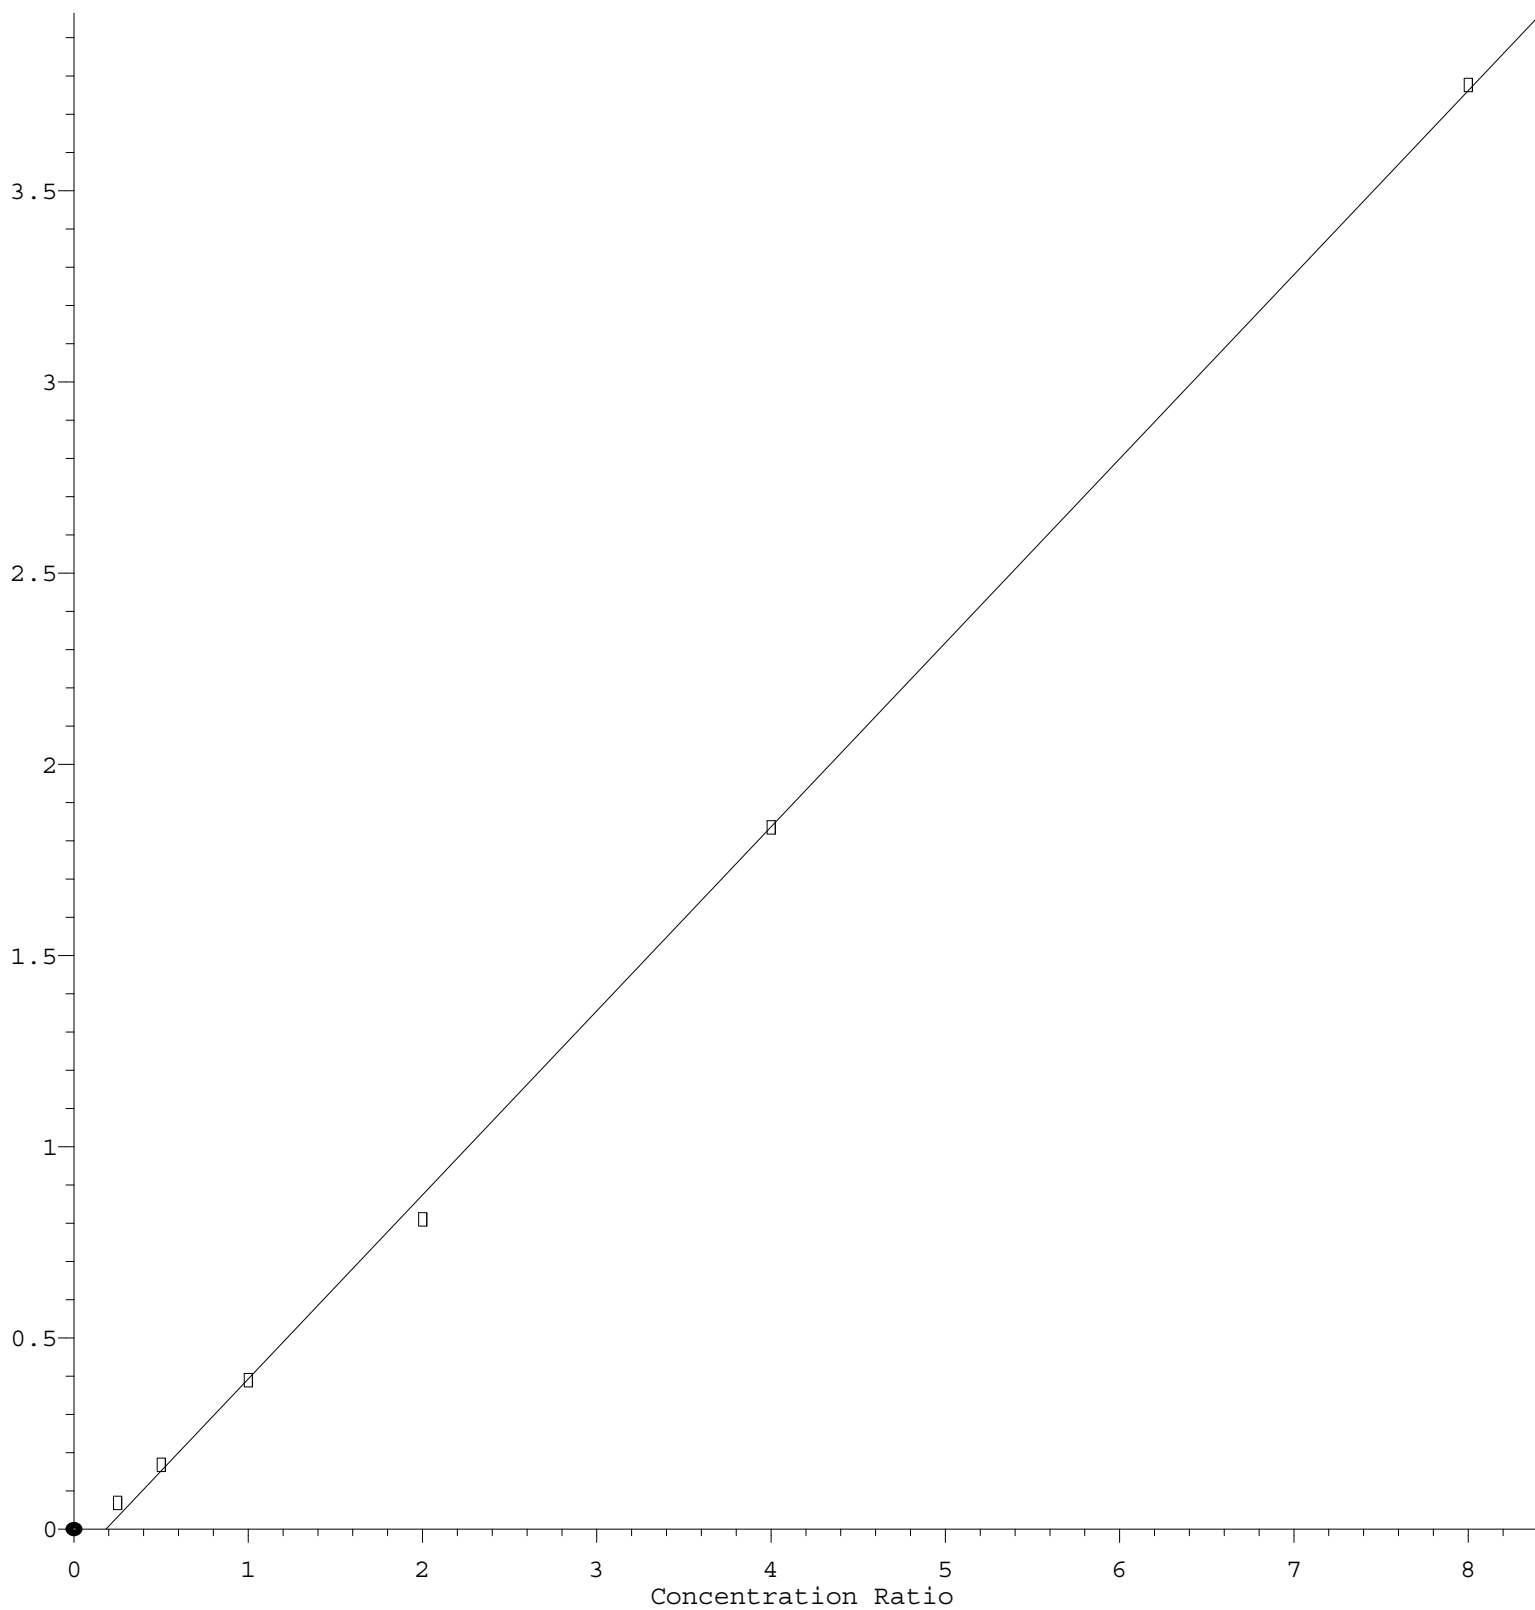

$$\text{Response} = 4.813\text{e-}001 * \text{Amt} - 8.867\text{e-}002$$


Coef of Det (r^2) = 0.999415 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE012419.M

Calibration Table Last Updated: Thu Jan 24 14:44:44 2019

Anthracene

Response Ratio

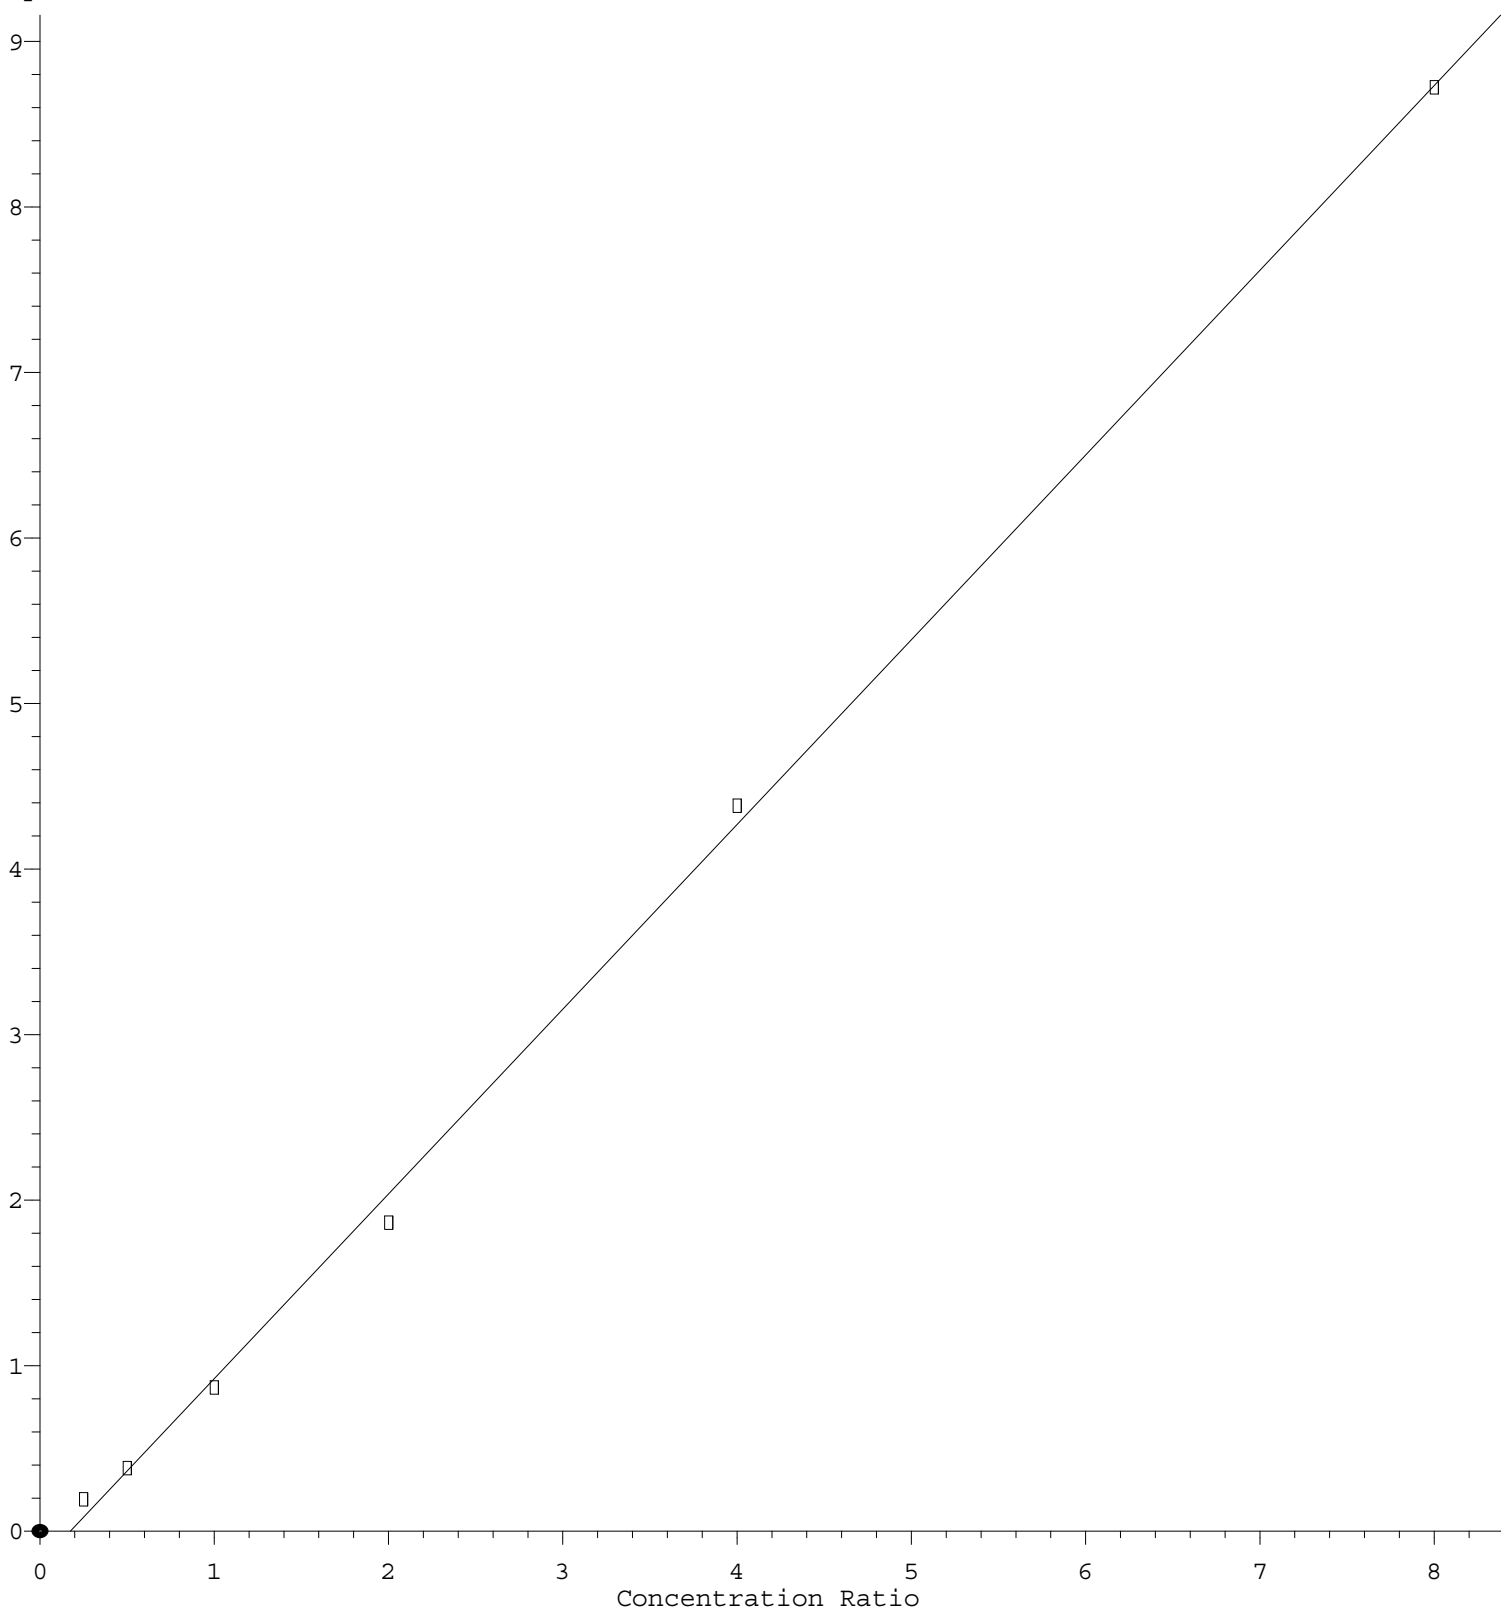

$$\text{Response} = 1.116\text{e}+000 * \text{Amt} - 1.946\text{e}-001$$


Coef of Det (r^2) = 0.998947 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE012419.M

Calibration Table Last Updated: Thu Jan 24 14:44:44 2019

1,4-Dioxane

Response Ratio

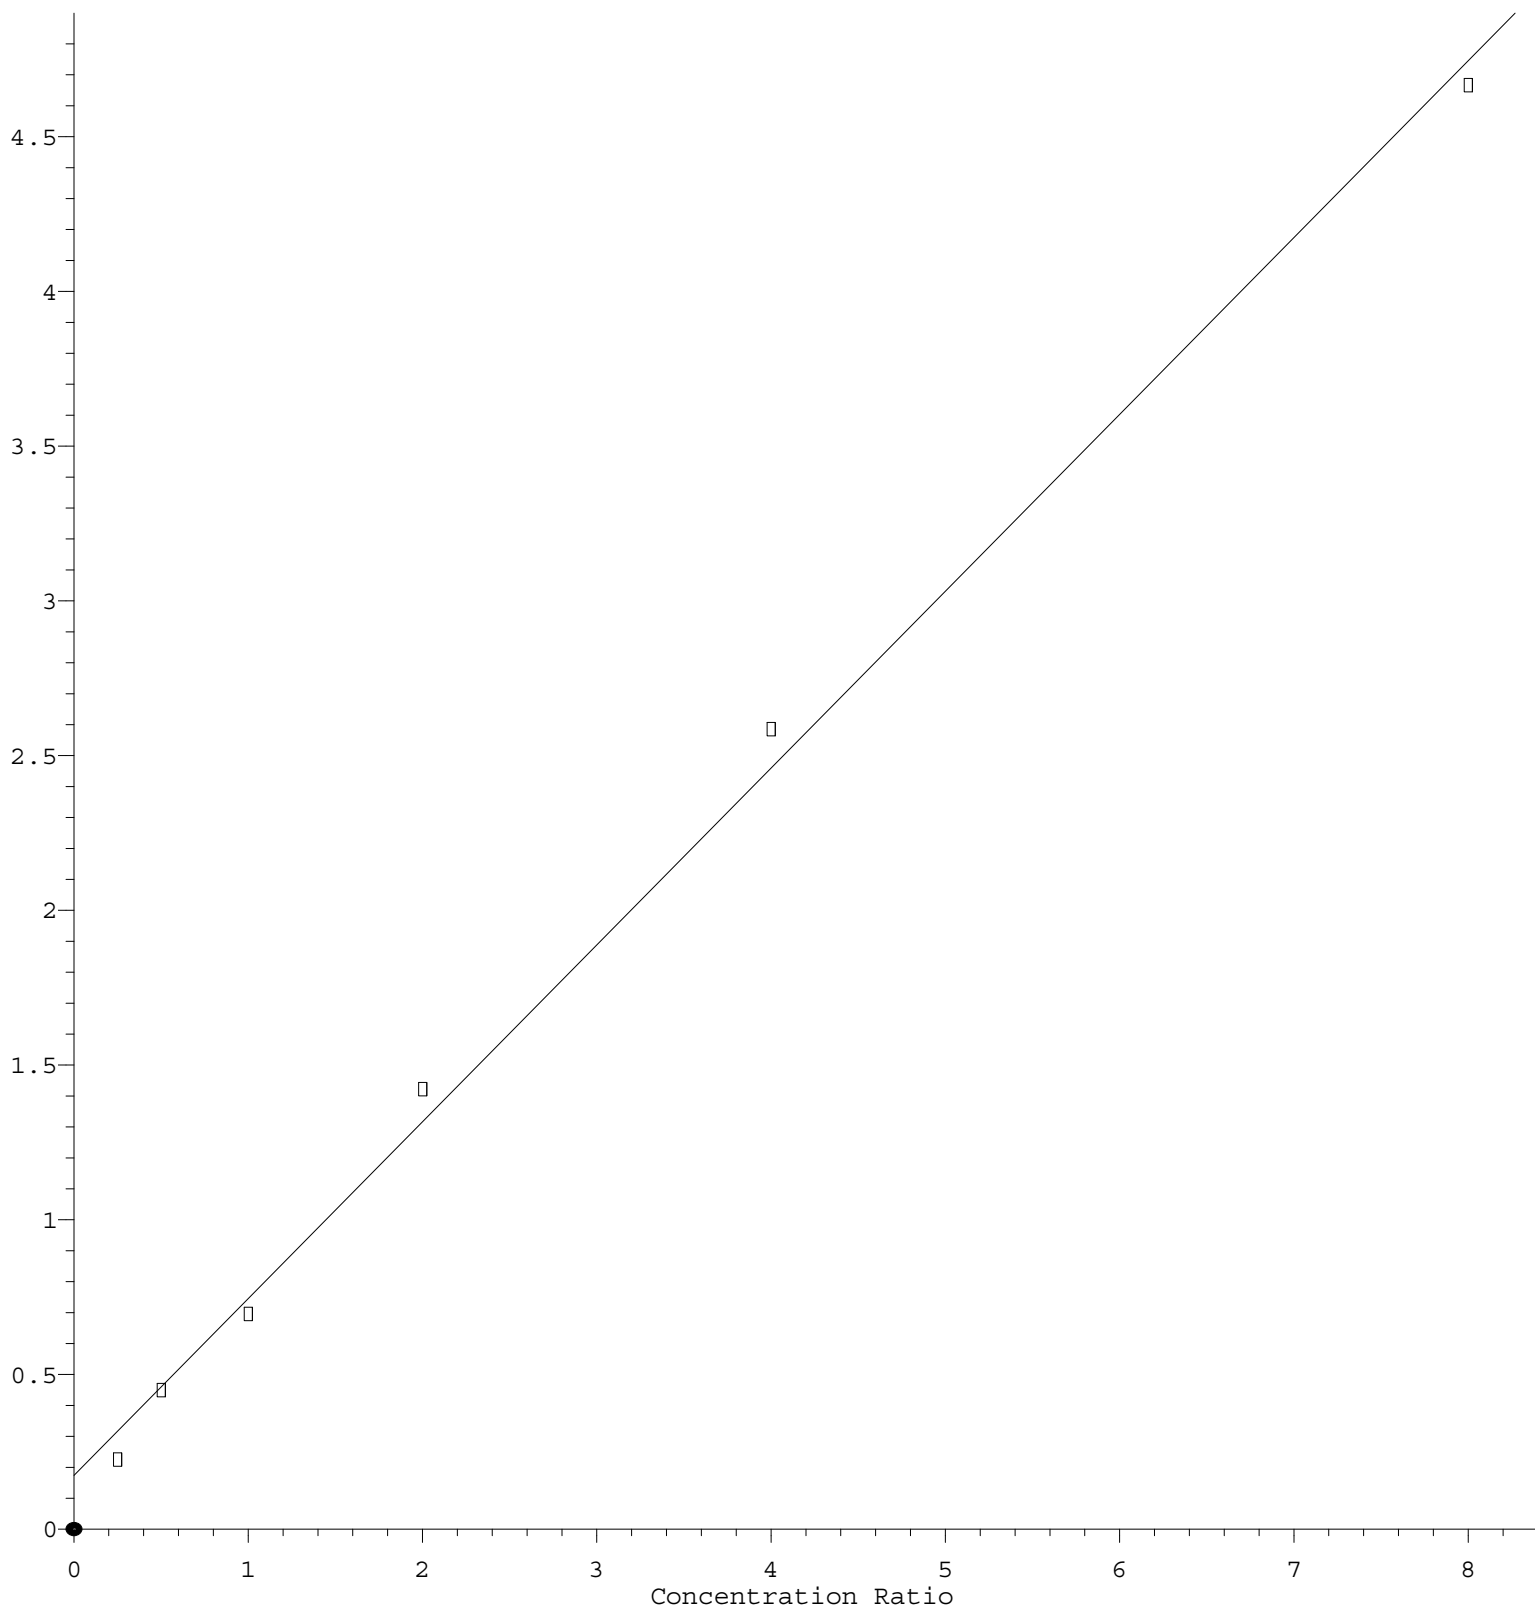

$$\text{Response} = 5.715\text{e-}001 * \text{Amt} + 1.738\text{e-}001$$

Coef of Det (r^2) = 0.996936 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE012419.M

Calibration Table Last Updated: Thu Jan 24 14:44:44 2019