

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE012419\
 Data File : BE098673.D
 Acq On : 24 Jan 2019 10:21
 Operator : SJ/JU
 Sample : SSTDICC0.1
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC0.1

Manual Integrations
 APPROVED

Sohil
 1/25/2019 10:06:31 AM

Quant Time: Jan 24 12:40:26 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE012419.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 24 12:37:26 2019
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.815	152	761	0.40	ng	0.00
7) Naphthalene-d8	10.615	136	3616	0.40	ng	# 0.01
13) Acenaphthene-d10	14.485	164	2473	0.40	ng	0.01
19) Phenanthrene-d10	17.229	188	5791	0.40	ng	# 0.00
27) Chrysene-d12	21.415	240	6605	0.40	ng	# 0.00
34) Perylene-d12	23.930	264	6355	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.420	112	247	0.12	ng	0.02
5) Phenol-d6	7.020	99	312	0.11	ng	0.02
8) Nitrobenzene-d5	9.004	82	347	0.12	ng	0.03
11) 2-Methylnaphthalene-d10	12.223	152	673	0.11	ng	0.01
14) 2,4,6-Tribromophenol	15.984	330	103	0.10	ng	0.00
15) 2-Fluorobiphenyl	13.102	172	1070	0.11	ng	0.00
25) Fluoranthene-d10	19.264	212	8614	0.12	ng	0.00
29) Terphenyl-d14	19.867	244	1634	0.11	ng	0.01
Target Compounds						Qvalue
2) 1,4-Dioxane	3.312	88	225	0.15	ng	# 80
3) n-Nitrosodimethylamine	3.692	42	68m	0.06	ng	
6) bis(2-Chloroethyl)ether	7.251	93	198	0.09	ng	# 51
9) Naphthalene	10.653	128	4226	0.12	ng	# 94
10) Hexachlorobutadiene	10.939	225	315	0.12	ng	96
12) 2-Methylnaphthalene	12.295	142	631	0.11	ng	95
16) Acenaphthylene	14.197	152	1163	0.11	ng	98
17) Acenaphthene	14.543	154	747	0.11	ng	98
18) Fluorene	15.529	166	995	0.11	ng	96
20) 4-Bromophenyl-phenylether	16.426	248	316	0.10	ng	98
21) Hexachlorobenzene	16.533	284	397	0.11	ng	95
23) Phenanthrene	17.269	178	1601	0.12	ng	97
24) Anthracene	17.376	178	1106	0.09	ng	# 94
26) Fluoranthene	19.293	202	2107	0.12	ng	99
28) Pyrene	19.655	202	2227	0.12	ng	100
30) Benzo(a)anthracene	21.402	228	1913	0.11	ng	# 94
31) Chrysene	21.451	228	2156	0.12	ng	96
32) Bis(2-ethylhexyl)phtha...	21.318	149	6146	0.16	ng	# 96
33) Indeno(1,2,3-cd)pyrene	26.588	276	1980	0.10	ng	97
35) Benzo(b)fluoranthene	23.164	252	1908	0.11	ng	# 80
36) Benzo(k)fluoranthene	23.210	252	2041	0.11	ng	# 80
37) Benzo(a)pyrene	23.823	252	1855	0.11	ng	# 77
38) Dibenzo(a,h)anthracene	26.609	278	1463m	0.10	ng	
39) Benzo(g,h,i)perylene	27.408	276	1869	0.11	ng	# 81

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE012419\
Data File : BE098673.D
Acq On : 24 Jan 2019 10:21
Operator : SJ/JU
Sample : SSTDICC0.1
Misc :
ALS Vial : 2 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
SSTDICC0.1

Manual Integrations
APPROVED

Sohil
1/25/2019 10:06:31 AM


Quant Time: Jan 24 12:40:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE012419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 24 12:37:26 2019
Response via : Initial Calibration

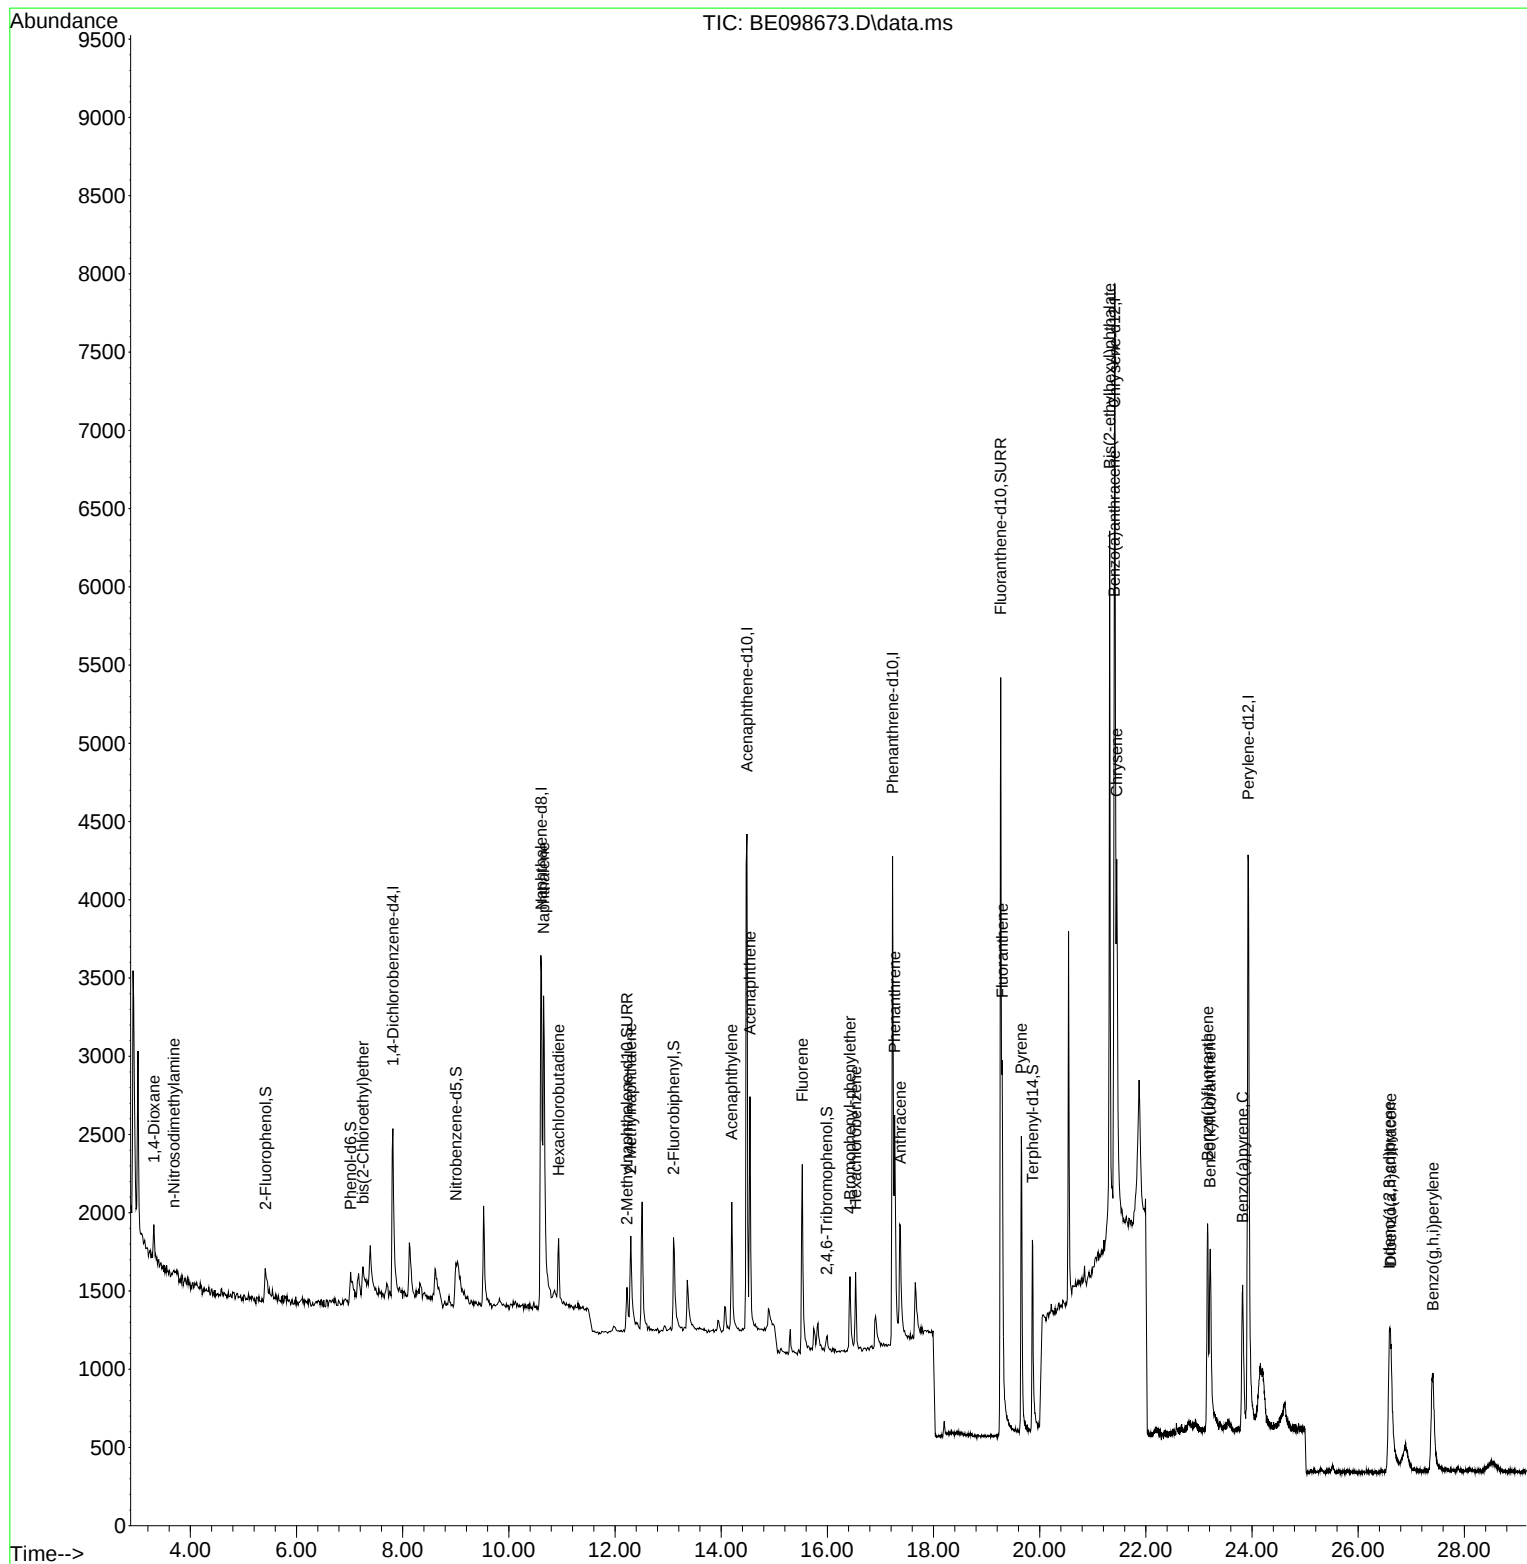

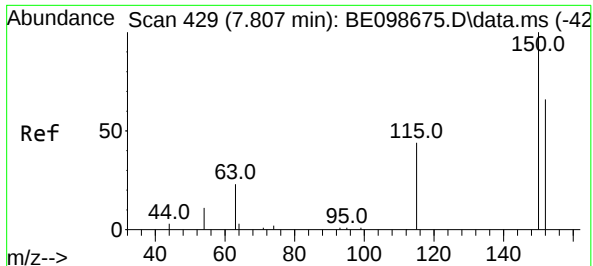

#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.815 min Scan# 430
 Delta R.T. 0.008 min
 Lab File: BE098673.D
 Acq: 24 Jan 2019 10:21

Instrument :
 BNA_E
 ClientSampled :
 SSTDICC0.1



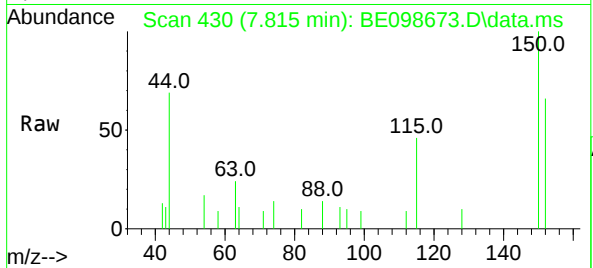


Tgt Ion: 152 Resp: 761

Ion	Ratio	Lower	Upper
152	100		
150	151.2	121.4	182.2
115	69.1	59.1	88.7

Manual Integrations
 APPROVED




Sohil
 1/25/2019 10:06:31 AM

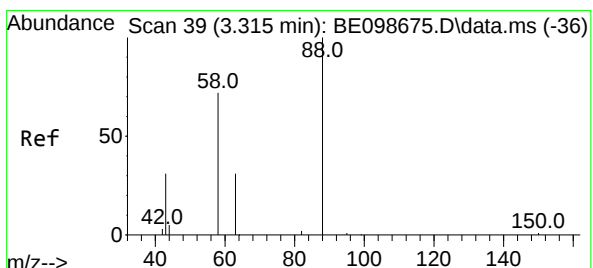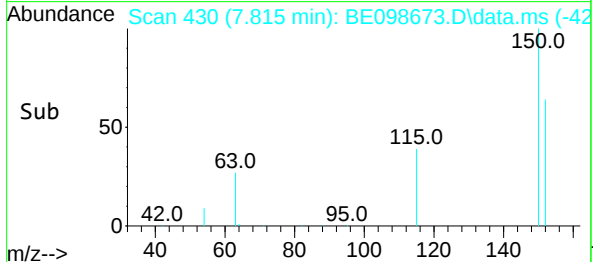

#2
 1,4-Dioxane
 Concen: 0.15 ng
 RT: 3.312 min Scan# 39
 Delta R.T. -0.003 min
 Lab File: BE098673.D
 Acq: 24 Jan 2019 10:21

Tgt Ion: 88 Resp: 225

Ion	Ratio	Lower	Upper
88	100		
58	63.1	73.9	110.9#
43	52.9	43.7	65.5

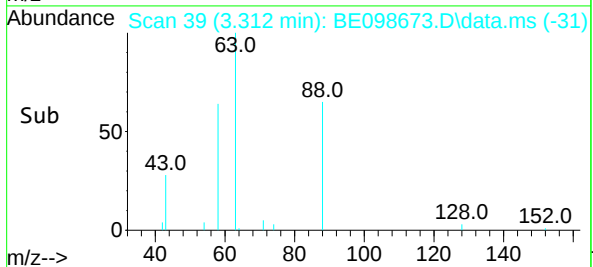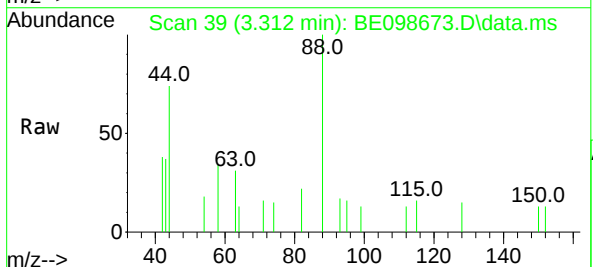







#3
n-Nitrosodimethylamine
Concen: 0.06 ng m
RT: 3.692 min Scan# 72
Delta R.T. 0.043 min
Lab File: BE098673.D
Acq: 24 Jan 2019 10:21

Tgt Ion: 42 Resp: 68
Ion Ratio Lower Upper
42 100
74 5.9 58.9 88.3#
44 33.8 0.0 0.0#

Instrument :
BNA_E
ClientSampled :
SSTDIC0.1




Manual Integrations
APPROVED


Sohil
1/25/2019 10:06:31 AM

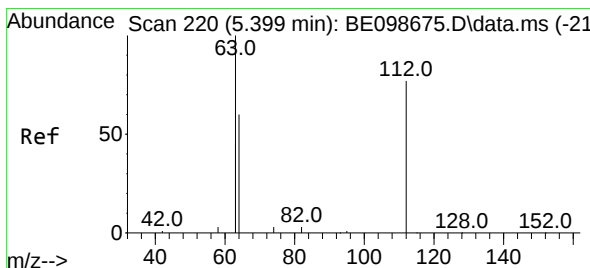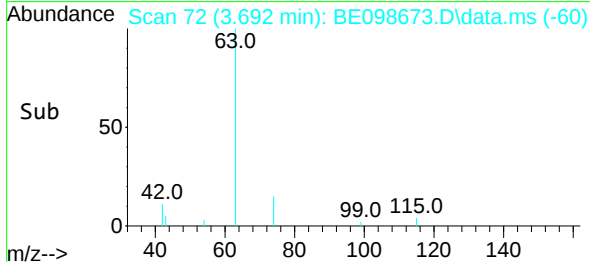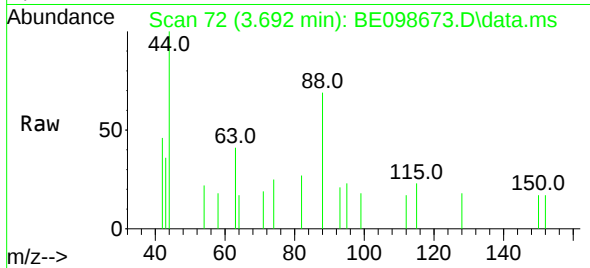

#4
2-Fluorophenol
Concen: 0.12 ng
RT: 5.420 min Scan# 222
Delta R.T. 0.020 min
Lab File: BE098673.D
Acq: 24 Jan 2019 10:21

Tgt Ion: 112 Resp: 247
Ion Ratio Lower Upper
112 100
64 67.2 62.9 94.3
63 175.3 152.2 228.4

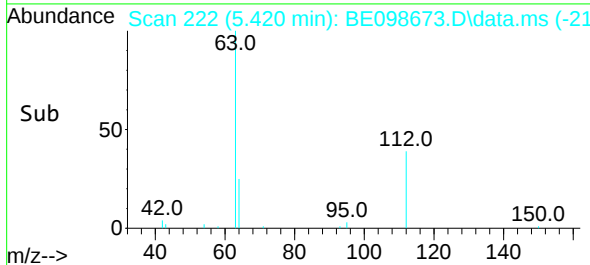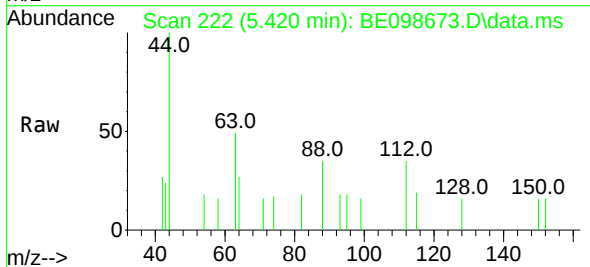







#5
Phenol-d6
Concen: 0.11 ng
RT: 7.020 min Scan# 361
Delta R.T. 0.020 min
Lab File: BE098673.D
Acq: 24 Jan 2019 10:21

Tgt Ion: 99 Resp: 312
Ion Ratio Lower Upper
99 100
42 34.6 24.6 37.0
71 50.3 35.1 52.7

Instrument :
BNA_E
ClientSampleId :
SSTDIC0.1




Manual Integrations
APPROVED

Sohil
1/25/2019 10:06:31 AM

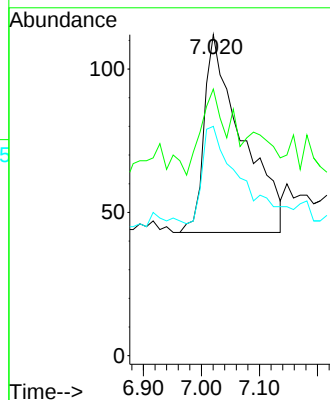

#6
bis(2-Chloroethyl)ether
Concen: 0.09 ng
RT: 7.251 min Scan# 381
Delta R.T. 0.009 min
Lab File: BE098673.D
Acq: 24 Jan 2019 10:21

Tgt Ion: 93 Resp: 198
Ion Ratio Lower Upper
93 100
63 224.7 267.3 400.9#
95 24.7 26.2 39.4#

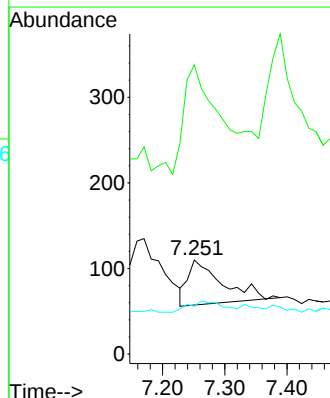







#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.615 min Scan# 650
Delta R.T. 0.013 min
Lab File: BE098673.D
Acq: 24 Jan 2019 10:21

Tgt Ion:	136	Resp:	3616
Ion Ratio	Lower	Upper	
136	100		
137	14.9	9.7	14.5#
54	42.4	35.5	53.3
68	6.8	5.0	7.6

Instrument :
BNA_E
ClientSampleId :
SSTDIC0.1




Manual Integrations
APPROVED


Sohil
1/25/2019 10:06:31 AM

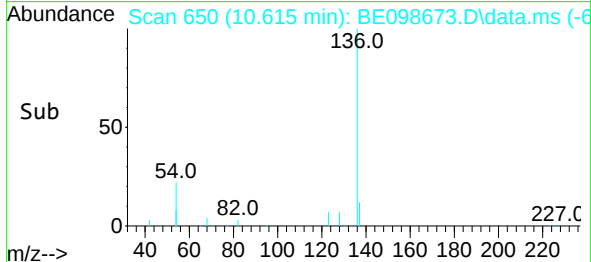

#8
Nitrobenzene-d5
Concen: 0.12 ng
RT: 9.004 min Scan# 526
Delta R.T. 0.026 min
Lab File: BE098673.D
Acq: 24 Jan 2019 10:21


Tgt Ion:	82	Resp:	347
Ion Ratio	Lower	Upper	
82	100		
128	237.8	96.5	144.7#
54	291.9	224.7	337.1

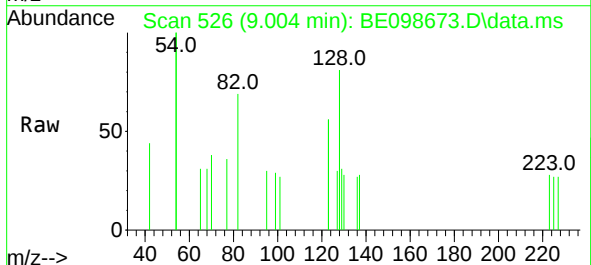



#9
Naphthalene
Concen: 0.12 ng
RT: 10.653 min Scan# 653
Delta R.T. 0.000 min
Lab File: BE098673.D
Acq: 24 Jan 2019 10:21




Instrument :
BNA_E
ClientSampleId :
SSTDIC0.1



Tgt Ion:128 Resp: 4226
Ion Ratio Lower Upper
128 100
129 5.1 2.6 3.8#
127 5.6 3.0 4.6#




Manual Integrations
APPROVED

Sohil
1/25/2019 10:06:31 AM

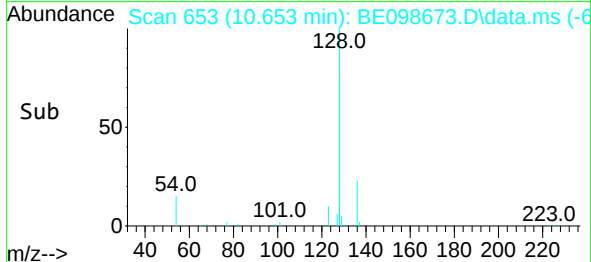

#10
Hexachlorobutadiene
Concen: 0.12 ng
RT: 10.939 min Scan# 675
Delta R.T. 0.000 min
Lab File: BE098673.D
Acq: 24 Jan 2019 10:21

Tgt Ion:225 Resp: 315
Ion Ratio Lower Upper
225 100
223 63.2 47.8 71.8
227 60.3 50.5 75.7

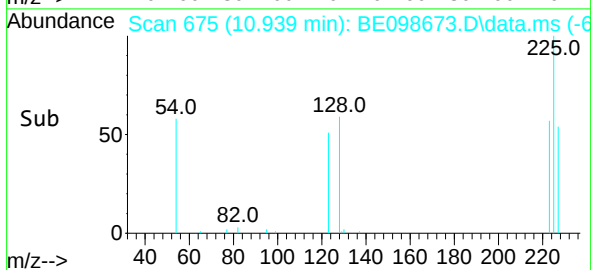







#11
2-Methylnaphthalene-d10
Concen: 0.11 ng
RT: 12.223 min Scan# 764
Delta R.T. 0.014 min
Lab File: BE098673.D
Acq: 24 Jan 2019 10:21

Instrument :
BNA_E
ClientSampleId :
SSTDICC0.1

Tgt Ion:152 Resp: 673
Ion Ratio Lower Upper
152 100
151 19.6 16.2 24.4




Manual Integrations
APPROVED


Sohil
1/25/2019 10:06:31 AM



#12
2-Methylnaphthalene
Concen: 0.11 ng
RT: 12.295 min Scan# 769
Delta R.T. 0.014 min
Lab File: BE098673.D
Acq: 24 Jan 2019 10:21

Tgt Ion:142 Resp: 631
Ion Ratio Lower Upper
142 100
141 84.0 70.0 105.0
115 48.6 35.2 52.8



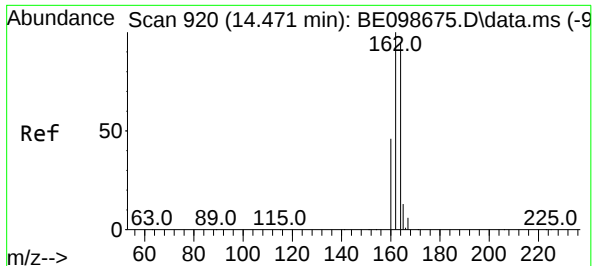

#13

Acenaphthene-d10

Concen: 0.40 ng

RT: 14.485 min Scan# 921

Delta R.T. 0.014 min

Lab File: BE098673.D

Acq: 24 Jan 2019 10:21

Tgt Ion:	164	Resp:	2473
Ion	Ratio	Lower	Upper
164	100		
162	96.1	80.5	120.7
160	45.4	40.1	60.1

Instrument :





BNA_E

ClientSampleId :

SSTDIC0.1

Manual Integrations
APPROVED

Sohil
1/25/2019 10:06:31 AM

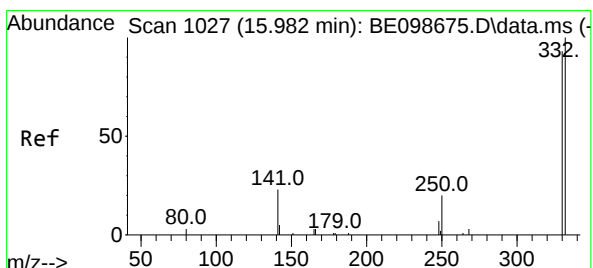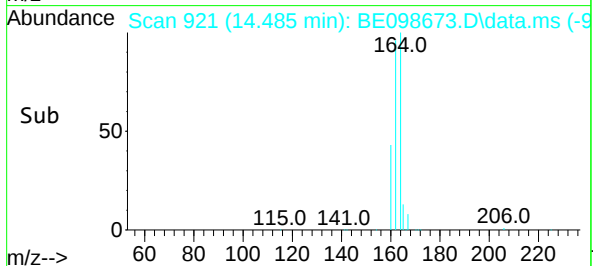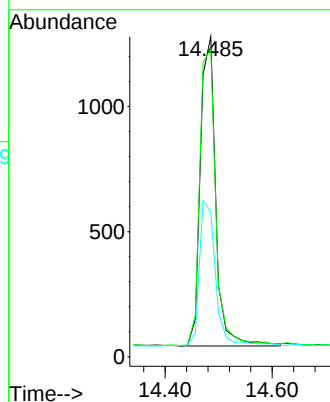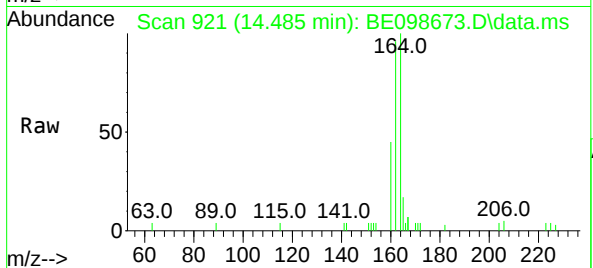

#14

2,4,6-Tribromophenol

Concen: 0.10 ng




RT: 15.984 min Scan# 1027


Delta R.T. 0.001 min

Lab File: BE098673.D

Acq: 24 Jan 2019 10:21

Tgt Ion:	330	Resp:	103
Ion	Ratio	Lower	Upper
330	100		
332	75.7	73.3	109.9
141	0.0	33.1	49.7

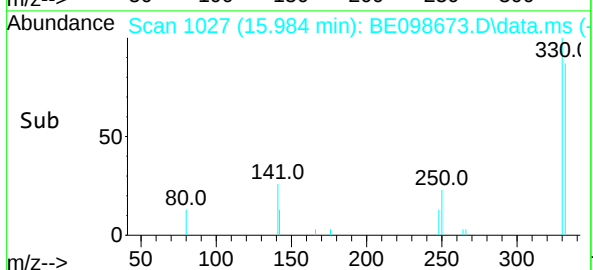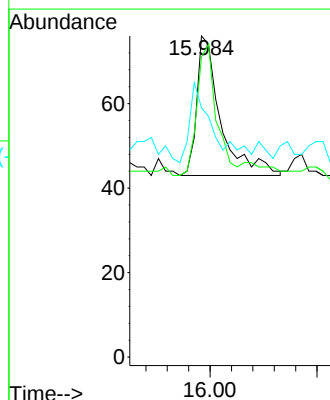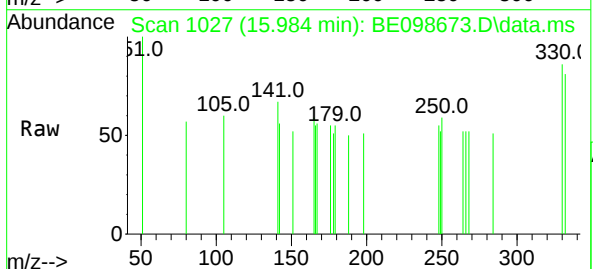







#15
2-Fluorobiphenyl
Concen: 0.11 ng
RT: 13.102 min Scan# 825
Delta R.T. -0.001 min
Lab File: BE098673.D
Acq: 24 Jan 2019 10:21

Tgt Ion:	172	Resp:	1070
Ion	Ratio	Lower	Upper
172	100		
171	41.6	29.0	43.4
170	34.2	20.8	31.2#

Instrument :
BNA_E
ClientSampleId :
SSTDIC0.1




Manual Integrations
APPROVED

Sohil
1/25/2019 10:06:31 AM

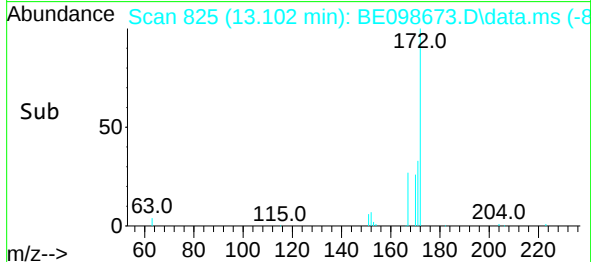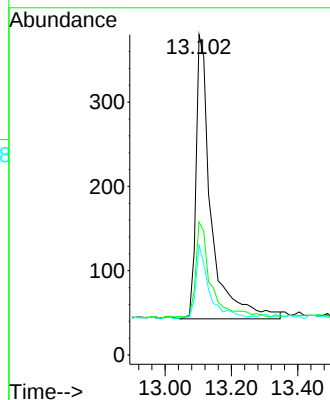

#16
Acenaphthylene
Concen: 0.11 ng
RT: 14.197 min Scan# 901
Delta R.T. -0.001 min
Lab File: BE098673.D
Acq: 24 Jan 2019 10:21

Tgt Ion:	152	Resp:	1163
Ion	Ratio	Lower	Upper
152	100		
151	21.0	16.3	24.5
153	14.4	10.7	16.1

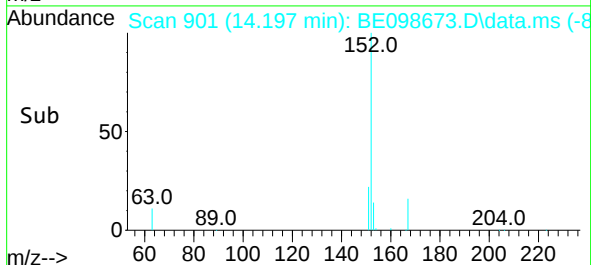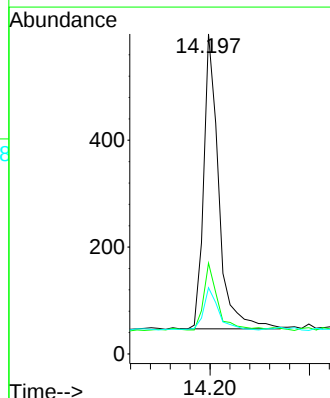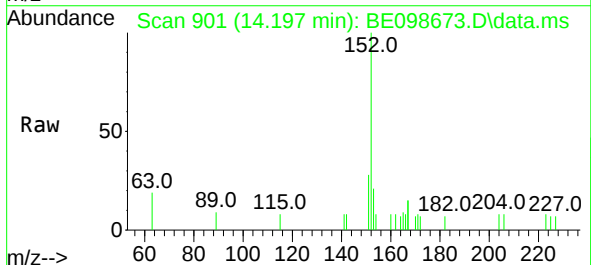



#17

Acenaphthene

Concen: 0.11 ng

RT: 14.543 min Scan# 925

Delta R.T. -0.001 min

Lab File: BE098673.D

Acq: 24 Jan 2019 10:21

Tgt Ion:	154	Resp:	747
Ion	Ratio	Lower	Upper
154	100		
153	119.5	93.9	140.9
152	59.4	45.8	68.8

Instrument :





BNA_E

ClientSampleId :

SSTDIC0.1

Manual Integrations
APPROVED

Sohil
1/25/2019 10:06:31 AM



#18

Fluorene

Concen: 0.11 ng




RT: 15.529 min Scan# 993


Delta R.T. 0.015 min

Lab File: BE098673.D

Acq: 24 Jan 2019 10:21


Tgt Ion:	166	Resp:	995
Ion	Ratio	Lower	Upper
166	100		
165	102.9	79.3	118.9
167	14.8	10.6	15.8

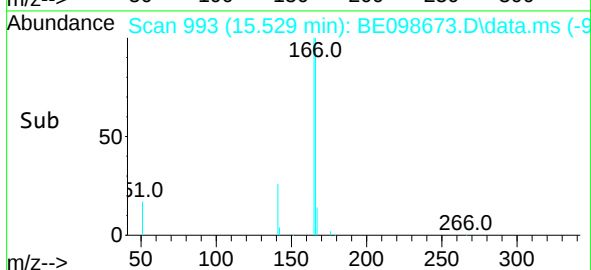

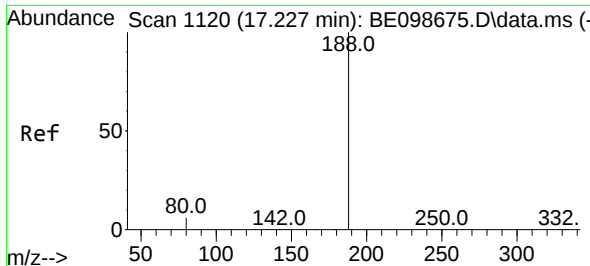

#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.229 min Scan# 1120
Delta R.T. 0.001 min
Lab File: BE098673.D
Acq: 24 Jan 2019 10:21




Instrument :
BNA_E
ClientSampleId :
SSTDIC0.1

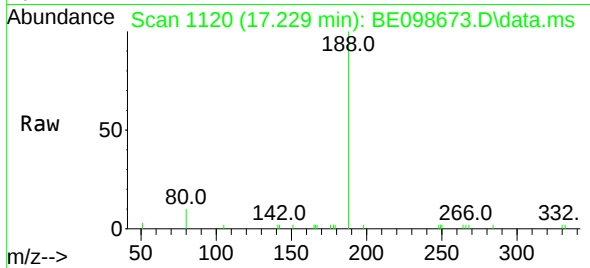


Tgt Ion:188 Resp: 5791
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 9.5 4.7 7.1#

Manual Integrations
APPROVED



Sohil
1/25/2019 10:06:31 AM

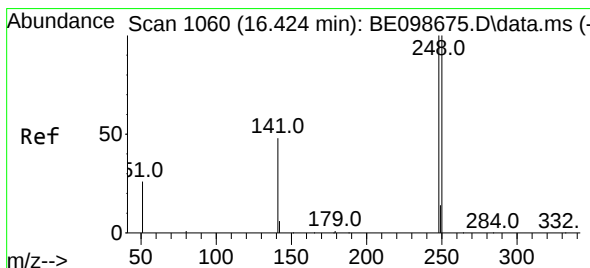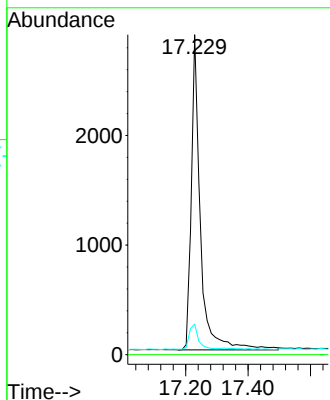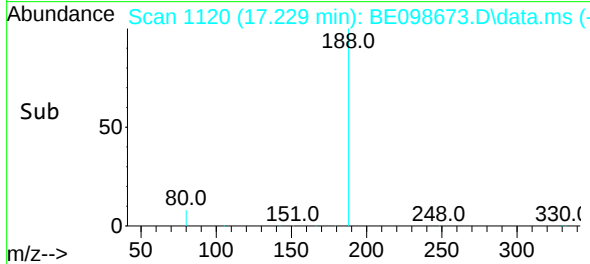


#20
4-Bromophenyl-phenylether
Concen: 0.10 ng
RT: 16.426 min Scan# 1060
Delta R.T. 0.001 min
Lab File: BE098673.D
Acq: 24 Jan 2019 10:21

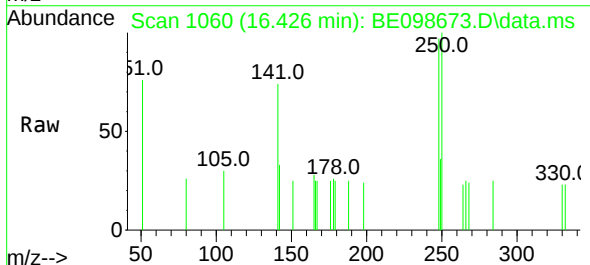


Tgt Ion:248 Resp: 316
Ion Ratio Lower Upper
248 100
250 102.7 80.2 120.4
141 76.1 60.5 90.7

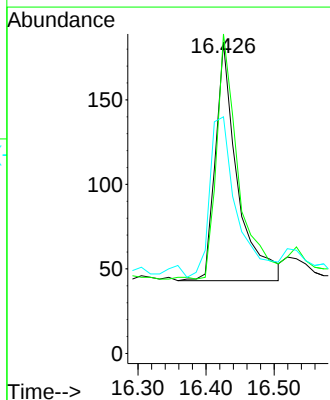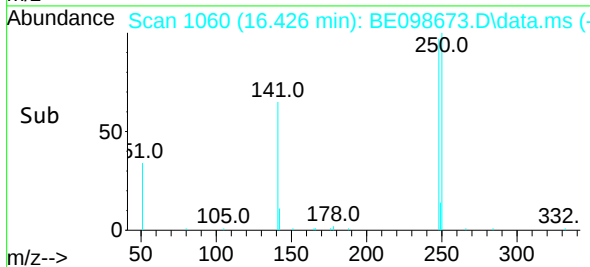



#21
Hexachlorobenzene
Concen: 0.11 ng
RT: 16.533 min Scan# 1068
Delta R.T. 0.001 min
Lab File: BE098673.D
Acq: 24 Jan 2019 10:21




Instrument :
BNA_E
ClientSampled :
SSTDIC0.1

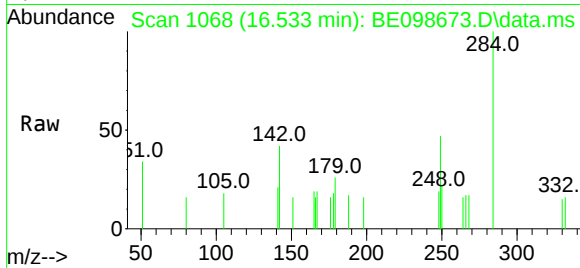


Tgt Ion:284 Resp: 397
Ion Ratio Lower Upper
284 100
142 33.0 25.5 38.3
249 37.5 26.6 39.8

Manual Integrations
APPROVED



Sohil
1/25/2019 10:06:31 AM

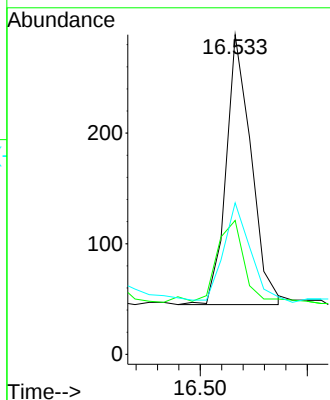


#23
Phenanthrene
Concen: 0.12 ng
RT: 17.269 min Scan# 1123
Delta R.T. 0.001 min
Lab File: BE098673.D
Acq: 24 Jan 2019 10:21

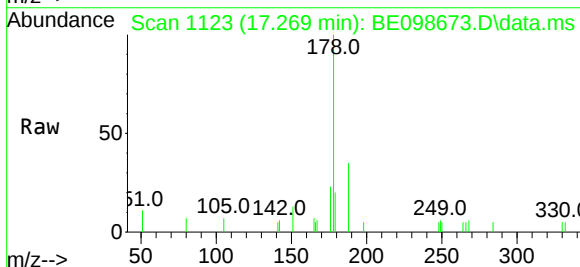


Tgt Ion:178 Resp: 1601
Ion Ratio Lower Upper
178 100
176 18.5 15.9 23.9
179 16.6 12.2 18.4


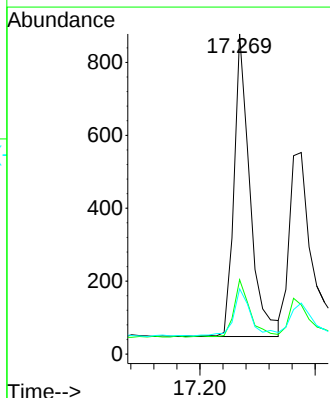






#24
 Anthracene
 Concen: 0.09 ng
 RT: 17.376 min Scan# 1131
 Delta R.T. 0.015 min
 Lab File: BE098673.D
 Acq: 24 Jan 2019 10:21

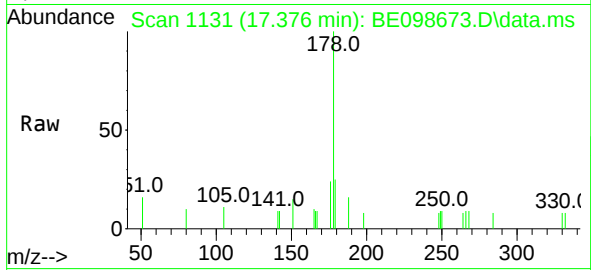



Tgt Ion:178 Resp: 1106
 Ion Ratio Lower Upper
 178 100
 176 21.1 14.9 22.3
 179 17.9 11.8 17.8#



#25
 Fluoranthene-d10
 Concen: 0.12 ng
 RT: 19.264 min Scan# 1392
 Delta R.T. 0.005 min
 Lab File: BE098673.D
 Acq: 24 Jan 2019 10:21




Tgt Ion:212 Resp: 8614
 Ion Ratio Lower Upper
 212 100
 106 2.0 1.7 2.5
 104 1.2 1.0 1.6




Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC0.1

Manual Integrations
 APPROVED




Sohil
 1/25/2019 10:06:31 AM




#26
Fluoranthene
Concen: 0.12 ng
RT: 19.293 min Scan# 1397
Delta R.T. 0.005 min
Lab File: BE098673.D
Acq: 24 Jan 2019 10:21





Tgt Ion:202 Resp: 2107
Ion Ratio Lower Upper
202 100
101 8.2 6.7 10.1
203 17.3 13.3 19.9



#27
Chrysene-d12
Concen: 0.40 ng
RT: 21.415 min Scan# 1634
Delta R.T. -0.000 min
Lab File: BE098673.D
Acq: 24 Jan 2019 10:21

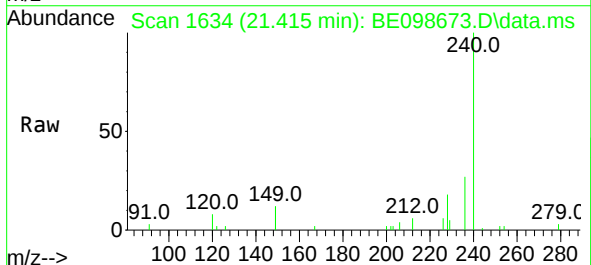


Tgt Ion:240 Resp: 6605
Ion Ratio Lower Upper
240 100
120 7.6 4.7 7.1#
236 27.3 21.9 32.9



Instrument :
BNA_E
ClientSampleId :
SSTDIC0.1

Manual Integrations
APPROVED

Sohil
1/25/2019 10:06:31 AM







#28
Pyrene
Concen: 0.12 ng
RT: 19.655 min Scan# 1460
Delta R.T. 0.005 min
Lab File: BE098673.D
Acq: 24 Jan 2019 10:21

Tgt Ion	Ratio	Lower	Upper
202	100		
200	21.4	17.0	25.6
203	17.0	13.8	20.8

Instrument :
BNA_E
ClientSampleId :
SSTDIC0.1




Manual Integrations
APPROVED


Sohil
1/25/2019 10:06:31 AM

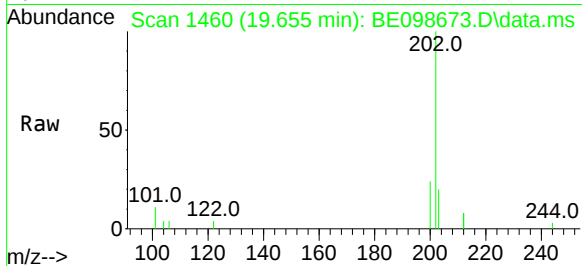


#29
Terphenyl-d14
Concen: 0.11 ng
RT: 19.867 min Scan# 1497
Delta R.T. 0.011 min
Lab File: BE098673.D
Acq: 24 Jan 2019 10:21

Tgt Ion	Ratio	Lower	Upper
244	100		
212	51.1	29.4	44.2#
122	12.3	7.1	10.7#



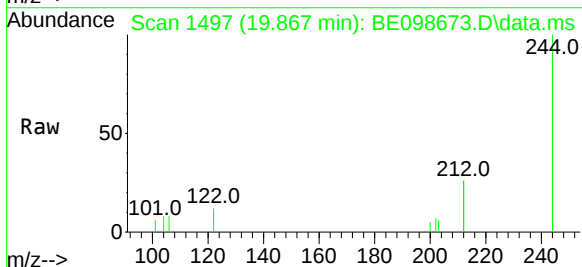





#30
Benzo(a)anthracene
Concen: 0.11 ng
RT: 21.402 min Scan# 1633
Delta R.T. 0.012 min
Lab File: BE098673.D
Acq: 24 Jan 2019 10:21





Tgt Ion:228 Resp: 1913
Ion Ratio Lower Upper
228 100
226 30.5 23.0 34.4
229 23.7 15.0 22.6#

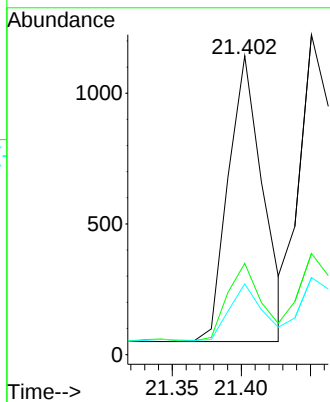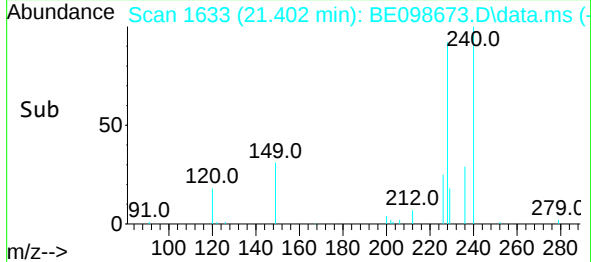

#31
Chrysene
Concen: 0.12 ng
RT: 21.451 min Scan# 1637
Delta R.T. -0.000 min
Lab File: BE098673.D
Acq: 24 Jan 2019 10:21

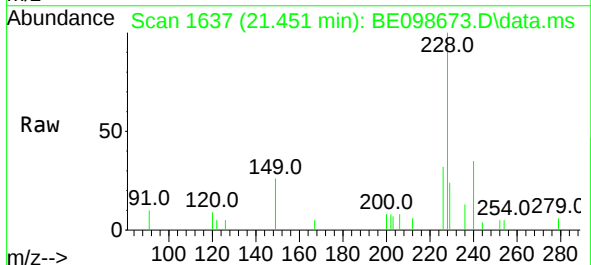


Tgt Ion:228 Resp: 2156
Ion Ratio Lower Upper
228 100
226 31.6 24.6 36.8
229 24.1 16.4 24.6

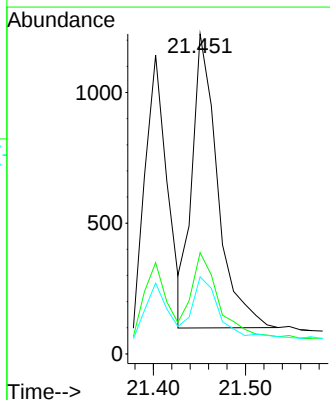


Instrument :
BNA_E
ClientSampled :
SSTDIC0.1

Manual Integrations
APPROVED



Sohil
1/25/2019 10:06:31 AM

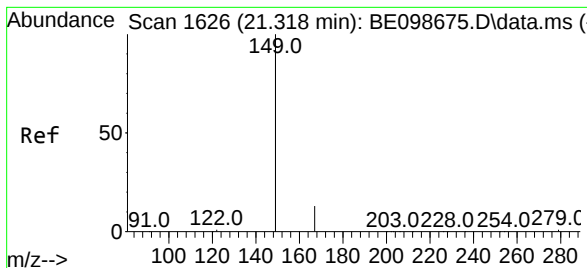

#32
 Bis(2-ethylhexyl)phthalate
 Concen: 0.16 ng
 RT: 21.318 min Scan# 1626
 Delta R.T. -0.000 min
 Lab File: BE098673.D
 Acq: 24 Jan 2019 10:21

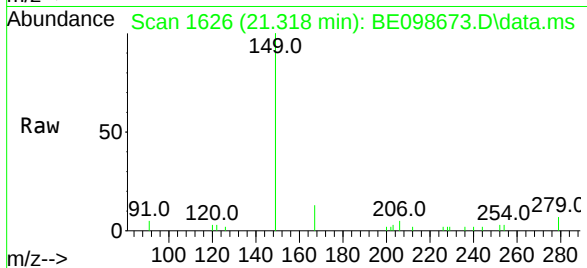


Tgt Ion:149 Resp: 6146
 Ion Ratio Lower Upper
 149 100
 167 5.8 5.4 8.2
 279 5.5 1.0 1.4#

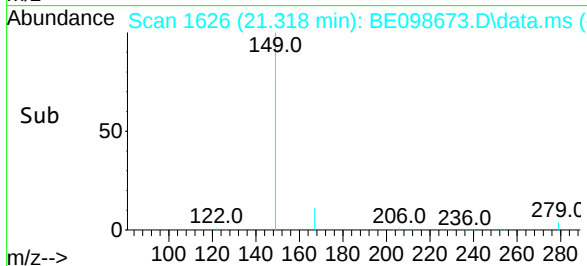


Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC0.1

Manual Integrations
 APPROVED



Sohil
 1/25/2019 10:06:31 AM

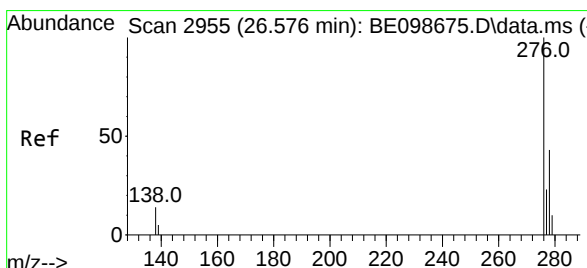


#33
 Indeno(1,2,3-cd)pyrene
 Concen: 0.10 ng
 RT: 26.588 min Scan# 2958
 Delta R.T. 0.011 min
 Lab File: BE098673.D
 Acq: 24 Jan 2019 10:21

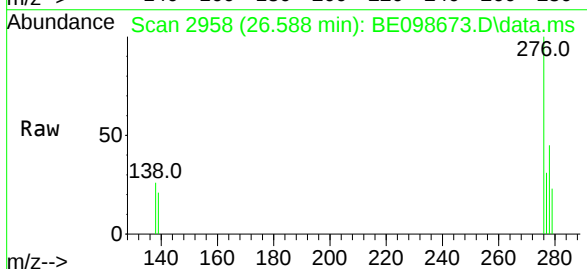


Tgt Ion:276 Resp: 1980
 Ion Ratio Lower Upper
 276 100
 138 14.0 13.3 19.9
 277 23.9 19.4 29.0



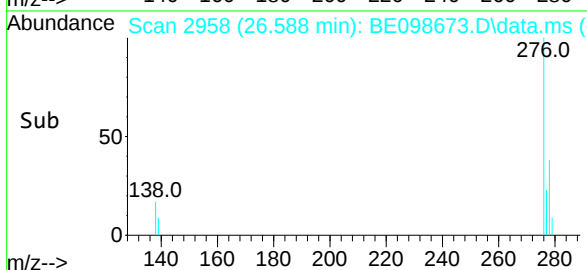





#34
Perylene-d12
Concen: 0.40 ng
RT: 23.930 min Scan# 2217
Delta R.T. 0.003 min
Lab File: BE098673.D
Acq: 24 Jan 2019 10:21





Tgt Ion:264 Resp: 6355
Ion Ratio Lower Upper
264 100
260 25.5 20.5 30.7
265 28.6 22.3 33.5



#35
Benzo(b)fluoranthene
Concen: 0.11 ng
RT: 23.164 min Scan# 2002
Delta R.T. 0.010 min
Lab File: BE098673.D
Acq: 24 Jan 2019 10:21

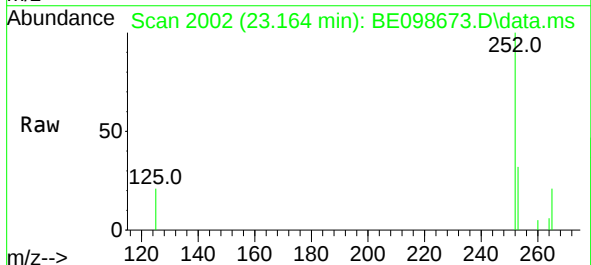


Tgt Ion:252 Resp: 1908
Ion Ratio Lower Upper
252 100
253 32.4 19.4 29.0#
125 20.9 8.2 12.4#



Instrument :
BNA_E
ClientSampleId :
SSTDIC0.1

Manual Integrations
APPROVED

Sohil
1/25/2019 10:06:31 AM







#36
Benzo(k)fluoranthene
Concen: 0.11 ng
RT: 23.210 min Scan# 2015
Delta R.T. 0.007 min
Lab File: BE098673.D
Acq: 24 Jan 2019 10:21

Tgt Ion:252 Resp: 2041
Ion Ratio Lower Upper
252 100
253 33.4 19.0 28.4#
125 16.3 7.0 10.4#

Instrument :
BNA_E
ClientSampleId :
SSTDIC0.1




Manual Integrations
APPROVED


Sohil
1/25/2019 10:06:31 AM



#37
Benzo(a)pyrene
Concen: 0.11 ng
RT: 23.823 min Scan# 2187
Delta R.T. 0.010 min
Lab File: BE098673.D
Acq: 24 Jan 2019 10:21

Tgt Ion:252 Resp: 1855
Ion Ratio Lower Upper
252 100
253 37.2 21.0 31.4#
125 21.2 9.2 13.8#

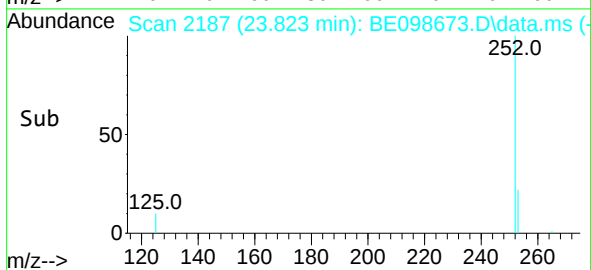







#38
Dibenzo(a,h)anthracene
Concen: 0.10 ng m
RT: 26.609 min Scan# 2964
Delta R.T. 0.011 min
Lab File: BE098673.D
Acq: 24 Jan 2019 10:21

Tgt Ion: 278 Resp: 1463
Ion Ratio Lower Upper
278 100
139 30.9 12.7 19.1#
279 42.5 22.0 33.0#

Instrument :
BNA_E
ClientSampled :
SSTDIC0.1

Manual Integrations
APPROVED

Sohil
1/25/2019 10:06:31 AM



#39
Benzo(g,h,i)perylene
Concen: 0.11 ng
RT: 27.408 min Scan# 3188
Delta R.T. 0.019 min
Lab File: BE098673.D
Acq: 24 Jan 2019 10:21

Tgt Ion: 276 Resp: 1869
Ion Ratio Lower Upper
276 100
277 33.9 20.3 30.5#
138 26.2 13.3 19.9#

