
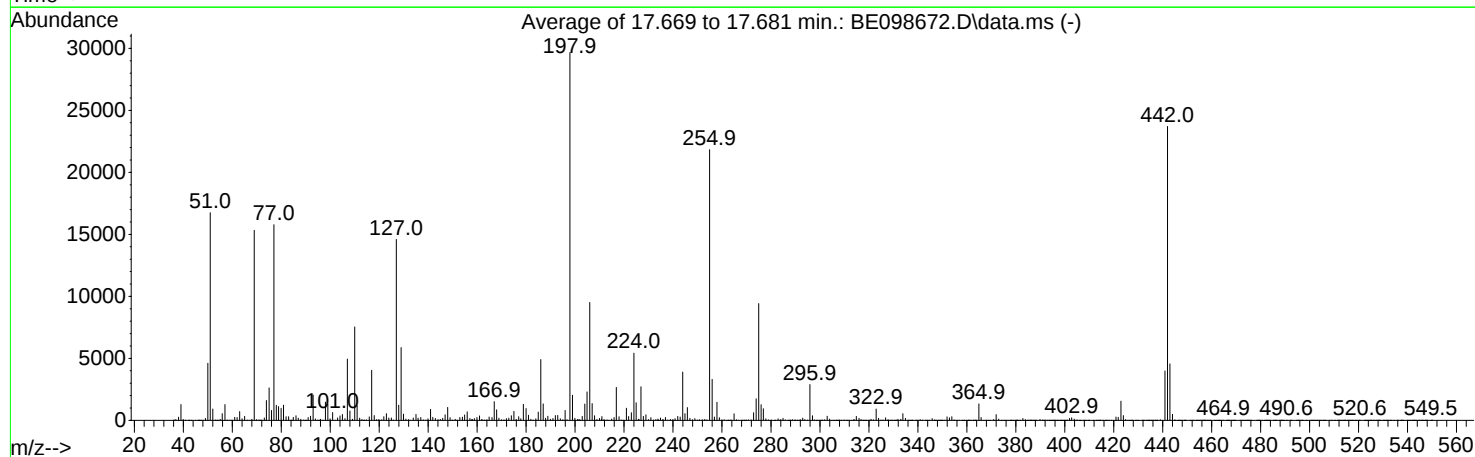


Data Path : Z:\svoasrv\HPCHEM1\BNA\_E\Data\BE012419\  
 Data File : BE098672.D  
 Acq On : 24 Jan 2019 9:42  
 Operator : SJ/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_E\METHODS\8270-SIM-BE012419.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Jan 24 14:44:44 2019

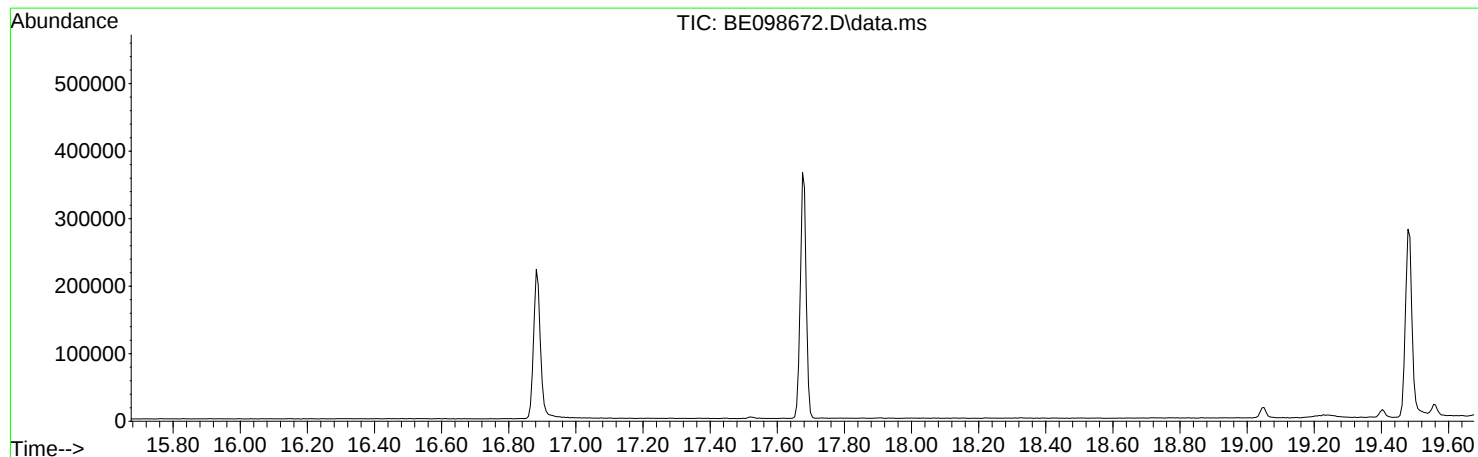

AutoFind: Scans 2567, 2568, 2569; Background Corrected with Scan 2558

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 56.5         | 16752      | PASS                |
| 68             | 69              | 0.00            | 2               | 0.6          | 96         | PASS                |
| 69             | 198             | 0.00            | 100             | 51.7         | 15329      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.4          | 59         | PASS                |
| 127            | 198             | 10              | 80              | 49.2         | 14590      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.2          | 49         | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 29665      | PASS                |
| 199            | 198             | 5               | 9               | 6.8          | 2024       | PASS                |
| 275            | 198             | 10              | 60              | 31.8         | 9420       | PASS                |
| 365            | 198             | 1               | 100             | 4.5          | 1328       | PASS                |
| 441            | 198             | 0.01            | 100             | 13.5         | 3991       | PASS                |
| 442            | 198             | 50              | 100             | 79.9         | 23698      | PASS                |
| 443            | 442             | 15              | 24              | 19.2         | 4561       | PASS                |