
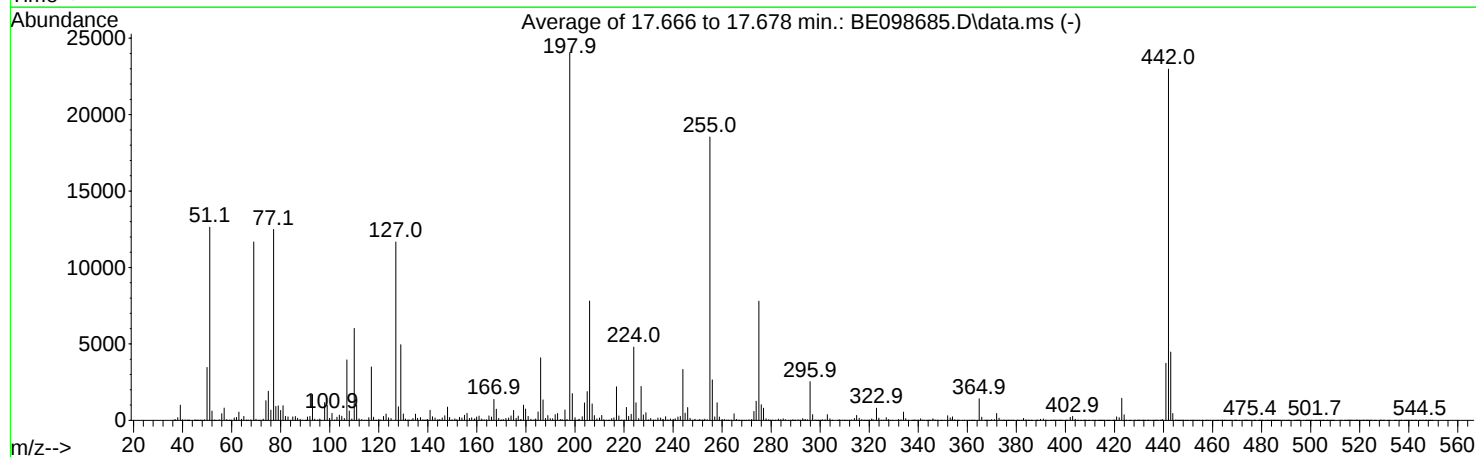


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE020119\
 Data File : BE098685.D
 Acq On : 1 Feb 2019 9:22
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE012419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 24 14:44:44 2019

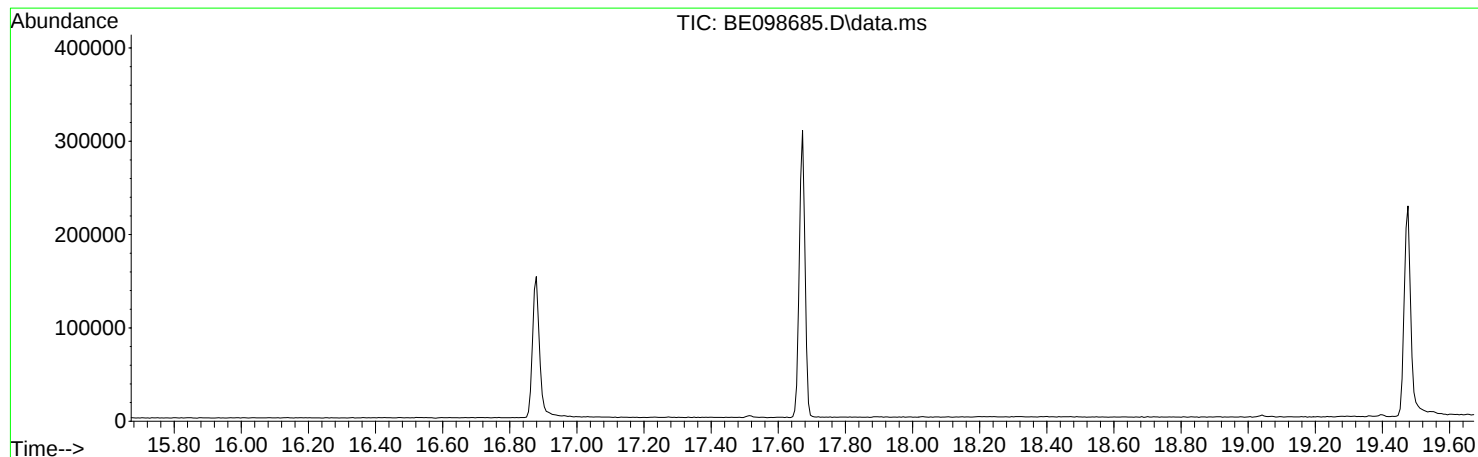

AutoFind: Scans 2566, 2567, 2568; Background Corrected with Scan 2554

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.5	12636	PASS
68	69	0.00	2	0.3	32	PASS
69	198	0.00	100	48.5	11667	PASS
70	69	0.00	2	0.6	75	PASS
127	198	10	80	48.5	11670	PASS
197	198	0.00	2	0.3	68	PASS
198	198	100	100	100.0	24063	PASS
199	198	5	9	7.2	1744	PASS
275	198	10	60	32.4	7800	PASS
365	198	1	100	5.9	1411	PASS
441	198	0.01	100	15.5	3733	PASS
442	198	50	100	95.5	22973	PASS
443	442	15	24	19.5	4473	PASS