
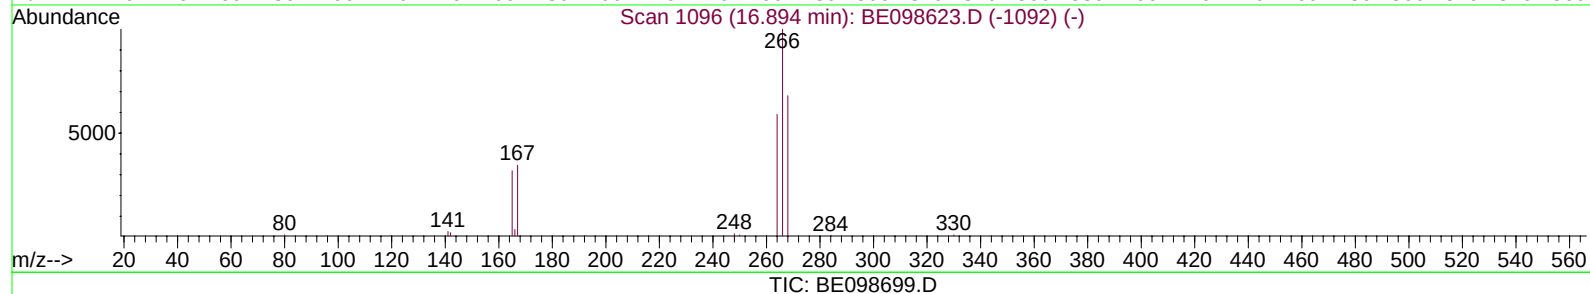
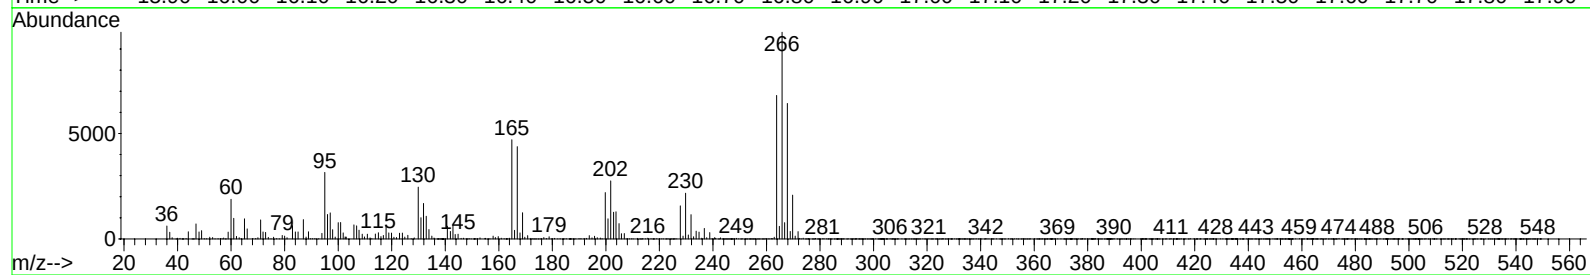


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE020419\
Data File : BE098699.D
Acq On : 4 Feb 2019 8:52
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 04 18:12:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE011519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 15 14:30:55 2019
Response via : Initial Calibration

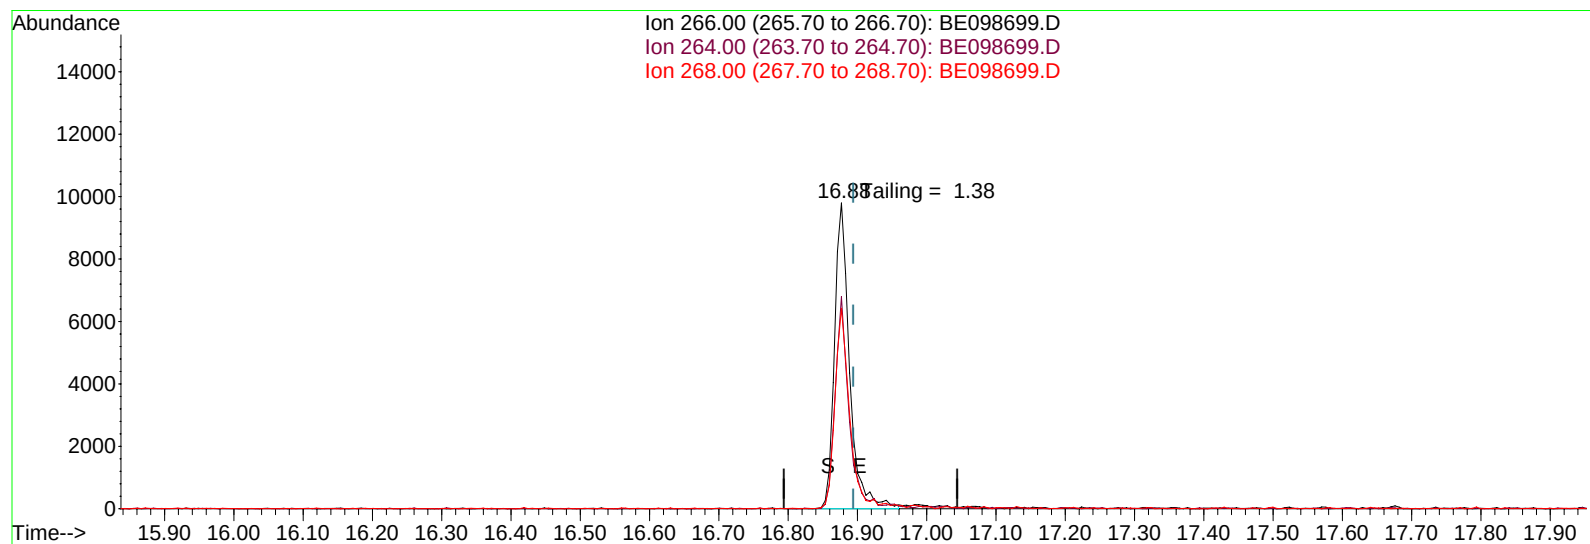

(22) Pentachlorophenol

16.877min (-0.017) 3099.60ng

response 14769

Ion	Exp%	Act%
266.00	100	100
264.00	67.10	69.41
268.00	74.80	65.57
0.00	0.00	0.00