
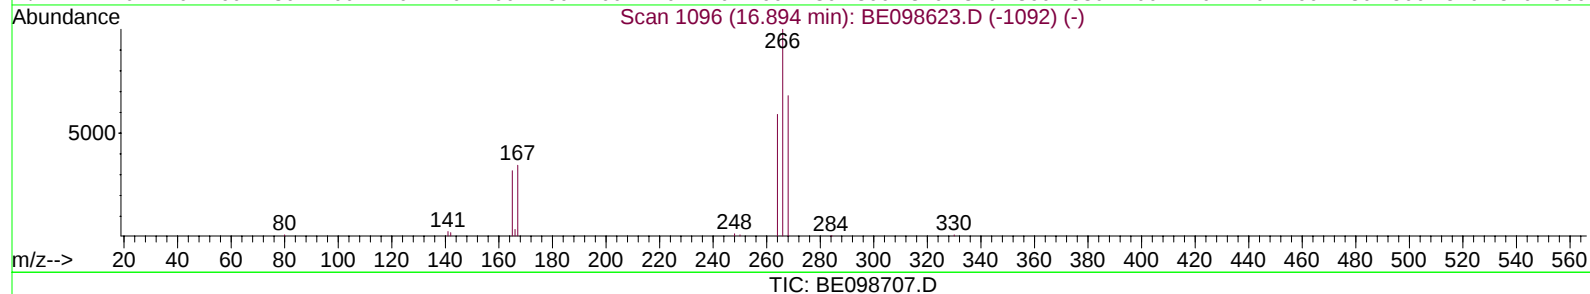
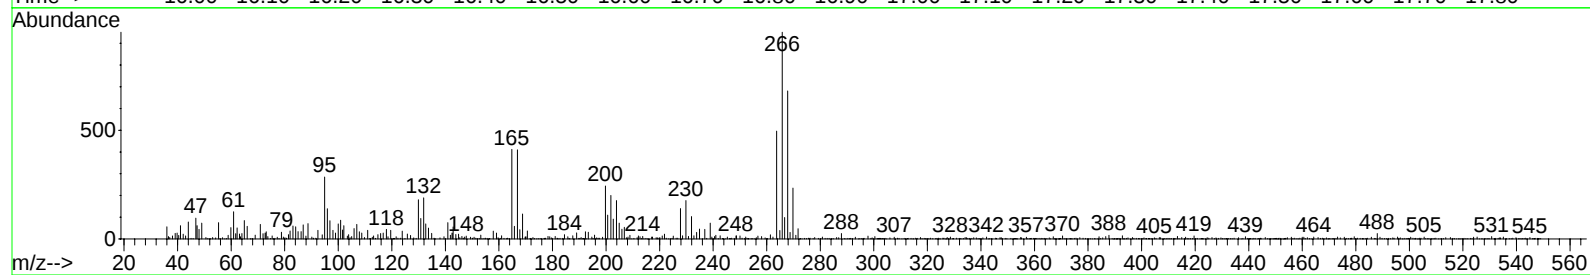


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE020419\  
 Data File : BE098707.D  
 Acq On : 4 Feb 2019 14:23  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 04 18:14:04 2019  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE011519.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Jan 15 14:30:55 2019  
 Response via : Initial Calibration

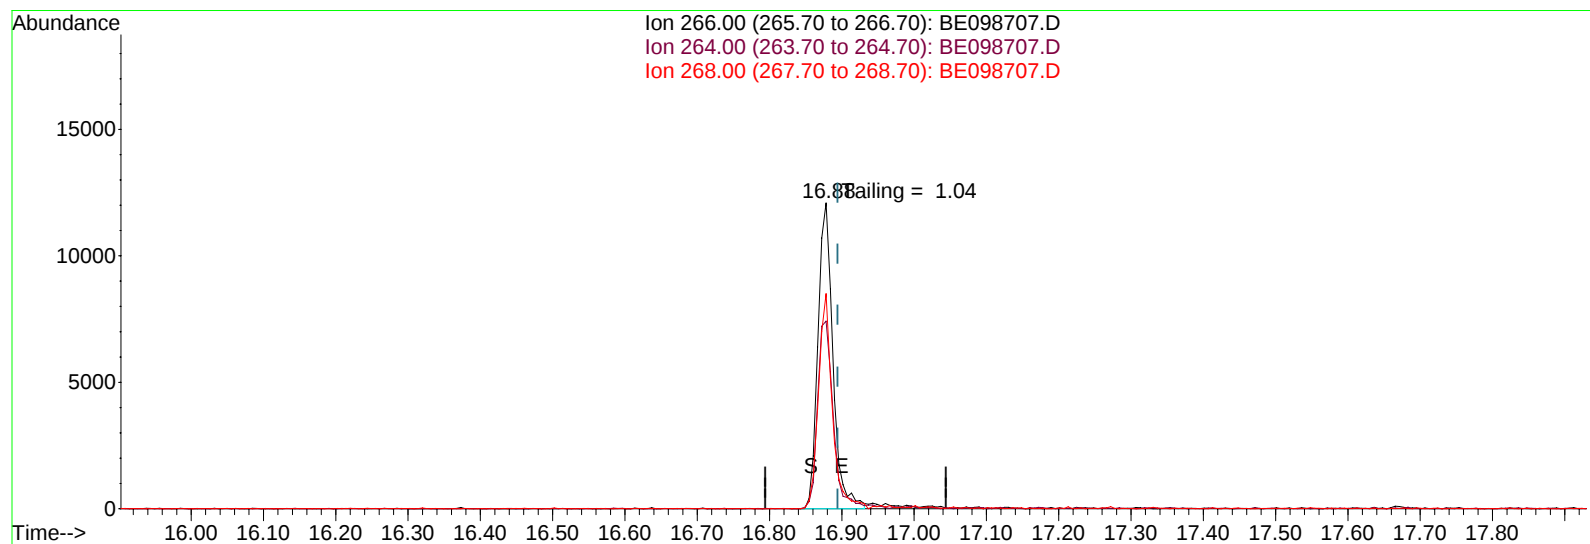

(22) Pentachlorophenol

16.902min (+0.008) 198.37ng m

response 682

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 266.00 | 100   | 100    |
| 264.00 | 67.10 | 52.16# |
| 268.00 | 74.80 | 71.61  |
| 0.00   | 0.00  | 0.00   |