
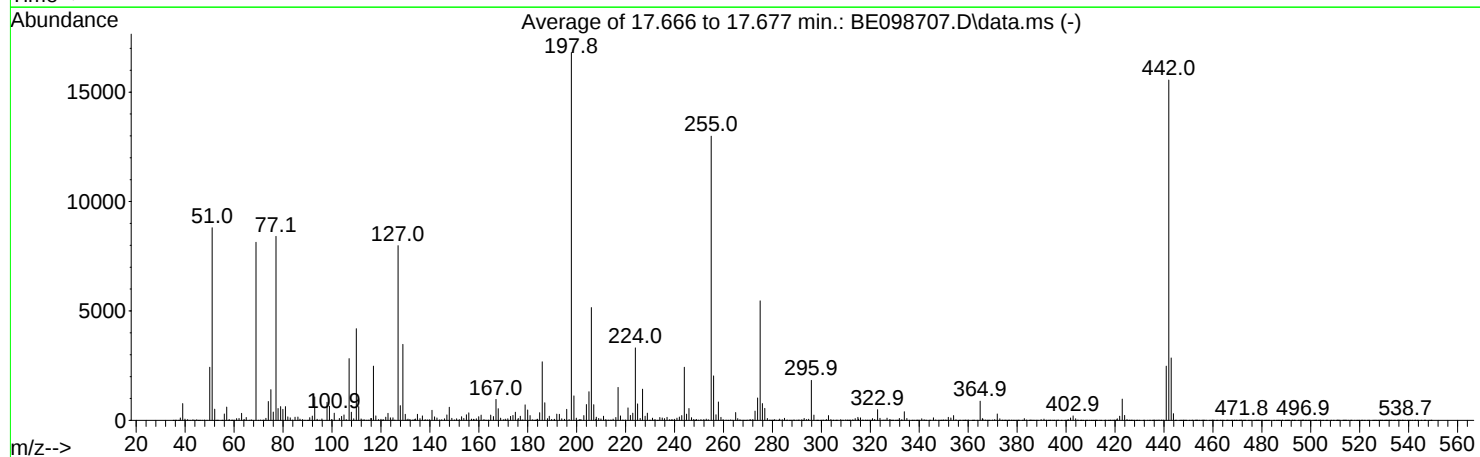


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE020419\
 Data File : BE098707.D
 Acq On : 4 Feb 2019 14:23
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE012419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 24 14:44:44 2019

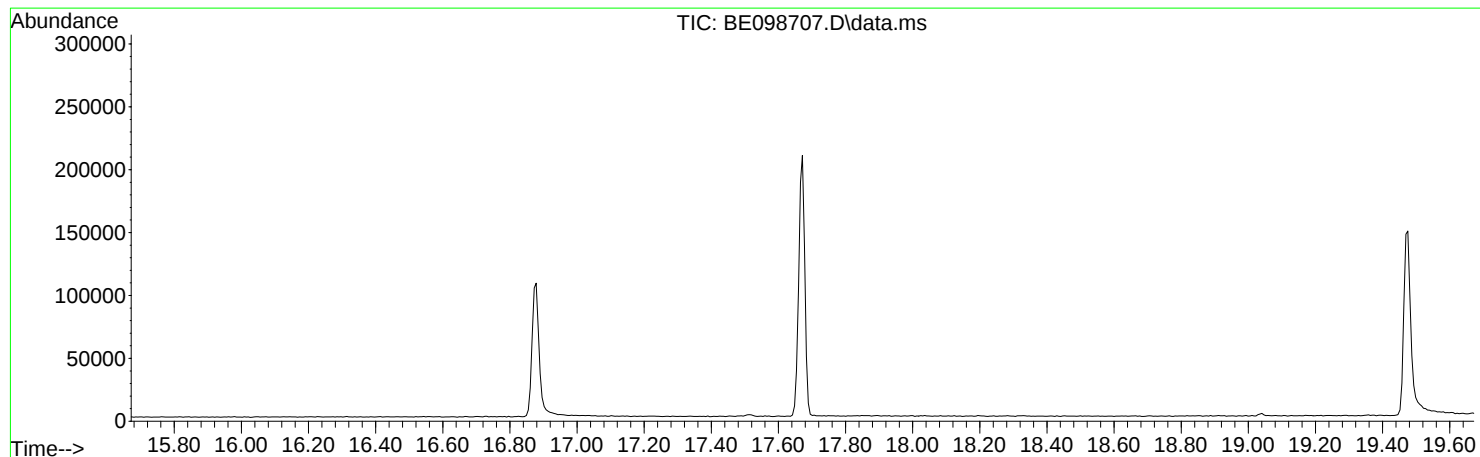

AutoFind: Scans 2566, 2567, 2568; Background Corrected with Scan 2555

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.4	8803	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	48.4	8138	PASS
70	69	0.00	2	0.1	9	PASS
127	198	10	80	47.5	7984	PASS
197	198	0.00	2	0.2	35	PASS
198	198	100	100	100.0	16810	PASS
199	198	5	9	6.7	1119	PASS
275	198	10	60	32.5	5464	PASS
365	198	1	100	5.2	876	PASS
441	198	0.01	100	14.7	2477	PASS
442	198	50	100	92.5	15556	PASS
443	442	15	24	18.3	2852	PASS