
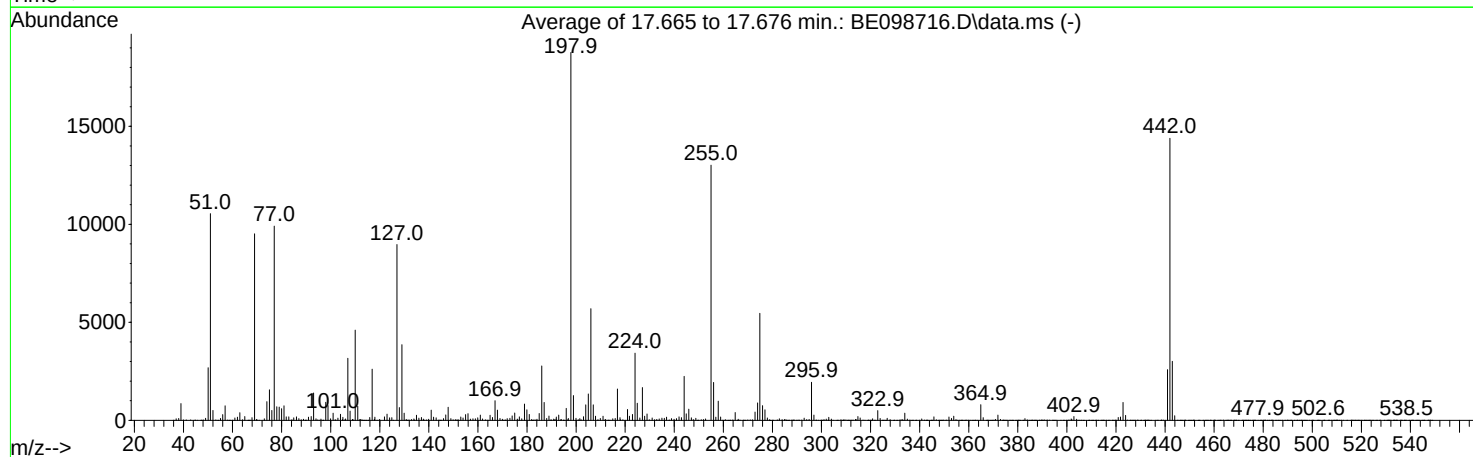


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE020719\
 Data File : BE098716.D
 Acq On : 7 Feb 2019 8:37
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE012419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 24 14:44:44 2019

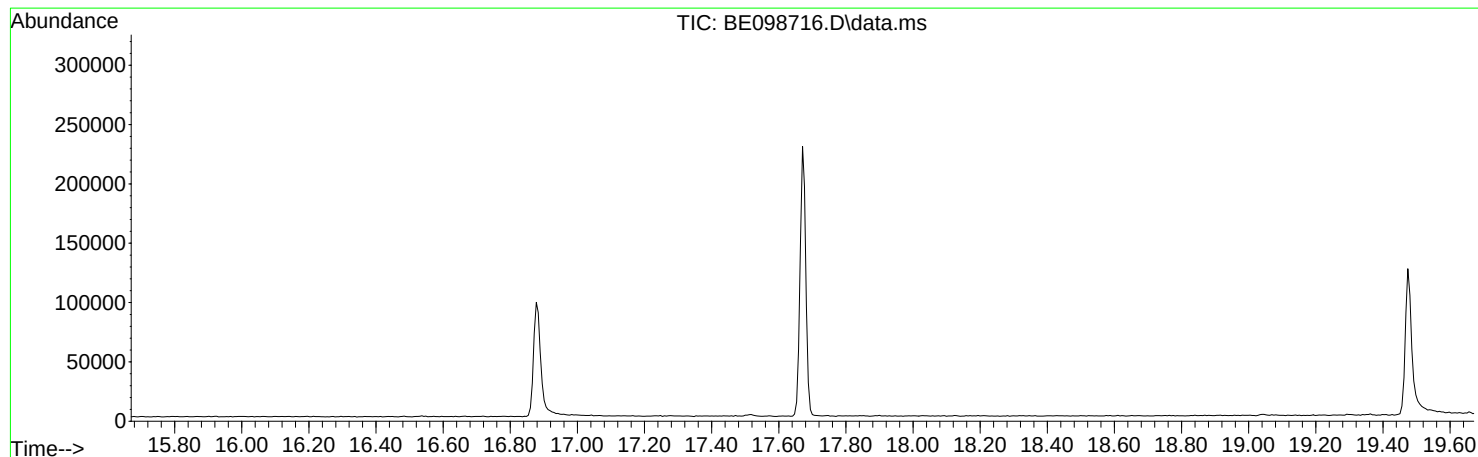

AutoFind: Scans 2566, 2567, 2568; Background Corrected with Scan 2560

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.2	10546	PASS
68	69	0.00	2	1.5	143	PASS
69	198	0.00	100	50.7	9516	PASS
70	69	0.00	2	0.5	46	PASS
127	198	10	80	47.8	8970	PASS
197	198	0.00	2	0.5	100	PASS
198	198	100	100	100.0	18763	PASS
199	198	5	9	6.8	1267	PASS
275	198	10	60	29.1	5461	PASS
365	198	1	100	4.3	803	PASS
441	198	0.01	100	13.8	2587	PASS
442	198	50	100	76.7	14386	PASS
443	442	15	24	20.9	3008	PASS