

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE021319\
 Data File : BE098730.D
 Acq On : 13 Feb 2019 16:50
 Operator : JU/SJ
 Sample : PB117079BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 PB117079BL

Quant Time: Feb 14 04:06:30 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE012419.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 24 14:44:44 2019
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.817	152	811	0.40	ng	0.00
7) Naphthalene-d8	10.615	136	3090	0.40	ng	# 0.01
13) Acenaphthene-d10	14.486	164	1839	0.40	ng	0.02
19) Phenanthrene-d10	17.241	188	4270	0.40	ng	# 0.01
27) Chrysene-d12	21.415	240	5435	0.40	ng	# 0.00
34) Perylene-d12	23.935	264	5031	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.410	112	959	0.40	ng	0.01
5) Phenol-d6	7.022	99	1158	0.33	ng	0.02
8) Nitrobenzene-d5	9.030	82	825	0.30	ng	0.05
11) 2-Methylnaphthalene-d10	12.224	152	2092	0.35	ng	0.02
14) 2,4,6-Tribromophenol	15.996	330	247	0.30	ng	0.01
15) 2-Fluorobiphenyl	13.117	172	2567	0.33	ng	0.01
25) Fluoranthene-d10	19.265	212	25126	0.41	ng	0.00
29) Terphenyl-d14	19.862	244	4267	0.31	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE021319\
Data File : BE098730.D
Acq On : 13 Feb 2019 16:50
Operator : JU/SJ
Sample : PB117079BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB117079BL

Quant Time: Feb 14 04:06:30 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE012419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 24 14:44:44 2019
Response via : Initial Calibration




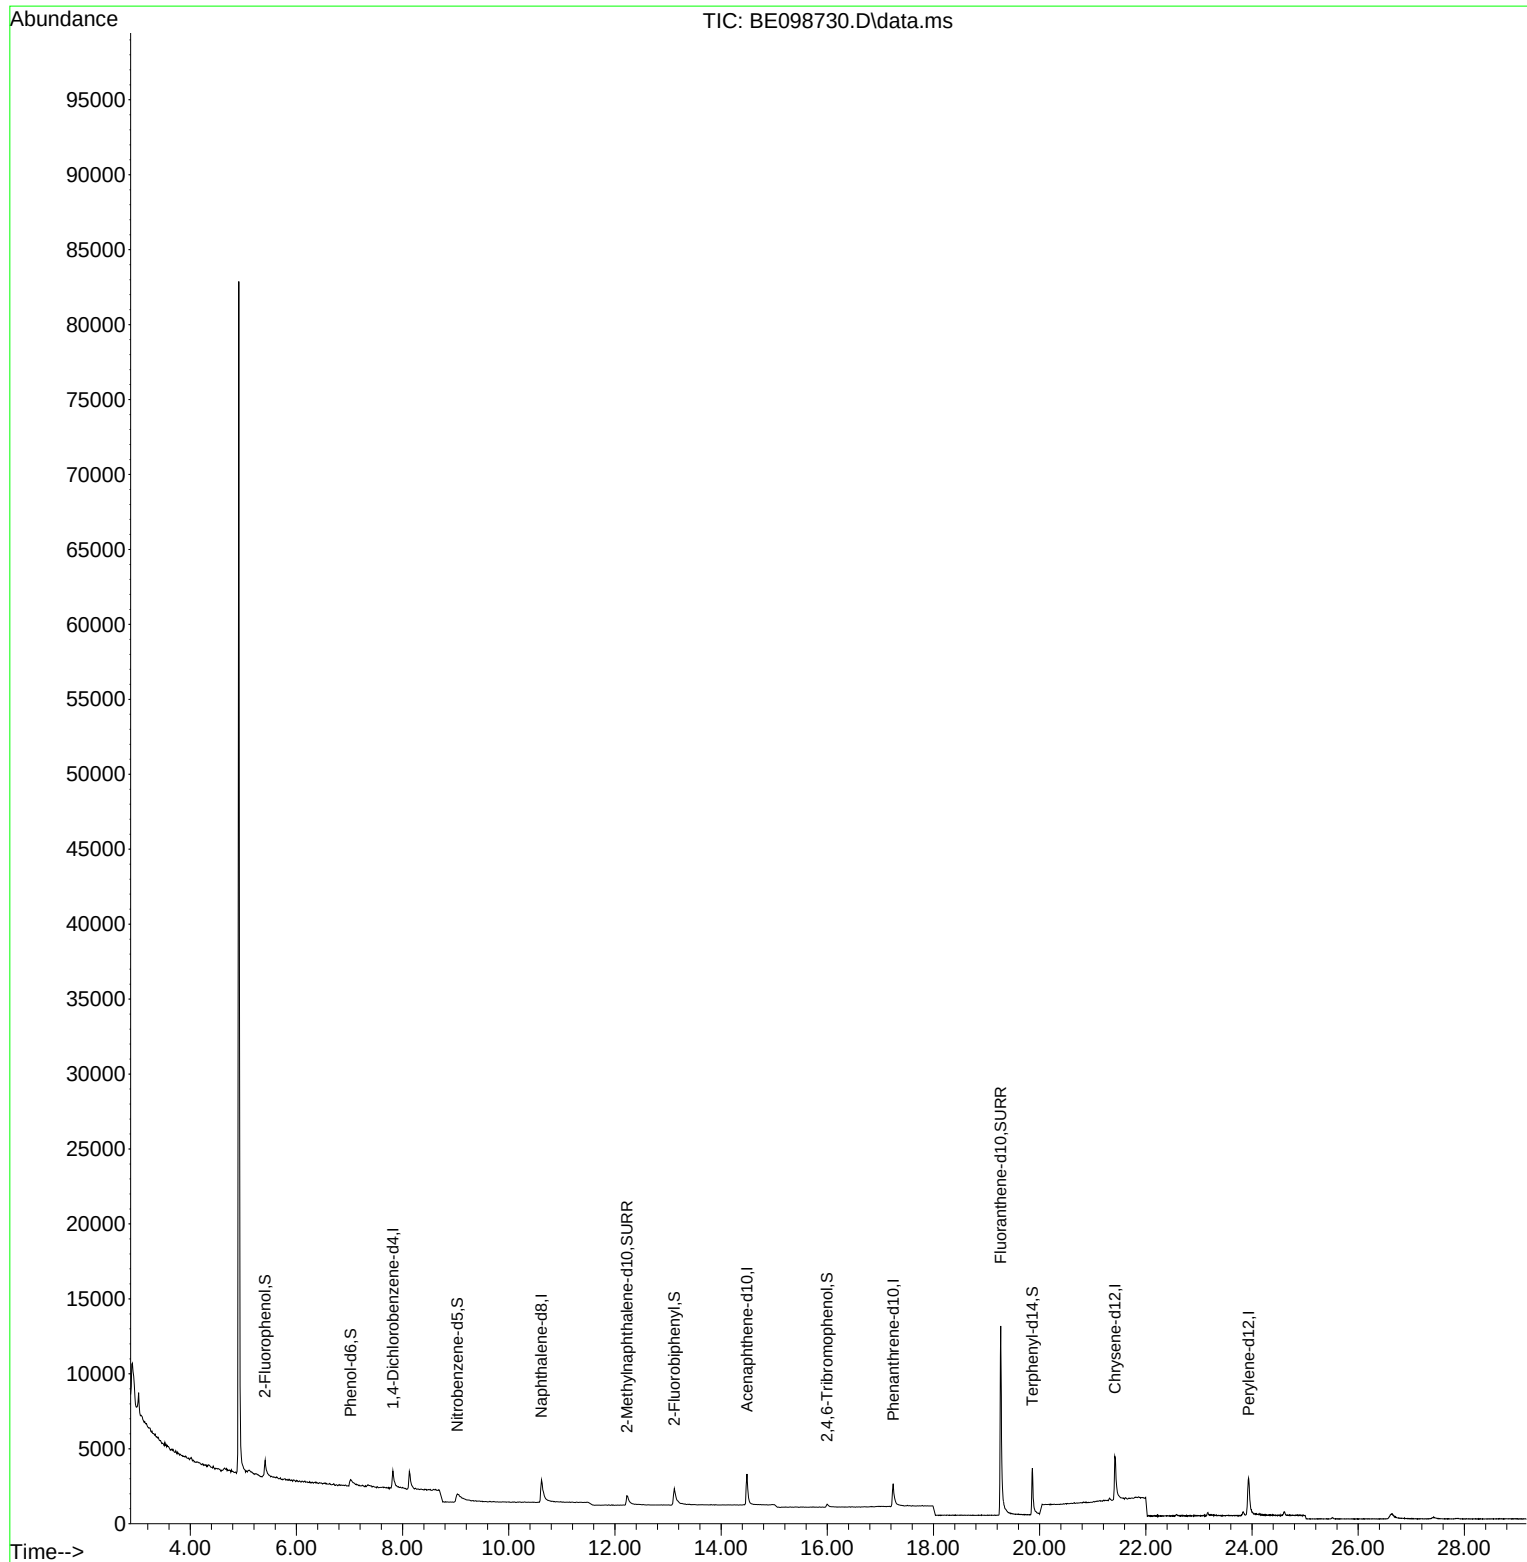


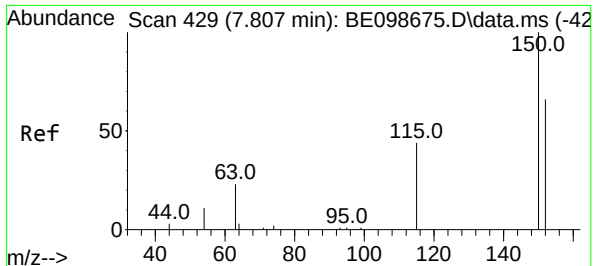

#1
1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.817 min Scan# 430
Delta R.T. 0.010 min
Lab File: BE098730.D
Acq: 13 Feb 2019 16:50




Instrument :
BNA_E
ClientSampled :
PB117079BL


Tgt Ion:152 Resp: 811
Ion Ratio Lower Upper
152 100
150 151.0 121.4 182.2
115 70.8 59.1 88.7

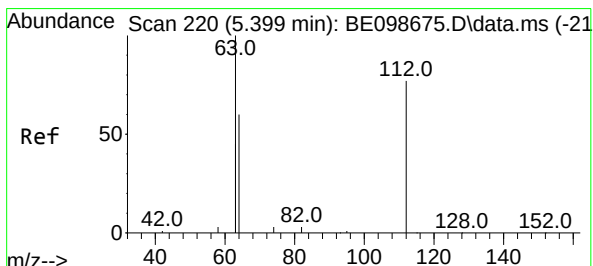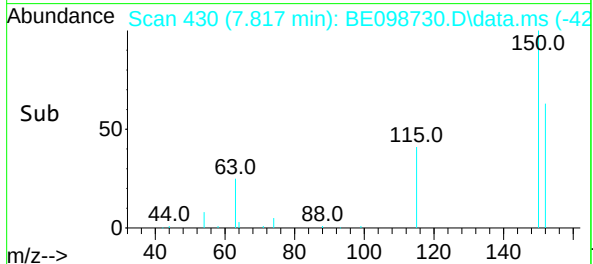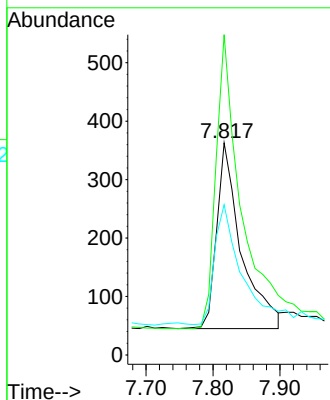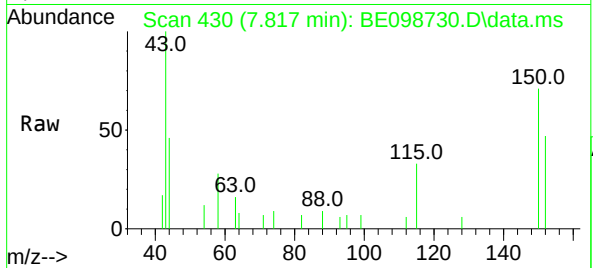

#4
2-Fluorophenol
Concen: 0.40 ng
RT: 5.410 min Scan# 221
Delta R.T. 0.011 min
Lab File: BE098730.D
Acq: 13 Feb 2019 16:50

Tgt Ion:112 Resp: 959
Ion Ratio Lower Upper
112 100
64 72.5 62.9 94.3
63 178.8 152.2 228.4


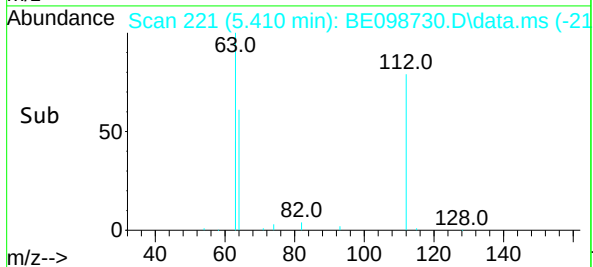
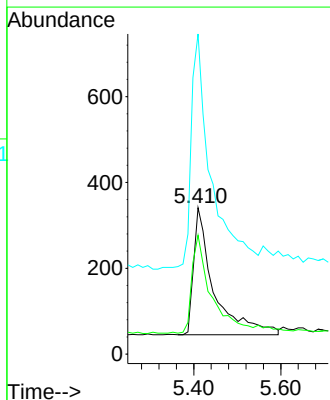
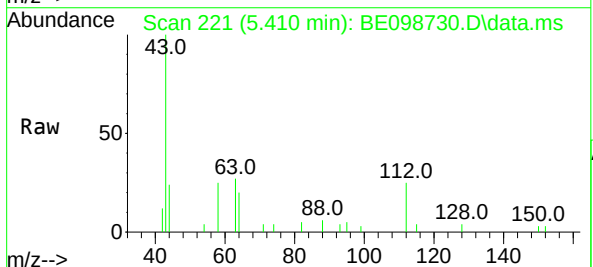


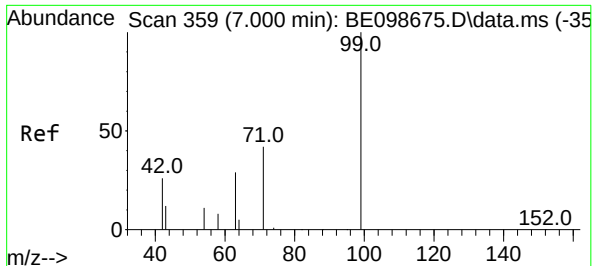

#5
Phenol-d6
Concen: 0.33 ng
RT: 7.022 min Scan# 361
Delta R.T. 0.022 min
Lab File: BE098730.D
Acq: 13 Feb 2019 16:50




Instrument :
BNA_E
ClientSampleId :
PB117079BL


Tgt Ion: 99 Resp: 1158
Ion Ratio Lower Upper
99 100
42 29.9 24.6 37.0
71 40.2 35.1 52.7

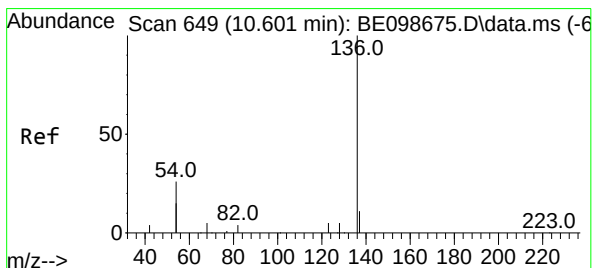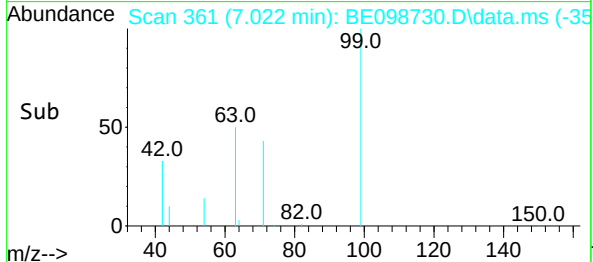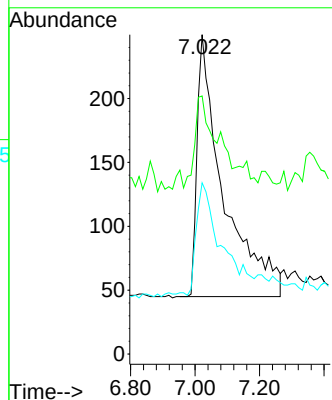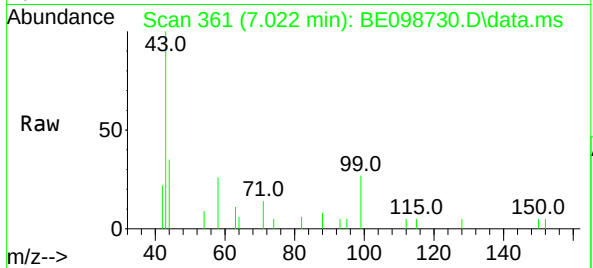

#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.615 min Scan# 650
Delta R.T. 0.014 min
Lab File: BE098730.D
Acq: 13 Feb 2019 16:50

Tgt Ion: 136 Resp: 3090
Ion Ratio Lower Upper
136 100
137 16.2 9.7 14.5#
54 76.1 35.5 53.3#
68 11.8 5.0 7.6#


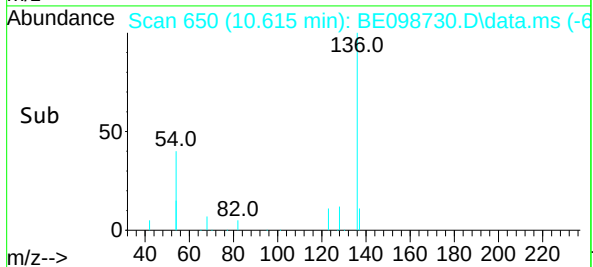
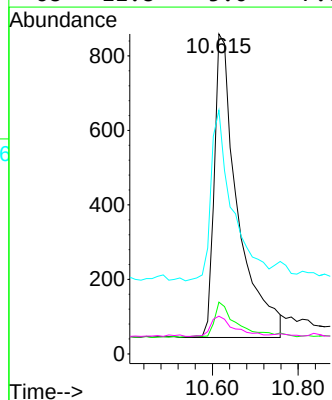
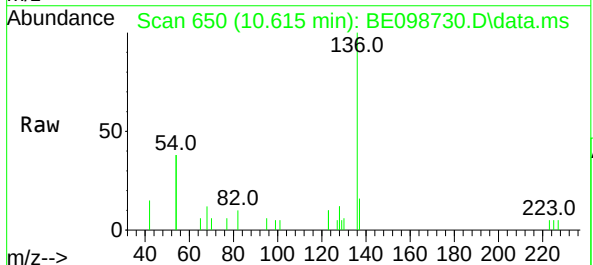


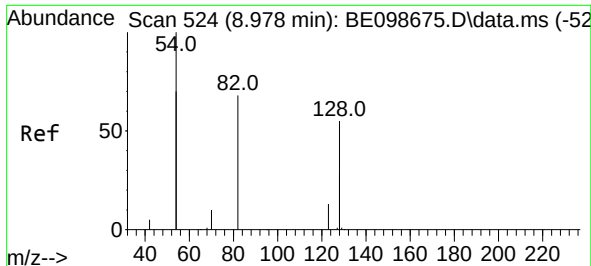

#8
Nitrobenzene-d5
Concen: 0.30 ng
RT: 9.030 min Scan# 528
Delta R.T. 0.052 min
Lab File: BE098730.D
Acq: 13 Feb 2019 16:50




Instrument :
BNA_E
ClientSampleId :
PB117079BL


Tgt Ion: 82 Resp: 825
Ion Ratio Lower Upper
82 100
128 202.5 96.5 144.7#
54 304.5 224.7 337.1

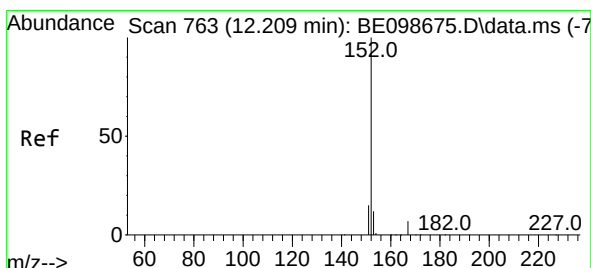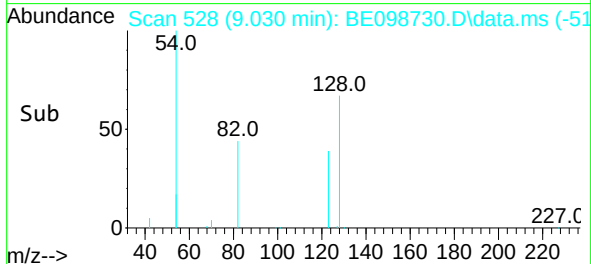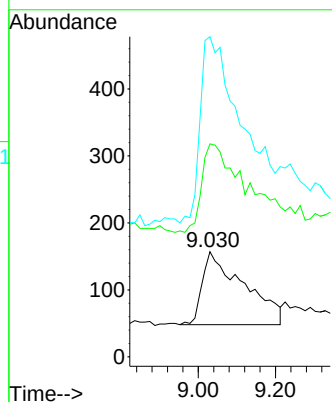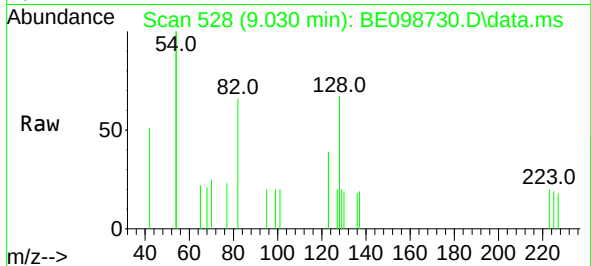

#11
2-Methylnaphthalene-d10
Concen: 0.35 ng
RT: 12.224 min Scan# 764
Delta R.T. 0.015 min
Lab File: BE098730.D
Acq: 13 Feb 2019 16:50

Tgt Ion: 152 Resp: 2092
Ion Ratio Lower Upper
152 100
151 19.0 16.2 24.4


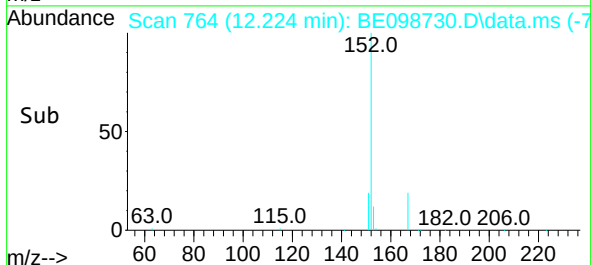
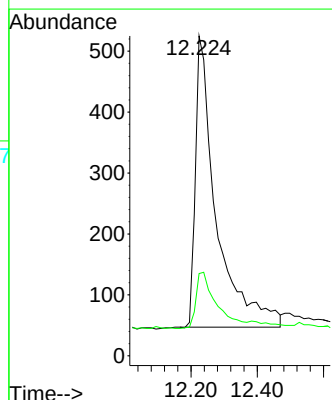
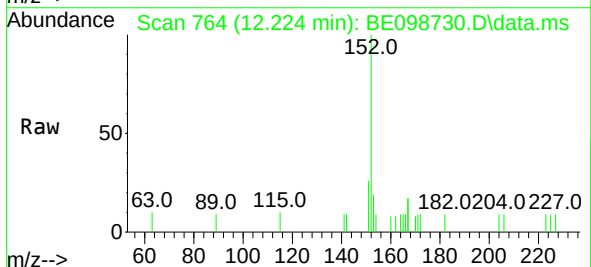


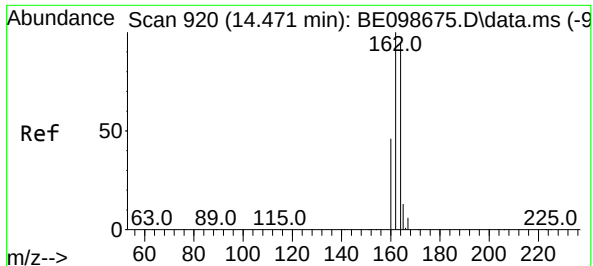

#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.486 min Scan# 921
Delta R.T. 0.015 min
Lab File: BE098730.D
Acq: 13 Feb 2019 16:50




Instrument :
BNA_E
ClientSampleId :
PB117079BL


Tgt Ion:	164	Resp:	1839
Ion	Ratio	Lower	Upper
164	100		
162	95.8	80.5	120.7
160	47.4	40.1	60.1

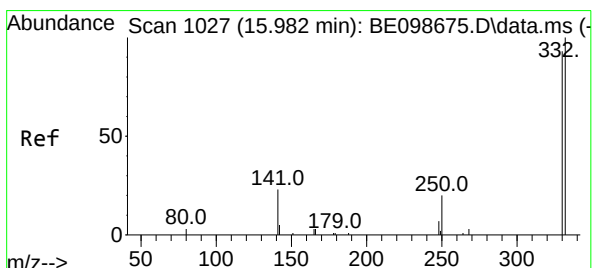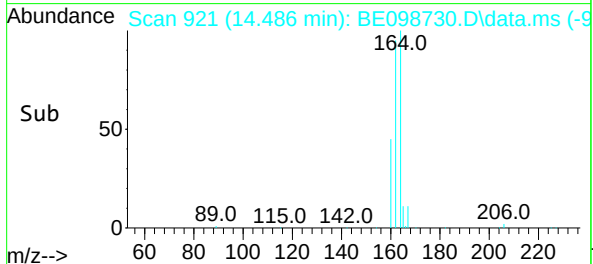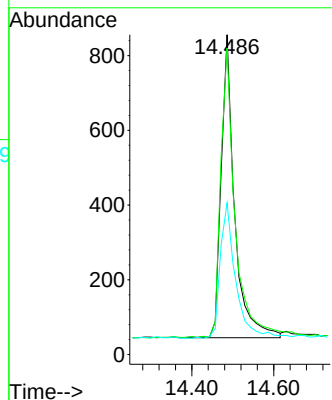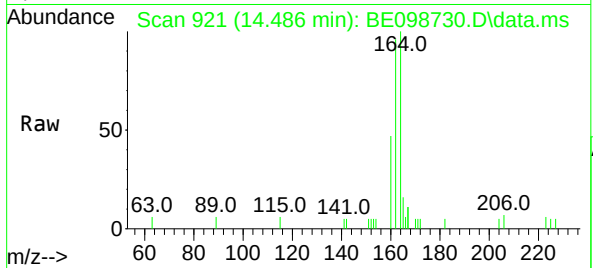

#14
2,4,6-Tribromophenol
Concen: 0.30 ng
RT: 15.996 min Scan# 1028
Delta R.T. 0.014 min
Lab File: BE098730.D
Acq: 13 Feb 2019 16:50

Tgt Ion:	330	Resp:	247
Ion	Ratio	Lower	Upper
330	100		
332	90.7	73.3	109.9
141	36.4	33.1	49.7


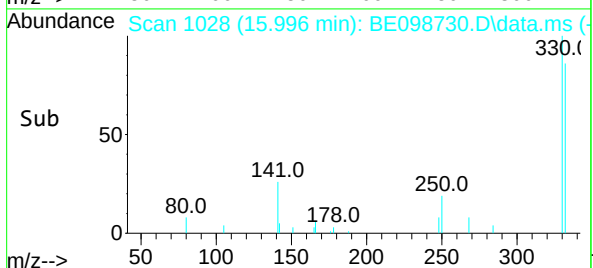
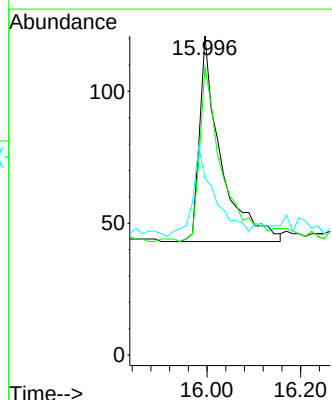
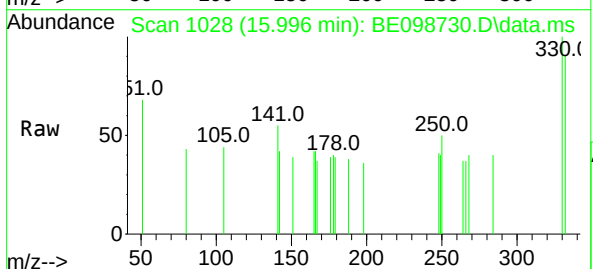


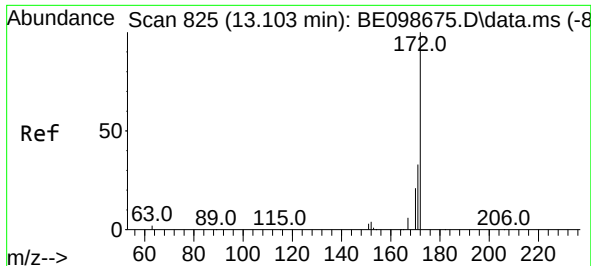

#15
2-Fluorobiphenyl
Concen: 0.33 ng
RT: 13.117 min Scan# 826
Delta R.T. 0.014 min
Lab File: BE098730.D
Acq: 13 Feb 2019 16:50




Instrument :
BNA_E
ClientSampleId :
PB117079BL


Tgt Ion:172	Resp:	2567
Ion Ratio	Lower	Upper
172	100	
171	37.4	29.0 43.4
170	26.5	20.8 31.2

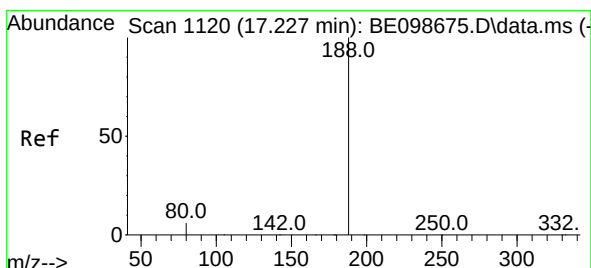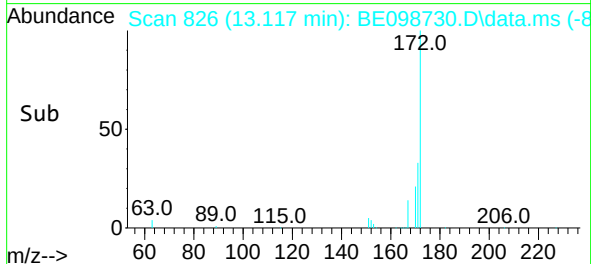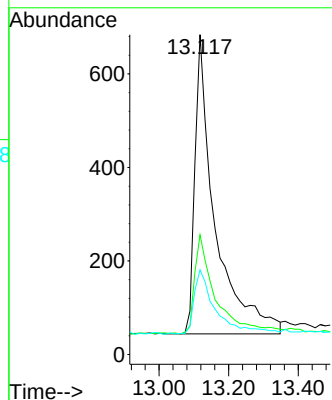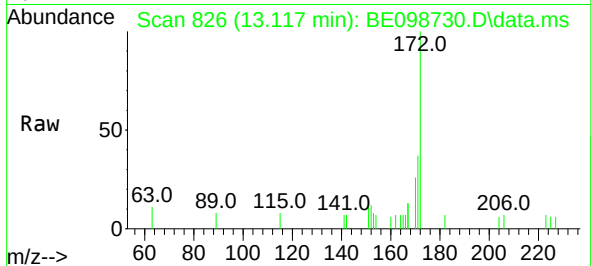

#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.241 min Scan# 1121
Delta R.T. 0.014 min
Lab File: BE098730.D
Acq: 13 Feb 2019 16:50

Tgt Ion:188	Resp:	4270
Ion Ratio	Lower	Upper
188	100	
94	0.0	0.0 0.0
80	9.9	4.7 7.1#


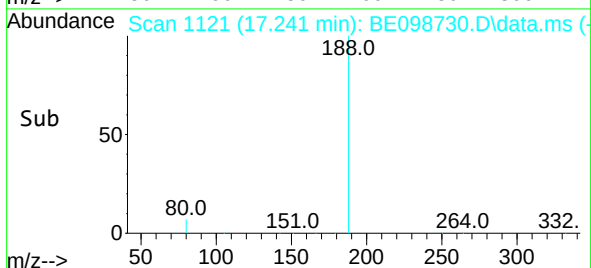
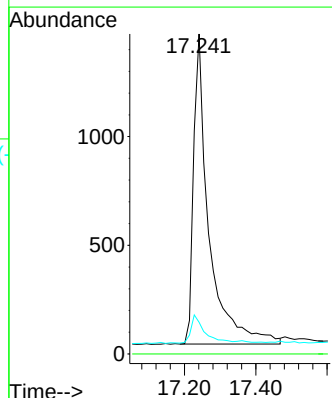
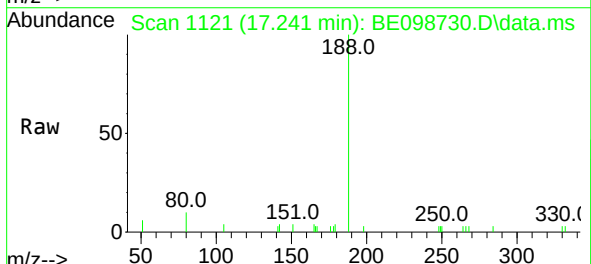


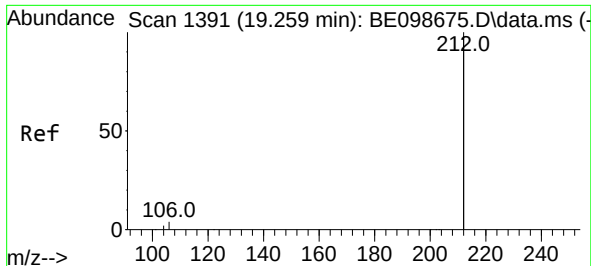

#25
Fluoranthene-d10
Concen: 0.41 ng
RT: 19.265 min Scan# 1392
Delta R.T. 0.006 min
Lab File: BE098730.D
Acq: 13 Feb 2019 16:50




Instrument :
BNA_E
ClientSampleId :
PB117079BL


Tgt Ion:212 Resp: 25126
Ion Ratio Lower Upper
212 100
106 2.0 1.7 2.5
104 1.2 1.0 1.6

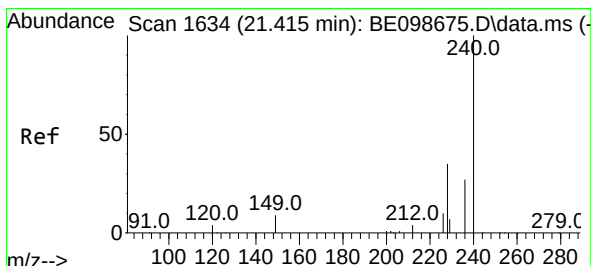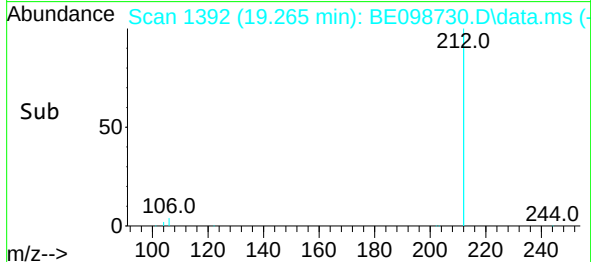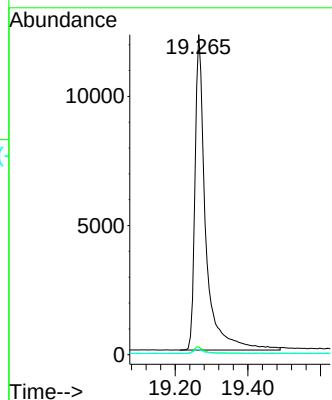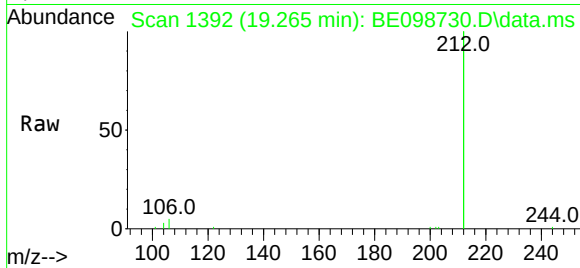

#27
Chrysene-d12
Concen: 0.40 ng
RT: 21.415 min Scan# 1634
Delta R.T. 0.000 min
Lab File: BE098730.D
Acq: 13 Feb 2019 16:50

Tgt Ion:240 Resp: 5435
Ion Ratio Lower Upper
240 100
120 12.2 4.7 7.1#
236 27.6 21.9 32.9


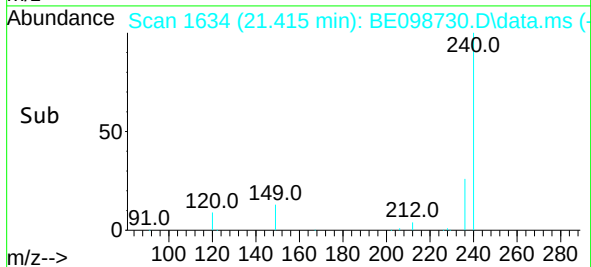
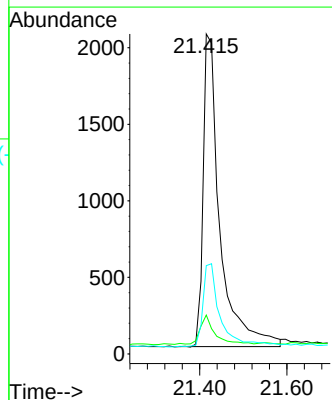
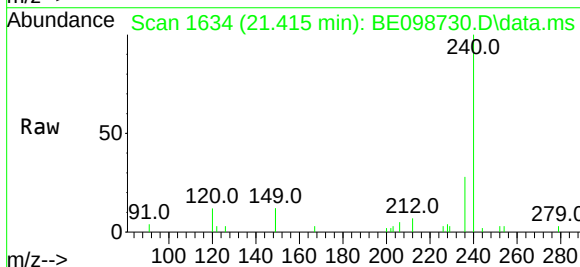


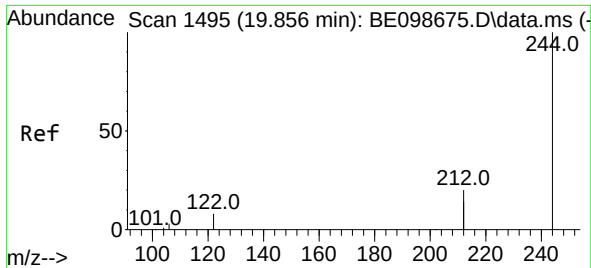

#29
Terphenyl-d14
Concen: 0.31 ng
RT: 19.862 min Scan# 1496
Delta R.T. 0.006 min
Lab File: BE098730.D
Acq: 13 Feb 2019 16:50

Instrument :
BNA_E
ClientSampleId :
PB117079BL

Tgt Ion:244 Resp: 4267
Ion Ratio Lower Upper
244 100
212 41.1 29.4 44.2
122 9.0 7.1 10.7

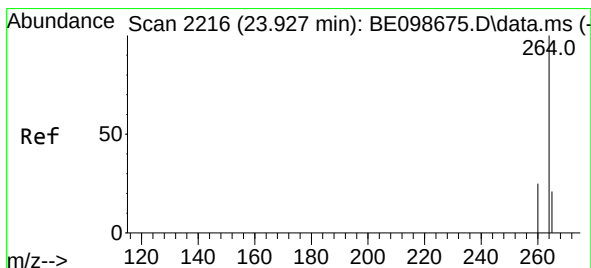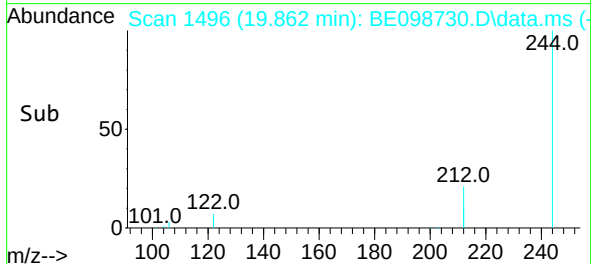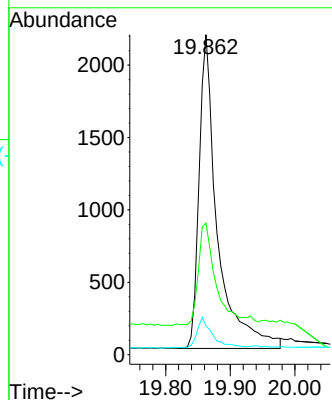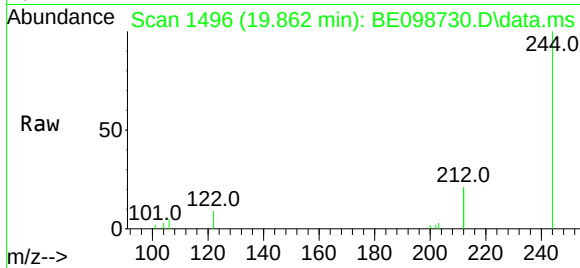

#34
Perylene-d12
Concen: 0.40 ng
RT: 23.935 min Scan# 2218
Delta R.T. 0.008 min
Lab File: BE098730.D
Acq: 13 Feb 2019 16:50

Tgt Ion:264 Resp: 5031
Ion Ratio Lower Upper
264 100
260 25.6 20.5 30.7
265 30.2 22.3 33.5

