
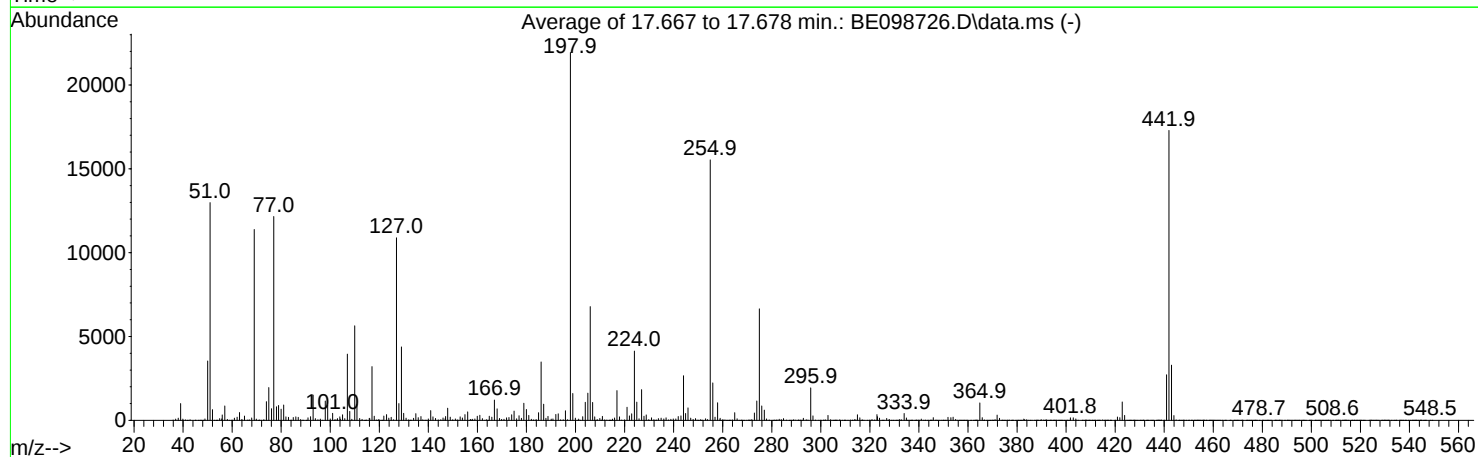


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE021319\
 Data File : BE098726.D
 Acq On : 13 Feb 2019 14:18
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE012419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 24 14:44:44 2019

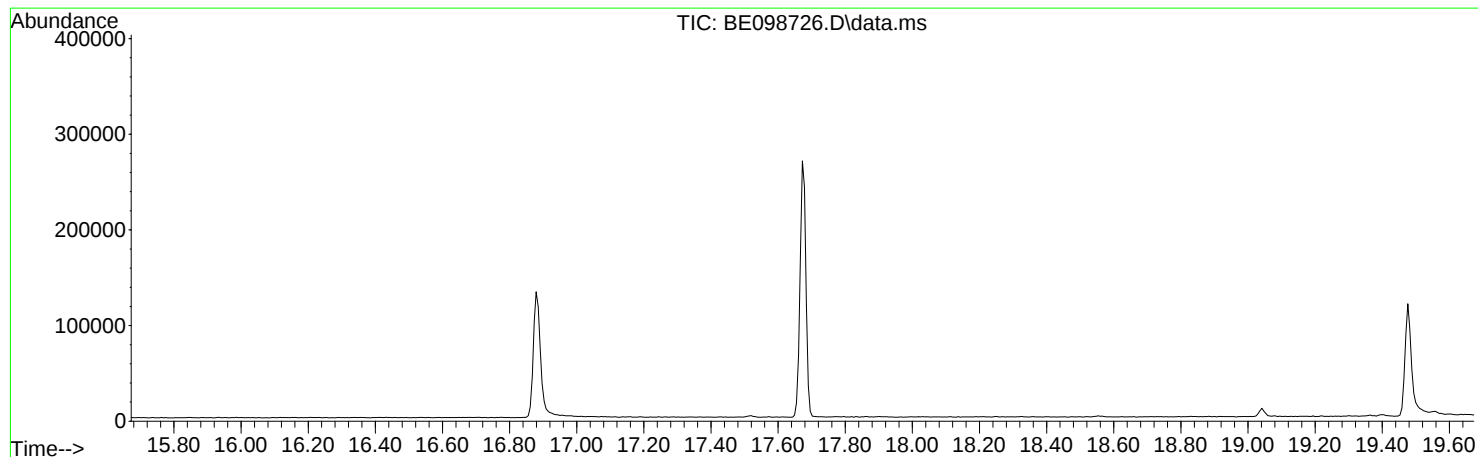

AutoFind: Scans 2566, 2567, 2568; Background Corrected with Scan 2554

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.2	12983	PASS
68	69	0.00	2	1.3	147	PASS
69	198	0.00	100	51.9	11387	PASS
70	69	0.00	2	0.6	72	PASS
127	198	10	80	49.6	10891	PASS
197	198	0.00	2	0.2	42	PASS
198	198	100	100	100.0	21937	PASS
199	198	5	9	7.3	1601	PASS
275	198	10	60	30.3	6652	PASS
365	198	1	100	4.7	1036	PASS
441	198	0.01	100	12.4	2718	PASS
442	198	50	100	78.8	17287	PASS
443	442	15	24	19.1	3296	PASS