

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE022019\
 Data File : BE098737.D
 Acq On : 20 Feb 2019 12:27
 Operator : JU/SJ
 Sample : PB117222BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 PB117222BL

Quant Time: Feb 20 13:02:28 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE012419.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 24 14:44:44 2019
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.827	152	1038	0.40	ng	0.02
7) Naphthalene-d8	10.626	136	3960	0.40	ng	# 0.03
13) Acenaphthene-d10	14.486	164	2357	0.40	ng	0.01
19) Phenanthrene-d10	17.241	188	5437	0.40	ng	# 0.01
27) Chrysene-d12	21.427	240	6387	0.40	ng	# 0.01
34) Perylene-d12	23.933	264	5860	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.420	112	1032	0.34	ng	0.02
5) Phenol-d6	7.032	99	972	0.22	ng	0.03
8) Nitrobenzene-d5	9.041	82	840	0.25	ng	0.06
11) 2-Methylnaphthalene-d10	12.238	152	2271	0.30	ng	0.03
14) 2,4,6-Tribromophenol	16.010	330	199	0.19	ng	0.03
15) 2-Fluorobiphenyl	13.117	172	2715	0.27	ng	0.01
25) Fluoranthene-d10	19.271	212	26165	0.34	ng	0.01
29) Terphenyl-d14	19.862	244	4269	0.27	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE022019\
Data File : BE098737.D
Acq On : 20 Feb 2019 12:27
Operator : JU/SJ
Sample : PB117222BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB117222BL

Quant Time: Feb 20 13:02:28 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE012419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 24 14:44:44 2019
Response via : Initial Calibration




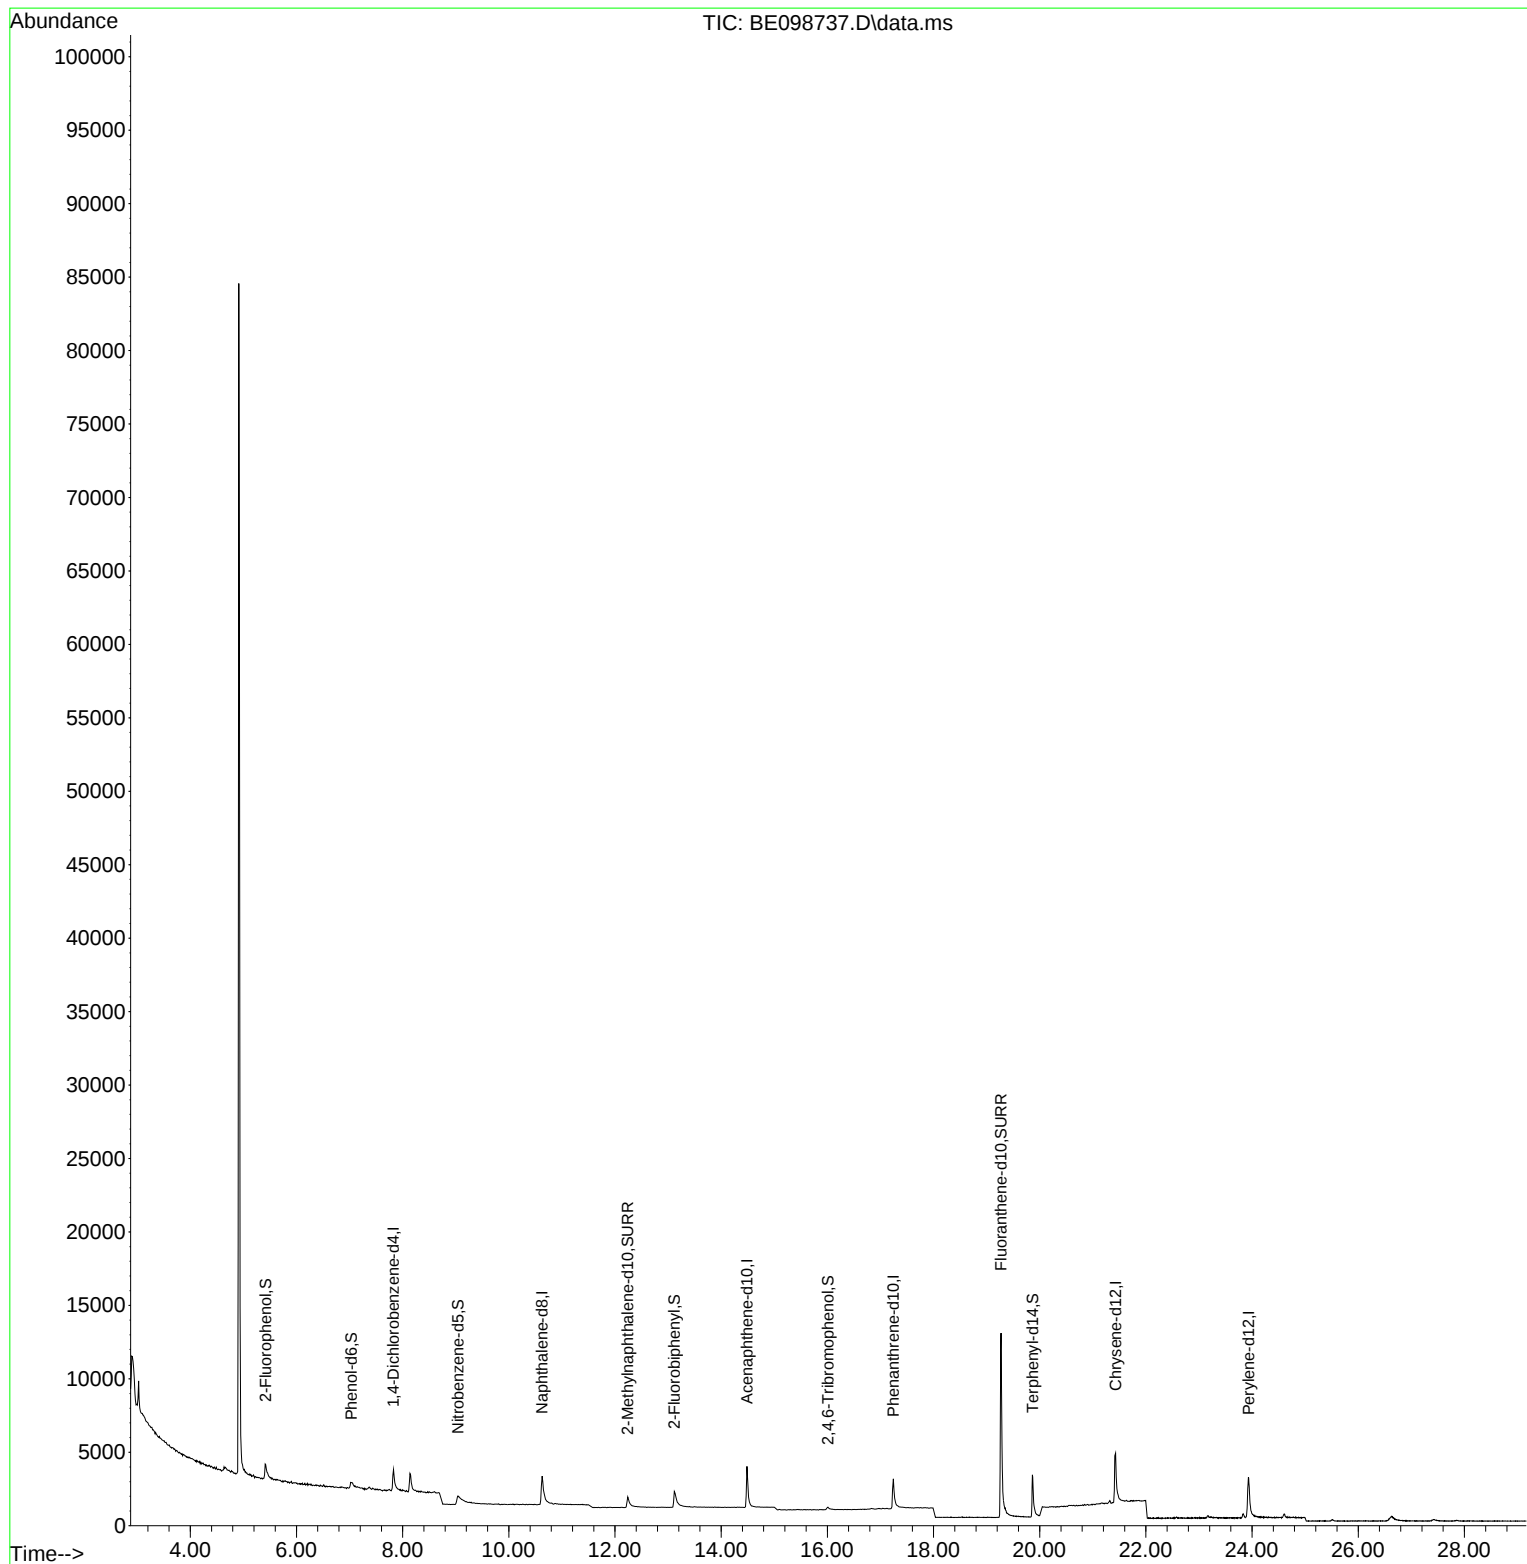


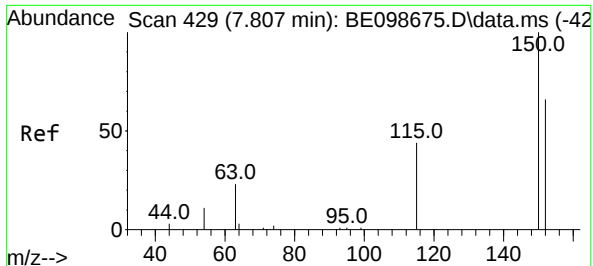

#1
1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.827 min Scan# 431
Delta R.T. 0.020 min
Lab File: BE098737.D
Acq: 20 Feb 2019 12:27




Instrument :
BNA_E
ClientSampleId :
PB117222BL


Tgt Ion:152 Resp: 1038
Ion Ratio Lower Upper
152 100
150 147.4 121.4 182.2
115 70.0 59.1 88.7

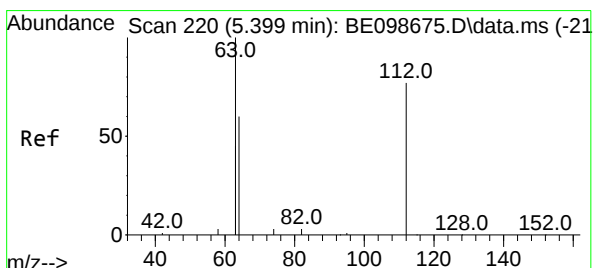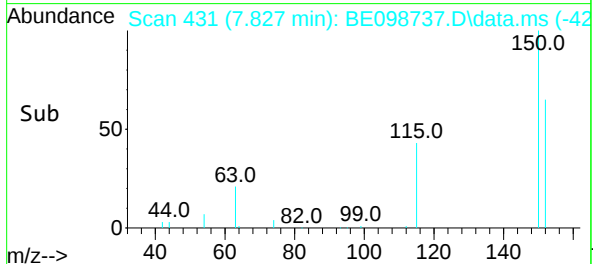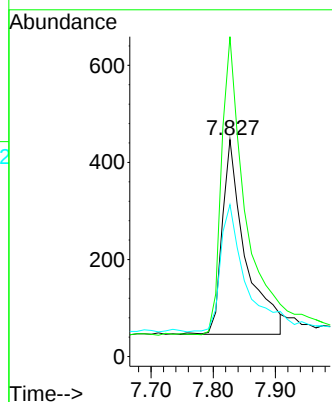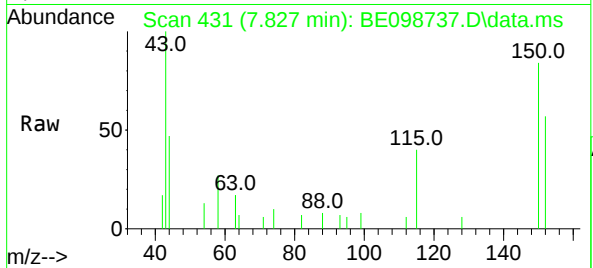

#4
2-Fluorophenol
Concen: 0.34 ng
RT: 5.420 min Scan# 222
Delta R.T. 0.021 min
Lab File: BE098737.D
Acq: 20 Feb 2019 12:27

Tgt Ion:112 Resp: 1032
Ion Ratio Lower Upper
112 100
64 84.2 62.9 94.3
63 192.0 152.2 228.4


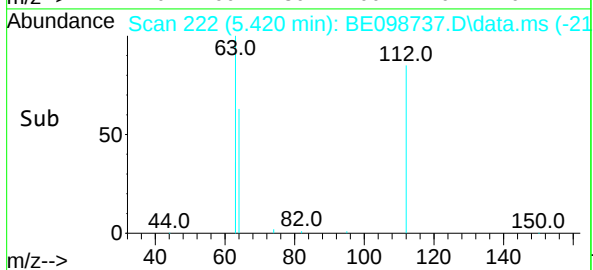
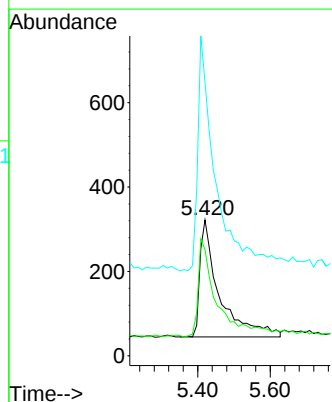
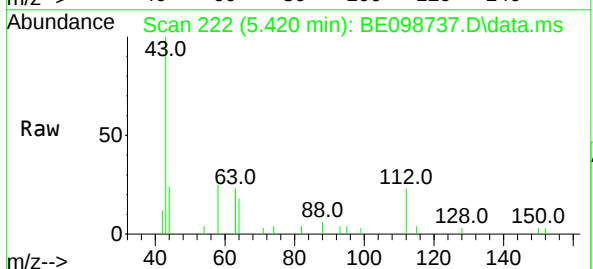


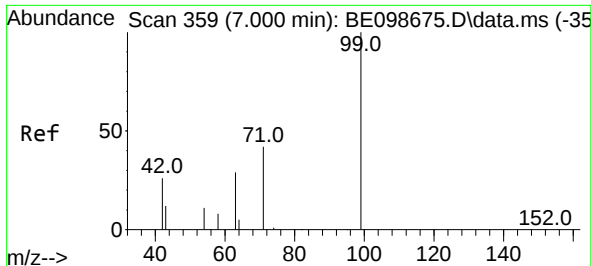

#5
Phenol-d6
Concen: 0.22 ng
RT: 7.032 min Scan# 362
Delta R.T. 0.032 min
Lab File: BE098737.D
Acq: 20 Feb 2019 12:27




Instrument :
BNA_E
ClientSampleId :
PB117222BL


Tgt Ion: 99 Resp: 972
Ion Ratio Lower Upper
99 100
42 40.9 24.6 37.0#
71 52.1 35.1 52.7

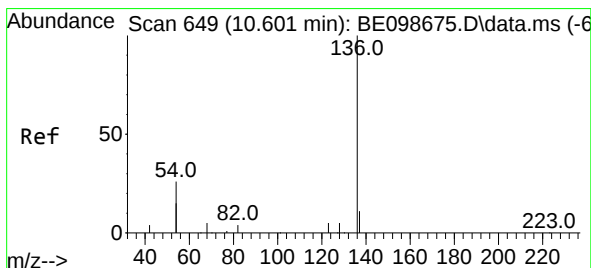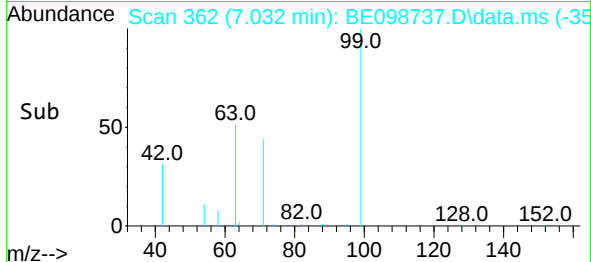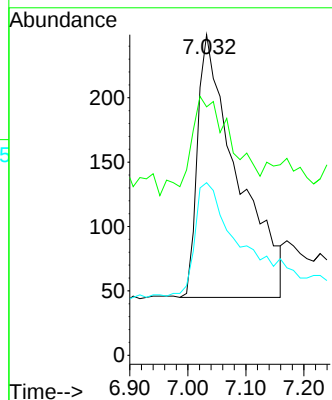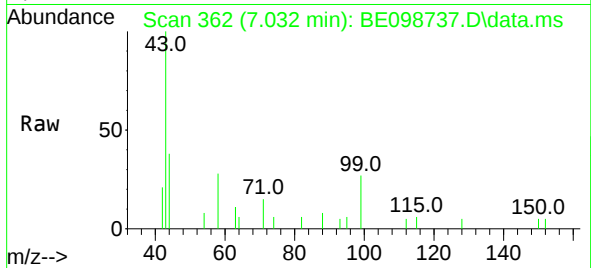

#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.626 min Scan# 651
Delta R.T. 0.025 min
Lab File: BE098737.D
Acq: 20 Feb 2019 12:27

Tgt Ion: 136 Resp: 3960
Ion Ratio Lower Upper
136 100
137 14.9 9.7 14.5#
54 60.2 35.5 53.3#
68 9.6 5.0 7.6#


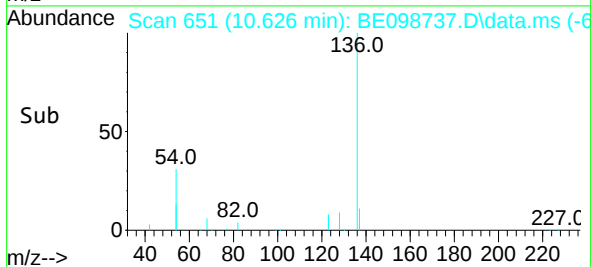
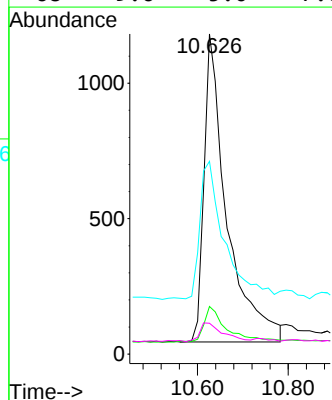
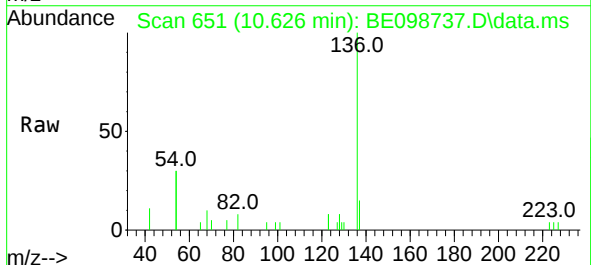


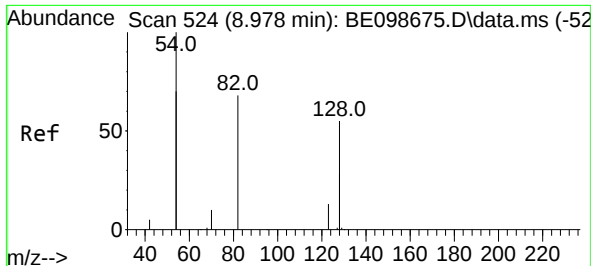

#8
Nitrobenzene-d5
Concen: 0.25 ng
RT: 9.041 min Scan# 529
Delta R.T. 0.063 min
Lab File: BE098737.D
Acq: 20 Feb 2019 12:27




Instrument :
BNA_E
ClientSampled :
PB117222BL


Tgt Ion: 82 Resp: 840
Ion Ratio Lower Upper
82 100
128 196.3 96.5 144.7#
54 308.5 224.7 337.1

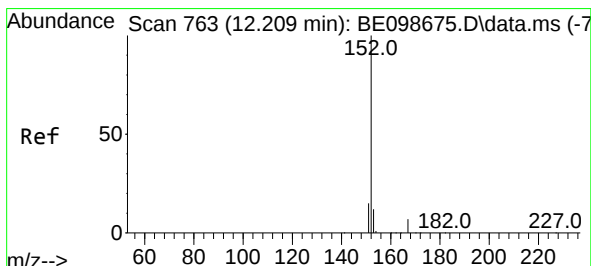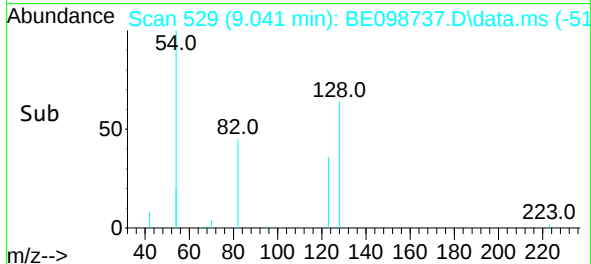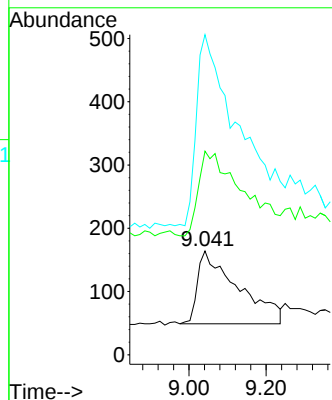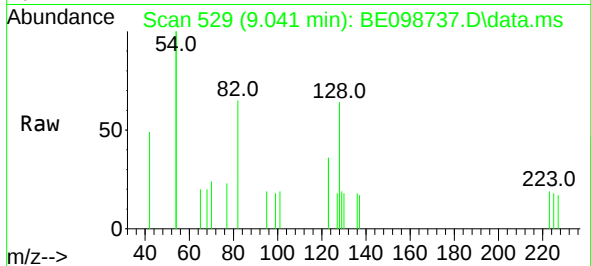

#11
2-Methylnaphthalene-d10
Concen: 0.30 ng
RT: 12.238 min Scan# 765
Delta R.T. 0.029 min
Lab File: BE098737.D
Acq: 20 Feb 2019 12:27


Tgt Ion: 152 Resp: 2271
Ion Ratio Lower Upper
152 100
151 17.4 16.2 24.4

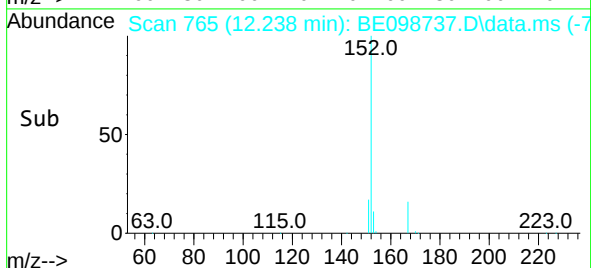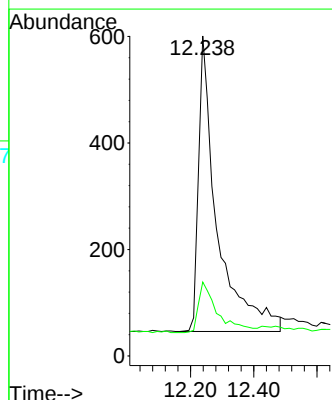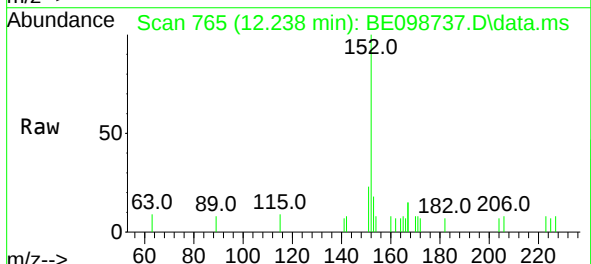



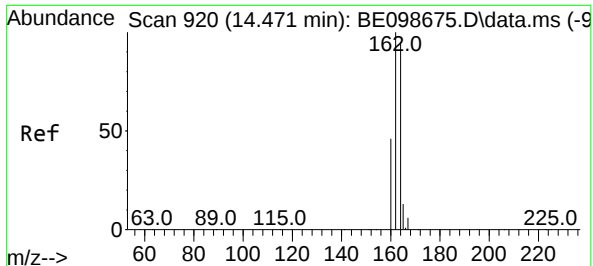


#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.486 min Scan# 921
Delta R.T. 0.015 min
Lab File: BE098737.D
Acq: 20 Feb 2019 12:27

Instrument :
BNA_E
ClientSampleId :
PB117222BL



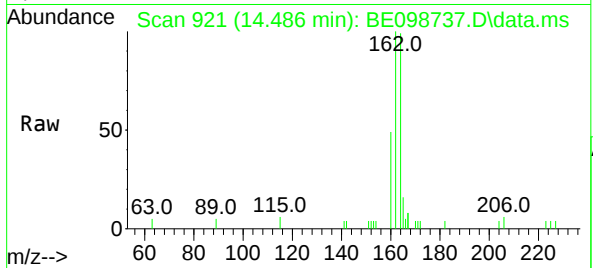



Tgt Ion:164 Resp: 2357
Ion Ratio Lower Upper
164 100
162 100.7 80.5 120.7
160 49.8 40.1 60.1

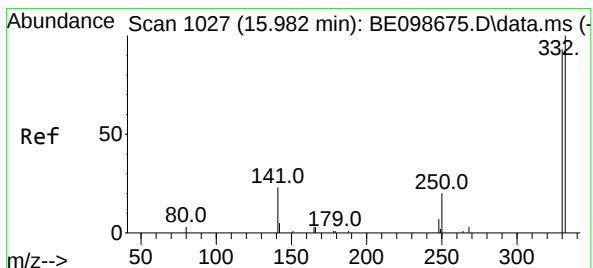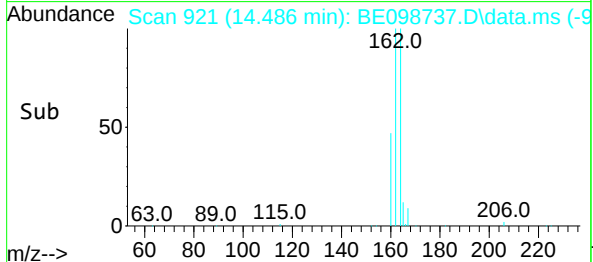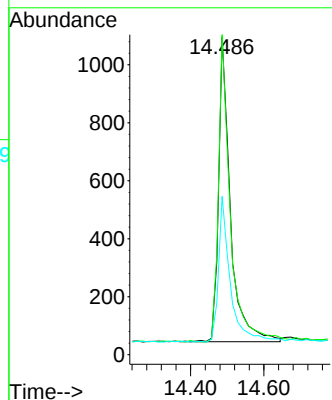

#14
2,4,6-Tribromophenol
Concen: 0.19 ng
RT: 16.010 min Scan# 1029
Delta R.T. 0.028 min
Lab File: BE098737.D
Acq: 20 Feb 2019 12:27

Tgt Ion:330 Resp: 199
Ion Ratio Lower Upper
330 100
332 111.6 73.3 109.9#
141 64.8 33.1 49.7#


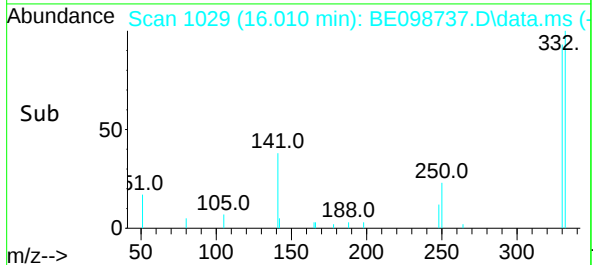
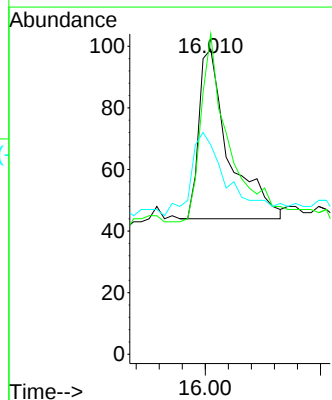
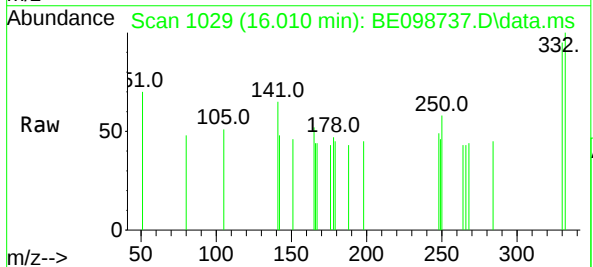


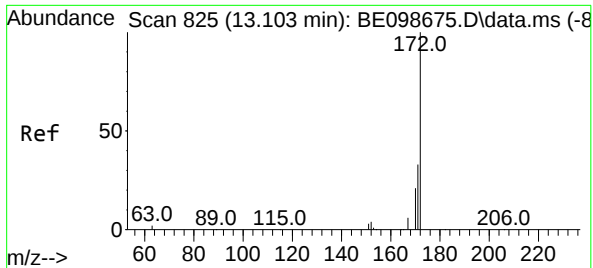

#15
2-Fluorobiphenyl
Concen: 0.27 ng
RT: 13.117 min Scan# 826
Delta R.T. 0.014 min
Lab File: BE098737.D
Acq: 20 Feb 2019 12:27




Instrument :
BNA_E
ClientSampleId :
PB117222BL


Tgt Ion:172	Resp:	2715
Ion Ratio	Lower	Upper
172	100	
171	37.3	29.0 43.4
170	27.4	20.8 31.2

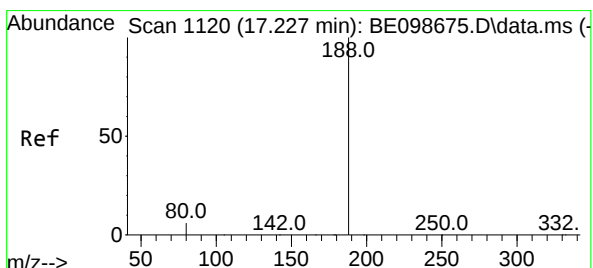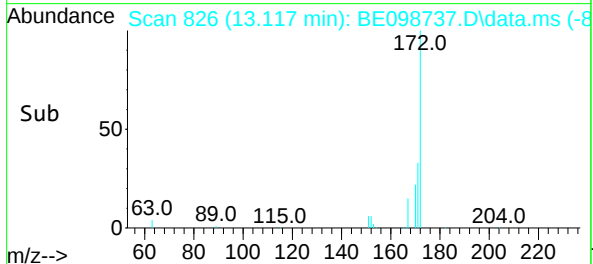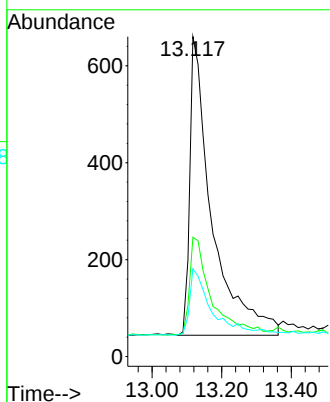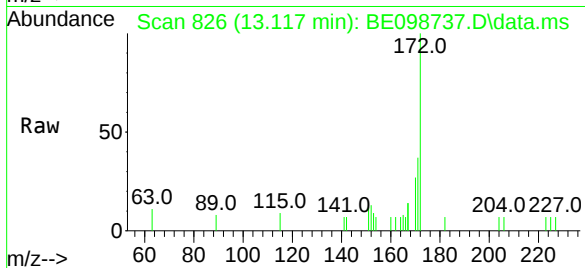

#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.241 min Scan# 1121
Delta R.T. 0.014 min
Lab File: BE098737.D
Acq: 20 Feb 2019 12:27

Tgt Ion:188	Resp:	5437
Ion Ratio	Lower	Upper
188	100	
94	0.0	0.0 0.0
80	10.0	4.7 7.1#


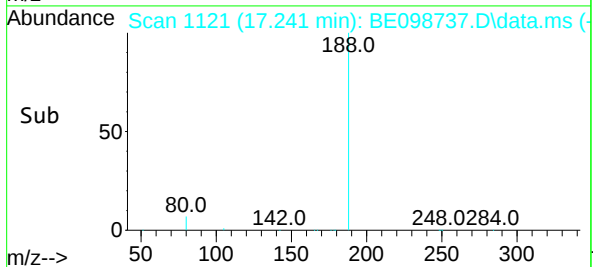
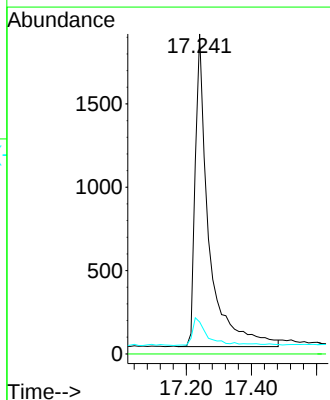
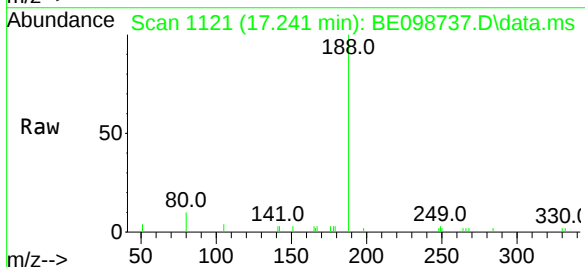


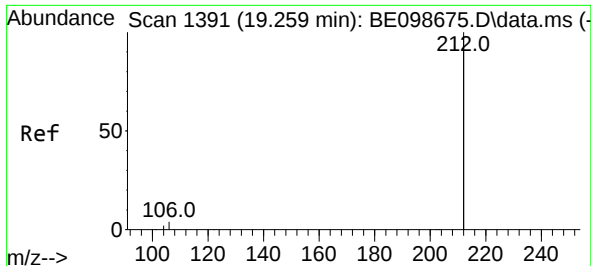

#25
Fluoranthene-d10
Concen: 0.34 ng
RT: 19.271 min Scan# 1393
Delta R.T. 0.012 min
Lab File: BE098737.D
Acq: 20 Feb 2019 12:27




Instrument :
BNA_E
ClientSampleId :
PB117222BL


Tgt Ion:212 Resp: 26165
Ion Ratio Lower Upper
212 100
106 2.0 1.7 2.5
104 1.2 1.0 1.6

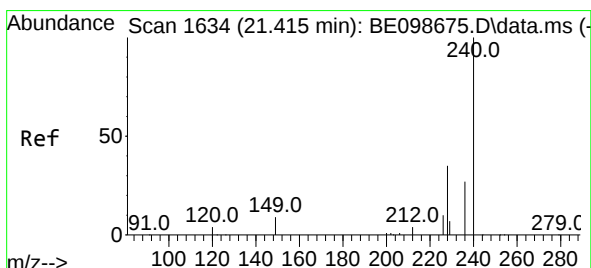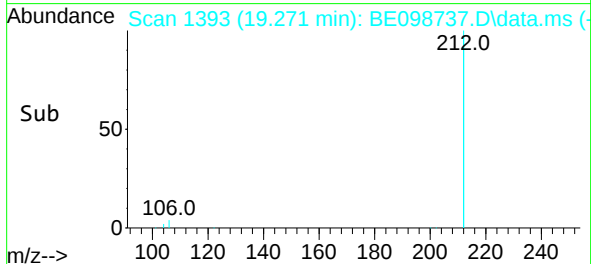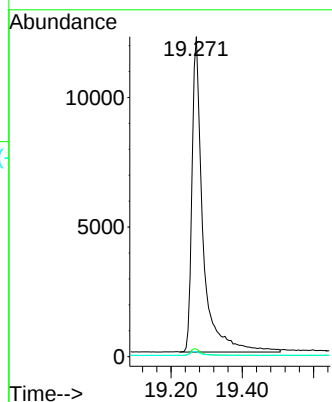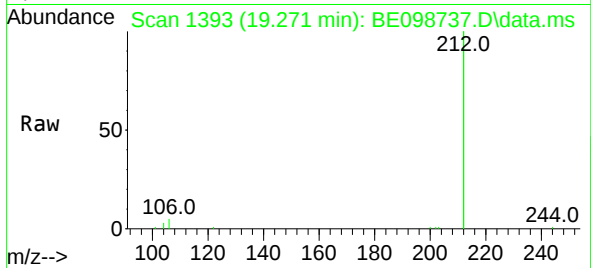

#27
Chrysene-d12
Concen: 0.40 ng
RT: 21.427 min Scan# 1635
Delta R.T. 0.012 min
Lab File: BE098737.D
Acq: 20 Feb 2019 12:27

Tgt Ion:240 Resp: 6387
Ion Ratio Lower Upper
240 100
120 7.5 4.7 7.1#
236 26.9 21.9 32.9


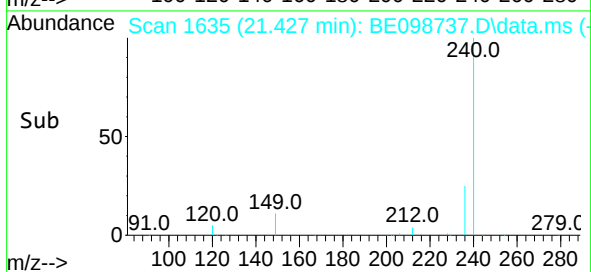
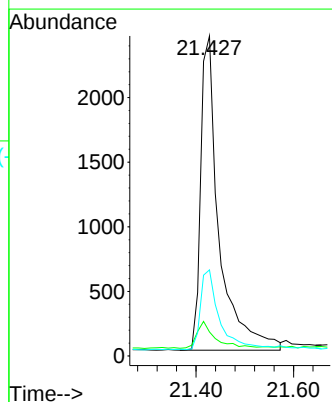
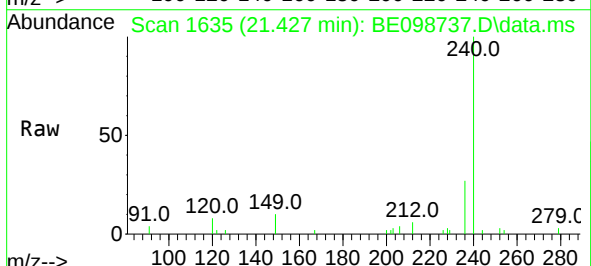


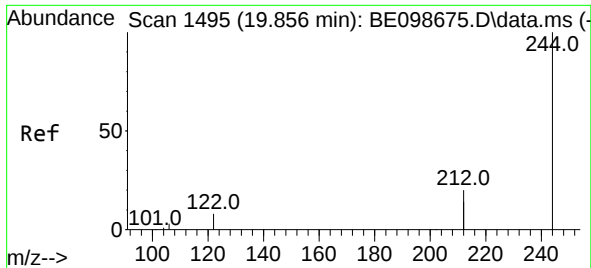

#29
Terphenyl-d14
Concen: 0.27 ng
RT: 19.862 min Scan# 1496
Delta R.T. 0.006 min
Lab File: BE098737.D
Acq: 20 Feb 2019 12:27

Instrument :
BNA_E
ClientSampleId :
PB117222BL

Tgt Ion:244	Resp:	4269
Ion Ratio	Lower	Upper
244	100	
212	43.4	29.4 44.2
122	10.4	7.1 10.7

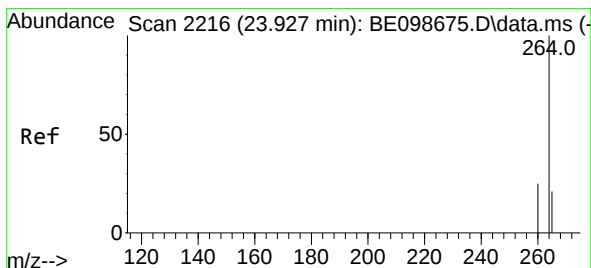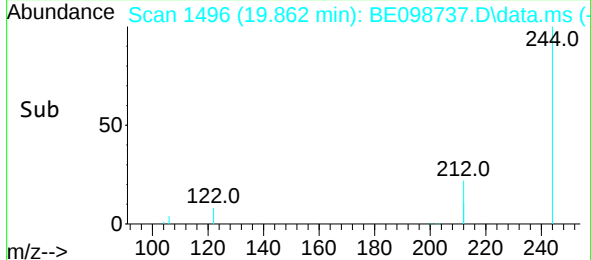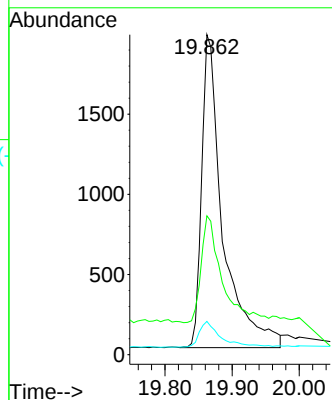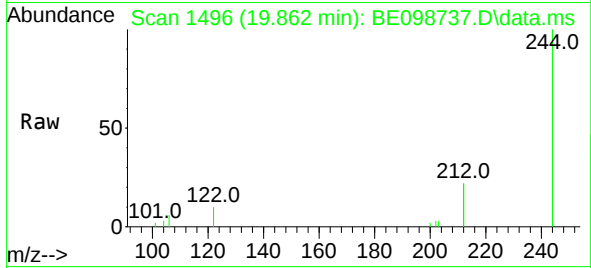

#34
Perylene-d12
Concen: 0.40 ng
RT: 23.933 min Scan# 2218
Delta R.T. 0.006 min
Lab File: BE098737.D
Acq: 20 Feb 2019 12:27

Tgt Ion:264	Resp:	5860
Ion Ratio	Lower	Upper
264	100	
260	26.4	20.5 30.7
265	28.9	22.3 33.5

