


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE022019\
 Data File : BE098734.D
 Acq On : 20 Feb 2019 10:19
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE012419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 24 14:44:44 2019

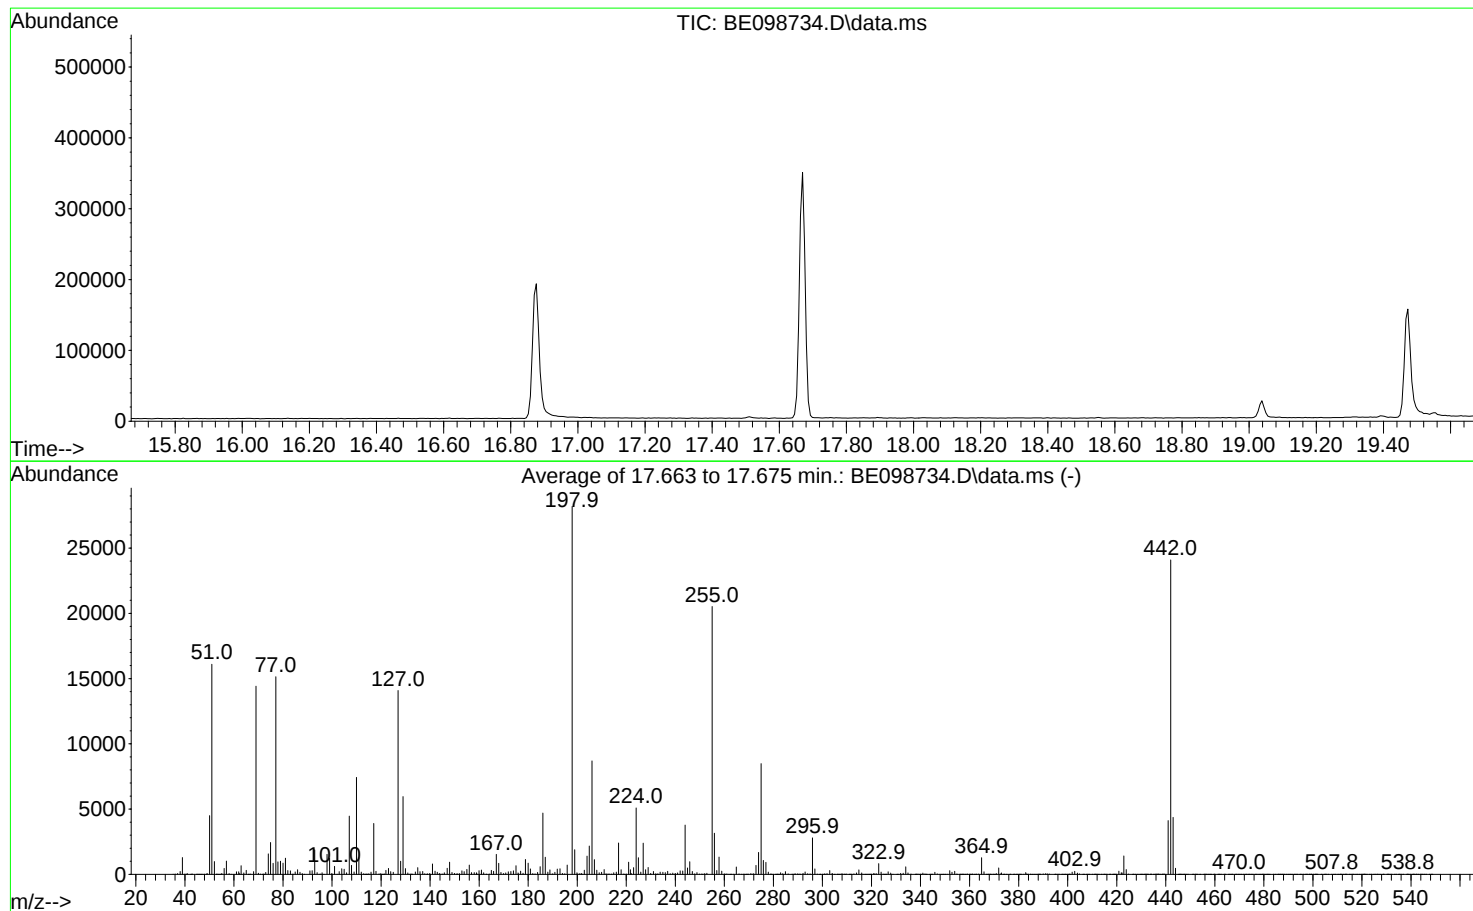

AutoFind: Scans 2566, 2567, 2568; Background Corrected with Scan 2558

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.1	16098	PASS
68	69	0.00	2	1.5	214	PASS
69	198	0.00	100	51.2	14419	PASS
70	69	0.00	2	0.6	90	PASS
127	198	10	80	50.0	14081	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	28186	PASS
199	198	5	9	6.7	1890	PASS
275	198	10	60	30.1	8484	PASS
365	198	1	100	4.5	1274	PASS
441	198	0.01	100	14.6	4114	PASS
442	198	50	100	85.5	24091	PASS
443	442	15	24	18.1	4370	PASS