

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE022619\
 Data File : BE098758.D
 Acq On : 26 Feb 2019 13:19
 Operator : JU/SJ
 Sample : SSTDICC0.8
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC0.8

Quant Time: Feb 26 13:51:56 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE022619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 26 13:42:02 2019
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.805	152	942	0.40	ng	0.00
7) Naphthalene-d8	10.601	136	4053	0.40	ng	0.00
13) Acenaphthene-d10	14.471	164	2510	0.40	ng	0.00
19) Phenanthrene-d10	17.215	188	6194	0.40	ng	#-0.01
27) Chrysene-d12	21.414	240	6745	0.40	ng	0.00
34) Perylene-d12	23.919	264	6298	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.398	112	1991	0.79	ng	0.00
5) Phenol-d6	6.988	99	3102	0.87	ng	0.00
8) Nitrobenzene-d5	8.964	82	3257	1.01	ng	-0.01
11) 2-Methylnaphthalene-d10	12.209	152	6016	0.90	ng	0.00
14) 2,4,6-Tribromophenol	15.970	330	846	0.77	ng	-0.01
15) 2-Fluorobiphenyl	13.088	172	8526	0.83	ng	0.00
25) Fluoranthene-d10	19.258	212	68341	0.89	ng	0.00
29) Terphenyl-d14	19.855	244	13052	0.87	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.314	88	1171	0.63	ng	92
3) n-Nitrosodimethylamine	3.636	42	1591	1.17	ng	# 13
6) bis(2-Chloroethyl)ether	7.230	93	2032	0.75	ng	92
9) Naphthalene	10.653	128	36005	0.89	ng	99
10) Hexachlorobutadiene	10.926	225	2302	0.80	ng	96
12) 2-Methylnaphthalene	12.281	142	5994	0.90	ng	98
16) Acenaphthylene	14.183	152	10306	0.95	ng	99
17) Acenaphthene	14.529	154	6124	0.90	ng	98
18) Fluorene	15.515	166	8473	0.96	ng	98
20) 4-Bromophenyl-phenylether	16.412	248	2801	0.85	ng	93
21) Hexachlorobenzene	16.532	284	3190	0.81	ng	94
22) Pentachlorophenol	16.894	266	630	0.54	ng	96
23) Phenanthrene	17.255	178	13349	0.91	ng	99
24) Anthracene	17.349	178	11068	0.88	ng	98
26) Fluoranthene	19.287	202	17008	0.90	ng	99
28) Pyrene	19.649	202	17254	0.93	ng	100
30) Benzo(a)anthracene	21.390	228	16000	0.88	ng	98
31) Chrysene	21.450	228	16525	0.88	ng	99
32) Bis(2-ethylhexyl)phtha...	21.317	149	31064	0.81	ng	100
33) Indeno(1,2,3-cd)pyrene	26.567	276	14501	0.75	ng	99
35) Benzo(b)fluoranthene	23.146	252	15522	0.90	ng	97
36) Benzo(k)fluoranthene	23.203	252	16575	0.88	ng	99
37) Benzo(a)pyrene	23.809	252	14705	0.87	ng	95
38) Dibenzo(a,h)anthracene	26.588	278	10012	0.67	ng	97
39) Benzo(g,h,i)perylene	27.376	276	13958	0.85	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE022619\
Data File : BE098758.D
Acq On : 26 Feb 2019 13:19
Operator : JU/SJ
Sample : SSTDICC0.8
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SSTDICC0.8

Quant Time: Feb 26 13:51:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE022619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 26 13:42:02 2019
Response via : Initial Calibration




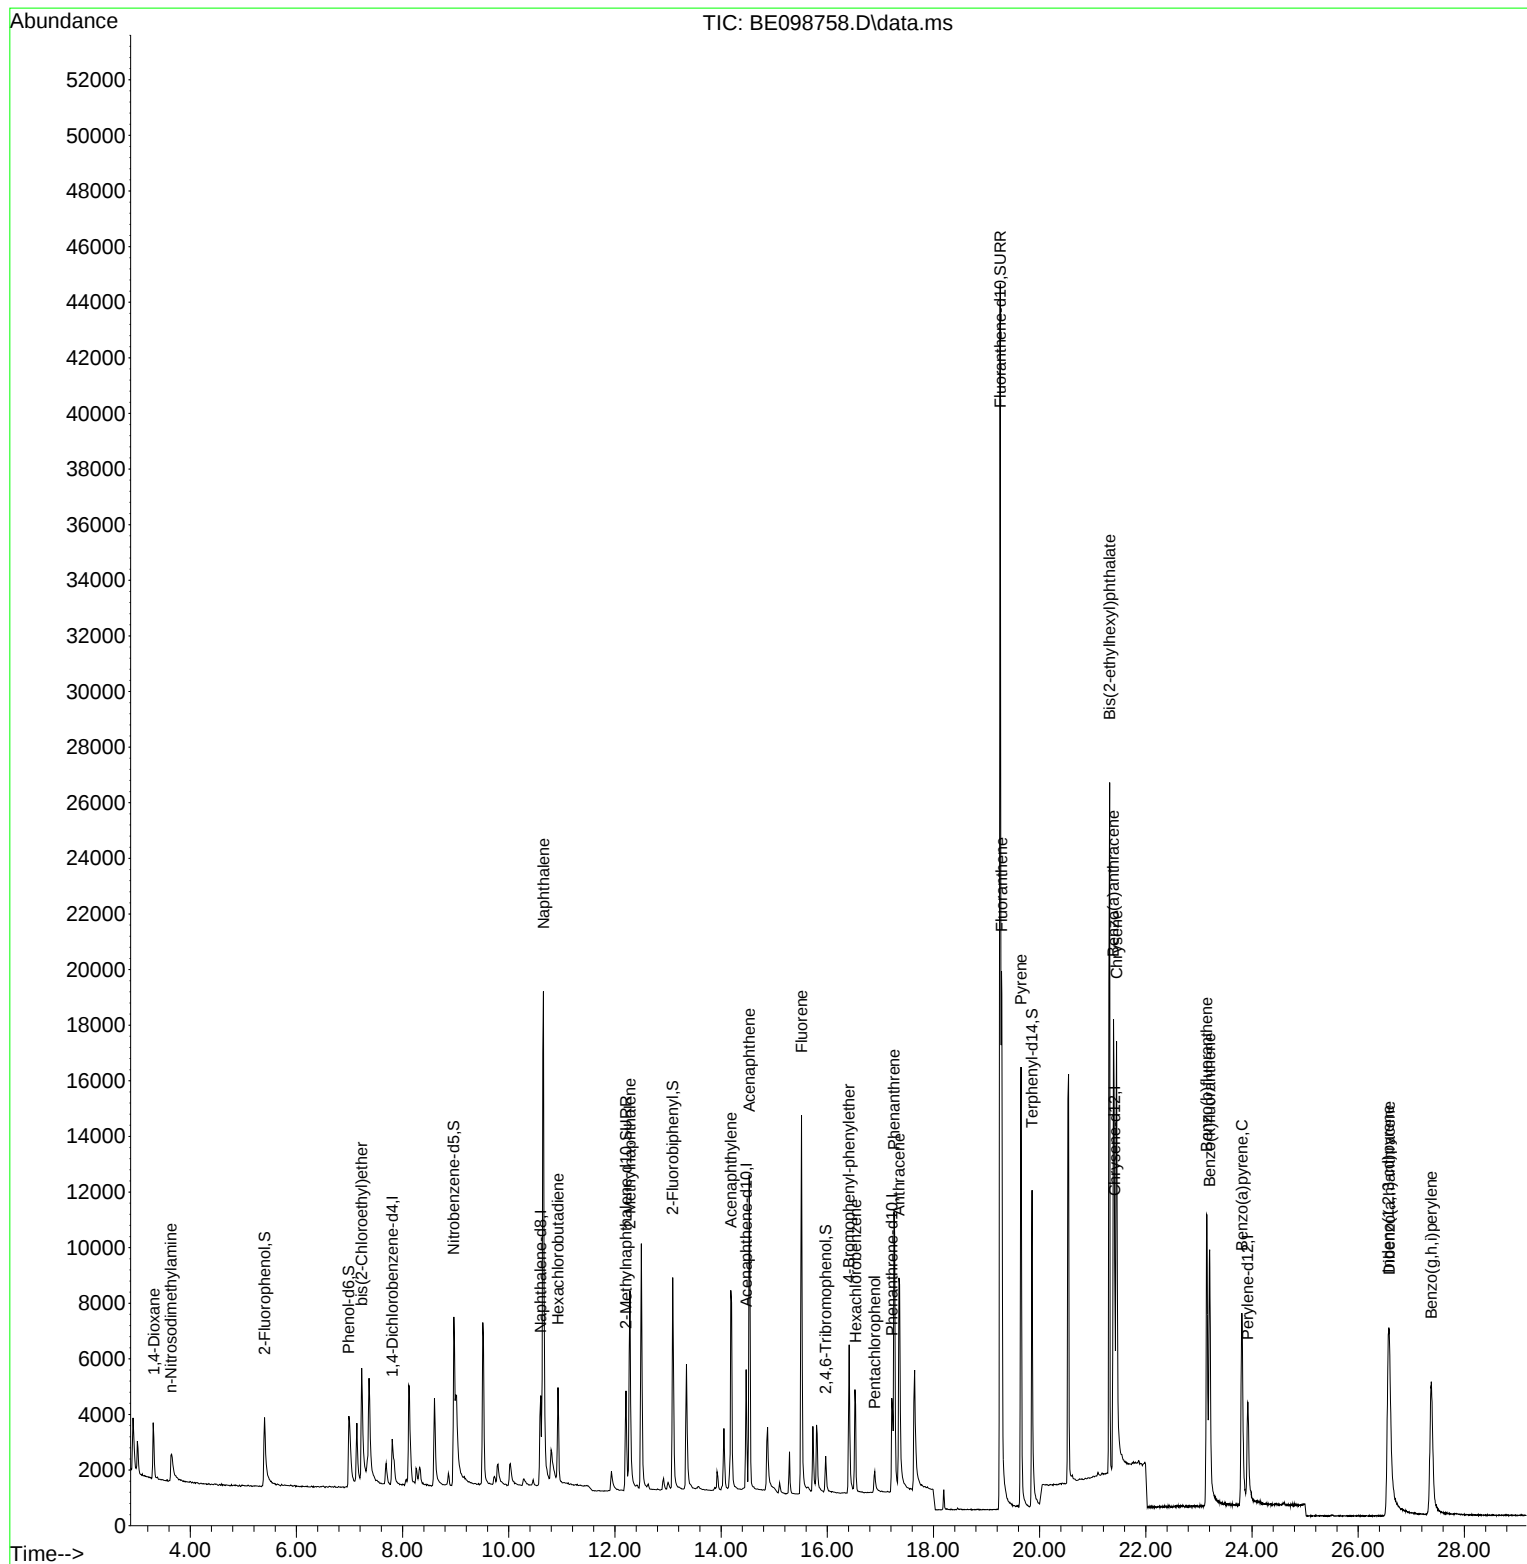




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.805 min Scan# 429
 Delta R.T. -0.010 min
 Lab File: BE098758.D
 Acq: 26 Feb 2019 13:19




Instrument :
 BNA_E
 ClientSampleID :
 SSTDICC0.8


Tgt Ion:152 Resp: 942
 Ion Ratio Lower Upper
 152 100
 150 154.7 121.4 182.2
 115 67.4 59.1 88.7

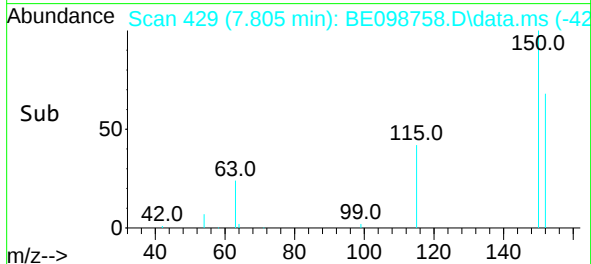

#2
 1,4-Dioxane
 Concen: 0.63 ng
 RT: 3.314 min Scan# 39
 Delta R.T. 0.002 min
 Lab File: BE098758.D
 Acq: 26 Feb 2019 13:19

Tgt Ion: 88 Resp: 1171
 Ion Ratio Lower Upper
 88 100
 58 103.2 73.9 110.9
 43 53.0 43.7 65.5


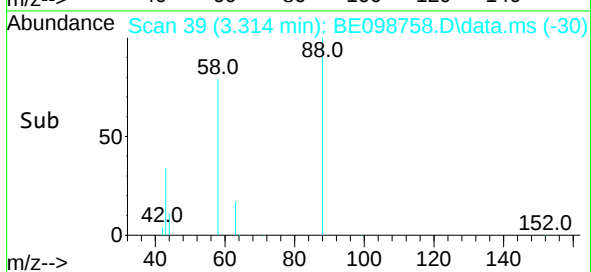




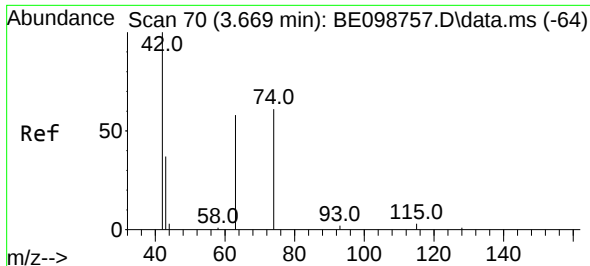

#3
n-Nitrosodimethylamine
Concen: 1.17 ng
RT: 3.636 min Scan# 67
Delta R.T. -0.033 min
Lab File: BE098758.D
Acq: 26 Feb 2019 13:19




Instrument :
BNA_E
ClientSampleId :
SSTDIC0.8


Tgt Ion: 42 Resp: 1591
Ion Ratio Lower Upper
42 100
74 0.0 58.9 88.3#
44 0.0 0.0 0.0

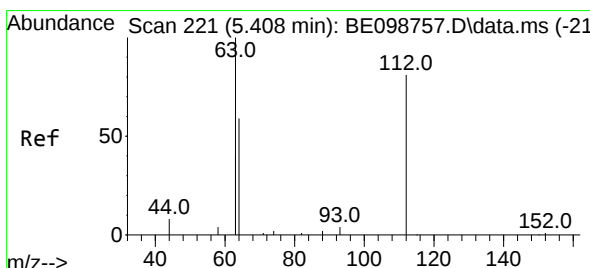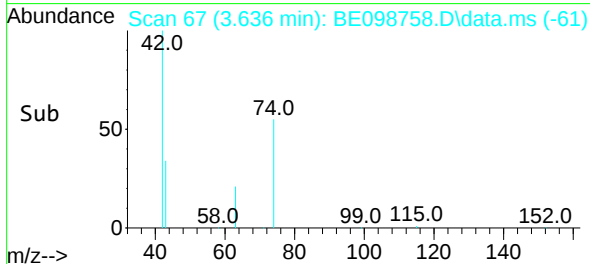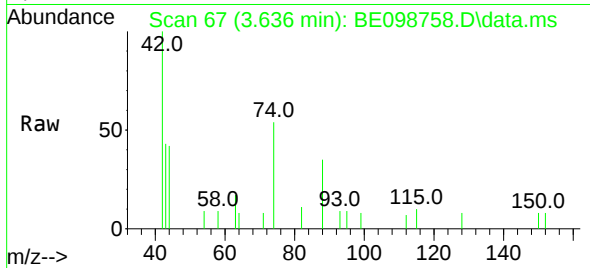

#4
2-Fluorophenol
Concen: 0.79 ng
RT: 5.398 min Scan# 220
Delta R.T. -0.010 min
Lab File: BE098758.D
Acq: 26 Feb 2019 13:19

Tgt Ion: 112 Resp: 1991
Ion Ratio Lower Upper
112 100
64 86.3 62.9 94.3
63 199.0 152.2 228.4


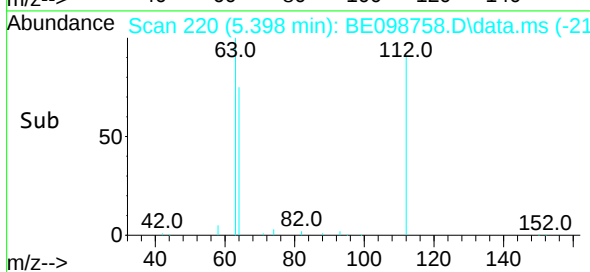

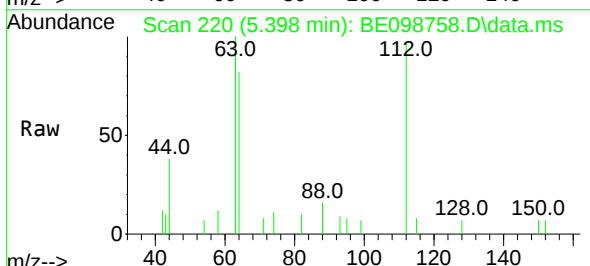


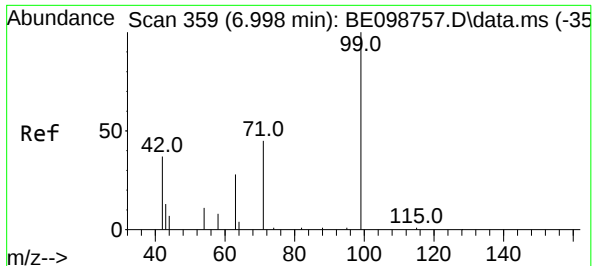

#5
Phenol-d6
Concen: 0.87 ng
RT: 6.988 min Scan# 358
Delta R.T. -0.010 min
Lab File: BE098758.D
Acq: 26 Feb 2019 13:19




Instrument :
BNA_E
ClientSampleId :
SSTDIC0.8


Tgt Ion: 99 Resp: 3102
Ion Ratio Lower Upper
99 100
42 31.1 24.6 37.0
71 49.7 35.1 52.7

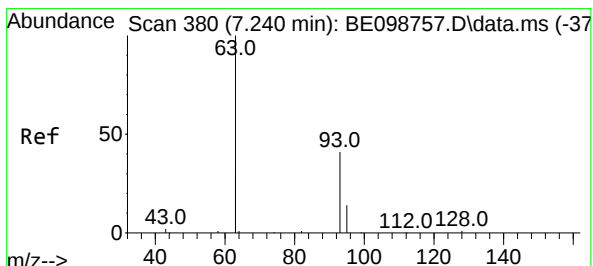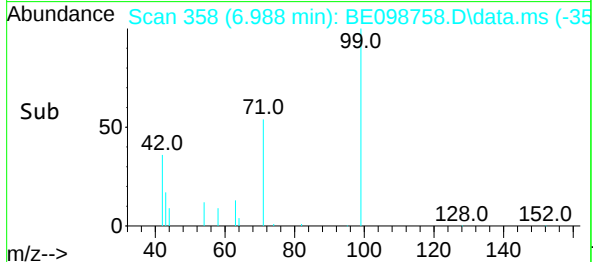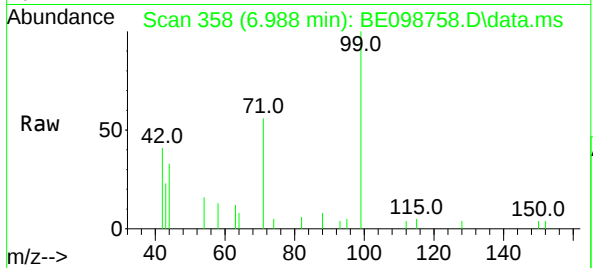

#6
bis(2-Chloroethyl)ether
Concen: 0.75 ng
RT: 7.230 min Scan# 379
Delta R.T. -0.010 min
Lab File: BE098758.D
Acq: 26 Feb 2019 13:19

Tgt Ion: 93 Resp: 2032
Ion Ratio Lower Upper
93 100
63 351.7 267.3 400.9
95 36.5 26.2 39.4


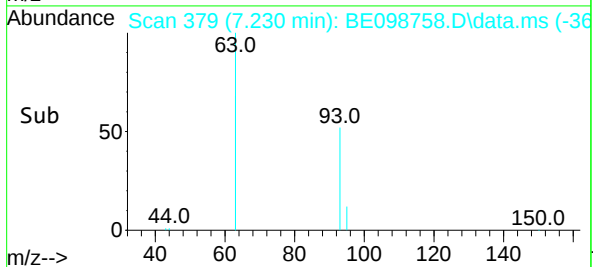

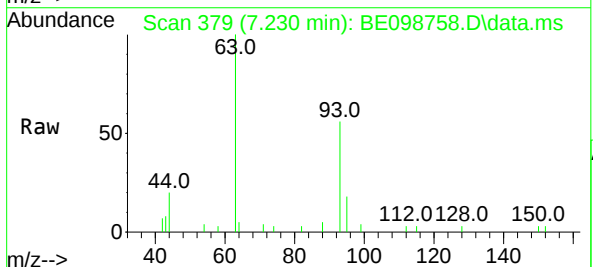




#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.601 min Scan# 649
Delta R.T. -0.001 min
Lab File: BE098758.D
Acq: 26 Feb 2019 13:19




Instrument :
BNA_E
ClientSampleId :
SSTDIC0.8


Tgt Ion:	136	Resp:	4053
Ion	Ratio	Lower	Upper
136	100		
137	12.3	9.7	14.5
54	42.9	35.5	53.3
68	6.5	5.0	7.6

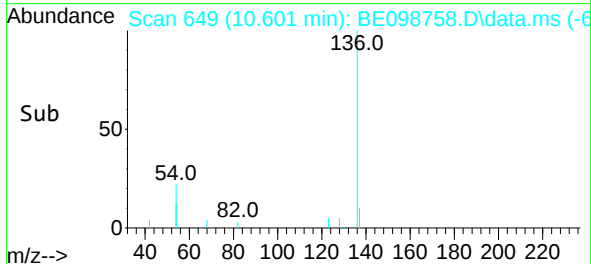

#8
Nitrobenzene-d5
Concen: 1.01 ng
RT: 8.964 min Scan# 523
Delta R.T. -0.014 min
Lab File: BE098758.D
Acq: 26 Feb 2019 13:19

Tgt Ion:	82	Resp:	3257
Ion	Ratio	Lower	Upper
82	100		
128	122.0	96.5	144.7
54	315.8	224.7	337.1


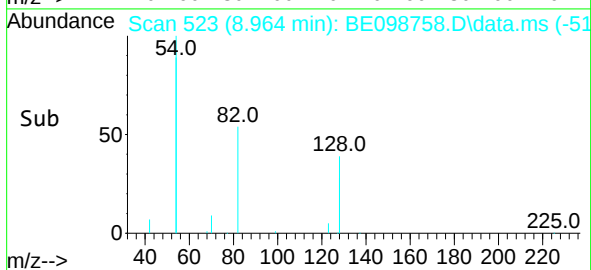

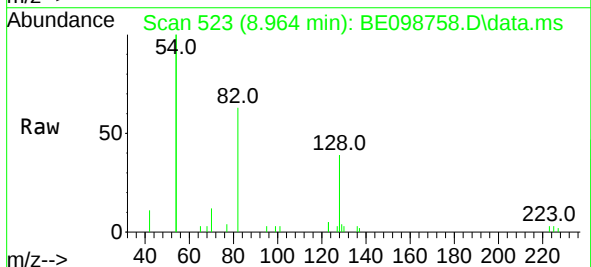




#9
Naphthalene
Concen: 0.89 ng
RT: 10.653 min Scan# 653
Delta R.T. -0.001 min
Lab File: BE098758.D
Acq: 26 Feb 2019 13:19




Instrument :
BNA_E
ClientSampleId :
SSTDIC0.8


Tgt Ion:128	Resp:	36005
Ion Ratio	Lower	Upper
128	100	
129	3.0	2.6 3.8
127	3.4	3.0 4.6

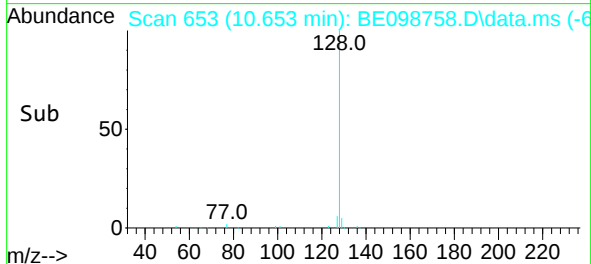

#10
Hexachlorobutadiene
Concen: 0.80 ng
RT: 10.926 min Scan# 674
Delta R.T. -0.001 min
Lab File: BE098758.D
Acq: 26 Feb 2019 13:19

Tgt Ion:225	Resp:	2302
Ion Ratio	Lower	Upper
225	100	
223	63.5	47.8 71.8
227	65.4	50.5 75.7


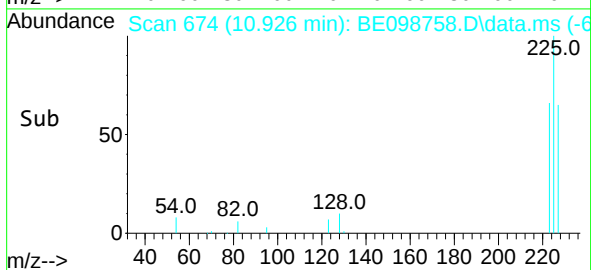

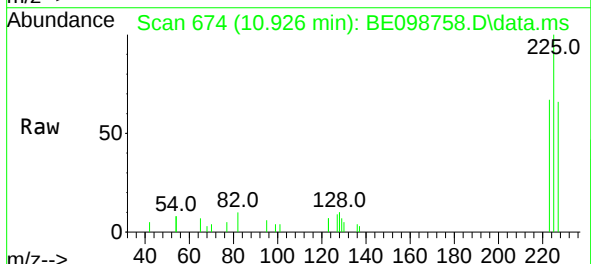




#11
2-Methylnaphthalene-d10
Concen: 0.90 ng
RT: 12.209 min Scan# 763
Delta R.T. -0.001 min
Lab File: BE098758.D
Acq: 26 Feb 2019 13:19




Instrument :
BNA_E
ClientSampleId :
SSTDIC0.8


Tgt Ion:152 Resp: 6016
Ion Ratio Lower Upper
152 100
151 19.8 16.2 24.4

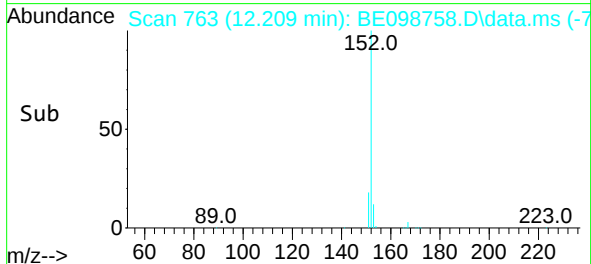

#12
2-Methylnaphthalene
Concen: 0.90 ng
RT: 12.281 min Scan# 768
Delta R.T. -0.001 min
Lab File: BE098758.D
Acq: 26 Feb 2019 13:19

Tgt Ion:142 Resp: 5994
Ion Ratio Lower Upper
142 100
141 85.5 70.0 105.0
115 45.1 35.2 52.8


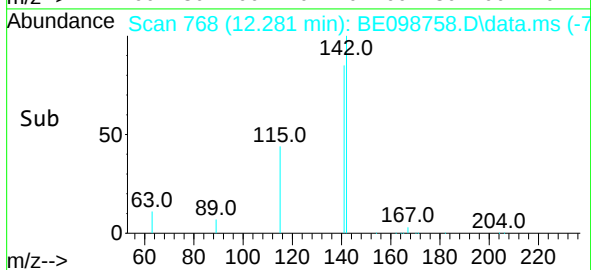

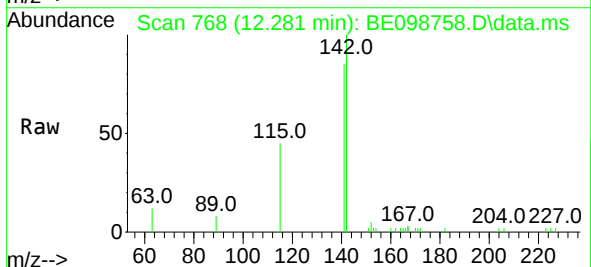


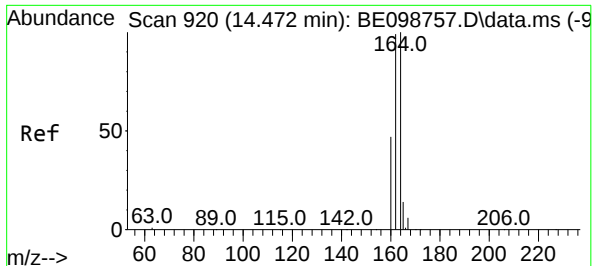

#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.471 min Scan# 920
Delta R.T. -0.001 min
Lab File: BE098758.D
Acq: 26 Feb 2019 13:19




Instrument :
BNA_E
ClientSampleId :
SSTDICC0.8


Tgt Ion:	164	Resp:	2510
Ion	Ratio	Lower	Upper
164	100		
162	103.9	80.5	120.7
160	47.4	40.1	60.1

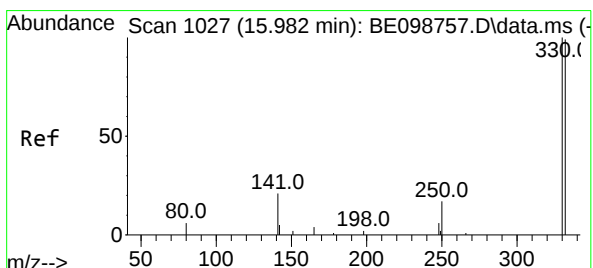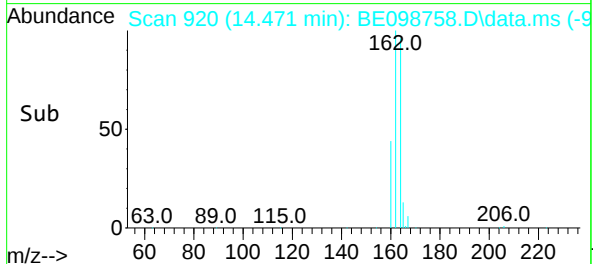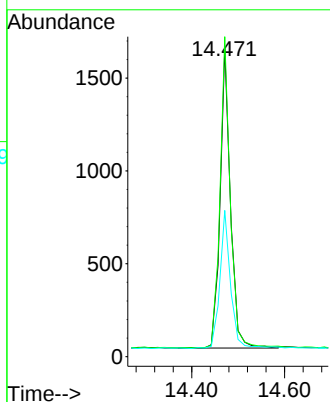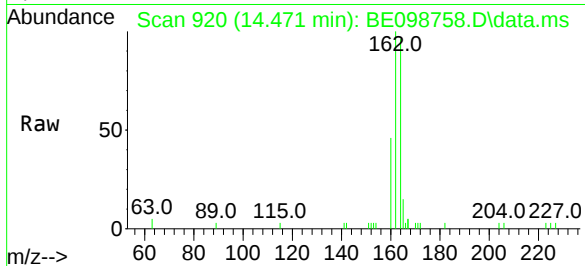

#14
2,4,6-Tribromophenol
Concen: 0.77 ng
RT: 15.970 min Scan# 1026
Delta R.T. -0.012 min
Lab File: BE098758.D
Acq: 26 Feb 2019 13:19

Tgt Ion:	330	Resp:	846
Ion	Ratio	Lower	Upper
330	100		
332	99.6	73.3	109.9
141	46.1	33.1	49.7


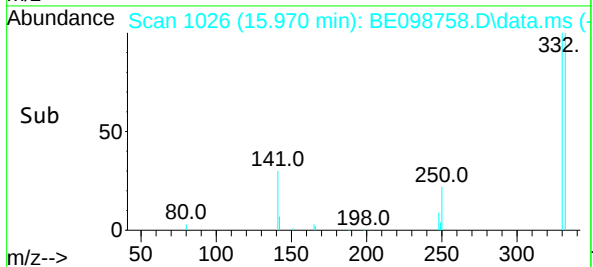
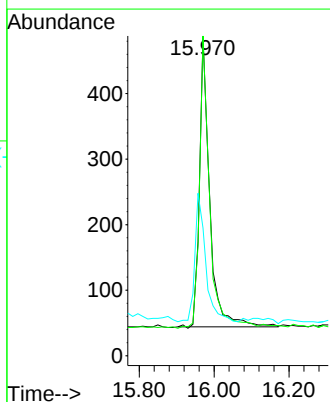
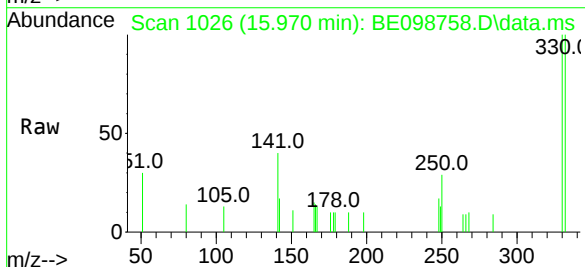


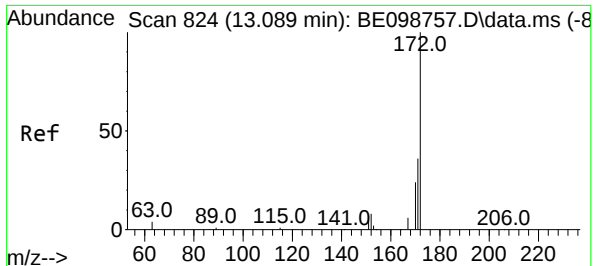

#15
2-Fluorobiphenyl
Concen: 0.83 ng
RT: 13.088 min Scan# 824
Delta R.T. -0.001 min
Lab File: BE098758.D
Acq: 26 Feb 2019 13:19




Instrument :
BNA_E
ClientSampleId :
SSTDIC0.8


Tgt Ion:	172	Resp:	8526
Ion Ratio	Lower	Upper	
172	100		
171	33.7	29.0	43.4
170	23.7	20.8	31.2

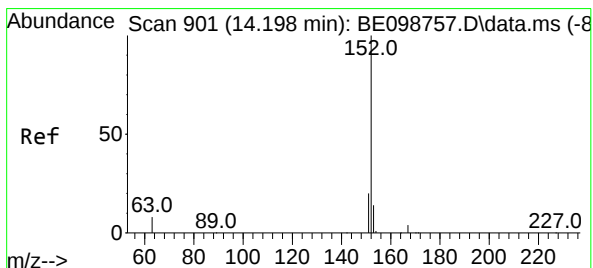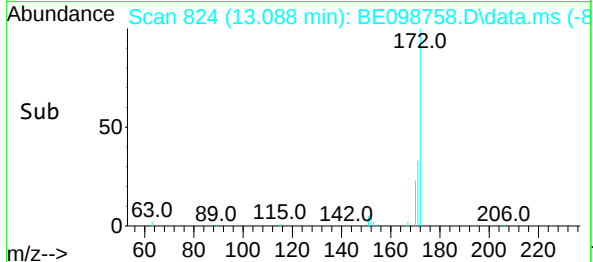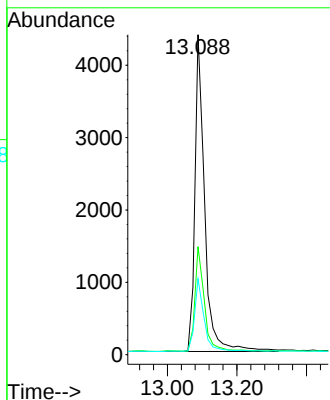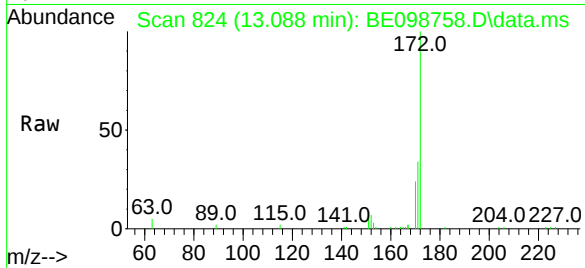

#16
Acenaphthylene
Concen: 0.95 ng
RT: 14.183 min Scan# 900
Delta R.T. -0.015 min
Lab File: BE098758.D
Acq: 26 Feb 2019 13:19

Tgt Ion:	152	Resp:	10306
Ion Ratio	Lower	Upper	
152	100		
151	20.0	16.3	24.5
153	12.9	10.7	16.1

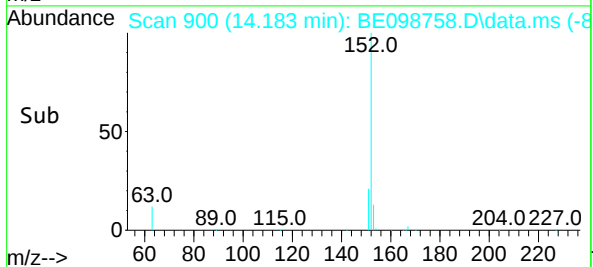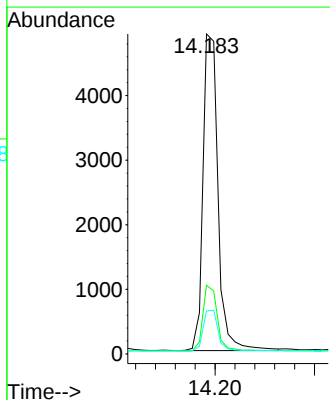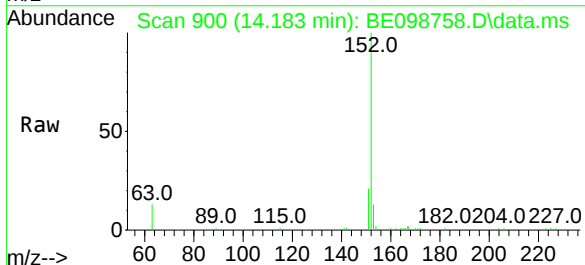

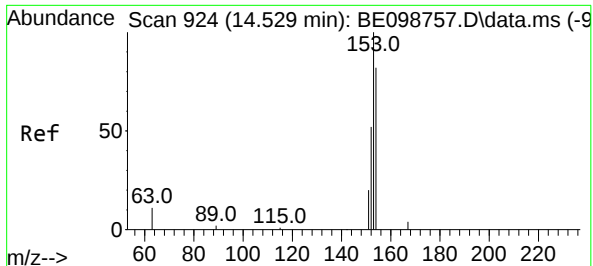

#17

Acenaphthene

Concen: 0.90 ng

RT: 14.529 min Scan# 924

Delta R.T. -0.001 min

Lab File: BE098758.D

Acq: 26 Feb 2019 13:19





Instrument :

BNA_E

ClientSampleId :

SSTDICC0.8

Tgt Ion:154	Resp:	6124	
Ion	Ratio	Lower	Upper
154	100		
153	116.7	93.9	140.9
152	54.7	45.8	68.8

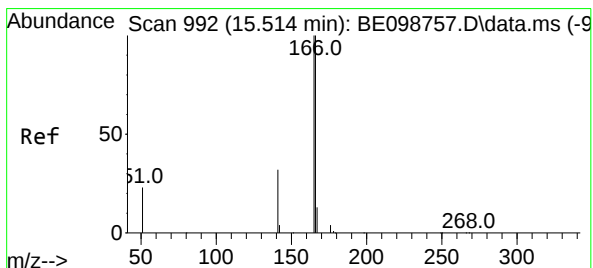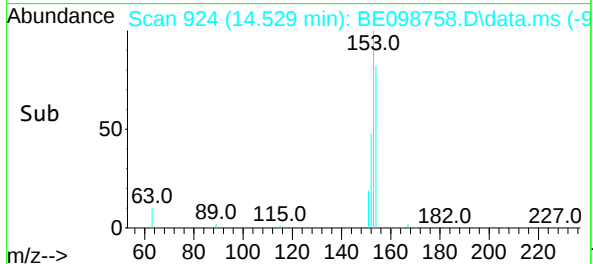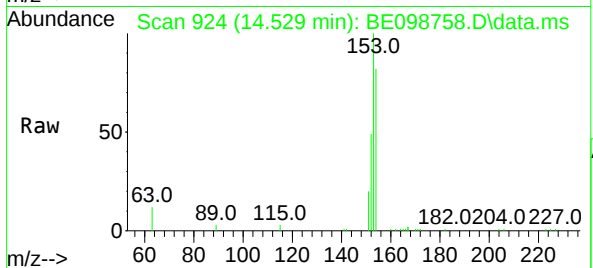

#18

Fluorene

Concen: 0.96 ng




RT: 15.515 min Scan# 992


Delta R.T. 0.001 min

Lab File: BE098758.D

Acq: 26 Feb 2019 13:19

Tgt Ion:166	Resp:	8473	
Ion	Ratio	Lower	Upper
166	100		
165	101.3	79.3	118.9
167	13.1	10.6	15.8


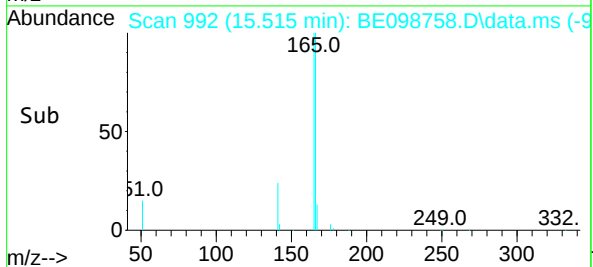

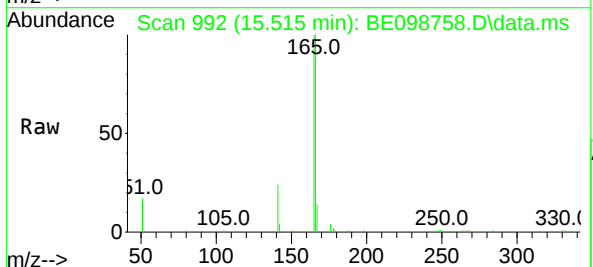




#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.215 min Scan# 1119
Delta R.T. -0.012 min
Lab File: BE098758.D
Acq: 26 Feb 2019 13:19




Instrument :
BNA_E
ClientSampleId :
SSTDICC0.8


Tgt Ion:188 Resp: 6194
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 12.4 4.7 7.1#

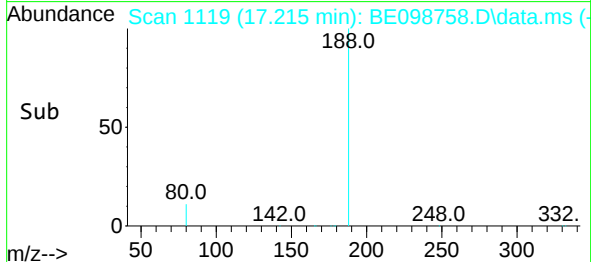

#20
4-Bromophenyl-phenylether
Concen: 0.85 ng
RT: 16.412 min Scan# 1059
Delta R.T. 0.001 min
Lab File: BE098758.D
Acq: 26 Feb 2019 13:19

Tgt Ion:248 Resp: 2801
Ion Ratio Lower Upper
248 100
250 93.3 80.2 120.4
141 69.0 60.5 90.7


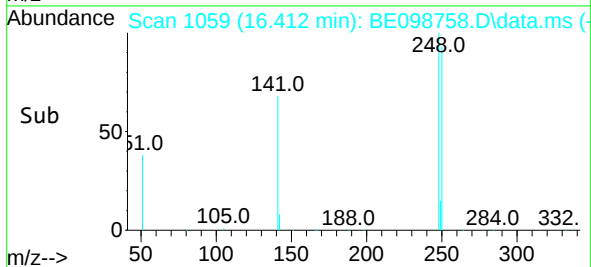

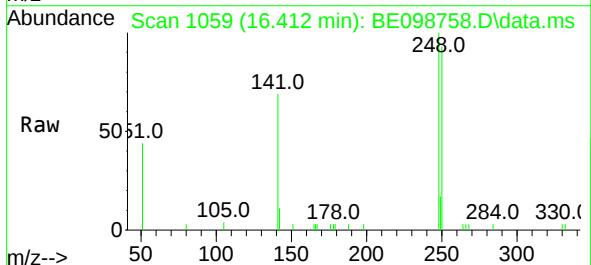




#21
Hexachlorobenzene
Concen: 0.81 ng
RT: 16.532 min Scan# 1068
Delta R.T. 0.001 min
Lab File: BE098758.D
Acq: 26 Feb 2019 13:19




Instrument :
BNA_E
ClientSampleId :
SSTDIC0.8


Tgt Ion:284 Resp: 3190
Ion Ratio Lower Upper
284 100
142 37.0 25.5 38.3
249 34.9 26.6 39.8

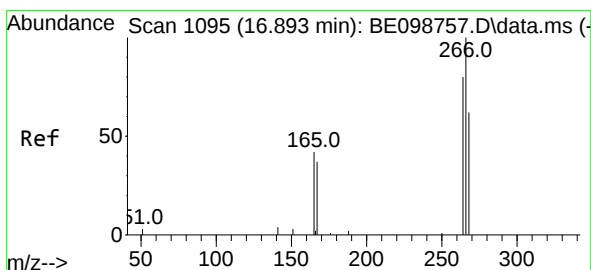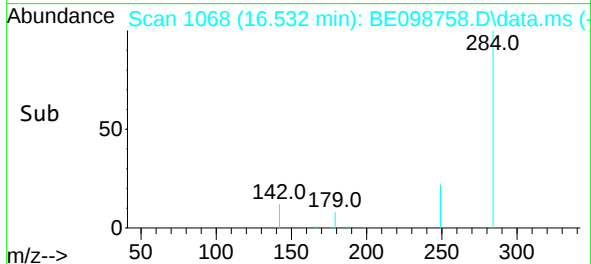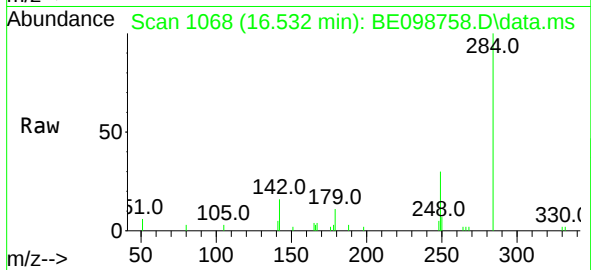

#22
Pentachlorophenol
Concen: 0.54 ng
RT: 16.894 min Scan# 1095
Delta R.T. 0.001 min
Lab File: BE098758.D
Acq: 26 Feb 2019 13:19

Tgt Ion:266 Resp: 630
Ion Ratio Lower Upper
266 100
264 71.7 53.7 80.5
268 76.6 59.8 89.8


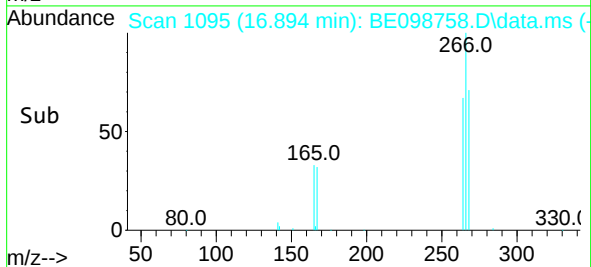

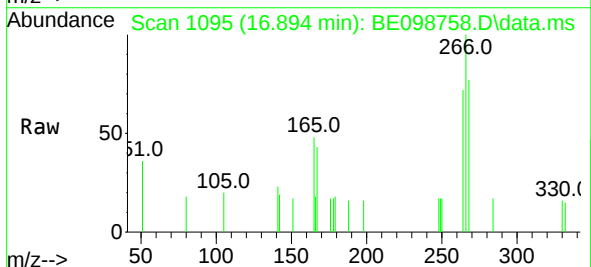


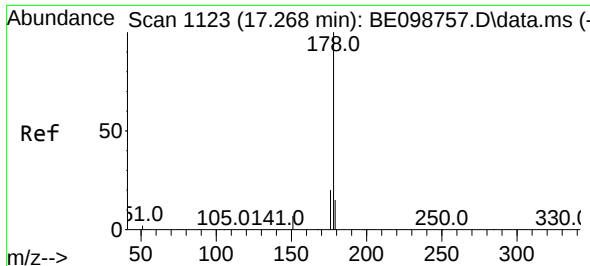

#23
Phenanthrene
Concen: 0.91 ng
RT: 17.255 min Scan# 1122
Delta R.T. -0.012 min
Lab File: BE098758.D
Acq: 26 Feb 2019 13:19




Instrument :
BNA_E
ClientSampleId :
SSTDICC0.8


Tgt Ion:178 Resp: 13349
Ion Ratio Lower Upper
178 100
176 19.6 15.9 23.9
179 15.6 12.2 18.4

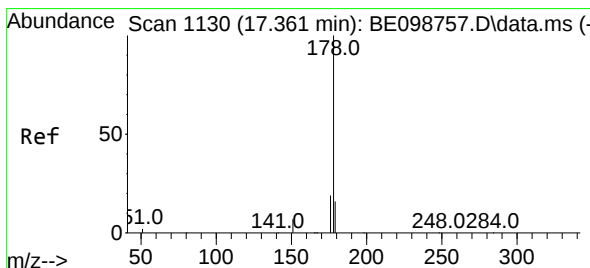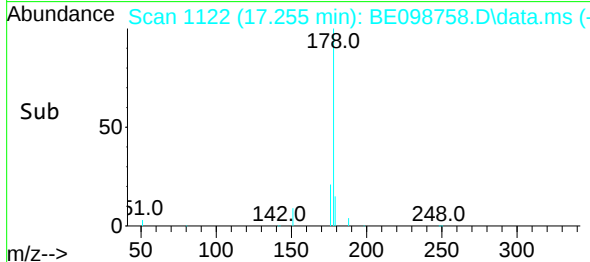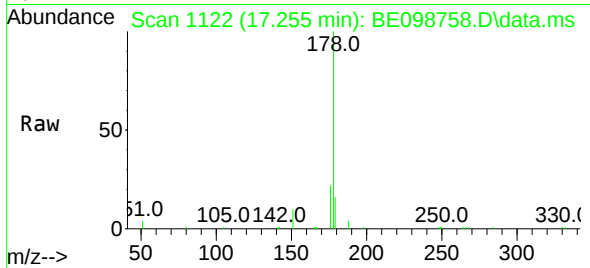

#24
Anthracene
Concen: 0.88 ng
RT: 17.349 min Scan# 1129
Delta R.T. -0.012 min
Lab File: BE098758.D
Acq: 26 Feb 2019 13:19

Tgt Ion:178 Resp: 11068
Ion Ratio Lower Upper
178 100
176 19.4 14.9 22.3
179 15.7 11.8 17.8


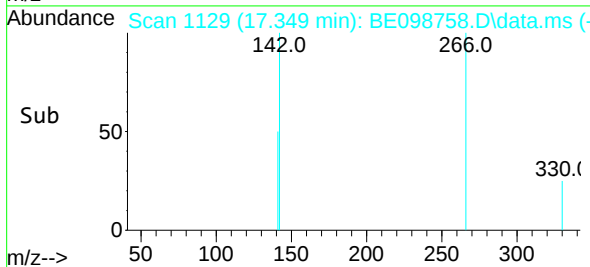

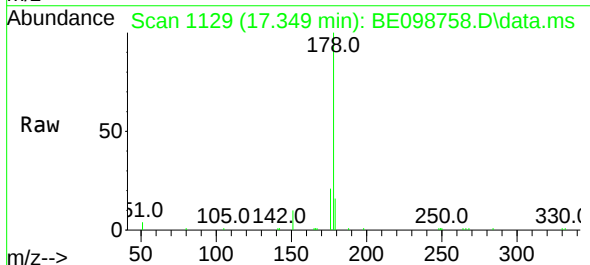




#25
Fluoranthene-d10
Concen: 0.89 ng
RT: 19.258 min Scan# 1391
Delta R.T. 0.005 min
Lab File: BE098758.D
Acq: 26 Feb 2019 13:19




Instrument :
BNA_E
ClientSampleId :
SSTDICC0.8


Tgt Ion:212 Resp: 68341
Ion Ratio Lower Upper
212 100
106 2.1 1.7 2.5
104 1.2 1.0 1.6

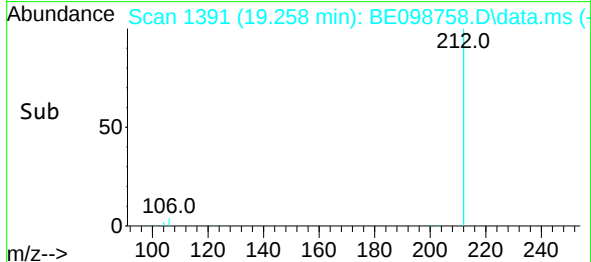

#26
Fluoranthene
Concen: 0.90 ng
RT: 19.287 min Scan# 1396
Delta R.T. -0.001 min
Lab File: BE098758.D
Acq: 26 Feb 2019 13:19

Tgt Ion:202 Resp: 17008
Ion Ratio Lower Upper
202 100
101 8.2 6.7 10.1
203 16.9 13.3 19.9


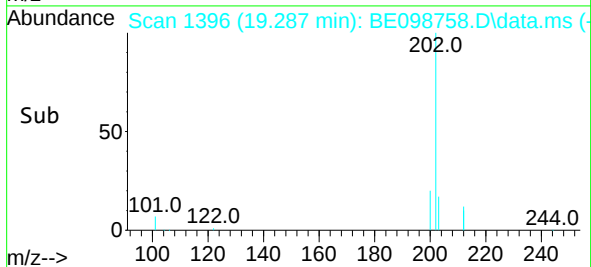

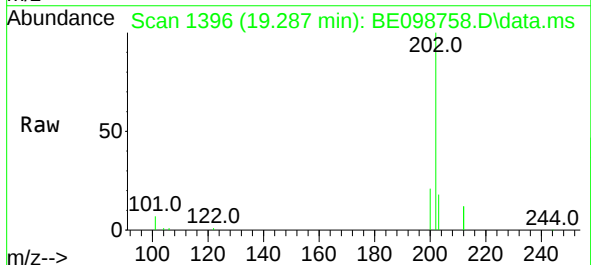


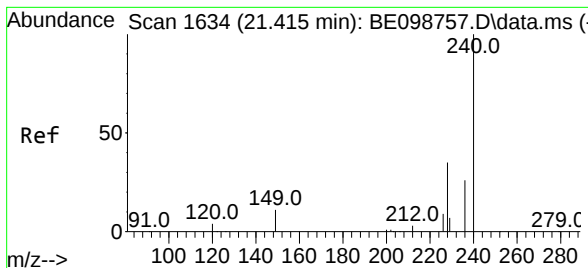

#27
Chrysene-d12
Concen: 0.40 ng
RT: 21.414 min Scan# 1634
Delta R.T. -0.001 min
Lab File: BE098758.D
Acq: 26 Feb 2019 13:19




Instrument :
BNA_E
ClientSampleId :
SSTDICC0.8


Tgt Ion:240 Resp: 6745
Ion Ratio Lower Upper
240 100
120 5.4 4.7 7.1
236 28.2 21.9 32.9

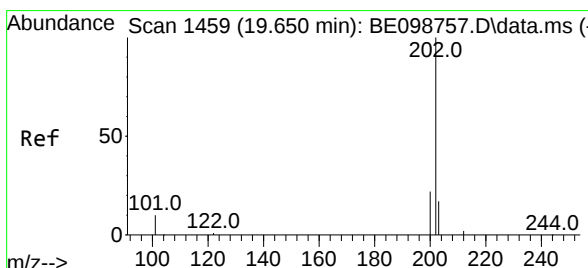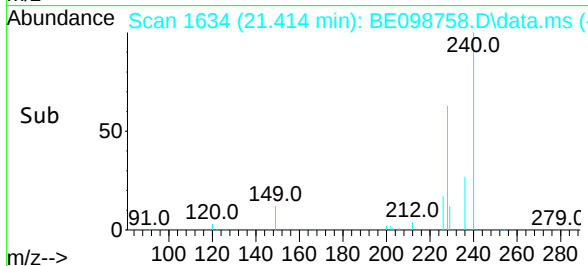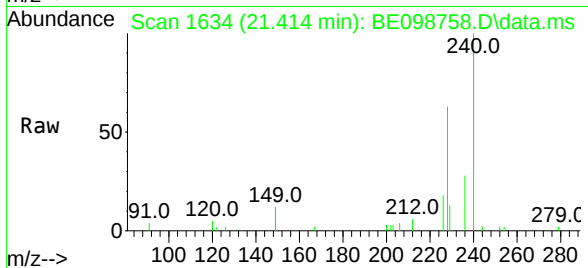

#28
Pyrene
Concen: 0.93 ng
RT: 19.649 min Scan# 1459
Delta R.T. -0.001 min
Lab File: BE098758.D
Acq: 26 Feb 2019 13:19

Tgt Ion:202 Resp: 17254
Ion Ratio Lower Upper
202 100
200 21.5 17.0 25.6
203 17.4 13.8 20.8


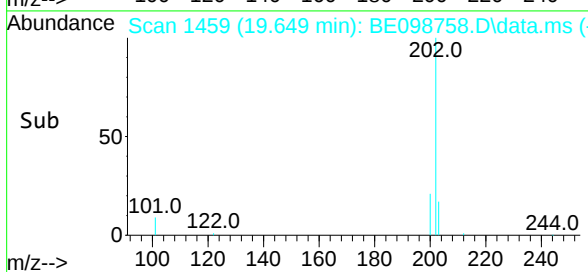

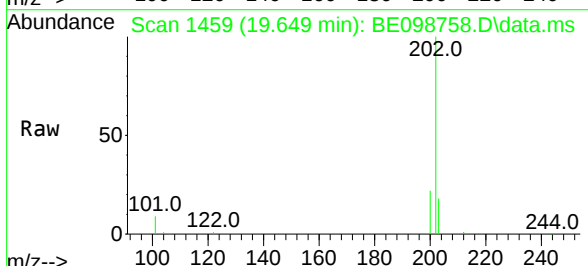




#29
Terphenyl-d14
Concen: 0.87 ng
RT: 19.855 min Scan# 1495
Delta R.T. -0.001 min
Lab File: BE098758.D
Acq: 26 Feb 2019 13:19




Instrument :
BNA_E
ClientSampleId :
SSTDIC0.8


Tgt Ion:244	Resp:	13052
Ion Ratio	Lower	Upper
244	100	
212	35.8	29.4 44.2
122	8.0	7.1 10.7



#30
Benzo(a)anthracene
Concen: 0.88 ng
RT: 21.390 min Scan# 1632
Delta R.T. -0.001 min
Lab File: BE098758.D
Acq: 26 Feb 2019 13:19

Tgt Ion:228	Resp:	16000
Ion Ratio	Lower	Upper
228	100	
226	28.0	23.0 34.4
229	20.1	15.0 22.6

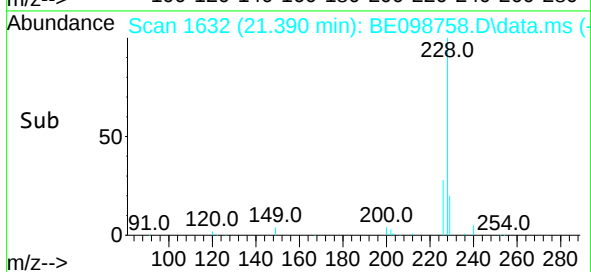

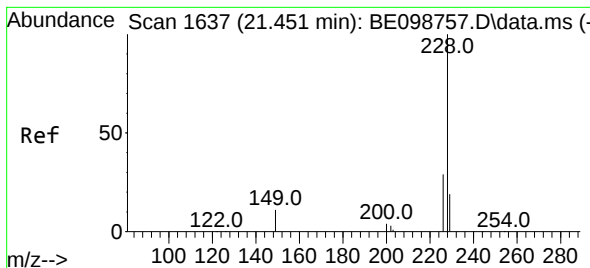

#31

Chrysene

Concen: 0.88 ng

RT: 21.450 min Scan# 1637

Delta R.T. -0.001 min

Lab File: BE098758.D

Acq: 26 Feb 2019 13:19





Instrument :

BNA_E

ClientSampleId :

SSTDIC0.8

Tgt Ion:228	Resp:	16525
Ion Ratio	Lower	Upper
228	100	
226	29.8	24.6 36.8
229	20.0	16.4 24.6

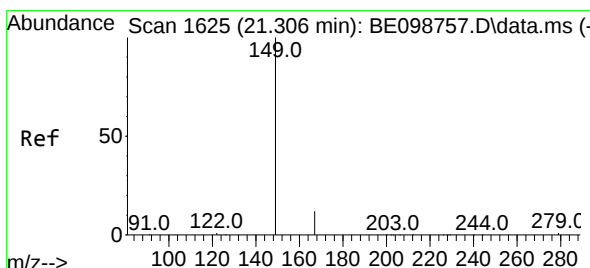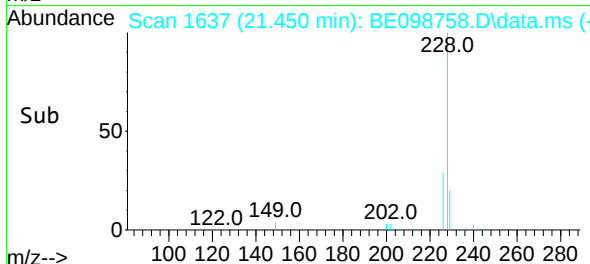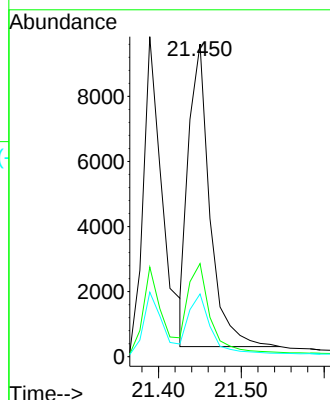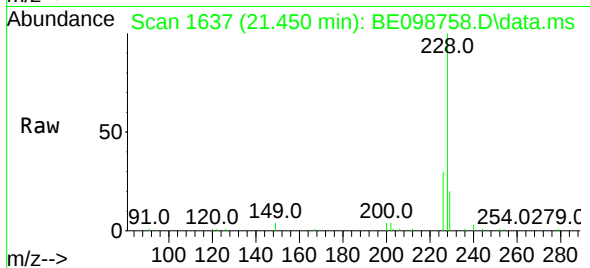

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.81 ng




RT: 21.317 min Scan# 1626


Delta R.T. 0.011 min

Lab File: BE098758.D

Acq: 26 Feb 2019 13:19

Tgt Ion:149	Resp:	31064
Ion Ratio	Lower	Upper
149	100	
167	6.8	5.4 8.2
279	1.1	1.0 1.4


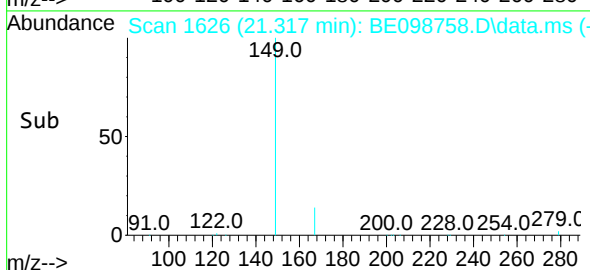
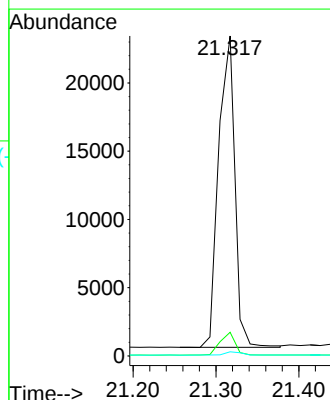
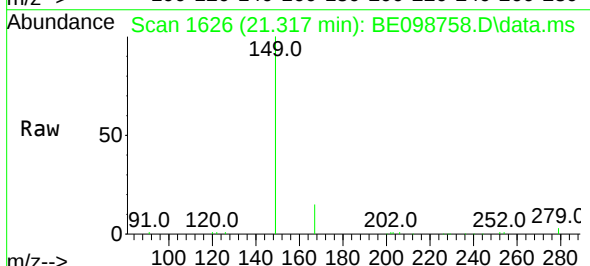




#33
Indeno(1,2,3-cd)pyrene
Concen: 0.75 ng
RT: 26.567 min Scan# 2952
Delta R.T. -0.004 min
Lab File: BE098758.D
Acq: 26 Feb 2019 13:19




Instrument :
BNA_E
ClientSampleId :
SSTDIC0.8


Tgt Ion:276 Resp: 14501
Ion Ratio Lower Upper
276 100
138 15.5 13.3 19.9
277 24.2 19.4 29.0



#34
Perylene-d12
Concen: 0.40 ng
RT: 23.919 min Scan# 2214
Delta R.T. -0.001 min
Lab File: BE098758.D
Acq: 26 Feb 2019 13:19

Tgt Ion:264 Resp: 6298
Ion Ratio Lower Upper
264 100
260 26.1 20.5 30.7
265 30.5 22.3 33.5


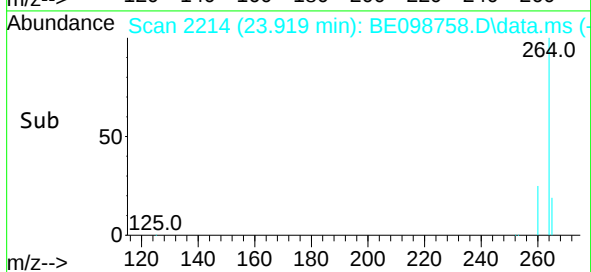






#35
Benzo(b)fluoranthene
Concen: 0.90 ng
RT: 23.146 min Scan# 1997
Delta R.T. -0.001 min
Lab File: BE098758.D
Acq: 26 Feb 2019 13:19




Instrument :
BNA_E
ClientSampleId :
SSTDIC0.8


Tgt Ion:252 Resp: 15522
Ion Ratio Lower Upper
252 100
253 22.9 19.4 29.0
125 8.4 8.2 12.4

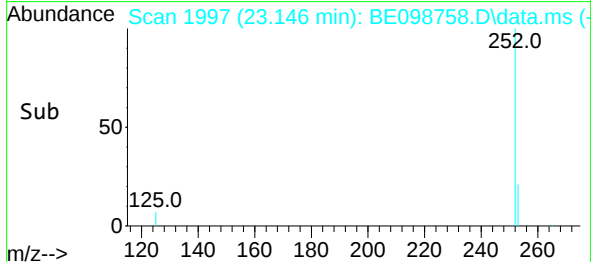

#36
Benzo(k)fluoranthene
Concen: 0.88 ng
RT: 23.203 min Scan# 2013
Delta R.T. 0.006 min
Lab File: BE098758.D
Acq: 26 Feb 2019 13:19

Tgt Ion:252 Resp: 16575
Ion Ratio Lower Upper
252 100
253 23.4 19.0 28.4
125 7.9 7.0 10.4


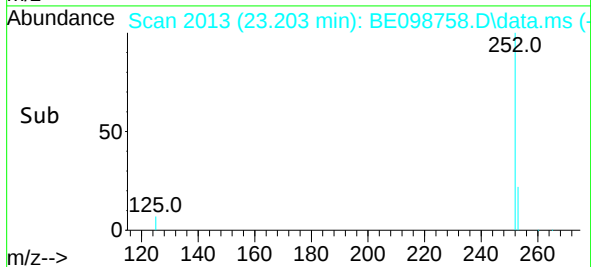

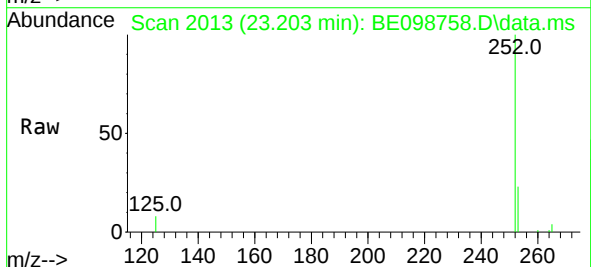




#37
Benzo(a)pyrene
Concen: 0.87 ng
RT: 23.809 min Scan# 2183
Delta R.T. 0.002 min
Lab File: BE098758.D
Acq: 26 Feb 2019 13:19




Instrument :
BNA_E
ClientSampleId :
SSTDICC0.8


Tgt Ion:252	Resp:	14705
Ion Ratio	Lower	Upper
252	100	
253	24.0	21.0 31.4
125	9.5	9.2 13.8

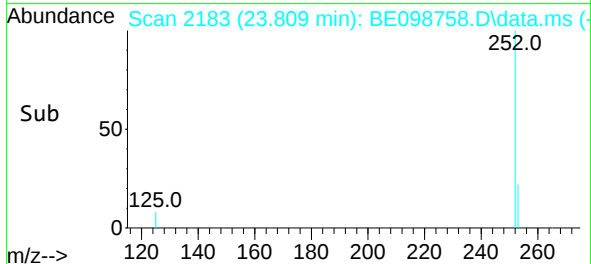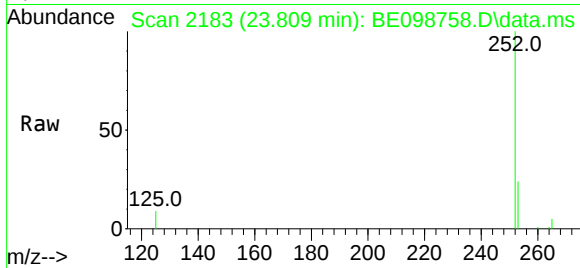

#38
Dibenzo(a,h)anthracene
Concen: 0.67 ng
RT: 26.588 min Scan# 2958
Delta R.T. -0.007 min
Lab File: BE098758.D
Acq: 26 Feb 2019 13:19


Tgt Ion:278	Resp:	10012
Ion Ratio	Lower	Upper
278	100	
139	13.3	12.7 19.1
279	26.6	22.0 33.0

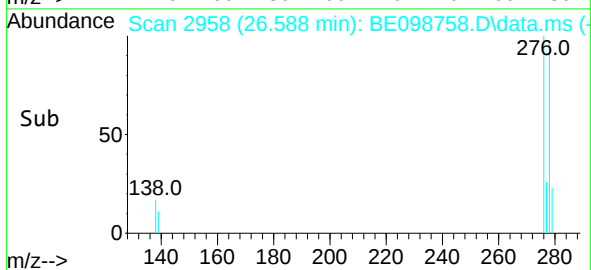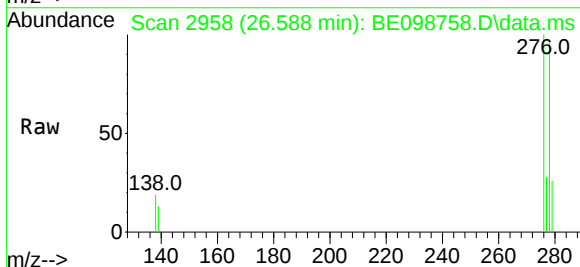



#39
Benzo(g,h,i)perylene
Concen: 0.85 ng
RT: 27.376 min Scan# 3179
Delta R.T. 0.003 min
Lab File: BE098758.D
Acq: 26 Feb 2019 13:19

Instrument :
BNA_E
ClientSampleId :
SSTDIC0.8

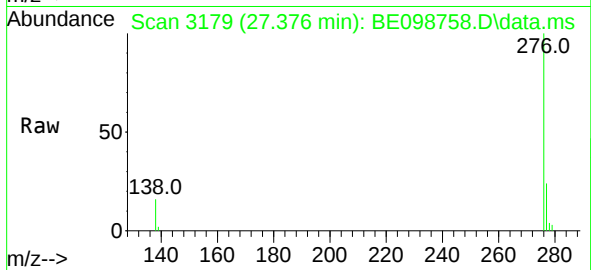

Tgt Ion:	276	Resp:	13958
Ion	Ratio	Lower	Upper
276	100		
277	24.0	20.3	30.5
138	15.9	13.3	19.9

