


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE022619\
Data File : BE098760.D
Acq On : 26 Feb 2019 14:34
Operator : JU/SJ
Sample : SSTDICC3.2
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2

Quant Time: Feb 26 15:06:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE022619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 26 14:06:40 2019
Response via : Initial Calibration



Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE022619\
 Data File : BE098760.D
 Acq On : 26 Feb 2019 14:34
 Operator : JU/SJ
 Sample : SSTDICC3.2
 Misc :
 ALS Vial : 7 Sample Multiplier: 1


Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC3.2

Quant Time: Feb 26 15:06:44 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE022619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 26 14:06:40 2019
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.803	152	1082	0.40	ng	-0.01
7) Naphthalene-d8	10.602	136	4169	0.40	ng	# 0.00
13) Acenaphthene-d10	14.471	164	2690	0.40	ng	0.00
19) Phenanthrene-d10	17.215	188	6107	0.40	ng	#-0.01
27) Chrysene-d12	21.402	240	7043	0.40	ng	#-0.01
34) Perylene-d12	23.920	264	6407	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.385	112	9478	3.28	ng	-0.02
5) Phenol-d6	6.985	99	14528	3.54	ng	-0.01
8) Nitrobenzene-d5	0.000	82	0d	0.00	ng	
11) 2-Methylnaphthalene-d10	12.195	152	26307	3.83	ng	-0.02
14) 2,4,6-Tribromophenol	0.000	330	0d	0.00	ng	
15) 2-Fluorobiphenyl	13.088	172	37624	3.42	ng	0.00
25) Fluoranthene-d10	19.253	212	293289	3.88	ng	0.00
29) Terphenyl-d14	19.850	244	58012	3.72	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.300	88	5158	2.42	ng	95
3) n-Nitrosodimethylamine	3.622	42	8606	5.50	ng	# 96
6) bis(2-Chloroethyl)ether	7.227	93	11041	3.55	ng	94
9) Naphthalene	10.641	128	157008	3.78	ng	99
10) Hexachlorobutadiene	10.927	225	9986	3.36	ng	98
12) 2-Methylnaphthalene	12.267	142	27737	4.03	ng	93
16) Acenaphthylene	14.183	152	47323	4.06	ng	99
17) Acenaphthene	14.528	154	26841	3.67	ng	99
18) Fluorene	15.515	166	37476	3.94	ng	99
20) 4-Bromophenyl-phenylether	16.412	248	12347	3.82	ng	# 82
21) Hexachlorobenzene	16.519	284	13687	3.51	ng	96
22) Pentachlorophenol	16.881	266	4095	3.58	ng	90
23) Phenanthrene	17.256	178	57166	3.95	ng	99
24) Anthracene	17.349	178	53068	4.28	ng	99
26) Fluoranthene	19.282	202	73665	3.96	ng	99
28) Pyrene	19.643	202	74582	3.85	ng	100
30) Benzo(a)anthracene	21.390	228	72765	3.84	ng	96
31) Chrysene	21.438	228	75834	3.86	ng	99
32) Bis(2-ethylhexyl)phtha...	21.305	149	145488	3.62	ng	100
33) Indeno(1,2,3-cd)pyrene	26.556	276	73935	3.65	ng	99
35) Benzo(b)fluoranthene	23.143	252	71552	4.09	ng	# 95
36) Benzo(k)fluoranthene	23.193	252	73344	3.84	ng	96
37) Benzo(a)pyrene	23.799	252	66823	3.89	ng	# 92
38) Dibenzo(a,h)anthracene	26.578	278	56093	3.69	ng	# 91
39) Benzo(g,h,i)perylene	27.366	276	64229	3.85	ng	97





(#) = qualifier out of range (m) = manual integration (+) = signals summed



#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.803 min Scan# 429
 Delta R.T. -0.012 min
 Lab File: BE098760.D
 Acq: 26 Feb 2019 14:34




Instrument :
 BNA_E
 ClientSampled :
 SSTDICC3.2


Tgt Ion: 152 Resp: 1082
 Ion Ratio Lower Upper
 152 100
 150 157.0 121.4 182.2
 115 68.3 59.1 88.7



#2
 1,4-Dioxane
 Concen: 2.42 ng
 RT: 3.300 min Scan# 38
 Delta R.T. -0.012 min
 Lab File: BE098760.D
 Acq: 26 Feb 2019 14:34

Tgt Ion: 88 Resp: 5158
 Ion Ratio Lower Upper
 88 100
 58 95.3 73.9 110.9
 43 49.4 43.7 65.5







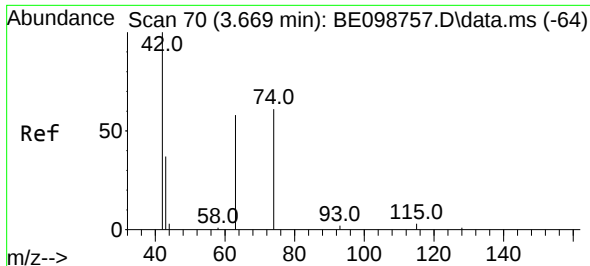

#3
n-Nitrosodimethylamine
Concen: 5.50 ng
RT: 3.622 min Scan# 66
Delta R.T. -0.047 min
Lab File: BE098760.D
Acq: 26 Feb 2019 14:34




Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2


Tgt Ion: 42 Resp: 8606
Ion Ratio Lower Upper
42 100
74 70.6 58.9 88.3
44 5.8 0.0 0.0#



#4
2-Fluorophenol
Concen: 3.28 ng
RT: 5.385 min Scan# 219
Delta R.T. -0.024 min
Lab File: BE098760.D
Acq: 26 Feb 2019 14:34

Tgt Ion: 112 Resp: 9478
Ion Ratio Lower Upper
112 100
64 81.0 62.9 94.3
63 195.2 152.2 228.4









#5
Phenol-d6
Concen: 3.54 ng
RT: 6.985 min Scan# 358
Delta R.T. -0.012 min
Lab File: BE098760.D
Acq: 26 Feb 2019 14:34




Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2


Tgt Ion: 99 Resp: 14528
Ion Ratio Lower Upper
99 100
42 33.6 24.6 37.0
71 47.7 35.1 52.7



#6
bis(2-Chloroethyl)ether
Concen: 3.55 ng
RT: 7.227 min Scan# 379
Delta R.T. -0.012 min
Lab File: BE098760.D
Acq: 26 Feb 2019 14:34

Tgt Ion: 93 Resp: 11041
Ion Ratio Lower Upper
93 100
63 347.6 267.3 400.9
95 32.1 26.2 39.4









#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.602 min Scan# 650
Delta R.T. 0.000 min
Lab File: BE098760.D
Acq: 26 Feb 2019 14:34

Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2


Tgt Ion:	136	Resp:	4169
Ion	Ratio	Lower	Upper
136	100		
137	12.9	9.7	14.5
54	33.5	35.5	53.3#
68	5.6	5.0	7.6




#8
Nitrobenzene-d5
Concen: 0.00 ng
Expected RT: 8.98 min

Lab File: BE098760.D
Acq: 26 Feb 2019 14:34

Tgt Ion:	82
Sig	Exp Ratio
82	100
128	120.6
54	280.9









#9
Naphthalene
Concen: 3.78 ng
RT: 10.641 min Scan# 653
Delta R.T. -0.013 min
Lab File: BE098760.D
Acq: 26 Feb 2019 14:34




Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2


Tgt Ion:128 Resp: 157008
Ion Ratio Lower Upper
128 100
129 2.7 2.6 3.8
127 3.4 3.0 4.6



#10
Hexachlorobutadiene
Concen: 3.36 ng
RT: 10.927 min Scan# 675
Delta R.T. 0.000 min
Lab File: BE098760.D
Acq: 26 Feb 2019 14:34

Tgt Ion:225 Resp: 9986
Ion Ratio Lower Upper
225 100
223 62.1 47.8 71.8
227 64.0 50.5 75.7









#11
2-Methylnaphthalene-d10
Concen: 3.83 ng
RT: 12.195 min Scan# 763
Delta R.T. -0.015 min
Lab File: BE098760.D
Acq: 26 Feb 2019 14:34




Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2


Tgt Ion:152 Resp: 26307
Ion Ratio Lower Upper
152 100
151 19.0 16.2 24.4



#12
2-Methylnaphthalene
Concen: 4.03 ng
RT: 12.267 min Scan# 768
Delta R.T. -0.015 min
Lab File: BE098760.D
Acq: 26 Feb 2019 14:34


Tgt Ion:142 Resp: 27737
Ion Ratio Lower Upper
142 100
141 93.2 70.0 105.0
115 49.0 35.2 52.8





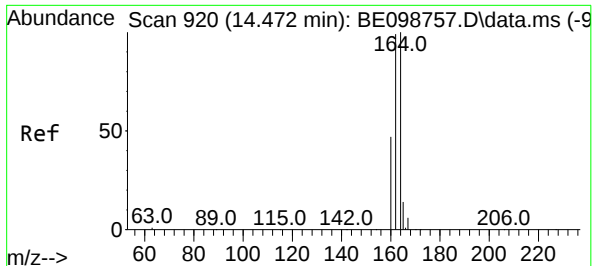


#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.471 min Scan# 921
Delta R.T. -0.001 min
Lab File: BE098760.D
Acq: 26 Feb 2019 14:34

Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2




Tgt Ion:164 Resp: 2690
Ion Ratio Lower Upper
164 100
162 95.2 80.5 120.7
160 44.9 40.1 60.1




#14
2,4,6-Tribromophenol
Concen: 0.00 ng
Expected RT: 15.98 min

Lab File: BE098760.D
Acq: 26 Feb 2019 14:34

Tgt Ion: 330
Sig Exp Ratio
330 100
332 91.6
141 41.4







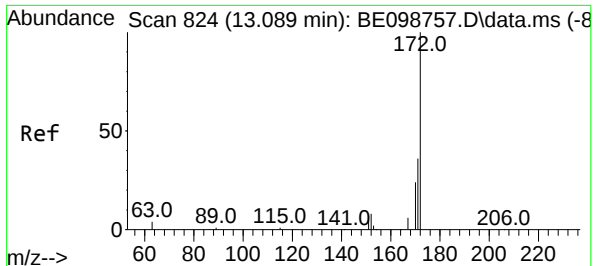

#15
2-Fluorobiphenyl
Concen: 3.42 ng
RT: 13.088 min Scan# 825
Delta R.T. -0.001 min
Lab File: BE098760.D
Acq: 26 Feb 2019 14:34




Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2


Tgt Ion:172	Resp:	37624
Ion Ratio	Lower	Upper
172	100	
171	32.8	29.0 43.4
170	21.9	20.8 31.2



#16
Acenaphthylene
Concen: 4.06 ng
RT: 14.183 min Scan# 901
Delta R.T. -0.015 min
Lab File: BE098760.D
Acq: 26 Feb 2019 14:34

Tgt Ion:152	Resp:	47323
Ion Ratio	Lower	Upper
152	100	
151	20.1	16.3 24.5
153	12.9	10.7 16.1



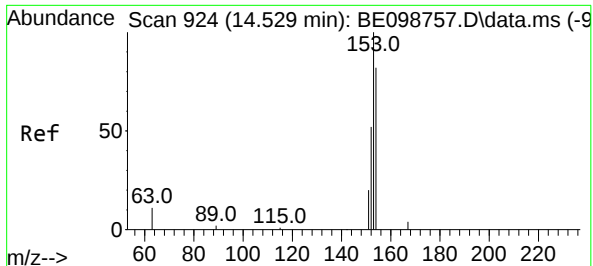

#17

Acenaphthene

Concen: 3.67 ng

RT: 14.528 min Scan# 925

Delta R.T. -0.001 min

Lab File: BE098760.D

Acq: 26 Feb 2019 14:34





Tgt Ion:154	Resp:	26841
Ion Ratio	Lower	Upper
154	100	
153	115.7	93.9 140.9
152	56.9	45.8 68.8

Instrument :

BNA_E

ClientSampleId :

SSTDICC3.2

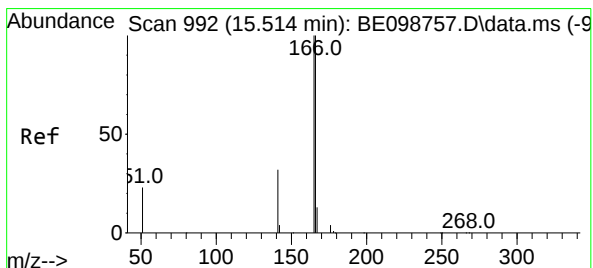

#18

Fluorene

Concen: 3.94 ng




RT: 15.515 min Scan# 993


Delta R.T. 0.001 min

Lab File: BE098760.D

Acq: 26 Feb 2019 14:34

Tgt Ion:166	Resp:	37476
Ion Ratio	Lower	Upper
166	100	
165	100.0	79.3 118.9
167	13.3	10.6 15.8









#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.215 min Scan# 1120
Delta R.T. -0.012 min
Lab File: BE098760.D
Acq: 26 Feb 2019 14:34




Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2


Tgt Ion:188 Resp: 6107
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 9.1 4.7 7.1#



#20
4-Bromophenyl-phenylether
Concen: 3.82 ng
RT: 16.412 min Scan# 1060
Delta R.T. 0.001 min
Lab File: BE098760.D
Acq: 26 Feb 2019 14:34

Tgt Ion:248 Resp: 12347
Ion Ratio Lower Upper
248 100
250 107.1 80.2 120.4
141 46.5 60.5 90.7#









#21
Hexachlorobenzene
Concen: 3.51 ng
RT: 16.519 min Scan# 1068
Delta R.T. -0.012 min
Lab File: BE098760.D
Acq: 26 Feb 2019 14:34




Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2


Tgt Ion:284 Resp: 13687
Ion Ratio Lower Upper
284 100
142 34.5 25.5 38.3
249 35.5 26.6 39.8



#22
Pentachlorophenol
Concen: 3.58 ng
RT: 16.881 min Scan# 1095
Delta R.T. -0.012 min
Lab File: BE098760.D
Acq: 26 Feb 2019 14:34

Tgt Ion:266 Resp: 4095
Ion Ratio Lower Upper
266 100
264 61.4 53.7 80.5
268 64.2 59.8 89.8







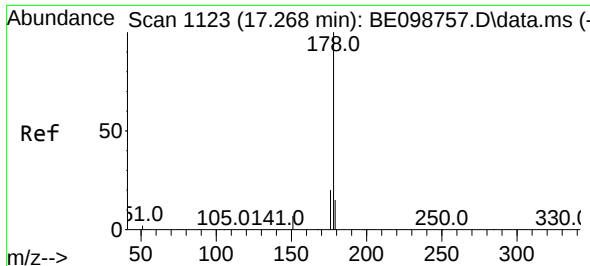

#23
Phenanthrene
Concen: 3.95 ng
RT: 17.256 min Scan# 1123
Delta R.T. -0.012 min
Lab File: BE098760.D
Acq: 26 Feb 2019 14:34




Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2


Tgt Ion:178 Resp: 57166
Ion Ratio Lower Upper
178 100
176 19.5 15.9 23.9
179 15.2 12.2 18.4

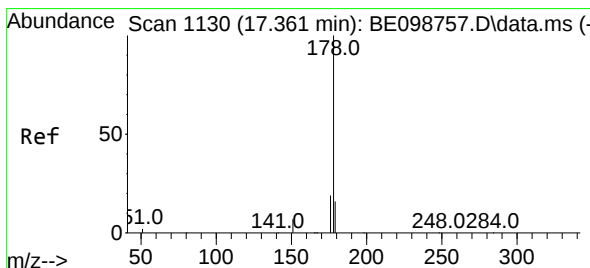

#24
Anthracene
Concen: 4.28 ng
RT: 17.349 min Scan# 1130
Delta R.T. -0.012 min
Lab File: BE098760.D
Acq: 26 Feb 2019 14:34

Tgt Ion:178 Resp: 53068
Ion Ratio Lower Upper
178 100
176 19.0 14.9 22.3
179 15.3 11.8 17.8









#25
Fluoranthene-d10
Concen: 3.88 ng
RT: 19.253 min Scan# 1391
Delta R.T. -0.001 min
Lab File: BE098760.D
Acq: 26 Feb 2019 14:34




Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2


Tgt Ion:212 Resp: 293289
Ion Ratio Lower Upper
212 100
106 2.1 1.7 2.5
104 1.2 1.0 1.6



#26
Fluoranthene
Concen: 3.96 ng
RT: 19.282 min Scan# 1396
Delta R.T. -0.006 min
Lab File: BE098760.D
Acq: 26 Feb 2019 14:34

Tgt Ion:202 Resp: 73665
Ion Ratio Lower Upper
202 100
101 8.0 6.7 10.1
203 17.2 13.3 19.9









#27
Chrysene-d12
Concen: 0.40 ng
RT: 21.402 min Scan# 1634
Delta R.T. -0.013 min
Lab File: BE098760.D
Acq: 26 Feb 2019 14:34




Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2


Tgt Ion:240 Resp: 7043
Ion Ratio Lower Upper
240 100
120 7.5 4.7 7.1#
236 27.7 21.9 32.9



#28
Pyrene
Concen: 3.85 ng
RT: 19.643 min Scan# 1459
Delta R.T. -0.006 min
Lab File: BE098760.D
Acq: 26 Feb 2019 14:34

Tgt Ion:202 Resp: 74582
Ion Ratio Lower Upper
202 100
200 21.6 17.0 25.6
203 17.4 13.8 20.8









#29
 Terphenyl-d14
 Concen: 3.72 ng
 RT: 19.850 min Scan# 1495
 Delta R.T. -0.006 min
 Lab File: BE098760.D
 Acq: 26 Feb 2019 14:34




Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC3.2


Tgt Ion:244	Resp:	58012
Ion Ratio	Lower	Upper
244	100	
212	34.1	29.4 44.2
122	7.5	7.1 10.7



#30
 Benzo(a)anthracene
 Concen: 3.84 ng
 RT: 21.390 min Scan# 1633
 Delta R.T. -0.001 min
 Lab File: BE098760.D
 Acq: 26 Feb 2019 14:34

Tgt Ion:228	Resp:	72765
Ion Ratio	Lower	Upper
228	100	
226	26.2	23.0 34.4
229	20.1	15.0 22.6



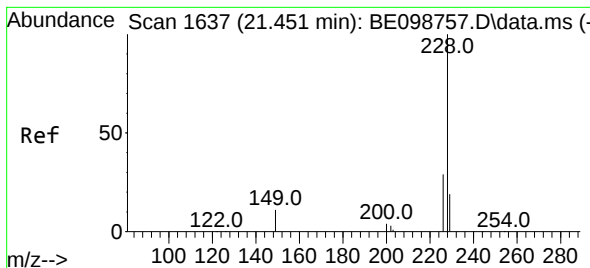

#31

Chrysene

Concen: 3.86 ng

RT: 21.438 min Scan# 1637

Delta R.T. -0.013 min

Lab File: BE098760.D

Acq: 26 Feb 2019 14:34

Tgt Ion:228 Resp: 75834

Ion Ratio Lower Upper

228 100

226 30.6 24.6 36.8





229 19.4 16.4 24.6

Instrument :

BNA_E

ClientSampleId :

SSTDICC3.2



#32

Bis(2-ethylhexyl)phthalate

Concen: 3.62 ng

RT: 21.305 min Scan# 1626

Delta R.T. -0.001 min

Lab File: BE098760.D

Acq: 26 Feb 2019 14:34




Tgt Ion:149 Resp: 145488


Ion Ratio Lower Upper

149 100

167 6.7 5.4 8.2

279 1.1 1.0 1.4









#33
Indeno(1,2,3-cd)pyrene
Concen: 3.65 ng
RT: 26.556 min Scan# 2950
Delta R.T. -0.014 min
Lab File: BE098760.D
Acq: 26 Feb 2019 14:34




Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2


Tgt Ion:276 Resp: 73935
Ion Ratio Lower Upper
276 100
138 16.3 13.3 19.9
277 25.1 19.4 29.0



#34
Perylene-d12
Concen: 0.40 ng
RT: 23.920 min Scan# 2215
Delta R.T. -0.001 min
Lab File: BE098760.D
Acq: 26 Feb 2019 14:34

Tgt Ion:264 Resp: 6407
Ion Ratio Lower Upper
264 100
260 26.6 20.5 30.7
265 30.2 22.3 33.5









#35
Benzo(b)fluoranthene
Concen: 4.09 ng
RT: 23.143 min Scan# 1997
Delta R.T. -0.004 min
Lab File: BE098760.D
Acq: 26 Feb 2019 14:34




Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2


Tgt Ion:252 Resp: 71552
Ion Ratio Lower Upper
252 100
253 22.3 19.4 29.0
125 7.0 8.2 12.4#



#36
Benzo(k)fluoranthene
Concen: 3.84 ng
RT: 23.193 min Scan# 2011
Delta R.T. -0.004 min
Lab File: BE098760.D
Acq: 26 Feb 2019 14:34

Tgt Ion:252 Resp: 73344
Ion Ratio Lower Upper
252 100
253 22.0 19.0 28.4
125 7.1 7.0 10.4









#37
Benzo(a)pyrene
Concen: 3.89 ng
RT: 23.799 min Scan# 2181
Delta R.T. -0.008 min
Lab File: BE098760.D
Acq: 26 Feb 2019 14:34




Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2


Tgt Ion:252 Resp: 66823
Ion Ratio Lower Upper
252 100
253 22.3 21.0 31.4
125 7.6 9.2 13.8#



#38
Dibenzo(a,h)anthracene
Concen: 3.69 ng
RT: 26.578 min Scan# 2956
Delta R.T. -0.018 min
Lab File: BE098760.D
Acq: 26 Feb 2019 14:34

Tgt Ion:278 Resp: 56093
Ion Ratio Lower Upper
278 100
139 10.8 12.7 19.1#
279 23.7 22.0 33.0





#39

Benzo(g,h,i)perylene


Concen: 3.85 ng

RT: 27.366 min Scan# 3177

Delta R.T. -0.007 min

Lab File: BE098760.D

Acq: 26 Feb 2019 14:34





Tgt Ion: 276 Resp: 64229

Ion Ratio Lower Upper

276 100

277 24.1 20.3 30.5

138 14.7 13.3 19.9



Instrument :

BNA_E

ClientSampleId :

SSTDICC3.2