
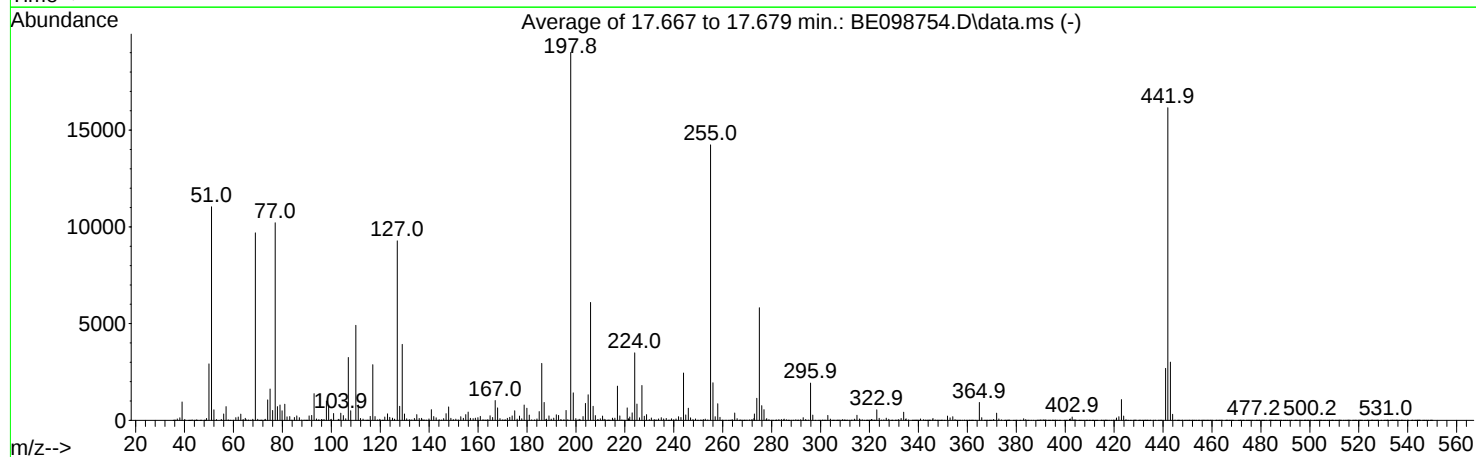


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE022619\
 Data File : BE098754.D
 Acq On : 26 Feb 2019 10:50
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE022619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 26 15:44:42 2019

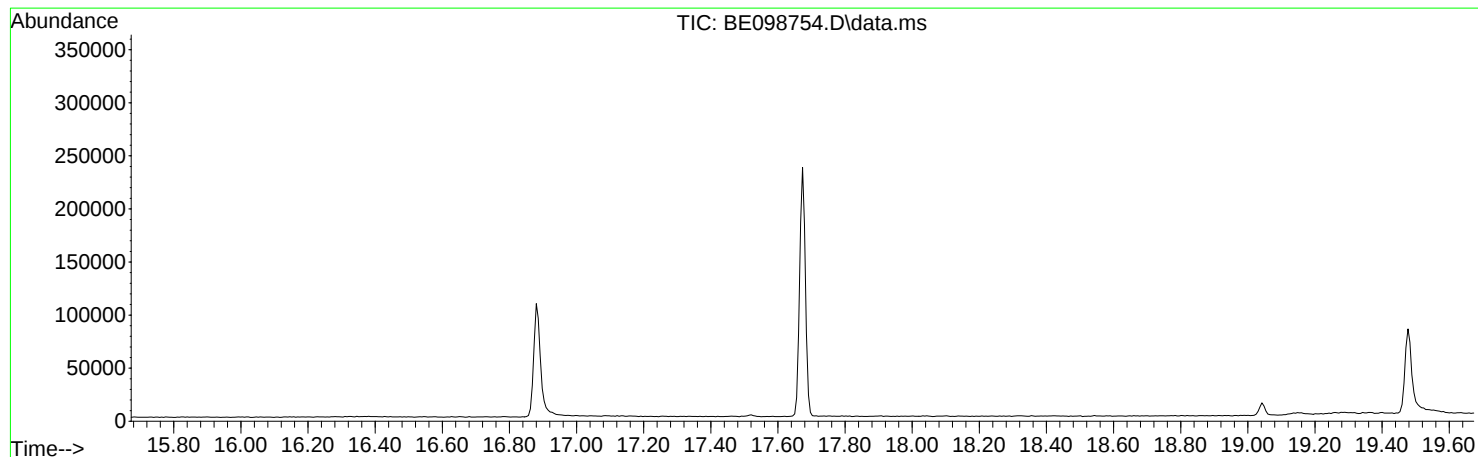

AutoFind: Scans 2566, 2567, 2568; Background Corrected with Scan 2559

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.1	11042	PASS
68	69	0.00	2	0.6	55	PASS
69	198	0.00	100	51.0	9690	PASS
70	69	0.00	2	0.6	61	PASS
127	198	10	80	48.8	9281	PASS
197	198	0.00	2	0.2	31	PASS
198	198	100	100	100.0	19012	PASS
199	198	5	9	7.5	1419	PASS
275	198	10	60	30.6	5825	PASS
365	198	1	100	4.9	925	PASS
441	198	0.01	100	14.1	2687	PASS
442	198	50	100	85.0	16159	PASS
443	442	15	24	18.6	3011	PASS