
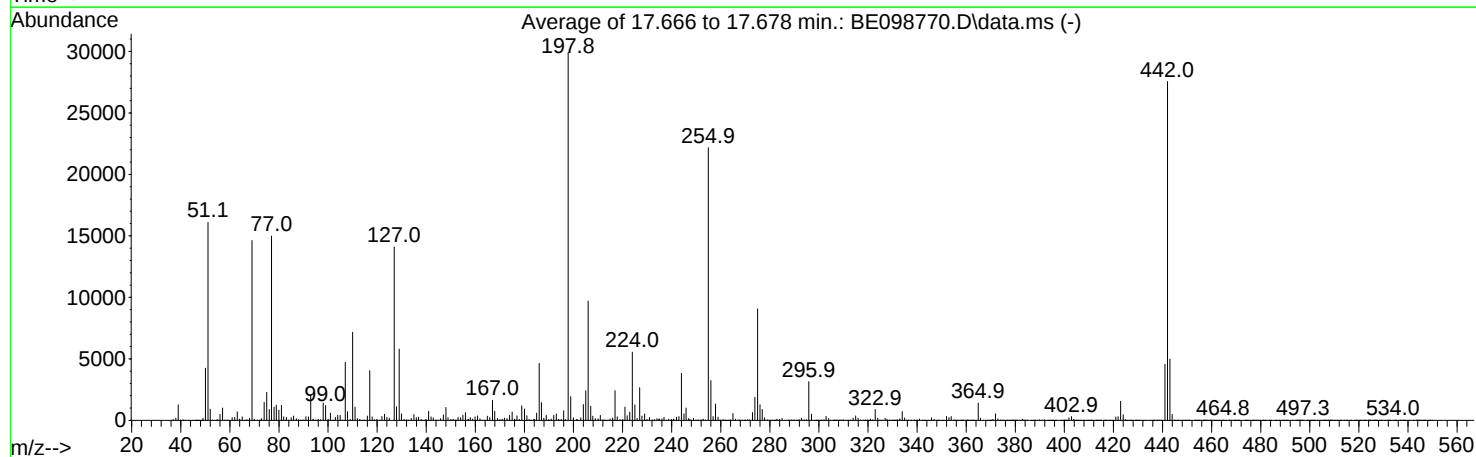


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE022719\
 Data File : BE098770.D
 Acq On : 27 Feb 2019 9:19
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE022619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 26 15:44:42 2019

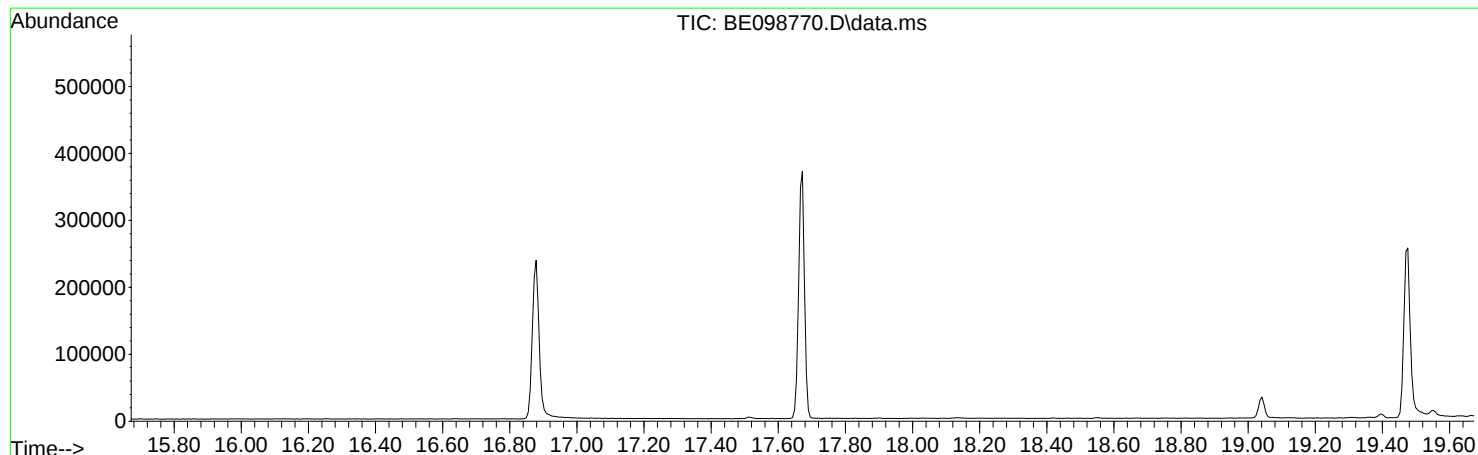

AutoFind: Scans 2566, 2567, 2568; Background Corrected with Scan 2559

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.8	16100	PASS
68	69	0.00	2	1.1	161	PASS
69	198	0.00	100	48.9	14631	PASS
70	69	0.00	2	0.6	90	PASS
127	198	10	80	47.2	14108	PASS
197	198	0.00	2	0.2	64	PASS
198	198	100	100	100.0	29913	PASS
199	198	5	9	6.4	1923	PASS
275	198	10	60	30.3	9070	PASS
365	198	1	100	4.7	1408	PASS
441	198	0.01	100	15.2	4553	PASS
442	198	50	100	92.1	27553	PASS
443	442	15	24	18.1	4982	PASS