



1,4-Dioxane

Response Ratio

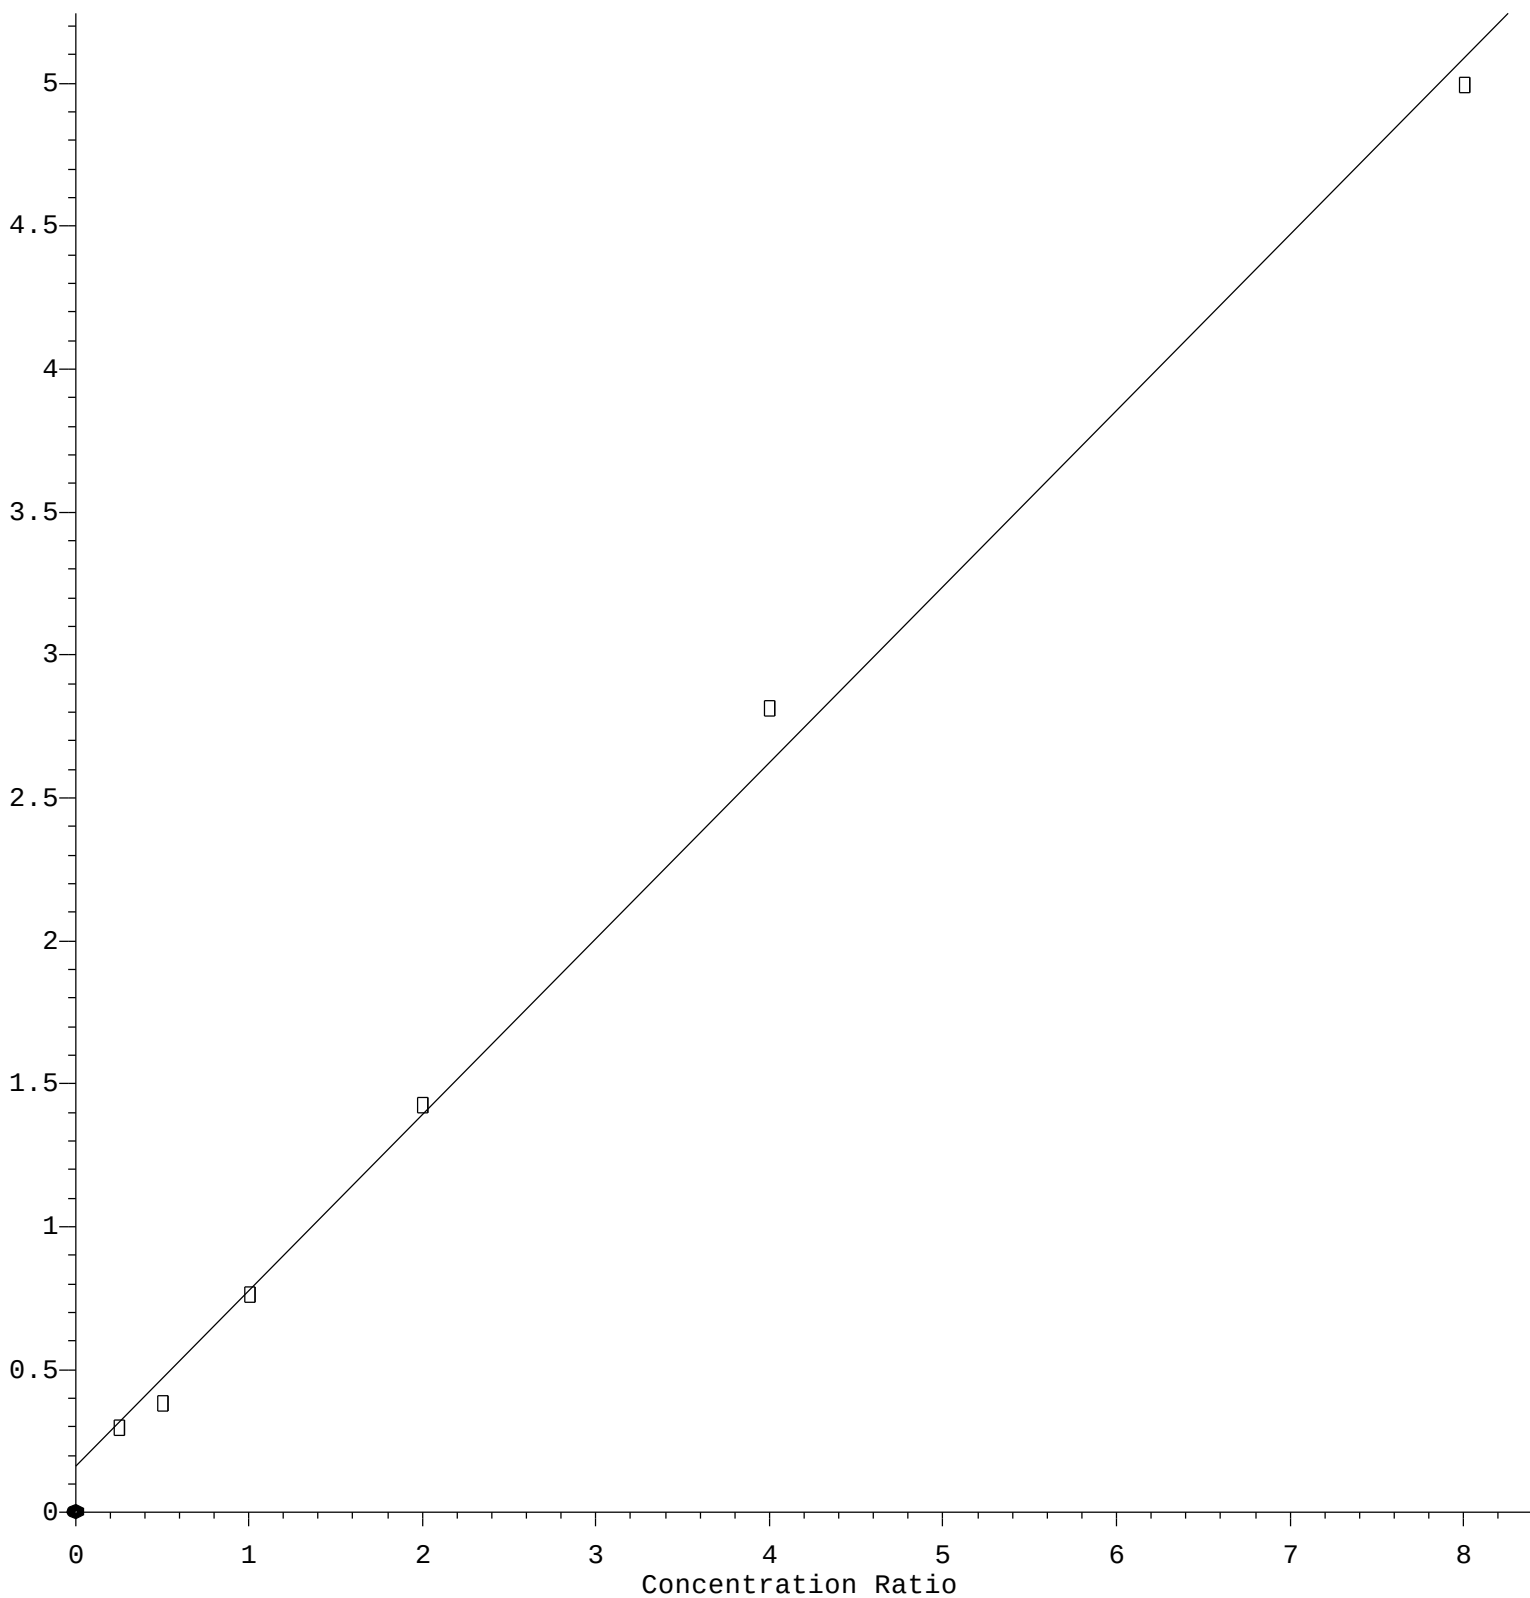

Response = 6.158e-001 * Amt + 1.606e-001
 Coef of Det (r^2) = 0.996795 Curve Fit: Linear
 Method Name: Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE030619.M
 Calibration Table Last Updated: Wed Mar 25 10:49:04 2015

Pentachlorophenol

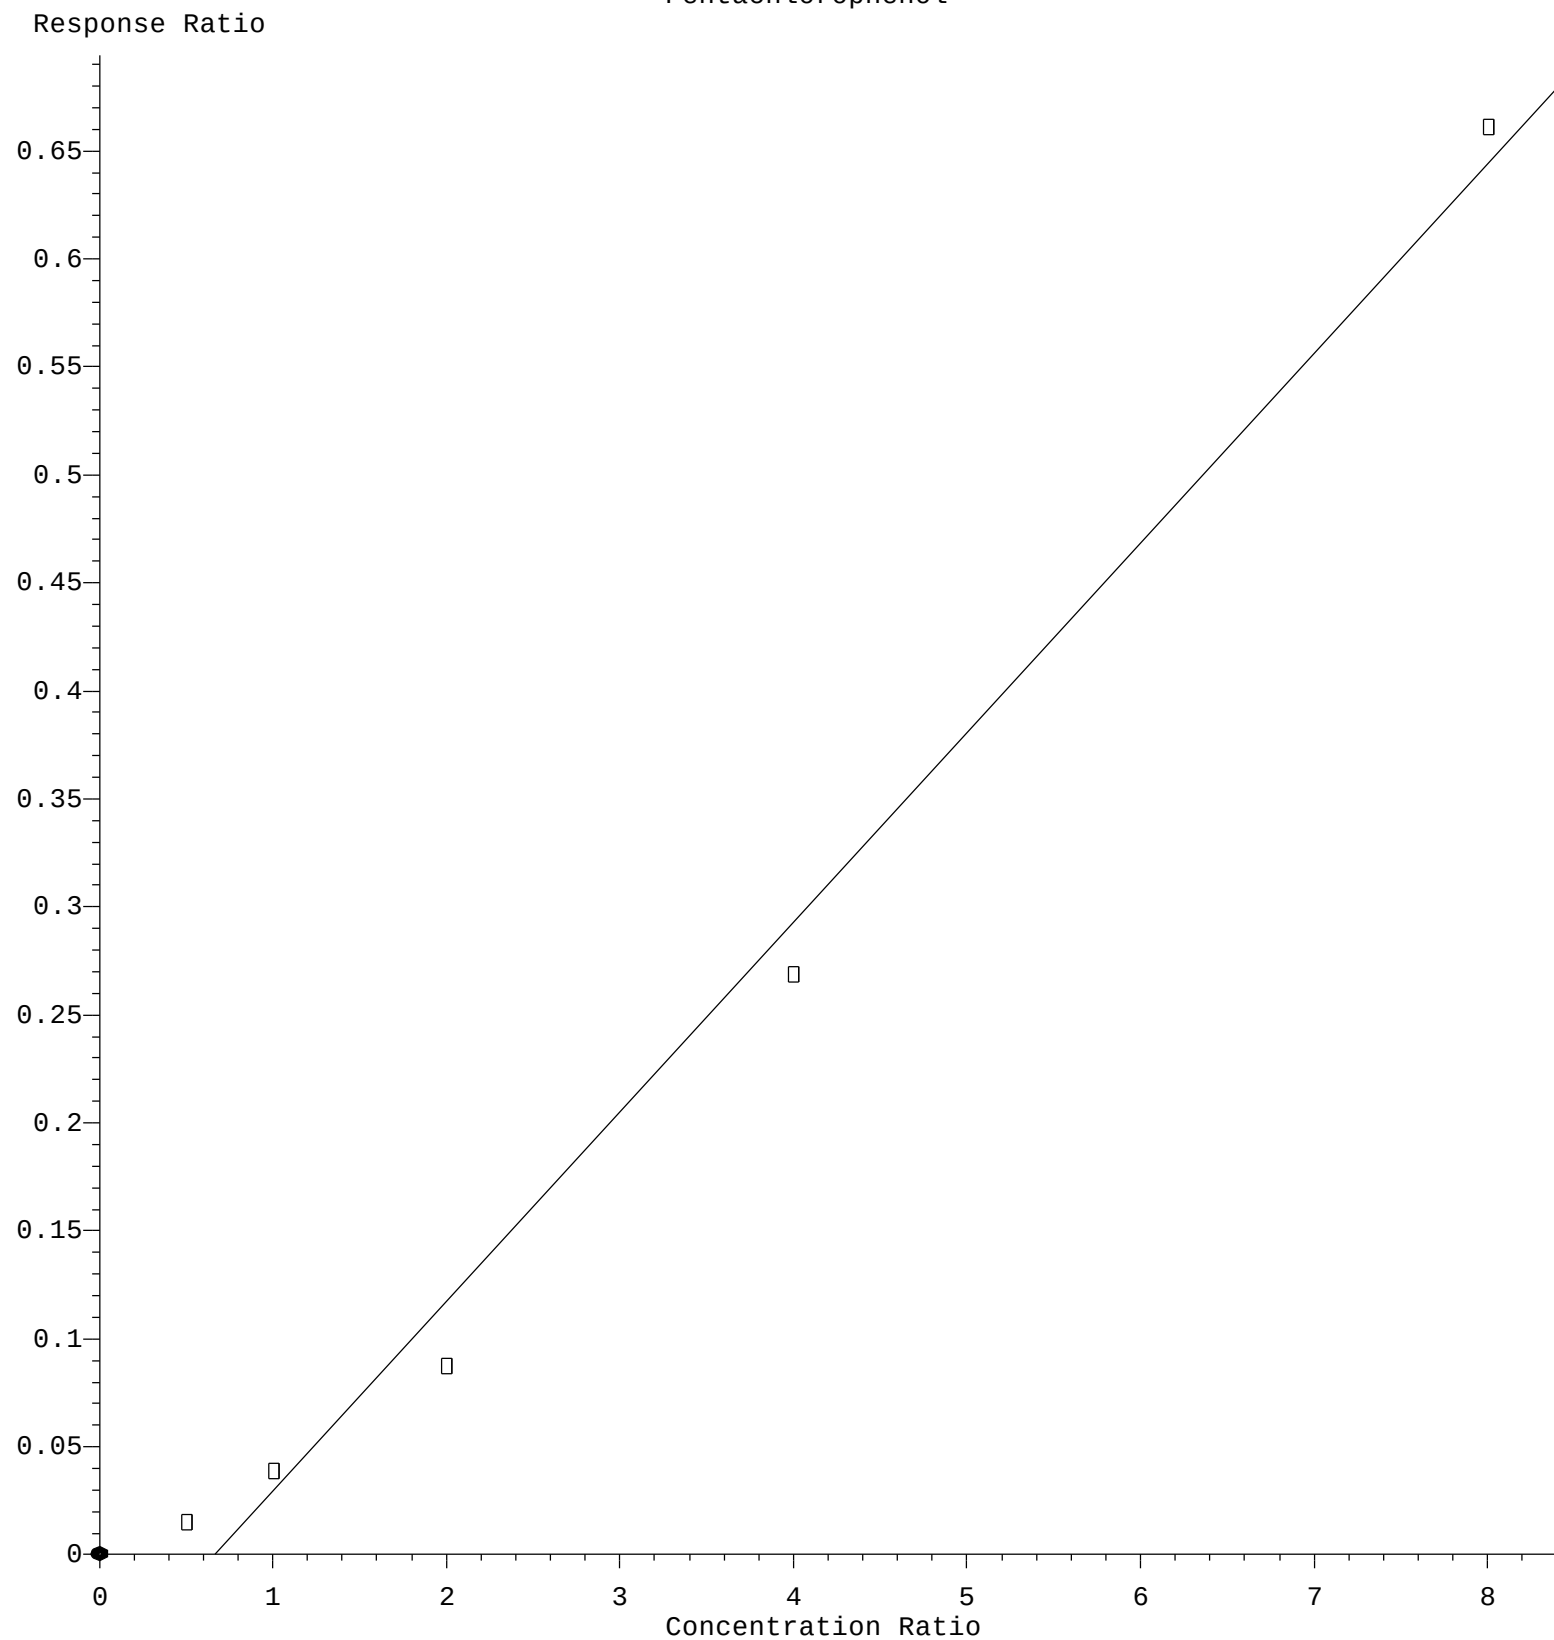

Response = 8.777e-002 * Amt - 5.804e-002
Coef of Det (r^2) = 0.990540 Curve Fit: Linear
Method Name: Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE030619.M
Calibration Table Last Updated: Wed Mar 25 10:49:04 2015