


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE030619\
 Data File : BE098791.D
 Acq On : 6 Mar 2019 10:14
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE030619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 06 15:33:24 2019

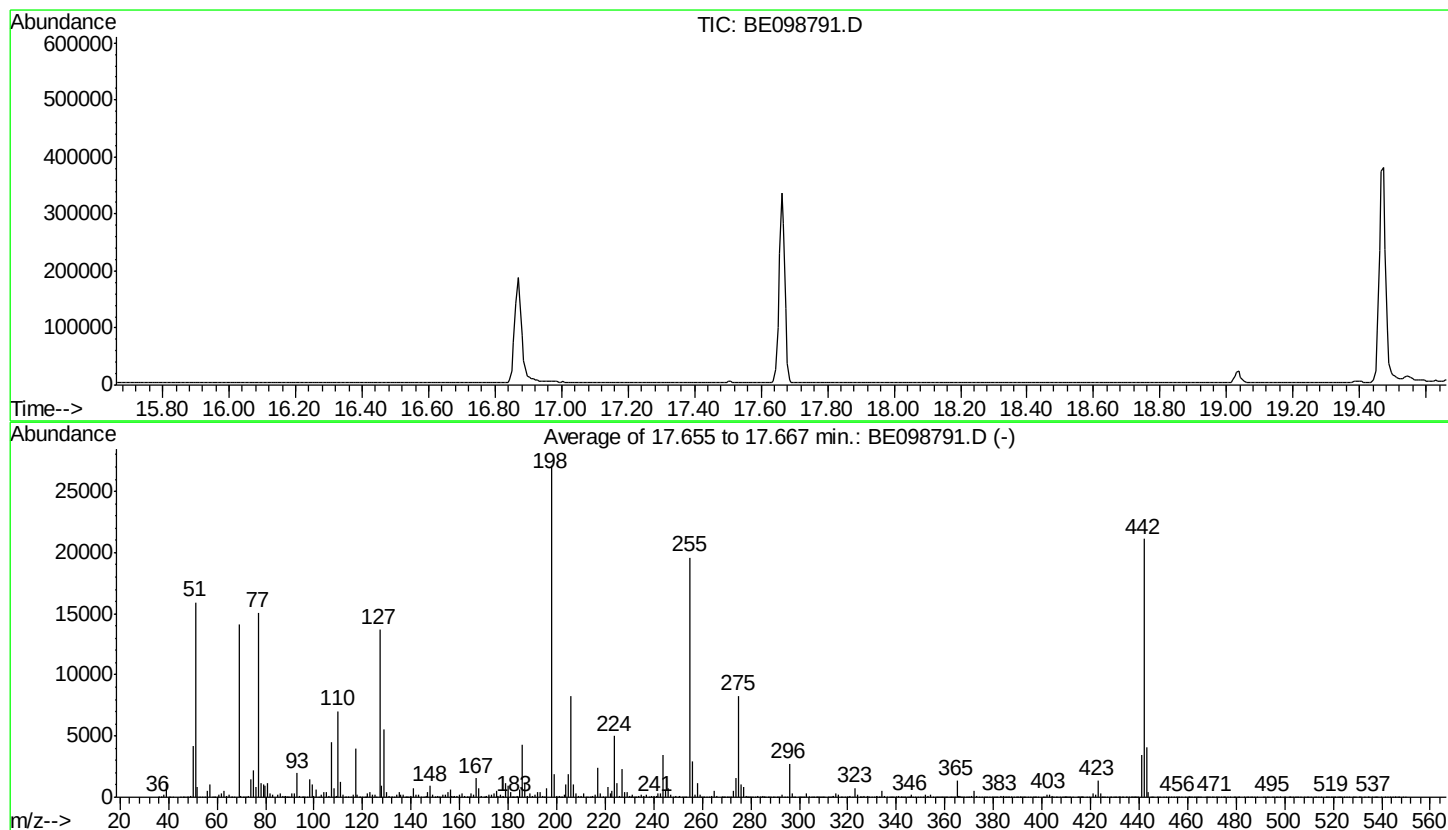

AutoFind: Scans 2564, 2565, 2566; Background Corrected with Scan 2557

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.7	15909	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	51.9	14082	PASS
70	69	0.00	2	0.6	80	PASS
127	198	10	80	50.4	13661	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	27109	PASS
199	198	5	9	7.1	1919	PASS
275	198	10	60	30.7	8318	PASS
365	198	1	100	4.9	1330	PASS
441	198	0.01	100	12.8	3473	PASS
442	198	50	100	77.9	21127	PASS
443	442	15	24	19.4	4095	PASS