

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE030819\
 Data File : BE098849.D
 Acq On : 9 Mar 2019 1:31
 Operator : JU/SJ
 Sample : K1793-12
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 RE126D1-20190306

Quant Time: Mar 09 03:52:17 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE030619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 06 15:33:24 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	768	0.40	ng	0.00
7) Naphthalene-d8	10.60	136	3094	0.40	ng	0.01
13) Acenaphthene-d10	14.46	164	2182	0.40	ng	0.00
19) Phenanthrene-d10	17.21	188	5690	0.40	ng	0.00
27) Chrysene-d12	21.40	240	6837	0.40	ng	0.00
34) Perylene-d12	23.90	264	6639	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.40	112	278	0.12	ng	0.01
5) Phenol-d6	7.01	99	252	0.08	ng	0.03
8) Nitrobenzene-d5	8.99	82	1115	0.34	ng	0.03
11) 2-Methylnaphthalene-d10	12.21	152	1993	0.35	ng	0.01
14) 2,4,6-Tribromophenol	15.97	330	369	0.34	ng	0.00
15) 2-Fluorobiphenyl	13.09	172	3690	0.41	ng	0.00
25) Fluoranthene-d10	19.24	212	31266	0.34	ng	0.00
29) Terphenyl-d14	19.84	244	7705	0.46	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.28	88	4883	4.026	ng	97
22) Pentachlorophenol	16.89	266	11	0.273	ng	93
32) Bis(2-ethylhexyl)phthalate	21.29	149	2975	0.066	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE030819\
Data File : BE098849.D
Acq On : 9 Mar 2019 1:31
Operator : JU/SJ
Sample : K1793-12
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
RE126D1-20190306

Quant Time: Mar 09 03:52:17 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE030619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 06 15:33:24 2019
Response via : Initial Calibration

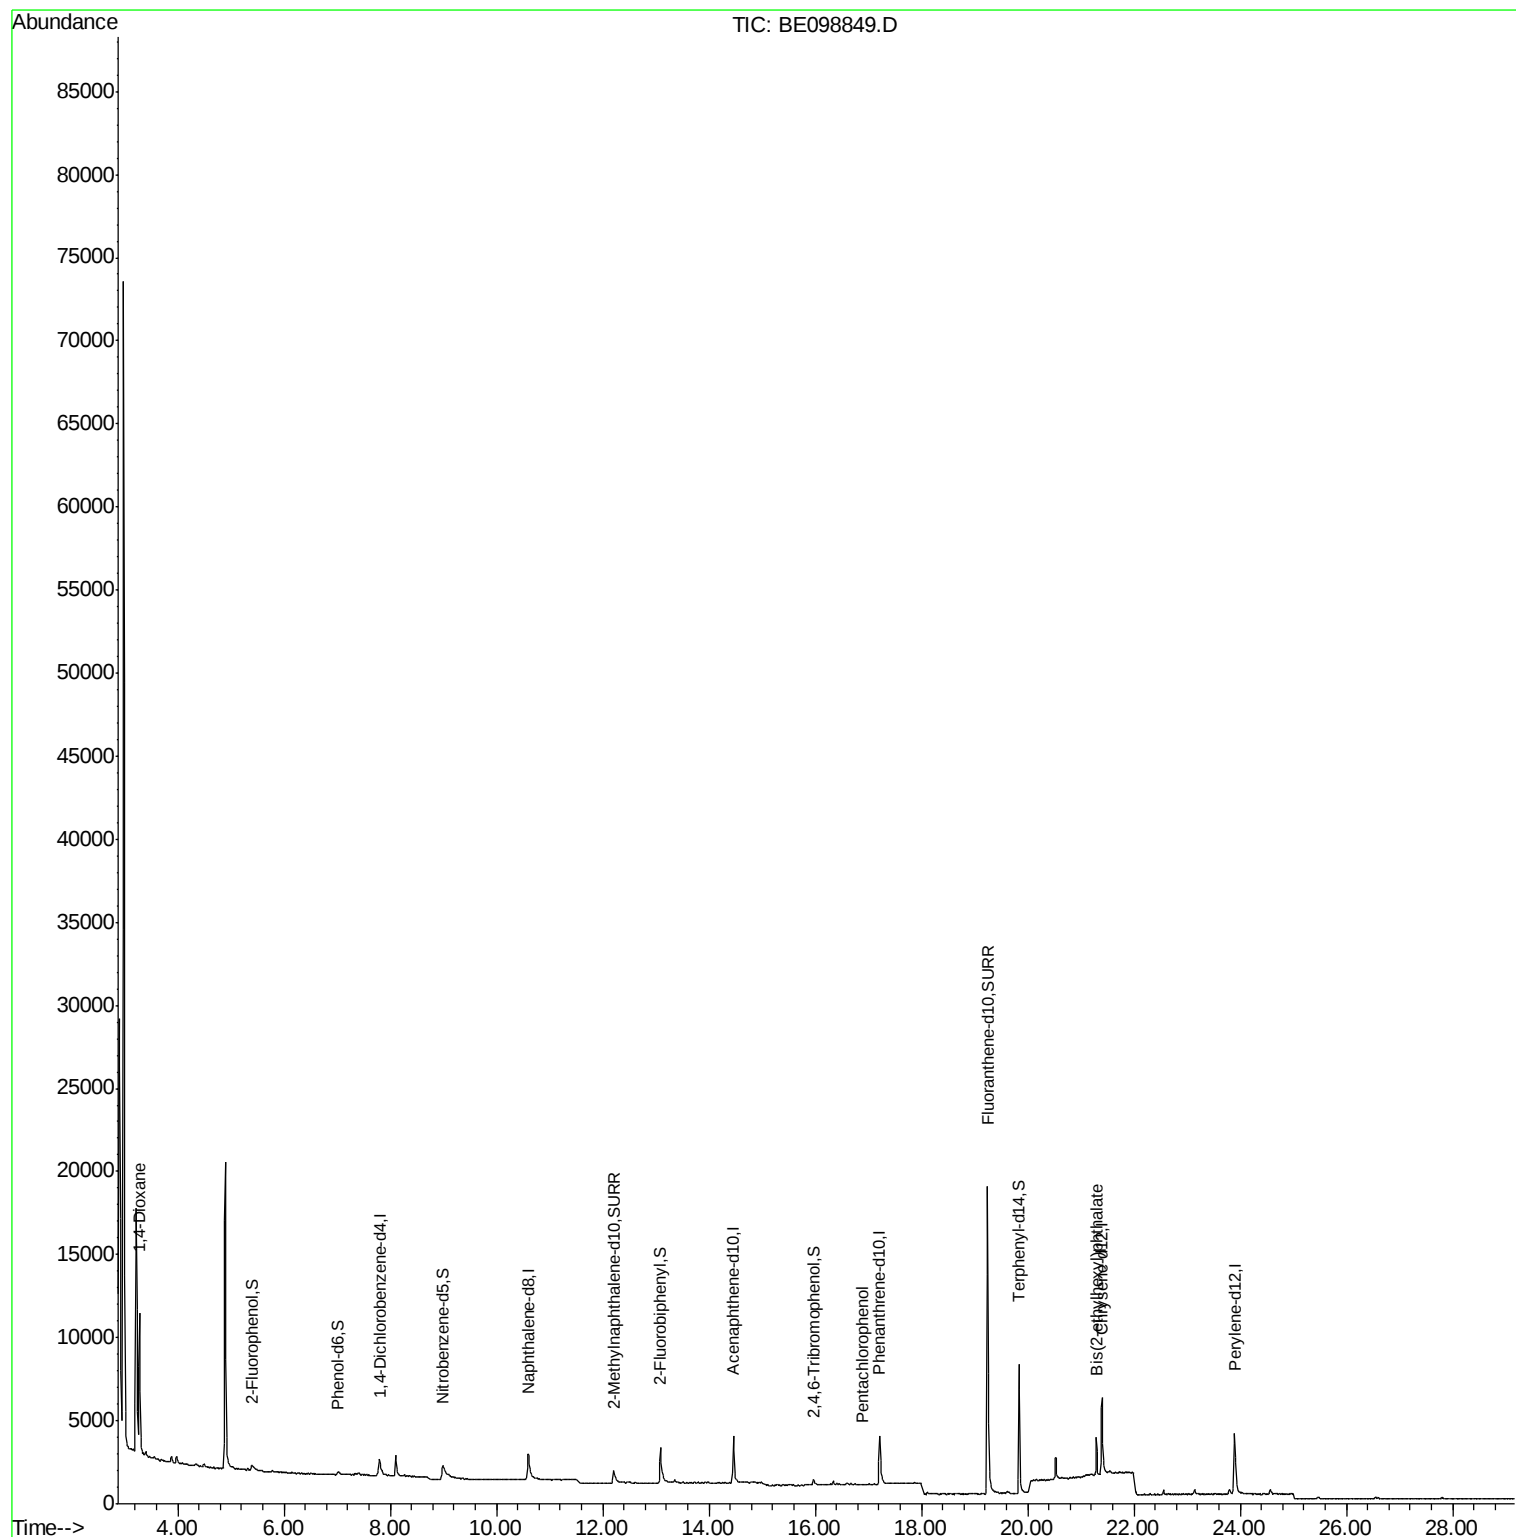

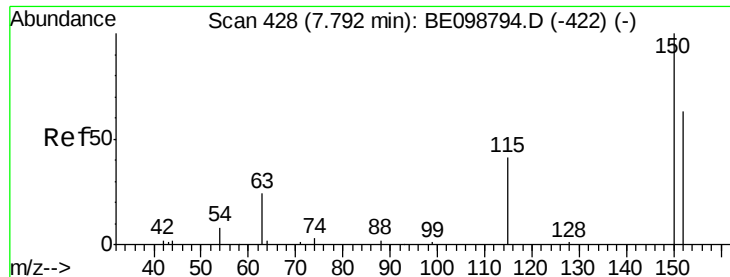


#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.79 min Scan# 428
Delta R.T. 0.00 min
Lab File: BE098849.D
Acq: 9 Mar 2019 1:31

Instrument :
BNA_E
ClientSampleId :
RE126D1-20190306

Tot Ion:152 Resp: 768
Ion Ratio Lower Upper
152 100
150 143.9 122.5 183.7
115 69.3 57.4 86.2

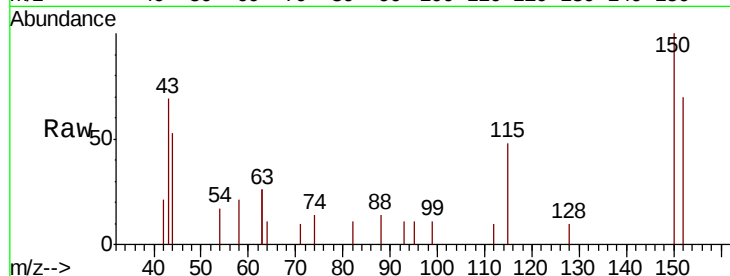


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

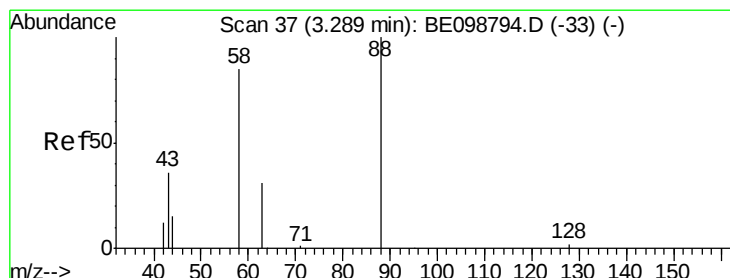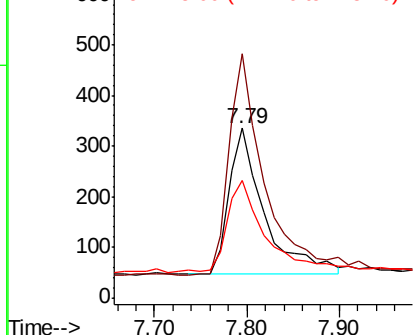



#2


1,4-Dioxane
Concen: 4.026 ng
RT: 3.28 min Scan# 36
Delta R.T. -0.01 min
Lab File: BE098849.D
Acq: 9 Mar 2019 1:31

Tgt Ion: 88 Resp: 4883
Ion Ratio Lower Upper
88 100
58 91.5 75.8 113.6
43 54.4 41.8 62.8

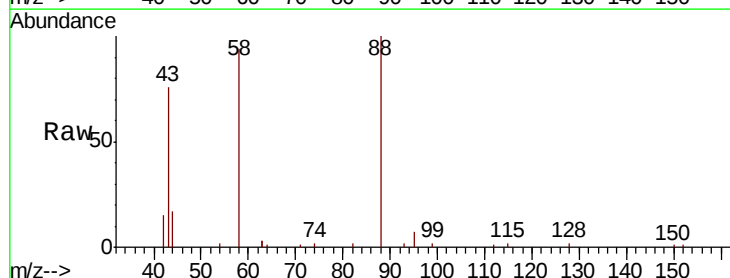

Abundance Ion 88.00 (87.70 to 88.70): BE0
Ion 58.00 (57.70 to 58.70): BE0
Ion 43.00 (42.70 to 43.70): BE0

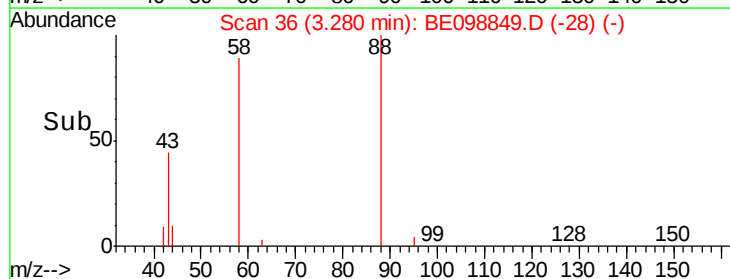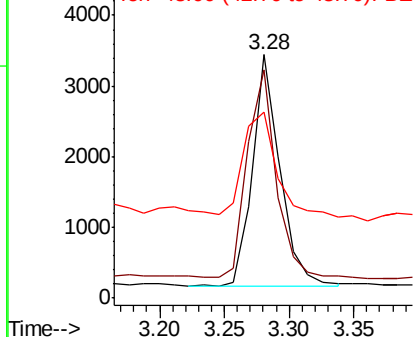

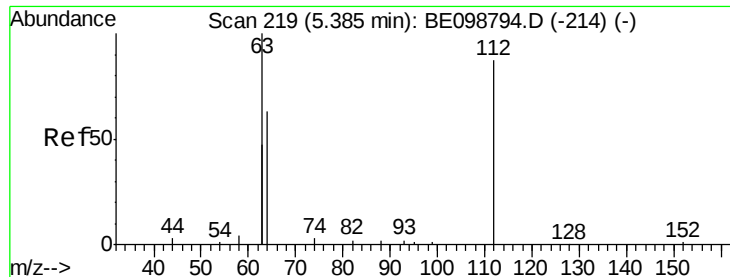

#4

2-Fluorophenol

Concen: 0.121 ng

RT: 5.40 min Scan# 220

Delta R.T. 0.01 min

Lab File: BE098849.D

Acq: 9 Mar 2019 1:31

Instrument :

BNA_E

ClientSampleId :

RE126D1-20190306


Tot Ion:112 Resp: 278

Ion Ratio Lower Upper

112 100

64 95.7 57.9 86.9#

63 207.9 158.3 237.5

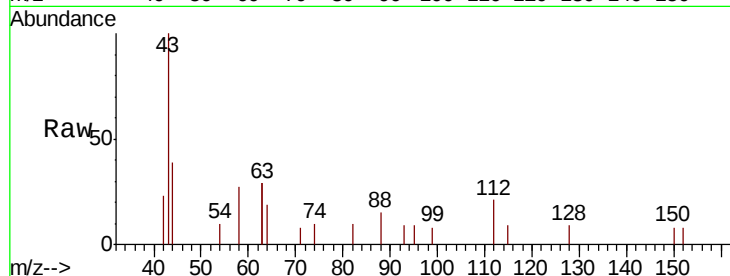

Abundance Ion 112.00 (111.70 to 112.70): BE0

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

400

300



200

100

0

5.30 5.35 5.40 5.45 5.50

Time-->

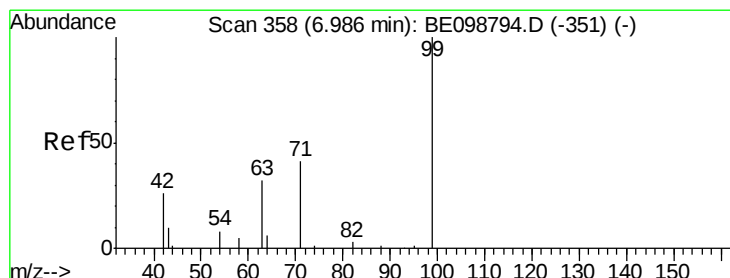

#5

Phenol-d6

Concen: 0.078 ng

RT: 7.01 min Scan# 360

Delta R.T. 0.03 min

Lab File: BE098849.D

Acq: 9 Mar 2019 1:31


Tgt Ion: 99 Resp: 252

Ion Ratio Lower Upper

99 100

42 0.0 24.2 36.2#

71 41.3 35.7 53.5

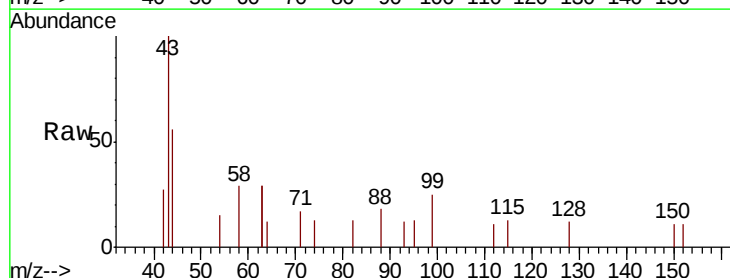

Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

150


100


50

0

6.90 7.00 7.10 7.20

Time-->



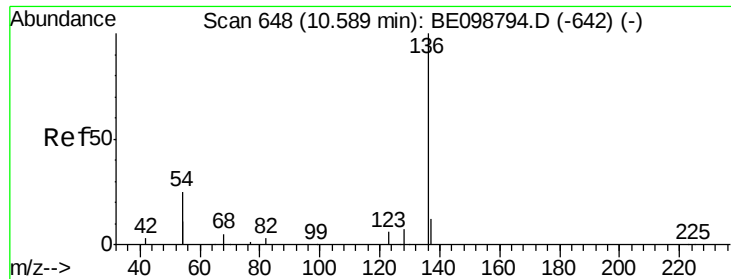

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.60 min Scan# 649

Delta R.T. 0.01 min

Lab File: BE098849.D

Acq: 9 Mar 2019 1:31

Instrument :

BNA_E

ClientSampleId :

RE126D1-20190306

Tot Ion:136 Resp: 3094


Ion Ratio Lower Upper

136 100

137 14.7 11.4 17.0

54 63.2 39.3 58.9#

68 11.5 6.7 10.1#



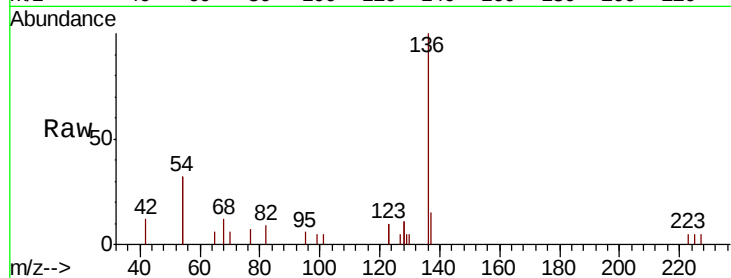


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

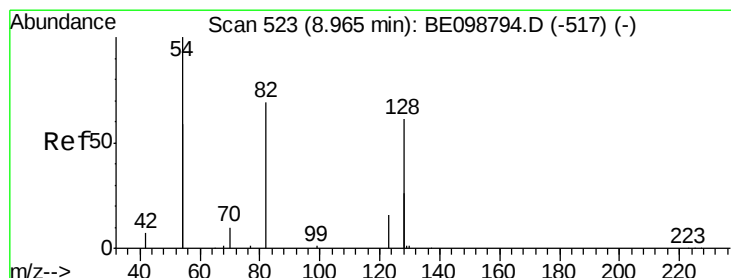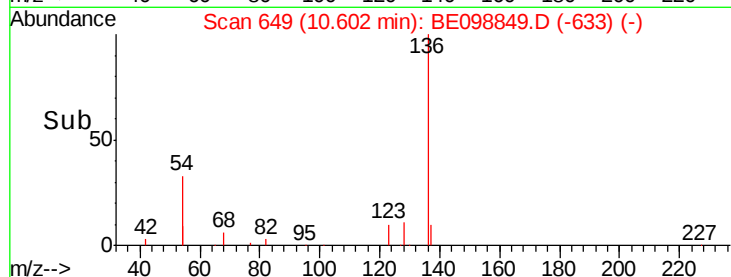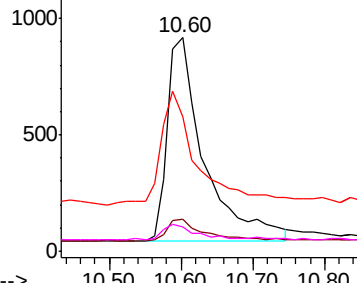

#8

Nitrobenzene-d5

Concen: 0.344 ng

RT: 8.99 min Scan# 525

Delta R.T. 0.03 min

Lab File: BE098849.D

Acq: 9 Mar 2019 1:31


Tgt Ion: 82 Resp: 1115

Ion Ratio Lower Upper

82 100

128 177.5 123.8 185.8



54 319.2 203.4 305.2#

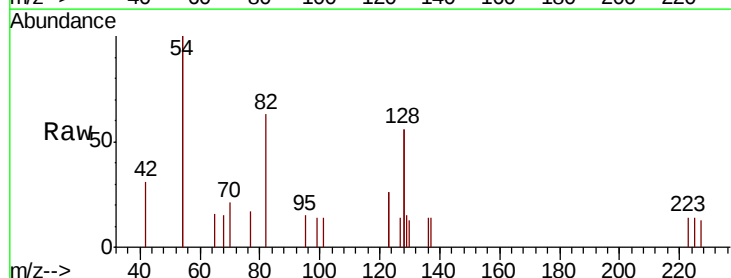


Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0



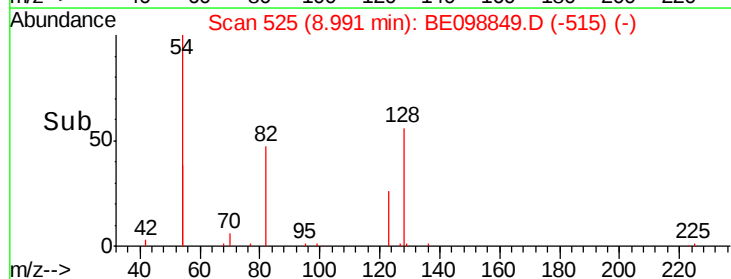
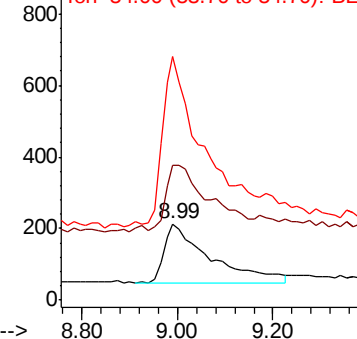


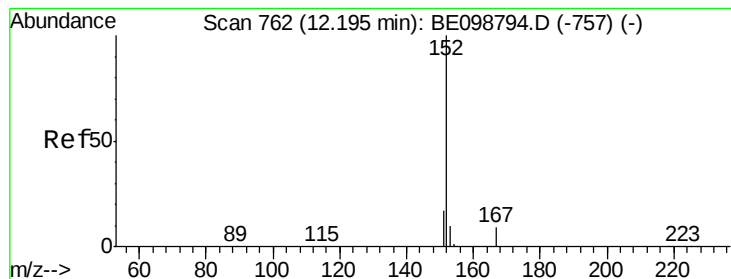

#11
 2-Methylnaphthalene-d10
 Concen: 0.349 ng
 RT: 12.21 min Scan# 763
 Delta R.T. 0.01 min
 Lab File: BE098849.D
 Acq: 9 Mar 2019 1:31




Instrument :
 BNA_E
 ClientSampleId :
 RE126D1-20190306


Tot Ion:152 Resp: 1993
 Ion Ratio Lower Upper
 152 100
 151 18.1 16.5 24.7

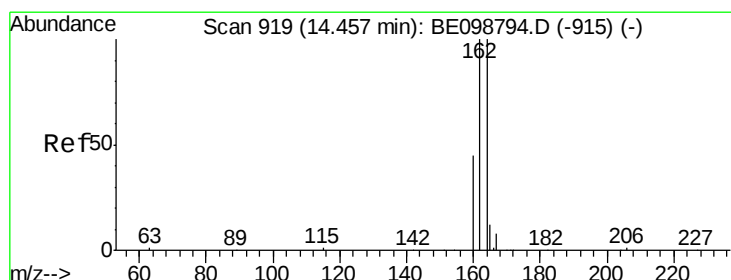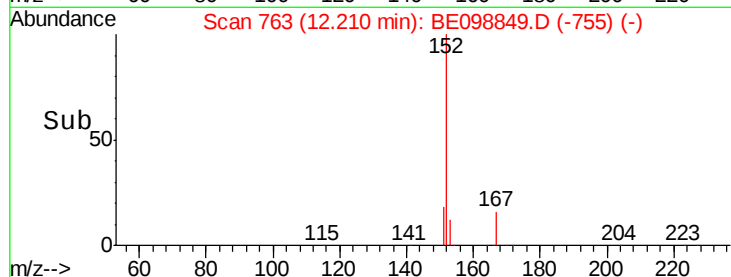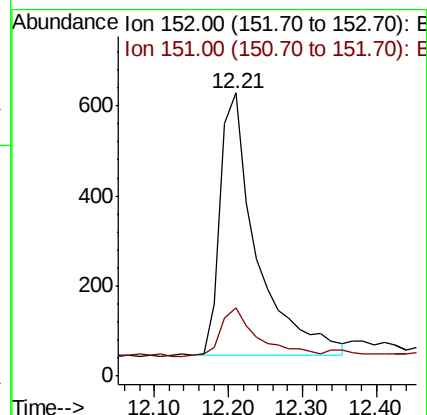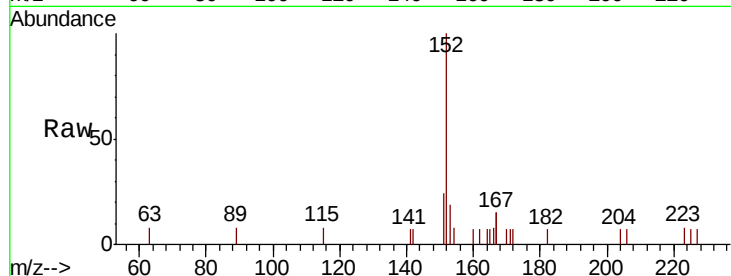

#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.46 min Scan# 919
 Delta R.T. 0.00 min
 Lab File: BE098849.D
 Acq: 9 Mar 2019 1:31

Tgt Ion:164 Resp: 2182
 Ion Ratio Lower Upper
 164 100
 162 100.8 80.2 120.2
 160 47.4 37.8 56.8


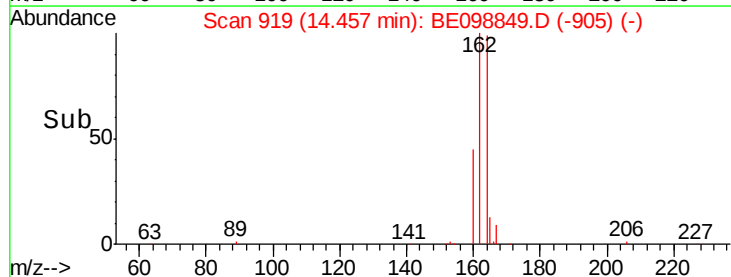
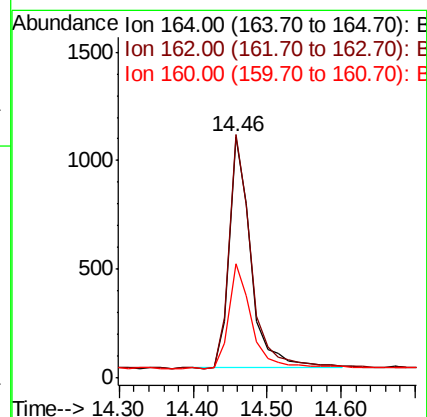
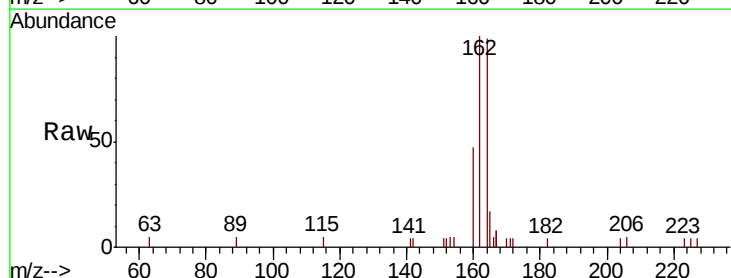




#14
 2,4,6-Tribromophenol
 Concen: 0.335 ng
 RT: 15.97 min Scan# 1026
 Delta R.T. -0.00 min
 Lab File: BE098849.D
 Acq: 9 Mar 2019 1:31




Instrument :
 BNA_E
 ClientSampleId :
 RE126D1-20190306


Tot Ion:330 Resp: 369
 Ion Ratio Lower Upper
 330 100
 332 93.5 77.6 116.4
 141 39.3 31.0 46.4

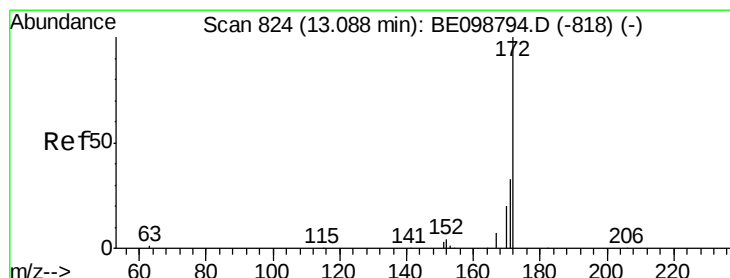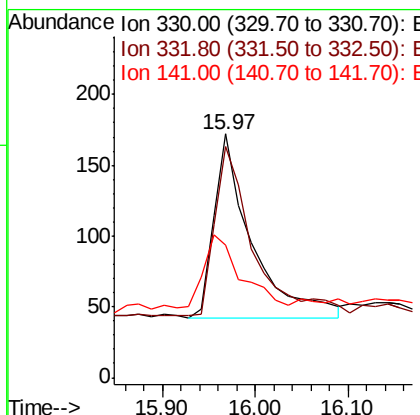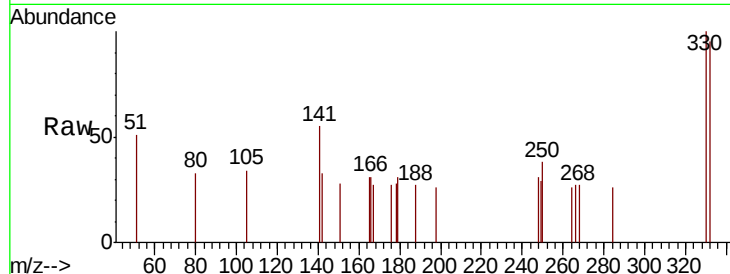

#15
 2-Fluorobiphenyl
 Concen: 0.408 ng
 RT: 13.09 min Scan# 824
 Delta R.T. 0.00 min
 Lab File: BE098849.D
 Acq: 9 Mar 2019 1:31

Tgt Ion:172 Resp: 3690
 Ion Ratio Lower Upper
 172 100
 171 35.8 28.0 42.0
 170 25.2 17.7 26.5

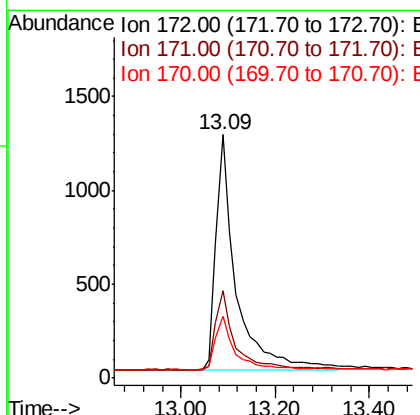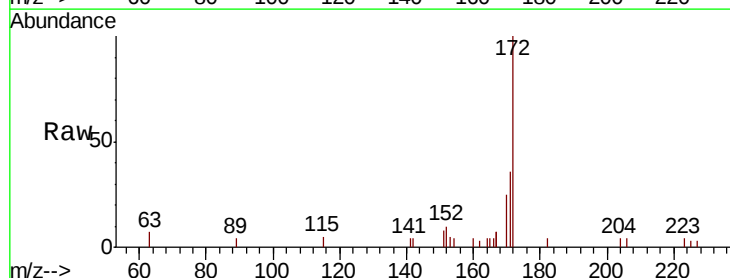

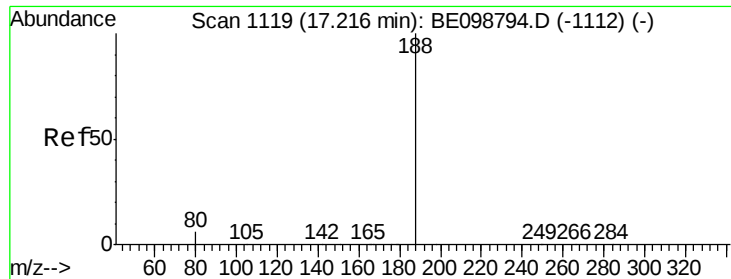

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.21 min Scan# 1119

Delta R.T. -0.00 min

Lab File: BE098849.D

Acq: 9 Mar 2019 1:31

Instrument :

BNA_E

ClientSampleId :

RE126D1-20190306





Tot Ion:188 Resp: 5690

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 8.8 6.3 9.5

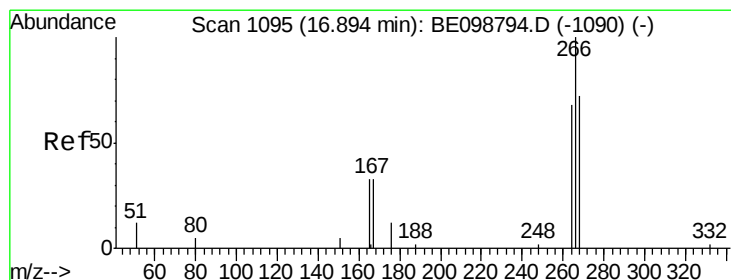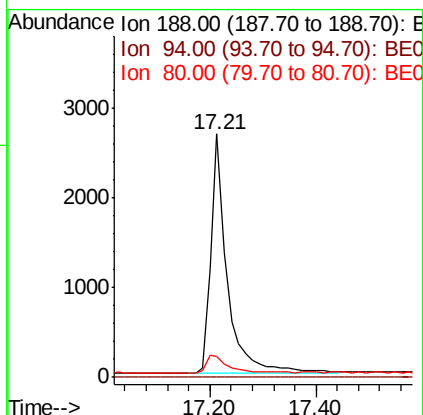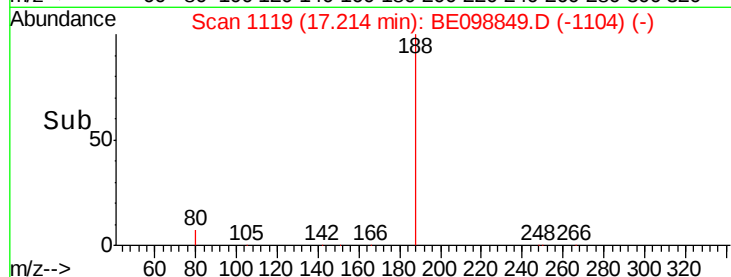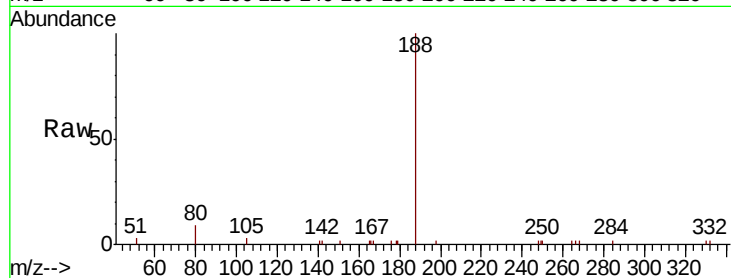

#22

Pentachlorophenol

Concen: 0.273 ng

RT: 16.89 min Scan# 1095

Delta R.T. -0.00 min

Lab File: BE098849.D

Acq: 9 Mar 2019 1:31




Tgt Ion:266 Resp: 11


Ion Ratio Lower Upper

266 100

264 88.0 66.6 100.0

268 96.0 69.8 104.8

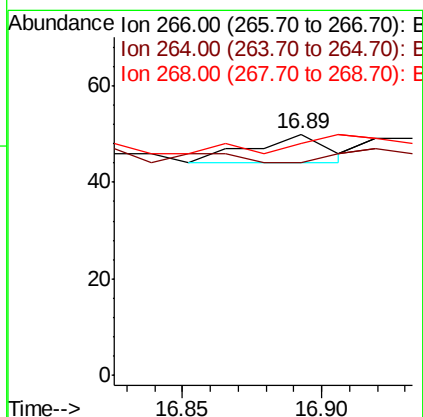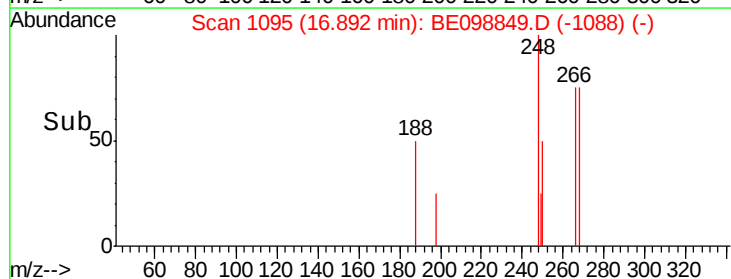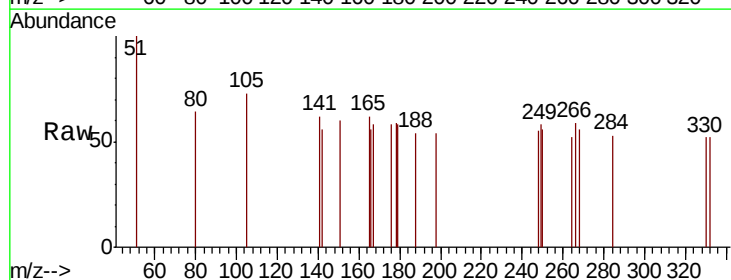

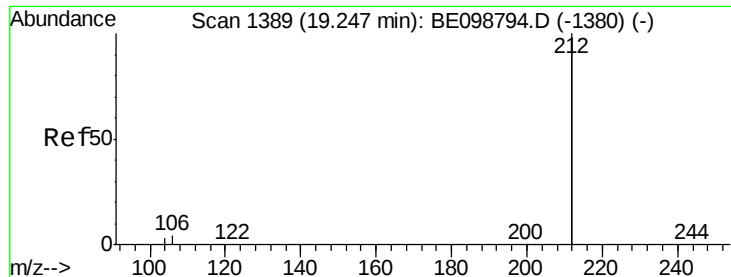

#25

Fluoranthene-d10

Concen: 0.344 ng

RT: 19.24 min Scan# 1388

Delta R.T. -0.00 min

Lab File: BE098849.D

Acq: 9 Mar 2019 1:31

Instrument :

BNA_E

ClientSampleId :

RE126D1-20190306


Tot Ion:212 Resp: 31266

Ion Ratio Lower Upper

212 100

106 2.4 1.8 2.8




104 1.4 1.0 1.6

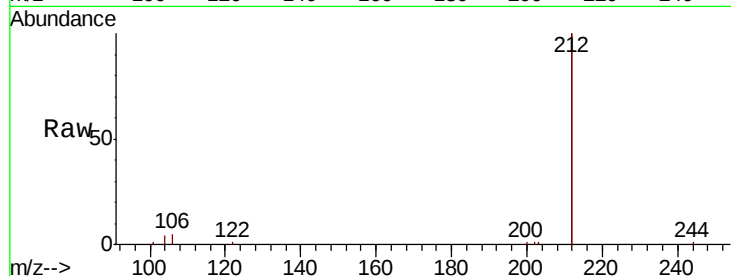

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

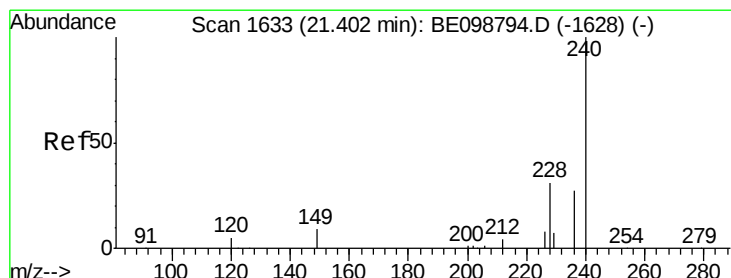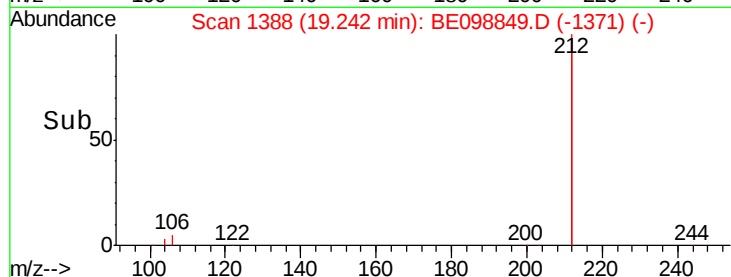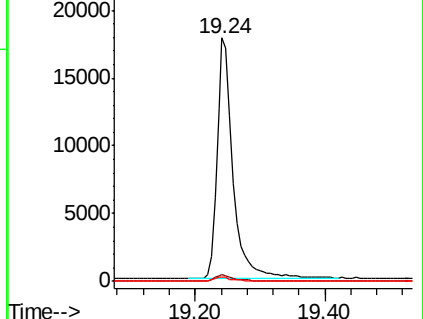

#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.40 min Scan# 1633

Delta R.T. 0.00 min

Lab File: BE098849.D

Acq: 9 Mar 2019 1:31


Tgt Ion:240 Resp: 6837

Ion Ratio Lower Upper

240 100

120 6.6 5.0 7.4



236 27.9 22.7 34.1

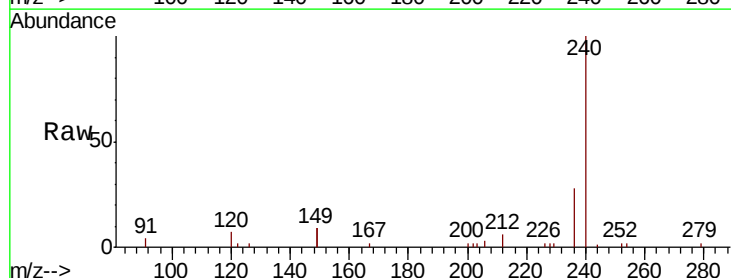


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

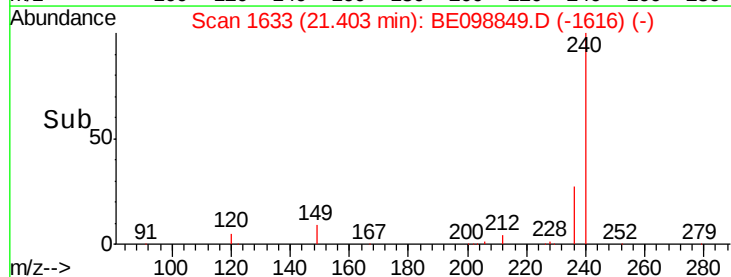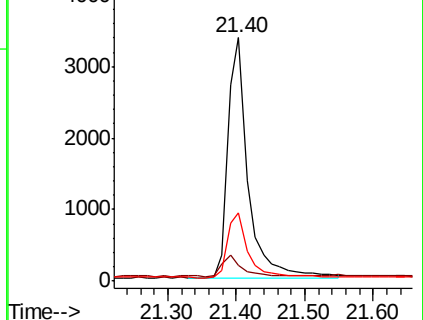

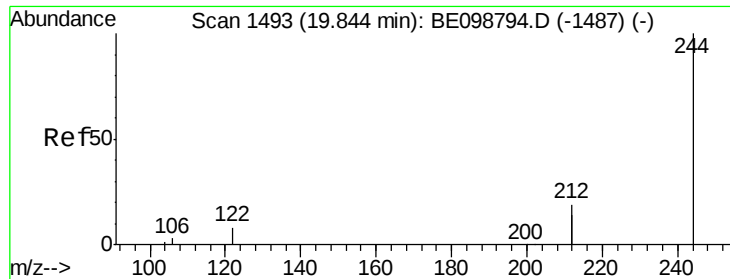

#29

Terphenyl-d14

Concen: 0.464 ng

RT: 19.84 min Scan# 1492

Delta R.T. -0.00 min

Lab File: BE098849.D

Acq: 9 Mar 2019 1:31

Instrument :

BNA_E

ClientSampleId :

RE126D1-20190306


Tot Ion:244 Resp: 7705

Ion Ratio Lower Upper

244 100

212 39.8 29.4 44.2




122 9.2 7.1 10.7

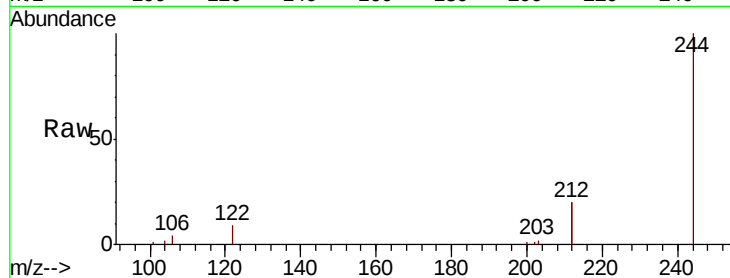

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

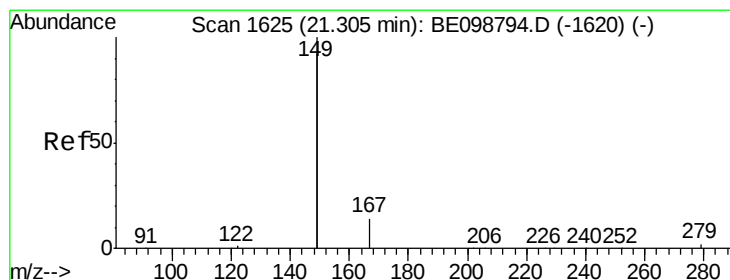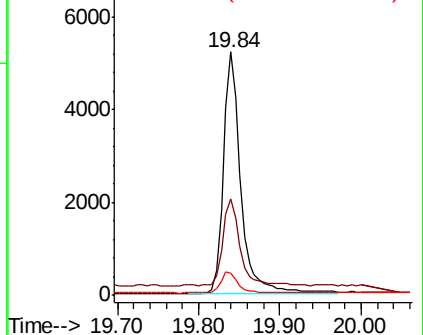

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.066 ng

RT: 21.29 min Scan# 1624

Delta R.T. -0.01 min

Lab File: BE098849.D

Acq: 9 Mar 2019 1:31


Tgt Ion:149 Resp: 2975

Ion Ratio Lower Upper

149 100

167 6.6 5.4 8.0



279 1.0 1.0 1.4



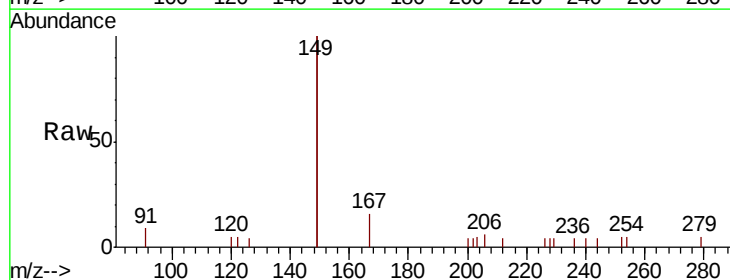


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

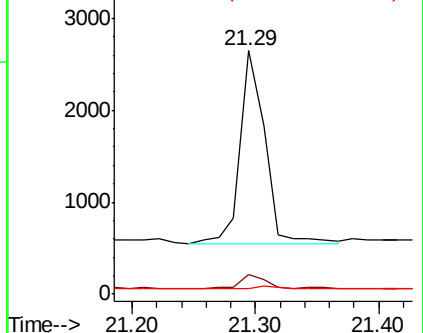

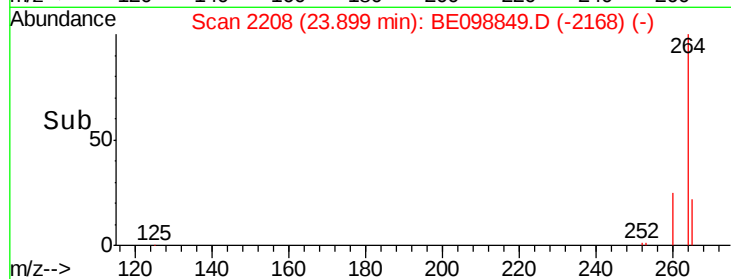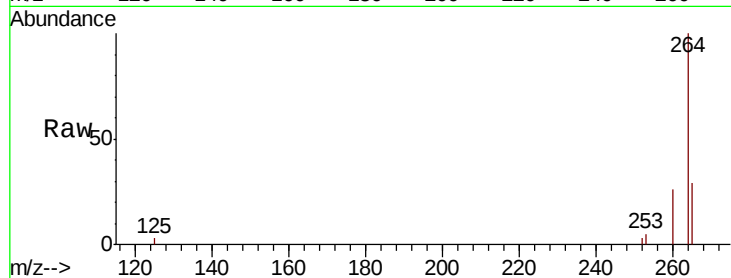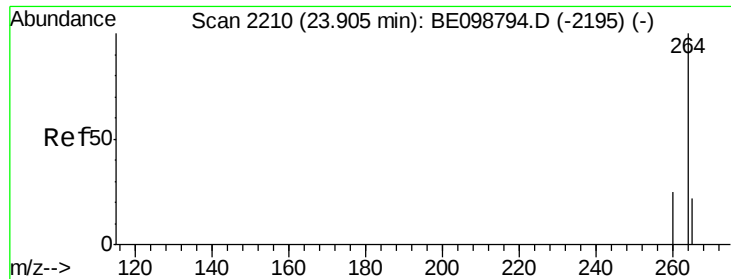

#34
Pervlene-d12
Concen: 0.400 ng
RT: 23.90 min Scan# 2208
Delta R.T. -0.01 min
Lab File: BE098849.D
Acq: 9 Mar 2019 1:31

Instrument :
BNA_E
ClientSampleId :
RE126D1-20190306

Tot Ion:264 Resp: 6639
Ion Ratio Lower Upper
264 100
260 26.4 21.2 31.8
265 29.4 24.6 36.8

