

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE030819\
 Data File : BE098831.D
 Acq On : 8 Mar 2019 10:42
 Operator : JU/SJ
 Sample : PB117716BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 PB117716BL

Quant Time: Mar 08 13:41:26 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE030619.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Mar 06 15:33:24 2019

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	649	0.40	ng	0.00
7) Naphthalene-d8	10.60	136	2675	0.40	ng	0.01
13) Acenaphthene-d10	14.47	164	1973	0.40	ng	0.01
19) Phenanthrene-d10	17.22	188	5303	0.40	ng	0.00
27) Chrysene-d12	21.40	240	6373	0.40	ng	0.00
34) Perylene-d12	23.90	264	6438	0.40	ng	0.00

System Monitoring Compounds

4) 2-Fluorophenol	5.40	112	448	0.23	ng	0.01
5) Phenol-d6	7.02	99	571	0.21	ng	0.04
8) Nitrobenzene-d5	9.03	82	333	0.12	ng	0.07
11) 2-Methylnaphthalene-d10	12.22	152	1143	0.23	ng	0.03
14) 2,4,6-Tribromophenol	15.98	330	158	0.16	ng	0.01
15) 2-Fluorobiphenyl	13.10	172	1773	0.22	ng	0.01
25) Fluoranthene-d10	19.25	212	18539	0.22	ng	0.00
29) Terphenyl-d14	19.85	244	3724	0.24	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE030819\
Data File : BE098831.D
Acq On : 8 Mar 2019 10:42
Operator : JU/SJ
Sample : PB117716BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB117716BL

Quant Time: Mar 08 13:41:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE030619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 06 15:33:24 2019
Response via : Initial Calibration




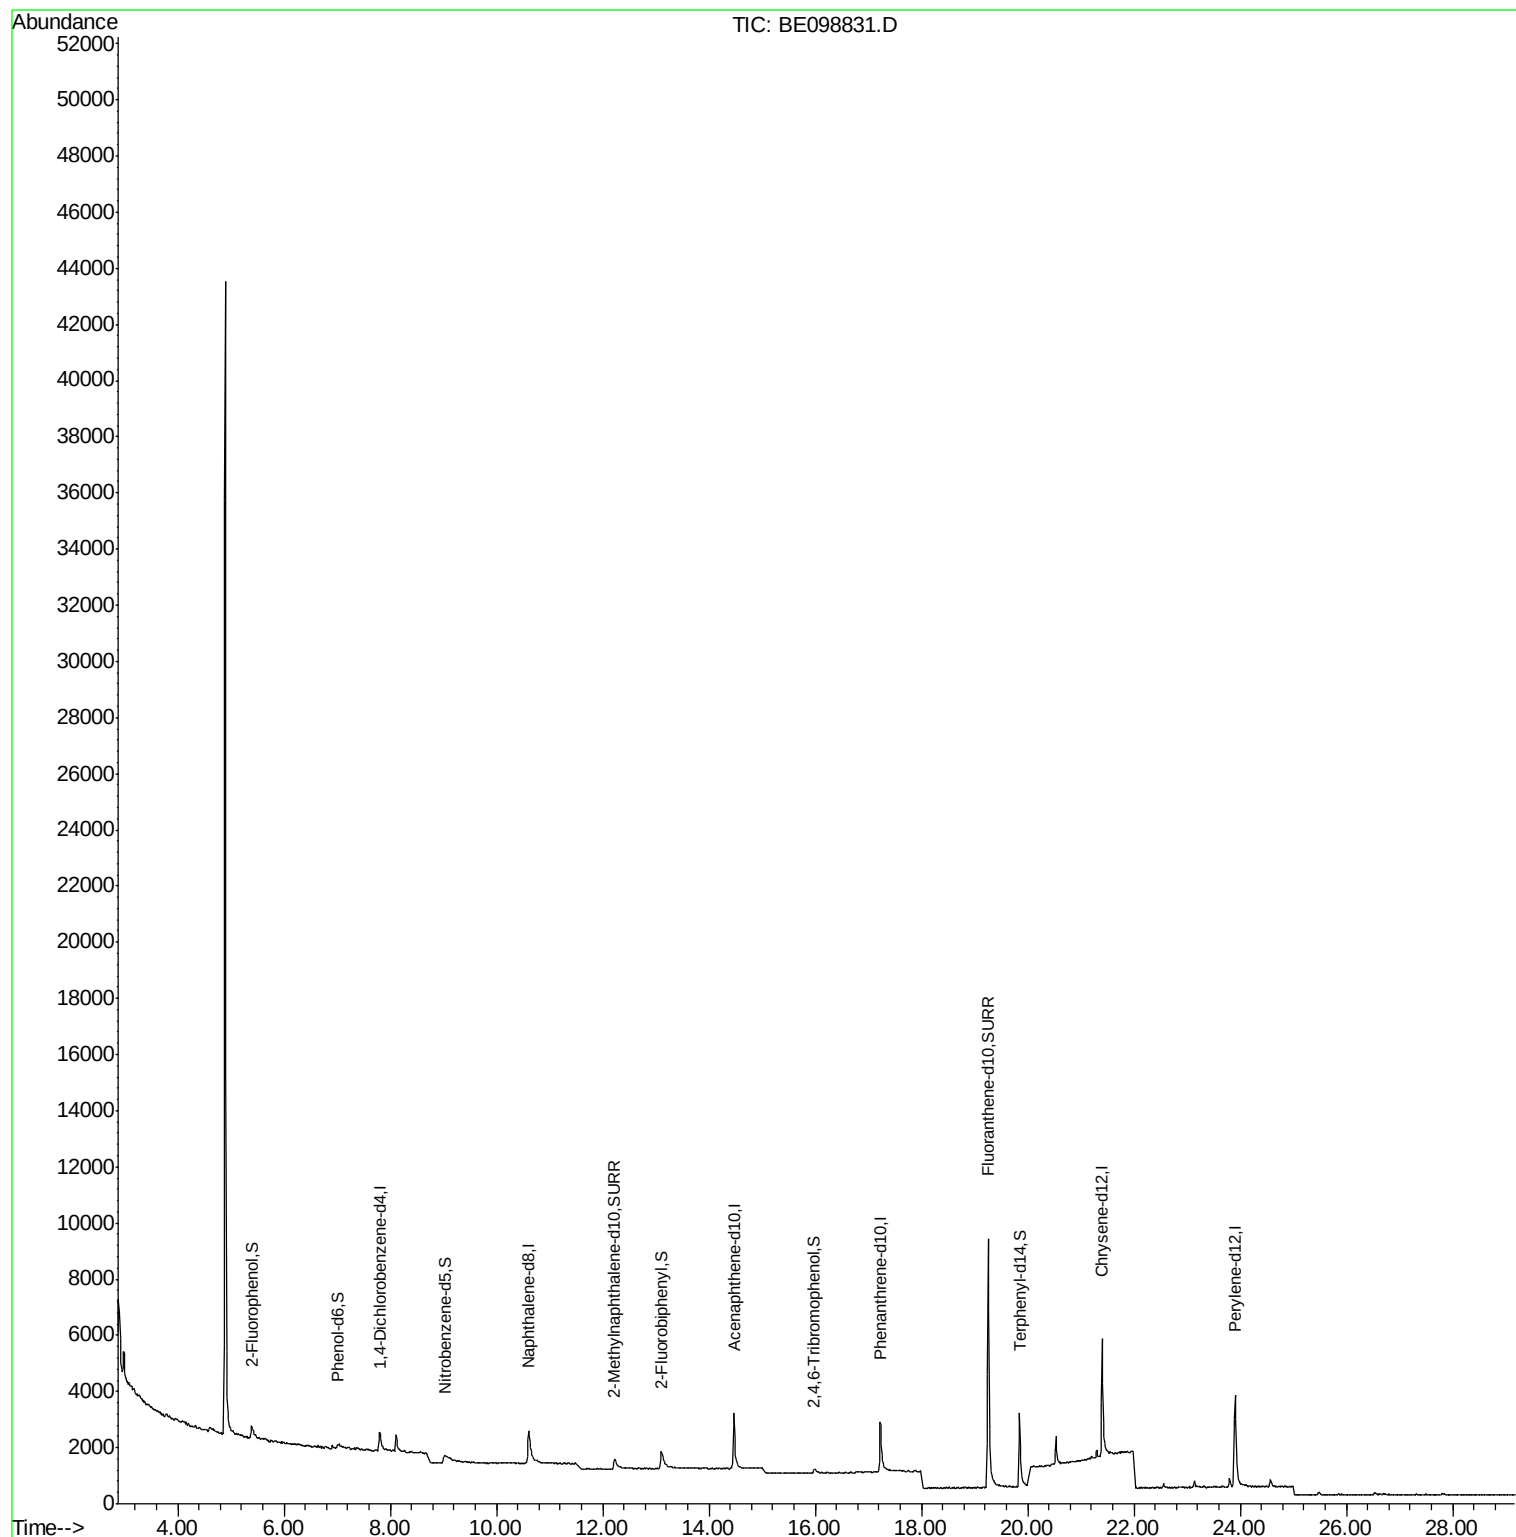


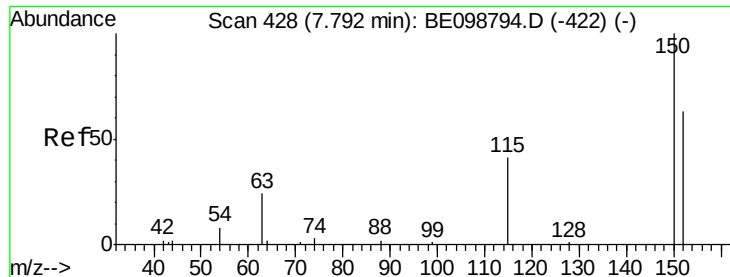

#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.79 min Scan# 428
 Delta R.T. 0.00 min
 Lab File: BE098831.D
 Acq: 8 Mar 2019 10:42




Instrument :
 BNA_E
 ClientSampleId :
 PB117716BL




Tgt Ion:152 Resp: 649
 Ion Ratio Lower Upper
 152 100
 150 153.5 122.5 183.7
 115 83.0 57.4 86.2

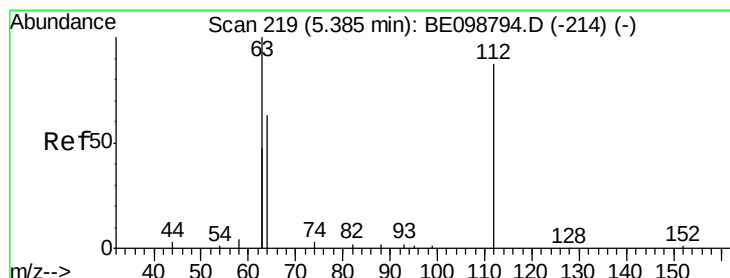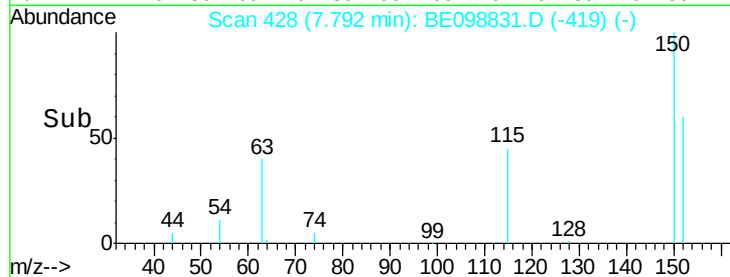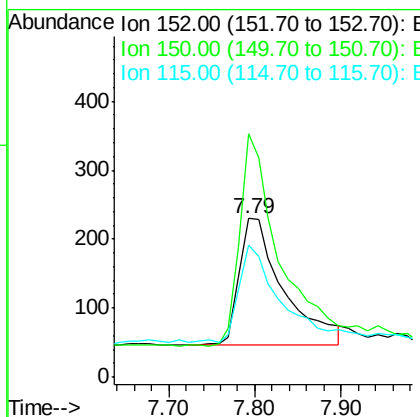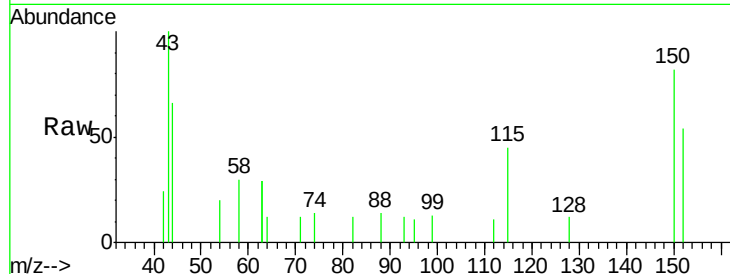

#4
 2-Fluorophenol
 Concen: 0.231 ng
 RT: 5.40 min Scan# 220
 Delta R.T. 0.01 min
 Lab File: BE098831.D
 Acq: 8 Mar 2019 10:42

Tgt Ion:112 Resp: 448
 Ion Ratio Lower Upper
 112 100
 64 83.7 57.9 86.9
 63 216.3 158.3 237.5


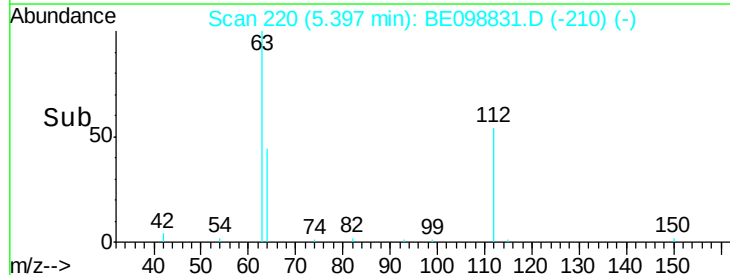
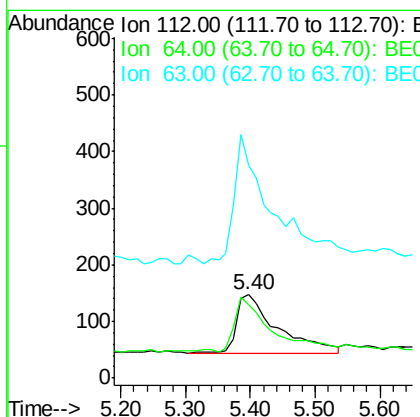
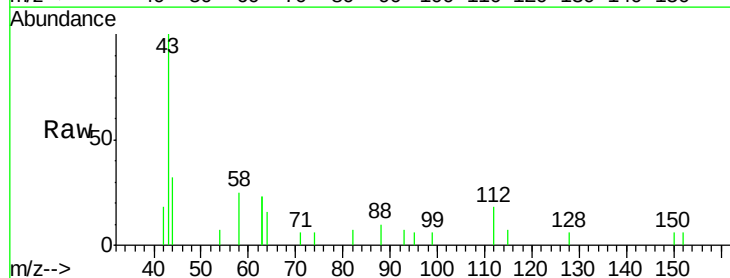


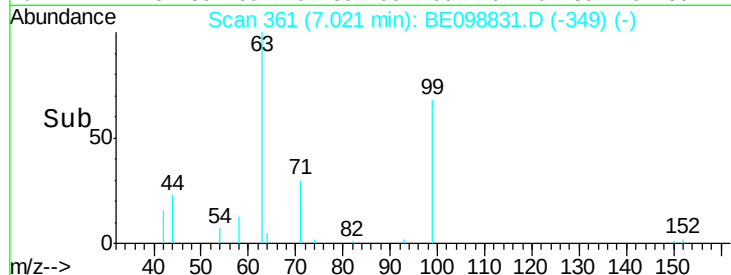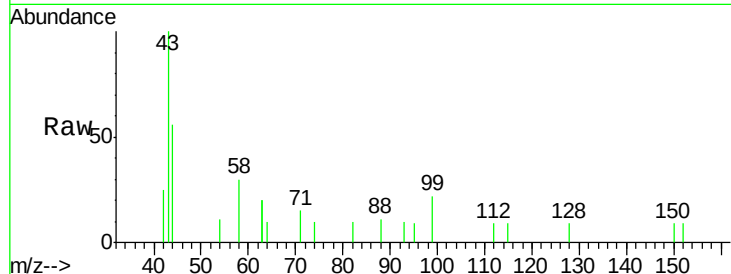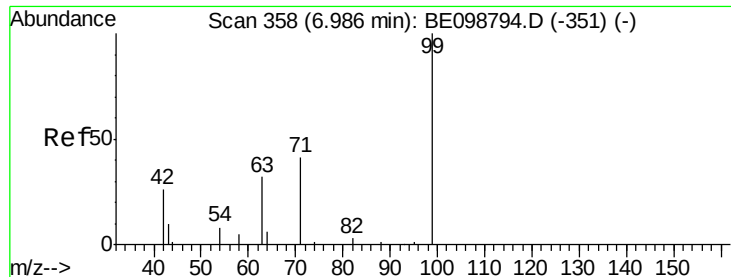

#5
 Phenol-d6
 Concen: 0.208 ng
 RT: 7.02 min Scan# 361
 Delta R.T. 0.04 min
 Lab File: BE098831.D
 Acq: 8 Mar 2019 10:42


Tgt Ion: 99 Resp: 571
 Ion Ratio Lower Upper
 99 100
 42 25.6 24.2 36.2
 71 22.6 35.7 53.5#


Instrument :
 BNA_E
 ClientSampleId :
 PB117716BL

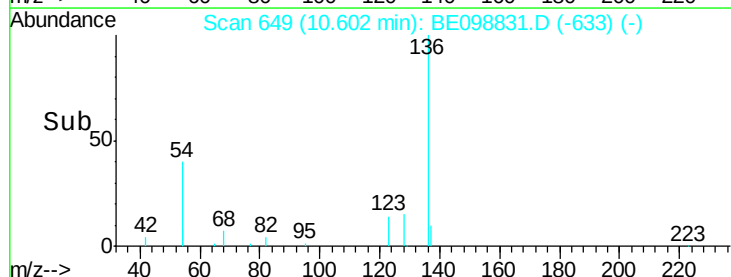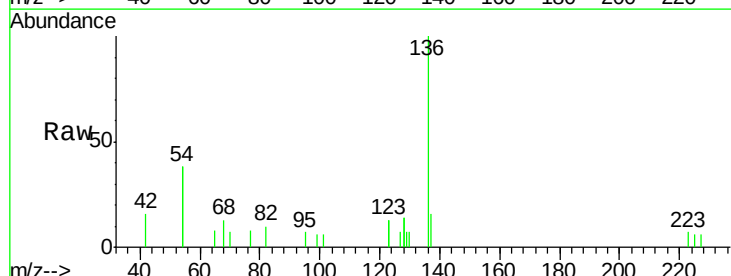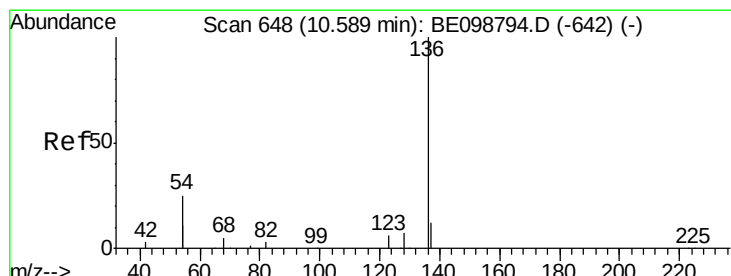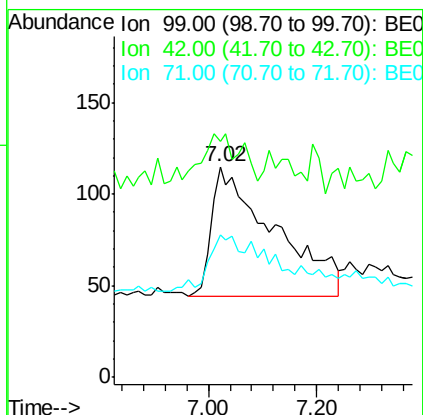

#7
 Naphthalene-d8
 Concen: 0.400 ng
 RT: 10.60 min Scan# 649
 Delta R.T. 0.01 min
 Lab File: BE098831.D
 Acq: 8 Mar 2019 10:42

Tgt Ion: 136 Resp: 2675
 Ion Ratio Lower Upper
 136 100
 137 15.6 11.4 17.0
 54 75.8 39.3 58.9#
 68 13.1 6.7 10.1#




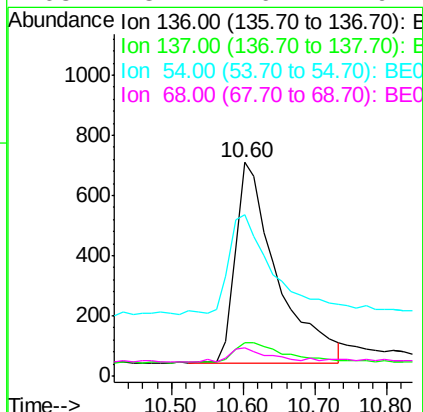


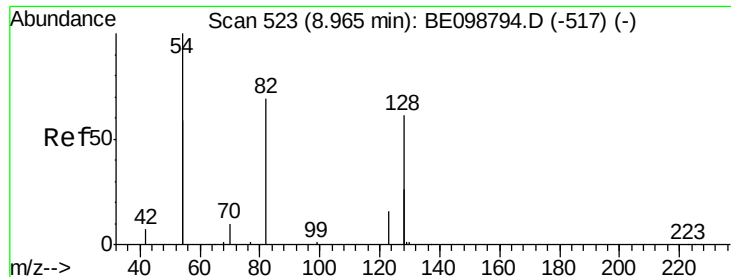

#8
 Nitrobenzene-d5
 Concen: 0.119 ng
 RT: 9.03 min Scan# 528
 Delta R.T. 0.07 min
 Lab File: BE098831.D
 Acq: 8 Mar 2019 10:42




Instrument :
 BNA_E
 ClientSampleId :
 PB117716BL


Tgt Ion: 82 Resp: 333
 Ion Ratio Lower Upper
 82 100
 128 251.9 123.8 185.8#
 54 332.7 203.4 305.2#

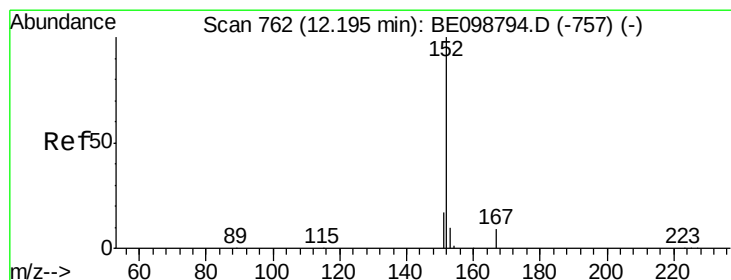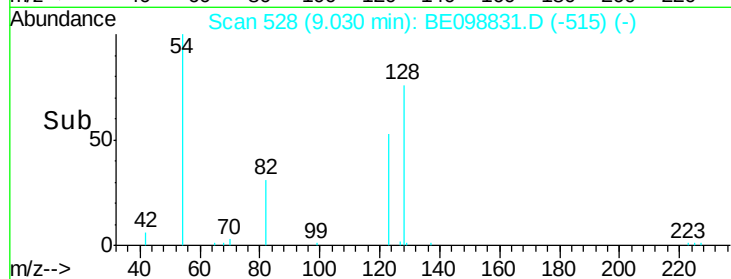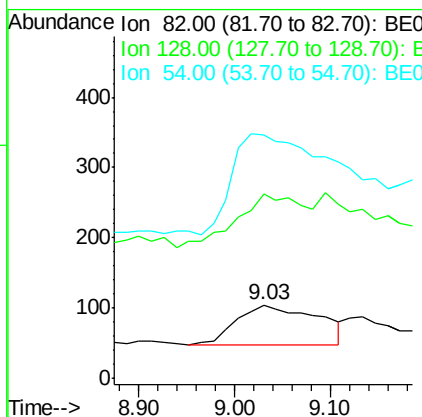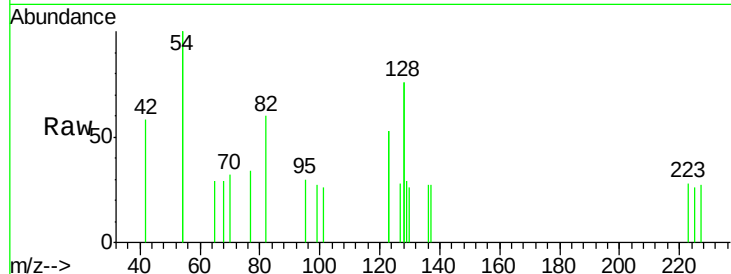

#11
 2-Methylnaphthalene-d10
 Concen: 0.231 ng
 RT: 12.22 min Scan# 764
 Delta R.T. 0.03 min
 Lab File: BE098831.D
 Acq: 8 Mar 2019 10:42

Tgt Ion: 152 Resp: 1143
 Ion Ratio Lower Upper
 152 100
 151 17.2 16.5 24.7


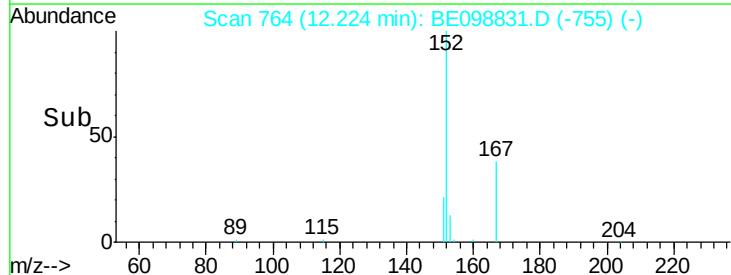
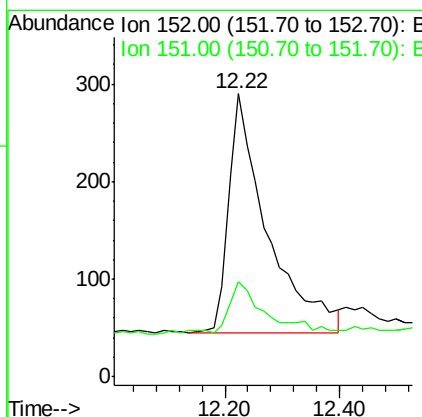
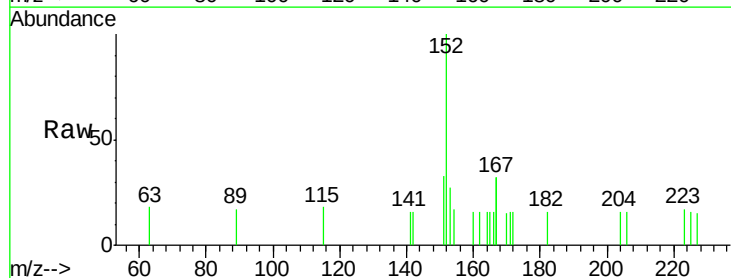


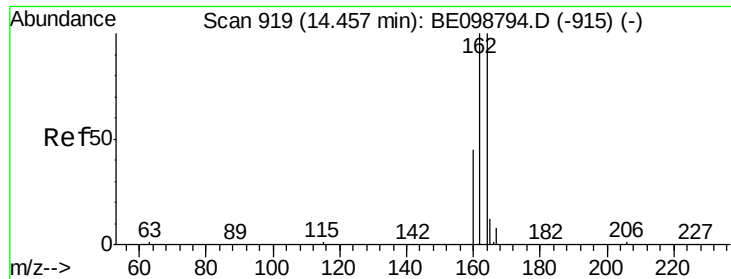

#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.47 min Scan# 920
 Delta R.T. 0.01 min
 Lab File: BE098831.D
 Acq: 8 Mar 2019 10:42




Instrument :
 BNA_E
 ClientSampleId :
 PB117716BL


Tgt Ion:164 Resp: 1973
 Ion Ratio Lower Upper
 164 100
 162 100.4 80.2 120.2
 160 47.8 37.8 56.8

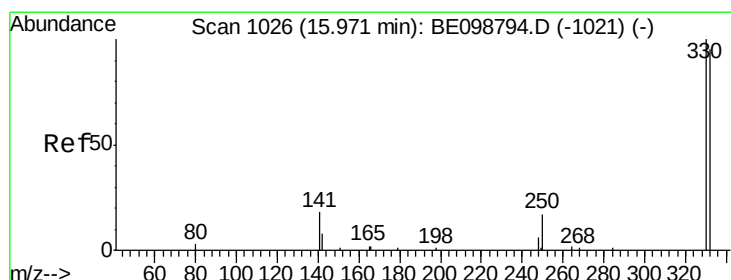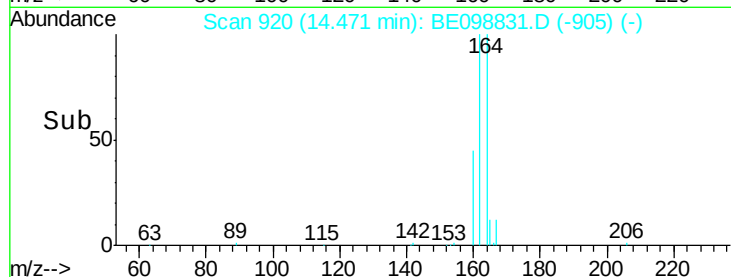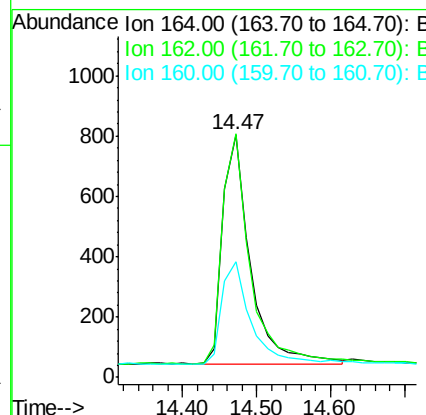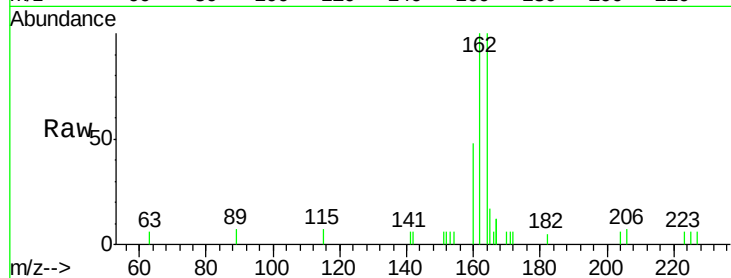

#14
 2,4,6-Tribromophenol
 Concen: 0.159 ng
 RT: 15.98 min Scan# 1027
 Delta R.T. 0.01 min
 Lab File: BE098831.D
 Acq: 8 Mar 2019 10:42

Tgt Ion:330 Resp: 158
 Ion Ratio Lower Upper
 330 100
 332 110.1 77.6 116.4
 141 31.6 31.0 46.4


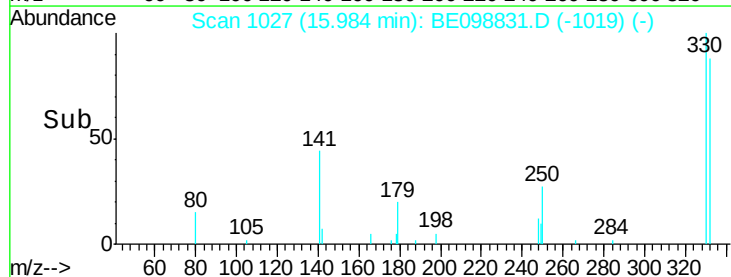
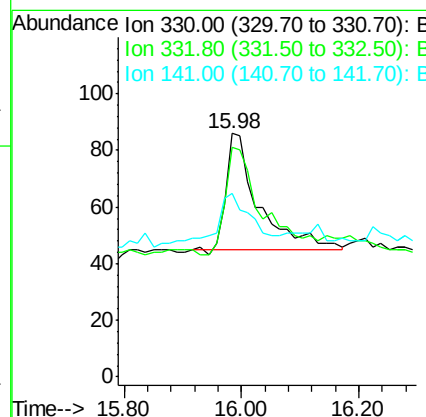
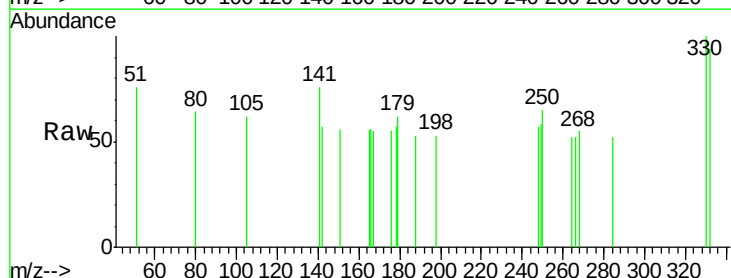


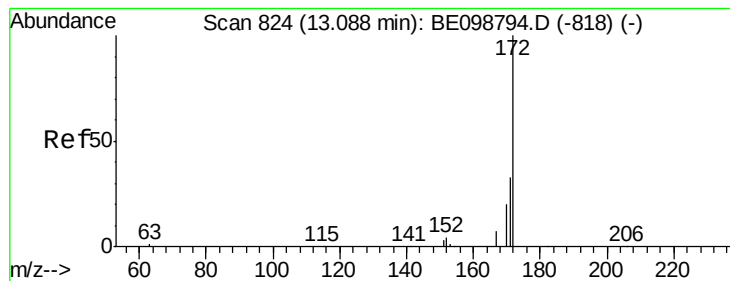

#15
2-Fluorobiphenyl
Concen: 0.217 ng
RT: 13.10 min Scan# 825
Delta R.T. 0.01 min
Lab File: BE098831.D
Acq: 8 Mar 2019 10:42




Instrument :
BNA_E
ClientSampleId :
PB117716BL


Tgt Ion:172 Resp: 1773
Ion Ratio Lower Upper
172 100
171 38.6 28.0 42.0
170 30.9 17.7 26.5#

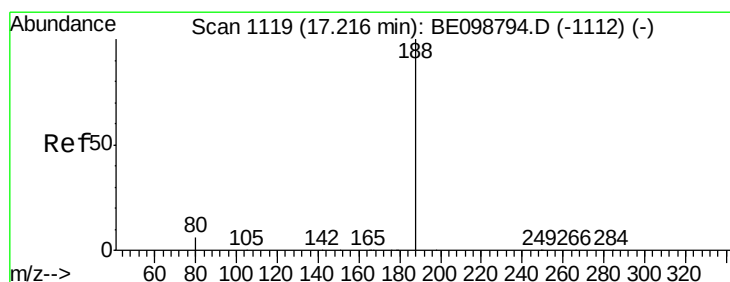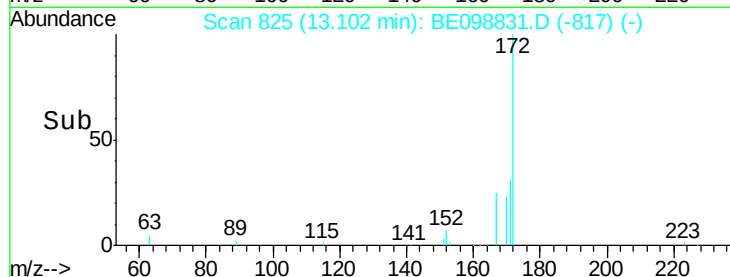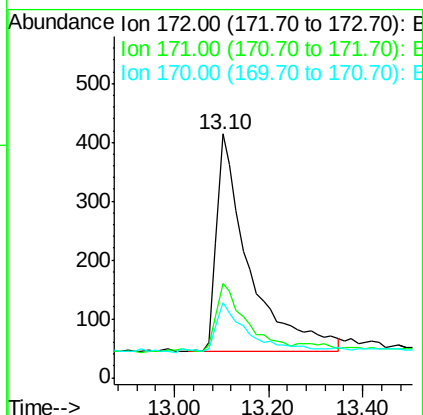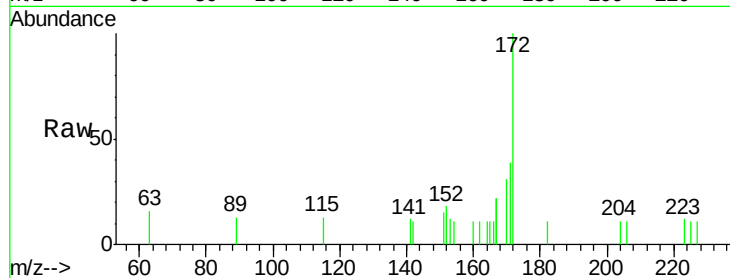

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.22 min Scan# 1119
Delta R.T. -0.00 min
Lab File: BE098831.D
Acq: 8 Mar 2019 10:42

Tgt Ion:188 Resp: 5303
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 13.2 6.3 9.5#

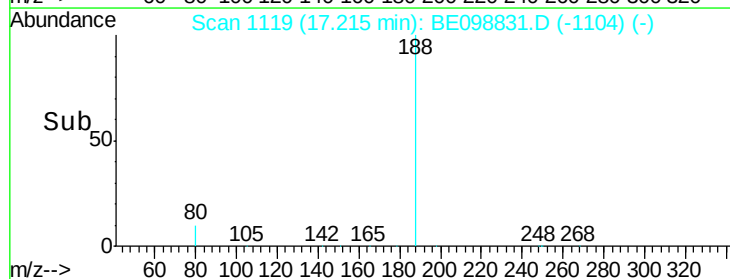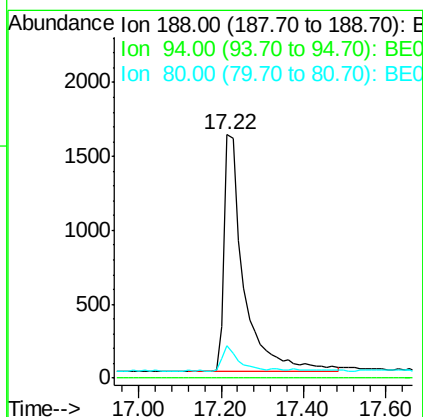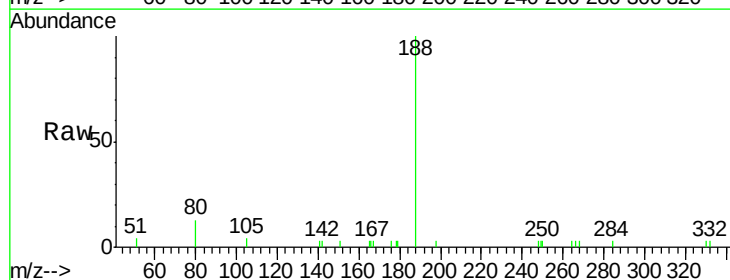

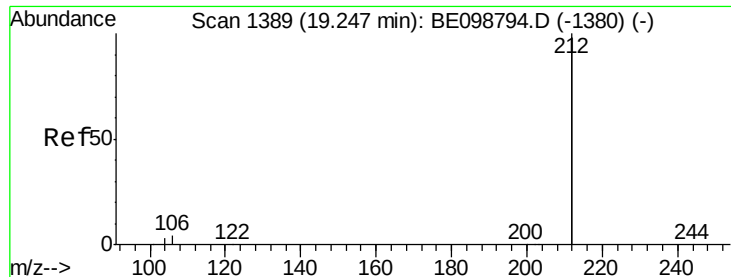

#25

Fluoranthene-d10

Concen: 0.219 ng

RT: 19.25 min Scan# 1390

Delta R.T. 0.01 min

Lab File: BE098831.D

Acq: 8 Mar 2019 10:42

Instrument :

BNA_E

ClientSampleId :

PB117716BL


Tgt Ion:212 Resp: 18539

Ion Ratio Lower Upper

212 100

106 2.4 1.8 2.8




104 1.3 1.0 1.6

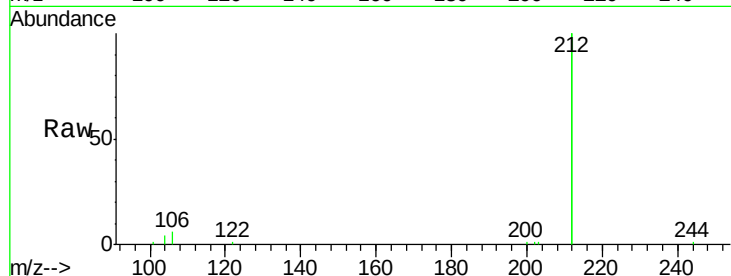

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

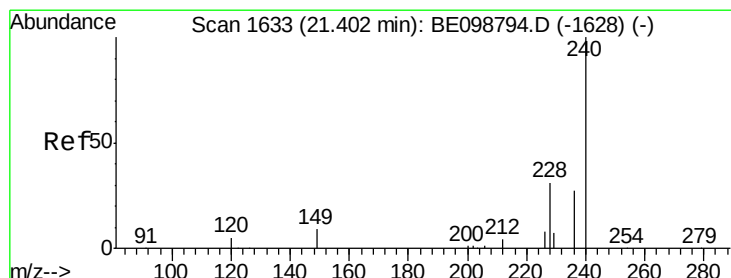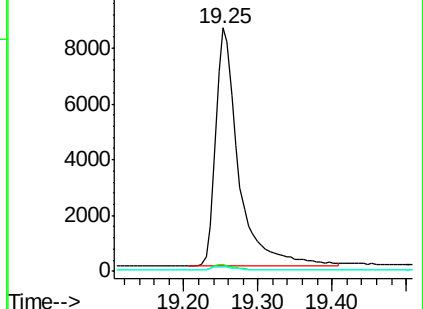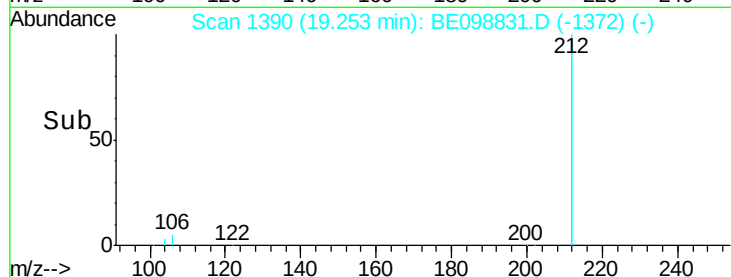

#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.40 min Scan# 1633

Delta R.T. 0.00 min

Lab File: BE098831.D

Acq: 8 Mar 2019 10:42


Tgt Ion:240 Resp: 6373

Ion Ratio Lower Upper

240 100

120 8.7 5.0 7.4#



236 27.5 22.7 34.1

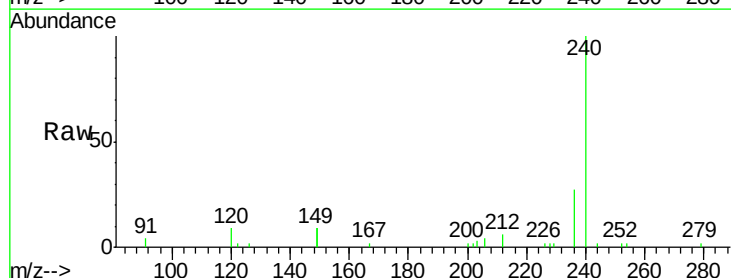


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

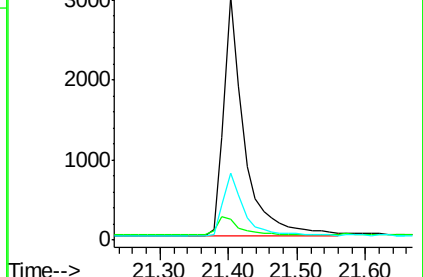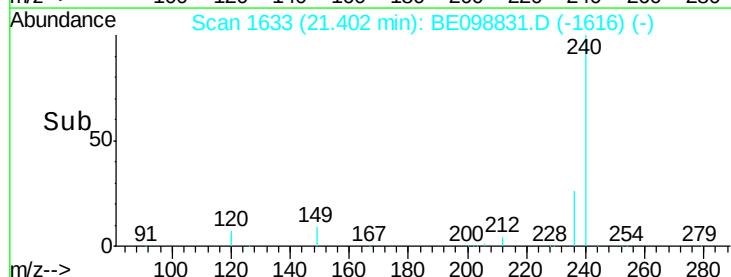

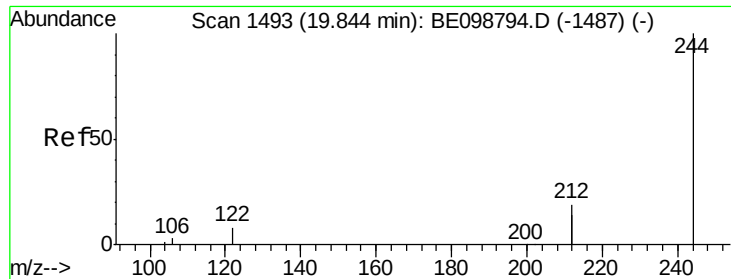

#29

Terphenyl-d14

Concen: 0.240 ng

RT: 19.85 min Scan# 1494

Delta R.T. 0.01 min

Lab File: BE098831.D

Acq: 8 Mar 2019 10:42

Instrument :

BNA_E

ClientSampleId :

PB117716BL


Tgt Ion:244 Resp: 3724

Ion Ratio Lower Upper




244 100

212 43.4 29.4 44.2

122 11.7 7.1 10.7#

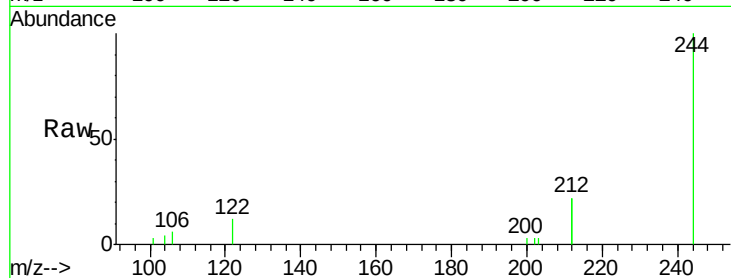

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

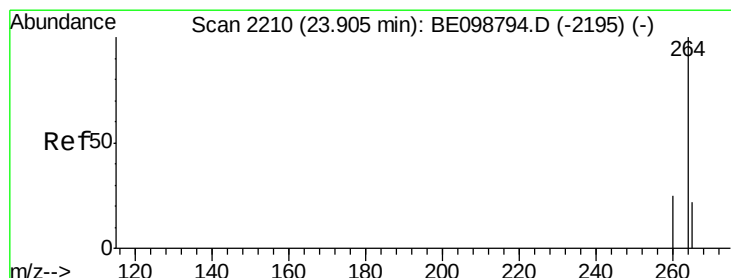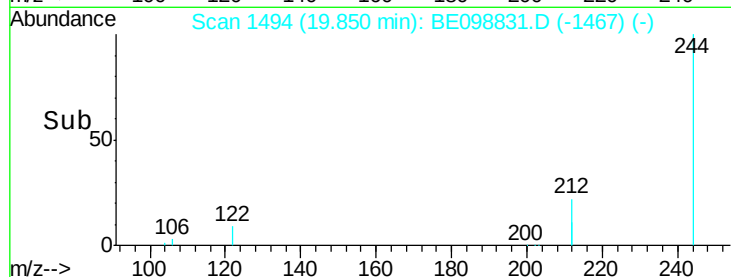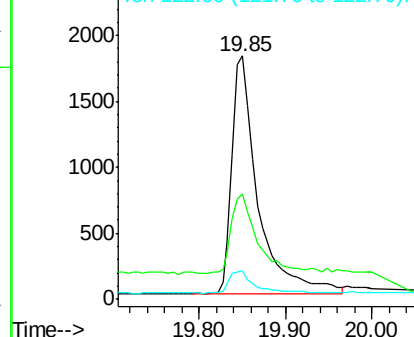

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.90 min Scan# 2209

Delta R.T. -0.00 min

Lab File: BE098831.D

Acq: 8 Mar 2019 10:42


Tgt Ion:264 Resp: 6438

Ion Ratio Lower Upper

264 100

260 25.8 21.2 31.8

265 30.3 24.6 36.8

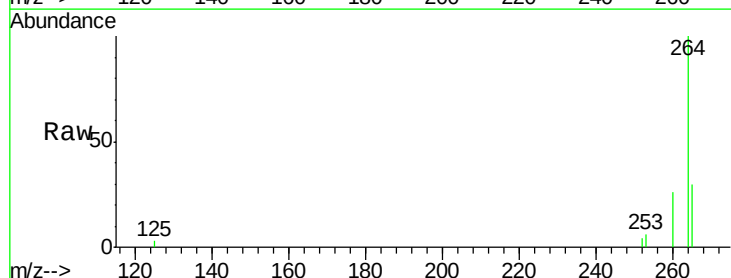

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

