


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE030819\
 Data File : BE098828.D
 Acq On : 8 Mar 2019 8:50
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE030619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 06 15:33:24 2019

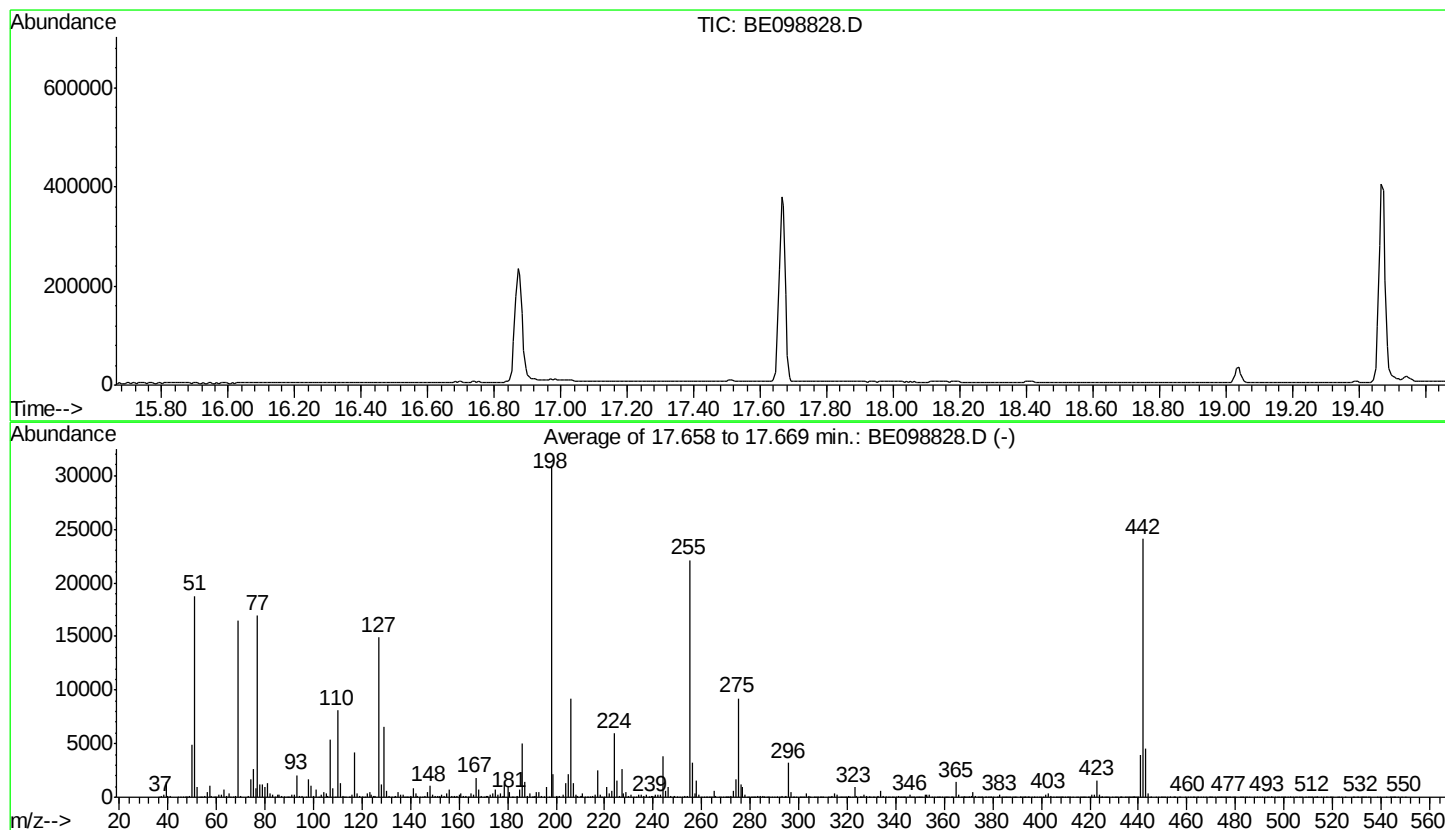

AutoFind: Scans 2565, 2566, 2567; Background Corrected with Scan 2558

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.7	18789	PASS
68	69	0.00	2	0.8	133	PASS
69	198	0.00	100	53.1	16438	PASS
70	69	0.00	2	0.5	87	PASS
127	198	10	80	48.1	14875	PASS
197	198	0.00	2	0.1	26	PASS
198	198	100	100	100.0	30938	PASS
199	198	5	9	7.2	2213	PASS
275	198	10	60	29.7	9204	PASS
365	198	1	100	4.5	1397	PASS
441	198	0.01	100	12.7	3937	PASS
442	198	50	100	78.0	24124	PASS
443	442	15	24	18.7	4512	PASS