


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE030819\
 Data File : BE098843.D
 Acq On : 8 Mar 2019 21:41
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE030619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 06 15:33:24 2019

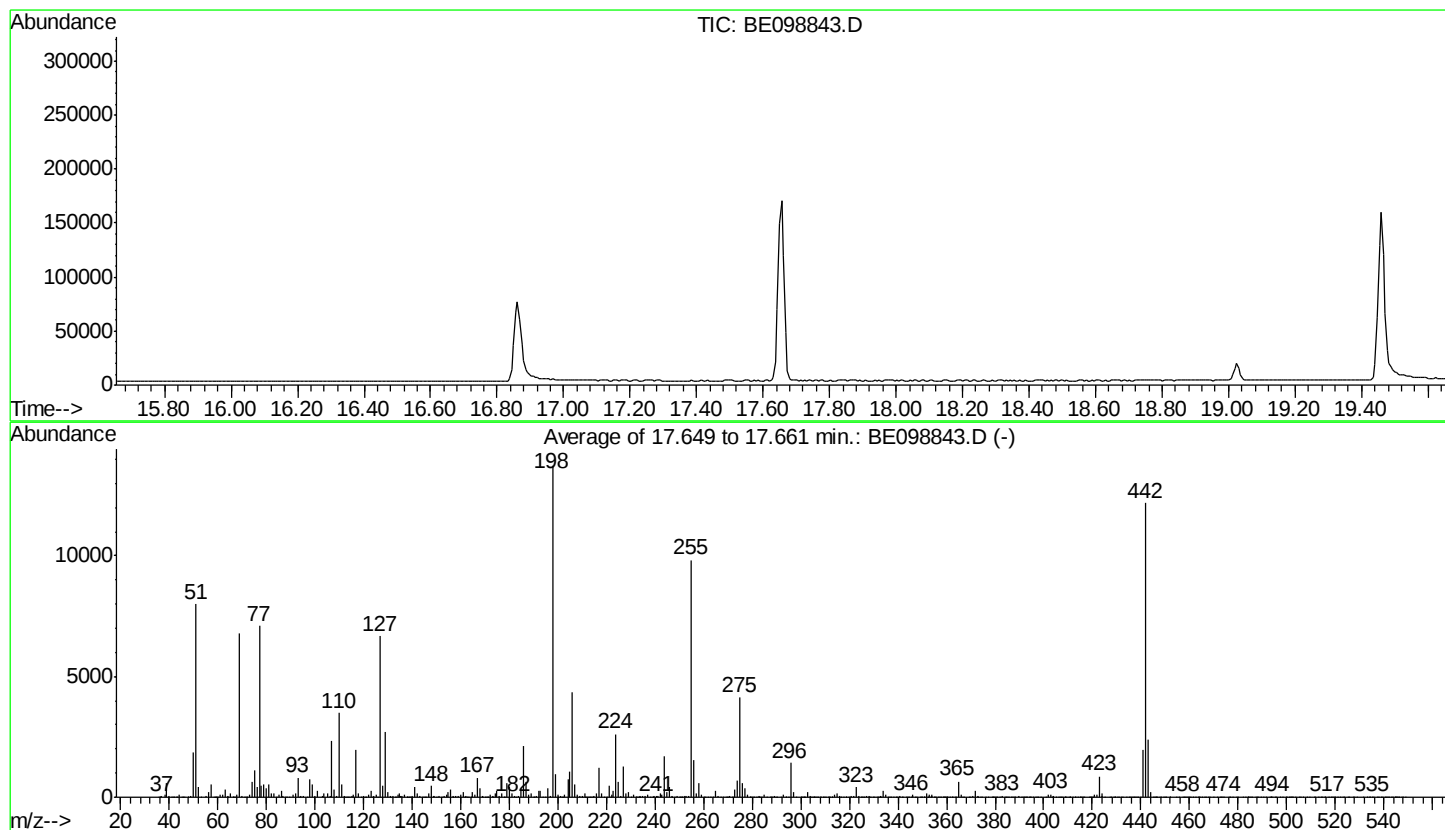

AutoFind: Scans 2563, 2564, 2565; Background Corrected with Scan 2552

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.2	7998	PASS
68	69	0.00	2	1.3	89	PASS
69	198	0.00	100	49.5	6799	PASS
70	69	0.00	2	0.5	37	PASS
127	198	10	80	48.5	6663	PASS
197	198	0.00	2	0.4	60	PASS
198	198	100	100	100.0	13740	PASS
199	198	5	9	7.0	955	PASS
275	198	10	60	30.1	4131	PASS
365	198	1	100	4.8	662	PASS
441	198	0.01	100	14.2	1955	PASS
442	198	50	100	88.6	12180	PASS
443	442	15	24	19.7	2404	PASS