
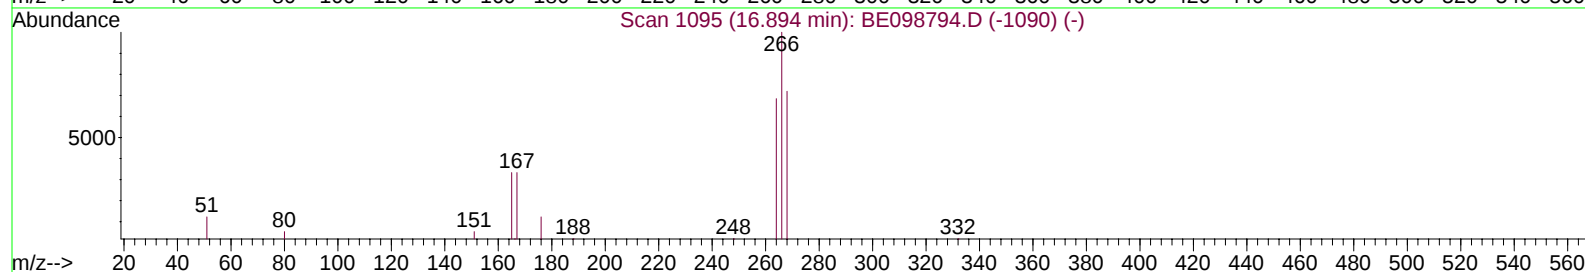
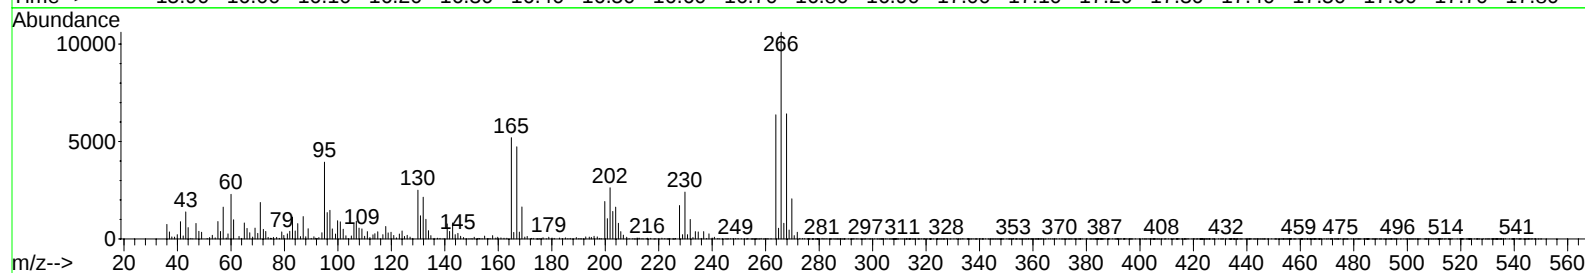


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE031119\
Data File : BE098856.D
Acq On : 11 Mar 2019 10:33
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 12 19:15:59 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE030619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 06 15:33:24 2019
Response via : Initial Calibration

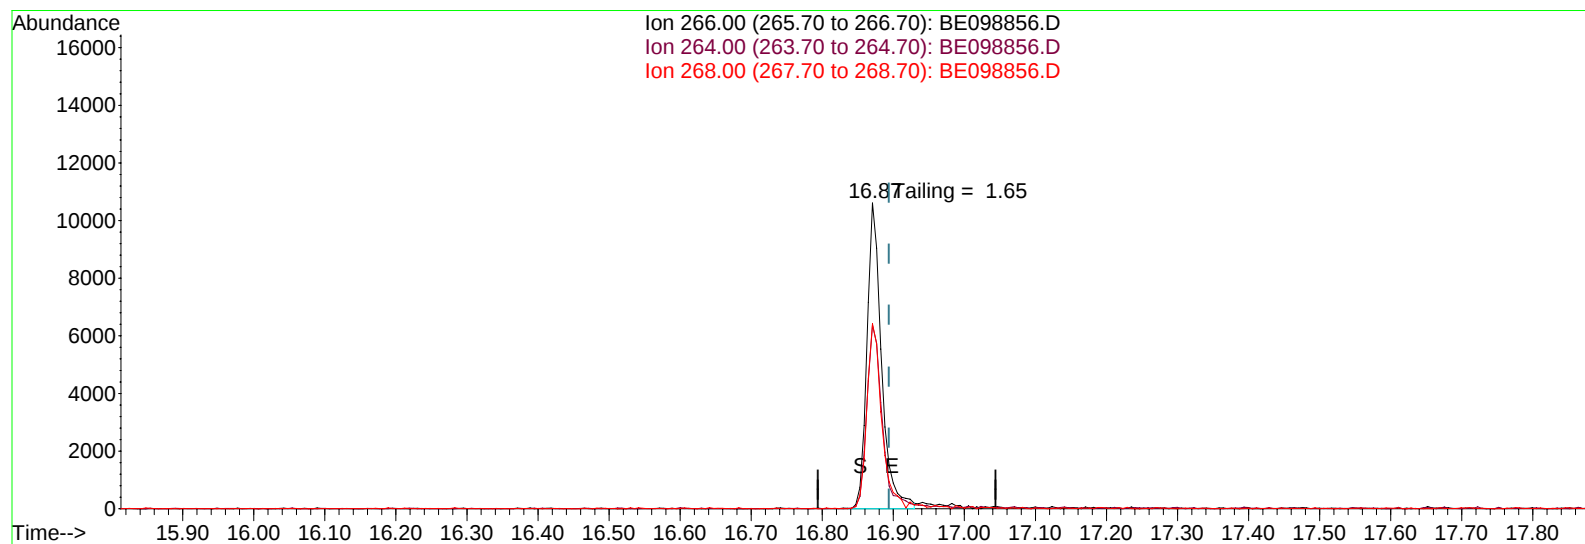

TIC: BE098856.D

(22) Pentachlorophenol

16.871min (-0.023) 3280.06ng

response 10795

Ion	Exp%	Act%
266.00	100	100
264.00	83.30	60.08#
268.00	87.30	60.51#
0.00	0.00	0.00