
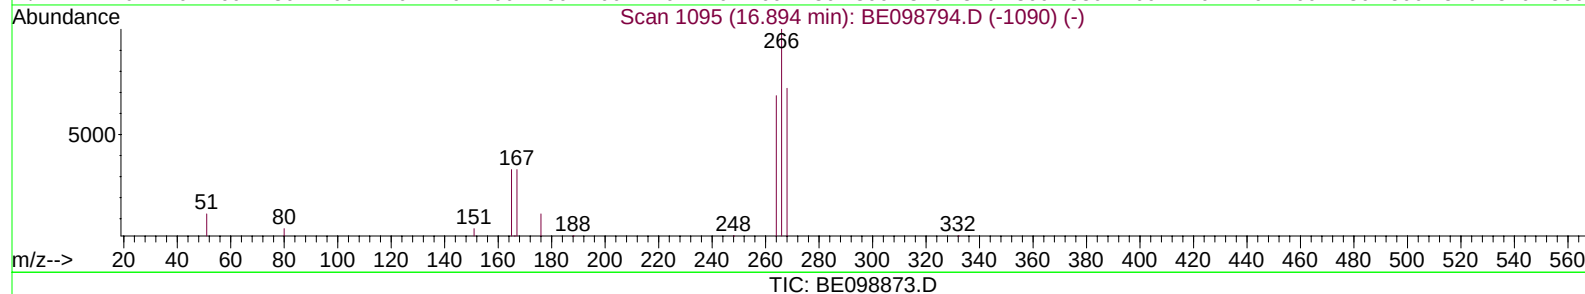
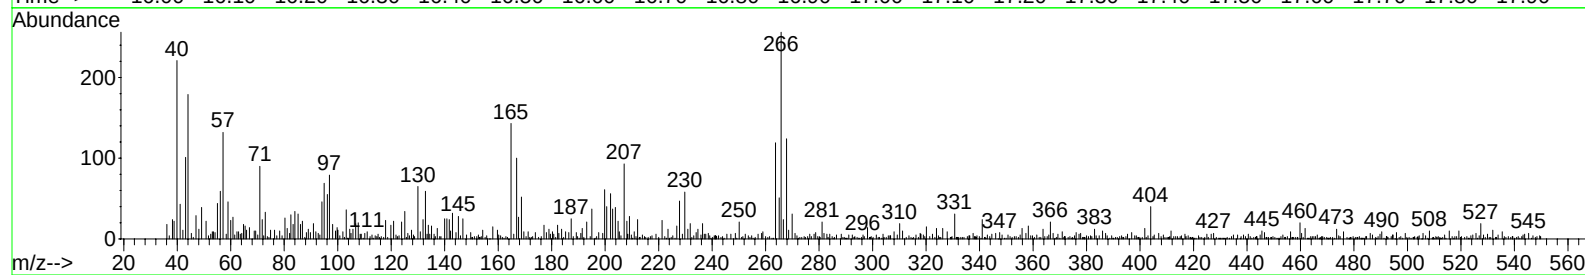


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE031119\
Data File : BE098873.D
Acq On : 11 Mar 2019 23:15
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 15 18:53:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE030619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 15 05:31:33 2019
Response via : Initial Calibration

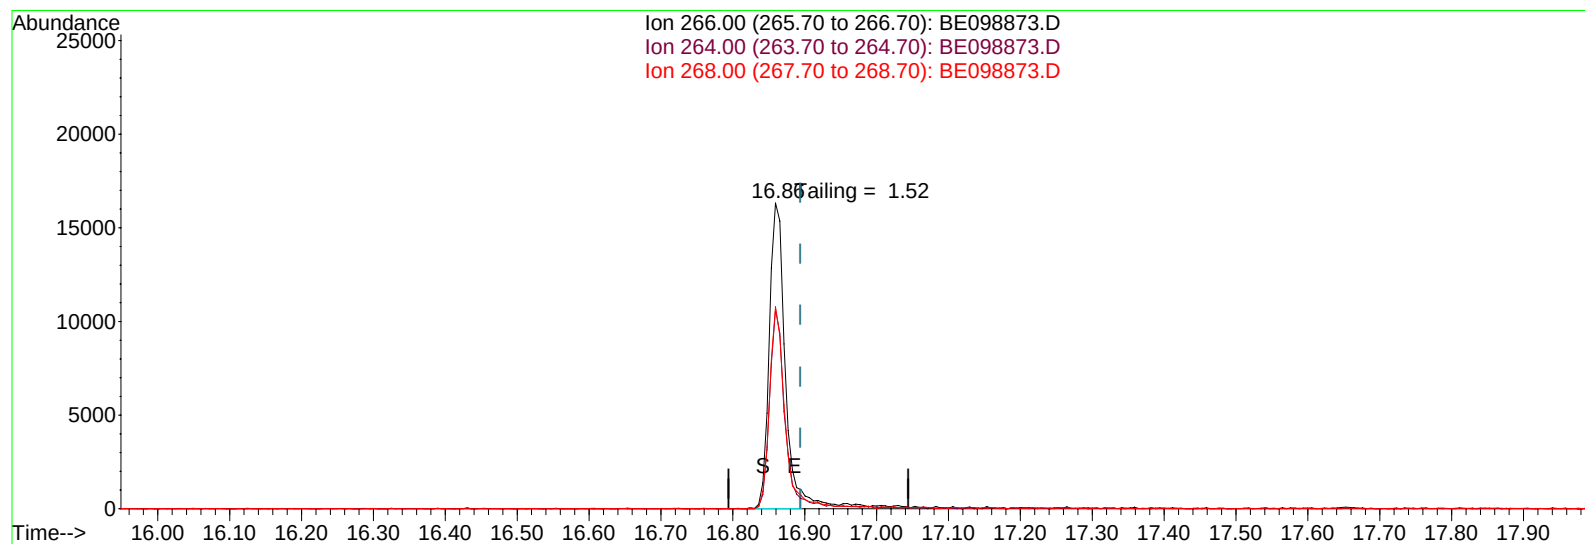

TIC: BE098873.D

(22) Pentachlorophenol

16.959min (+0.065) 68.15ng

response 283

Ion	Exp%	Act%
266.00	100	100
264.00	83.30	42.50#
268.00	87.30	48.21#
0.00	0.00	0.00