

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE031119\
 Data File : BE098861.D
 Acq On : 11 Mar 2019 13:39
 Operator : JU/SJ
 Sample : K1793-16DL 2X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 RE108D2-20190306DL

Manual Integrations
 APPROVED

Sohil
 3/12/2019 4:33:41 PM

Quant Time: Mar 12 08:09:01 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE030619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 06 15:33:24 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	701	0.40	ng	0.01
7) Naphthalene-d8	10.60	136	3357	0.40	ng	0.01
13) Acenaphthene-d10	14.46	164	2382	0.40	ng	0.00
19) Phenanthrene-d10	17.22	188	6358	0.40	ng	0.00
27) Chrysene-d12	21.40	240	7315	0.40	ng	0.00
34) Perylene-d12	23.90	264	7083	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.45	112	120m	0.06	ng	0.07
5) Phenol-d6	7.04	99	86m	0.03	ng	0.06
8) Nitrobenzene-d5	9.04	82	393	0.11	ng	0.08
11) 2-Methylnaphthalene-d10	12.22	152	1017	0.16	ng	0.03
14) 2,4,6-Tribromophenol	15.98	330	190	0.16	ng	0.01
15) 2-Fluorobiphenyl	13.10	172	1845	0.19	ng	0.01
25) Fluoranthene-d10	19.25	212	16805	0.17	ng	0.00
29) Terphenyl-d14	19.84	244	4109	0.23	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.28	88	3083	2.752	ng	Qvalue 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE031119\
Data File : BE098861.D
Acq On : 11 Mar 2019 13:39
Operator : JU/SJ
Sample : K1793-16DL 2X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
RE108D2-20190306DL

Manual Integrations
APPROVED

Sohil
3/12/2019 4:33:41 PM

Quant Time: Mar 12 08:09:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE030619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 06 15:33:24 2019
Response via : Initial Calibration

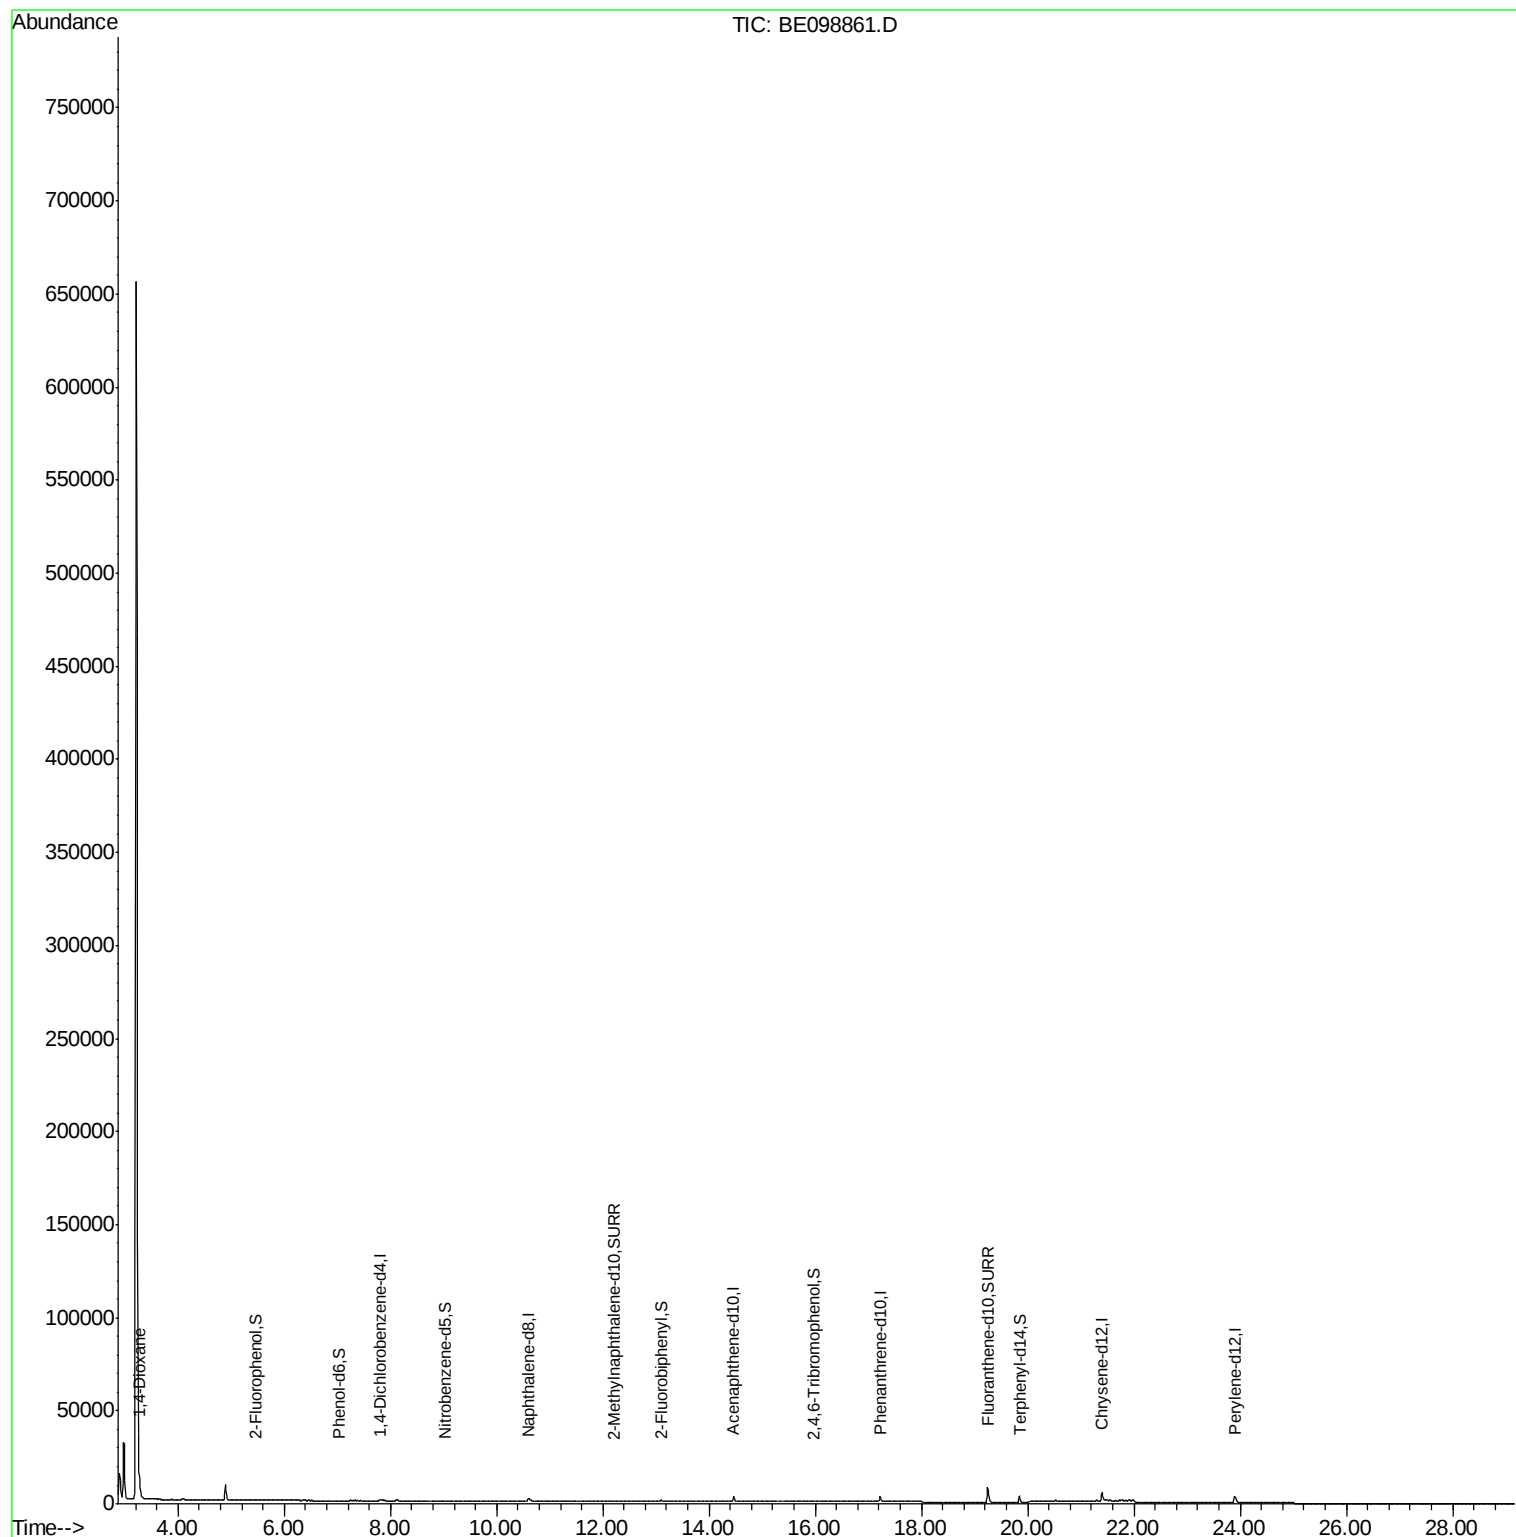



#1


1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.80 min Scan# 429
Delta R.T. 0.01 min
Lab File: BE098861.D
Acq: 11 Mar 2019 13:39

Instrument :
BNA_E
ClientSampleId :
RE108D2-20190306DL

Tot Ion	Ratio	Lower	Upper
152	100		
150	154.2	122.5	183.7
115	75.1	57.4	86.2

Manual Integrations
APPROVED

Sohil
3/12/2019 4:33:41 PM



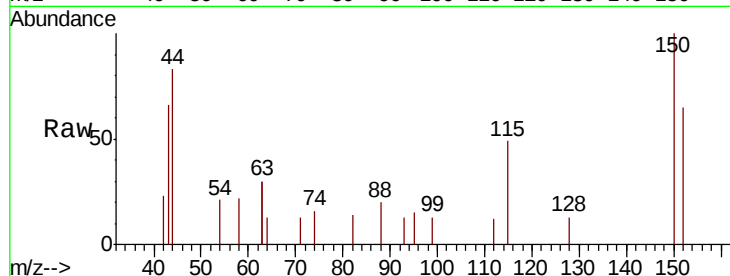


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

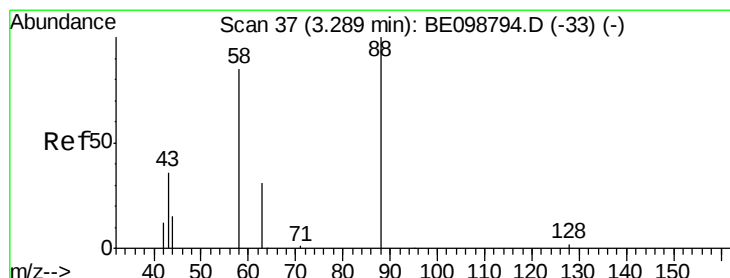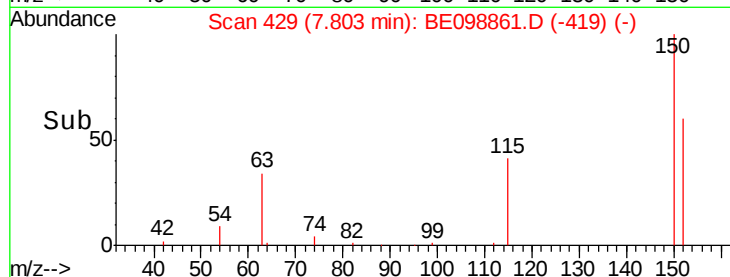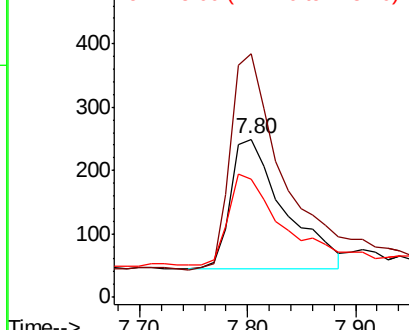

#2

1,4-Dioxane
Concen: 2.752 ng
RT: 3.28 min Scan# 36
Delta R.T. -0.01 min
Lab File: BE098861.D
Acq: 11 Mar 2019 13:39

Tgt Ion	Ratio	Lower	Upper
88	100		
58	89.6	75.8	113.6
43	54.2	41.8	62.8


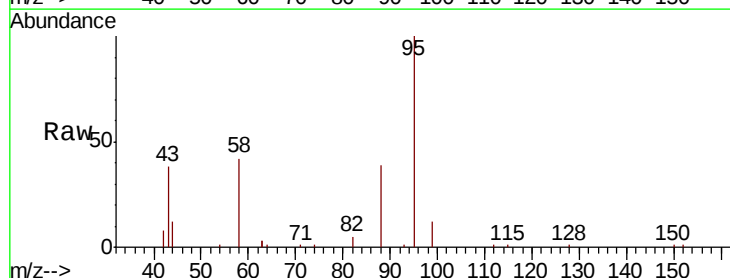



Abundance

Ion 88.00 (87.70 to 88.70): BE0

Ion 58.00 (57.70 to 58.70): BE0

Ion 43.00 (42.70 to 43.70): BE0

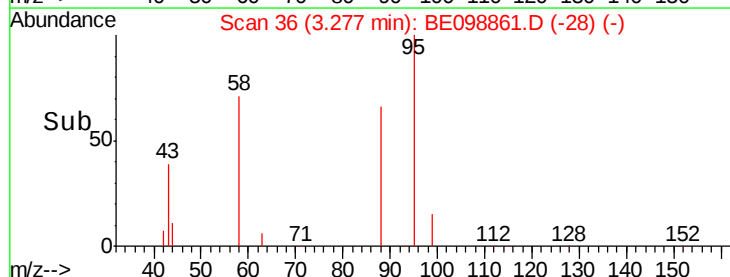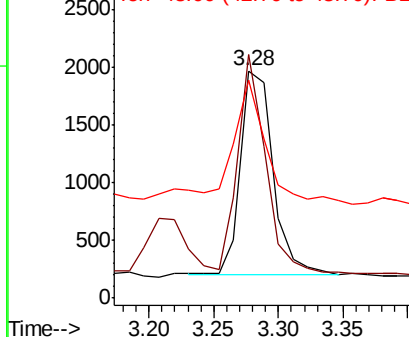

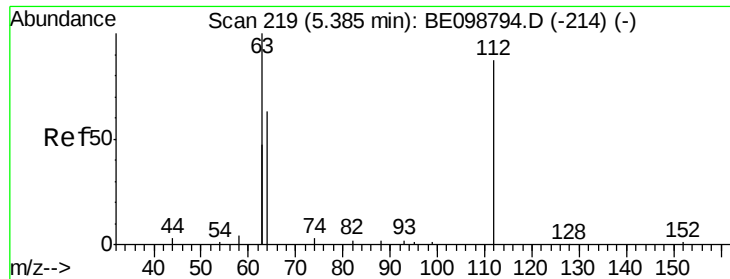

#4

2-Fluorophenol

Concen: 0.057 ng m

RT: 5.45 min Scan# 225

Delta R.T. 0.07 min

Lab File: BE098861.D

Acq: 11 Mar 2019 13:39

Instrument :

BNA_E





ClientSampleId :

RE108D2-20190306DL

Tot Ion:	112	Resp:	120
Ion Ratio	Lower	Upper	
112	100		
64	0.0	57.9	86.9#
63	0.0	158.3	237.5#

Manual Integrations
APPROVED

Sohil
3/12/2019 4:33:41 PM

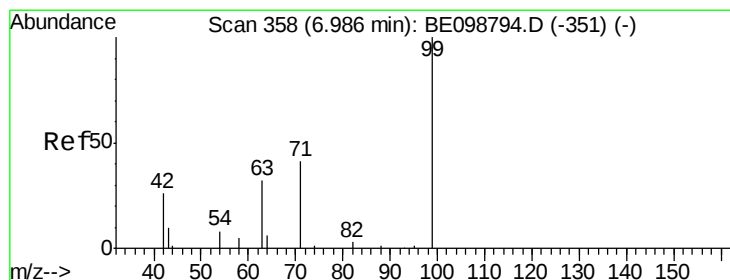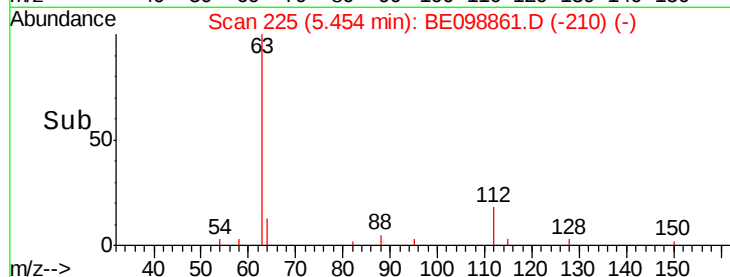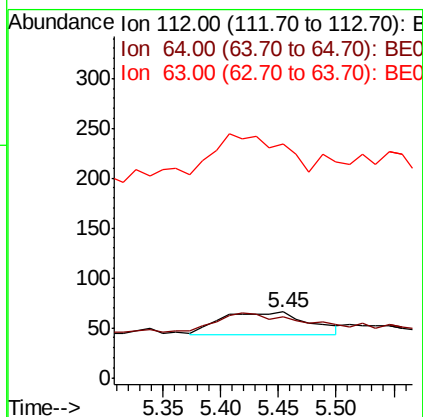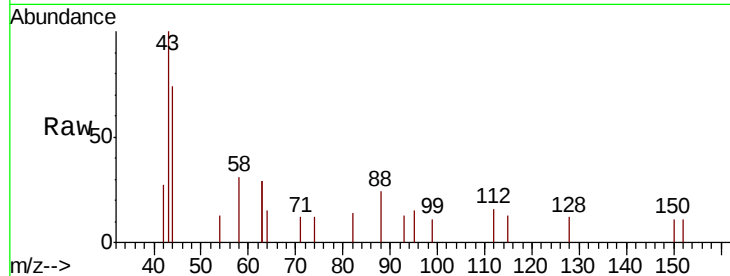

#5

Phenol-d6

Concen: 0.029 ng m




RT: 7.04 min Scan# 363

Delta R.T. 0.06 min

Lab File: BE098861.D

Acq: 11 Mar 2019 13:39

Tgt Ion:	99	Resp:	86
Ion Ratio	Lower	Upper	
99	100		
42	0.0	24.2	36.2#
71	0.0	35.7	53.5#

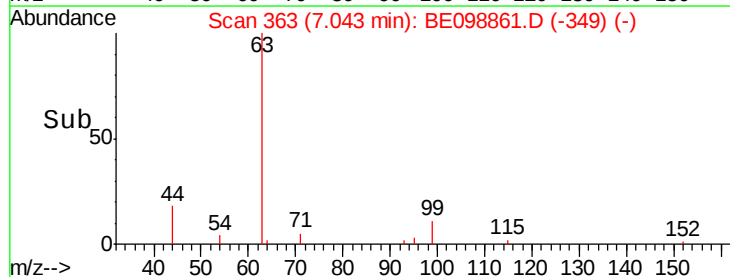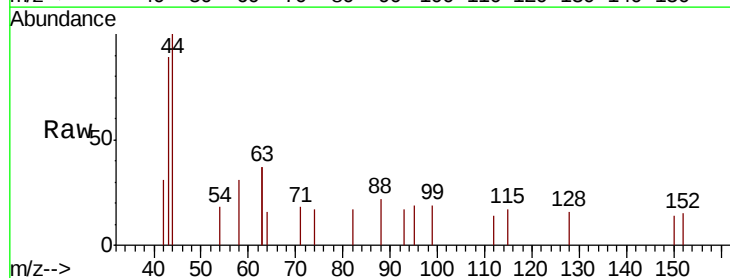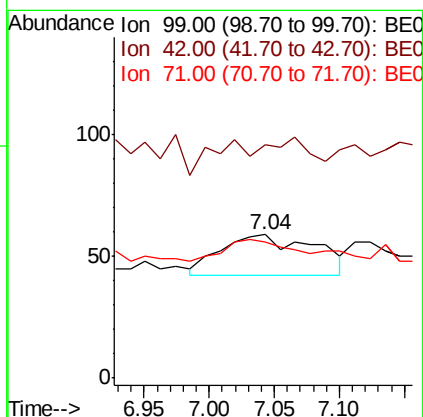



#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.60 min Scan# 650

Delta R.T. 0.01 min

Lab File: BE098861.D

Acq: 11 Mar 2019 13:39

Instrument :

BNA_E


ClientSampleId :

RE108D2-20190306DL

Tot Ion	Ratio	Lower	Upper
136	100		
137	13.7	11.4	17.0
54	57.9	39.3	58.9
68	10.1	6.7	10.1

Manual Integrations
APPROVED

Sohil
3/12/2019 4:33:41 PM

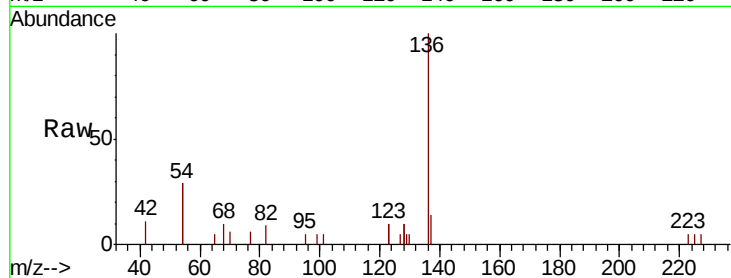




Abundance

Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

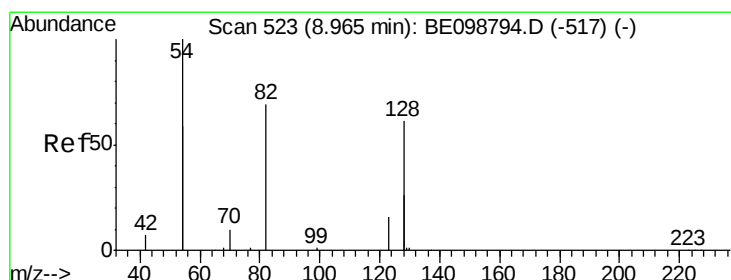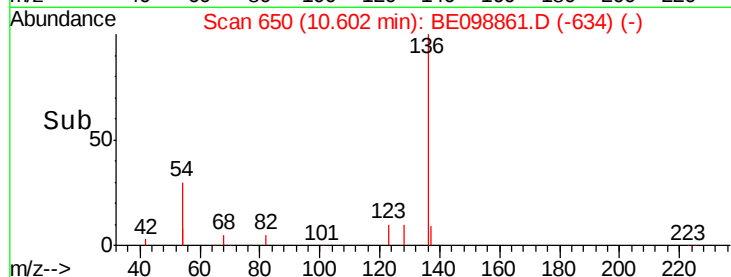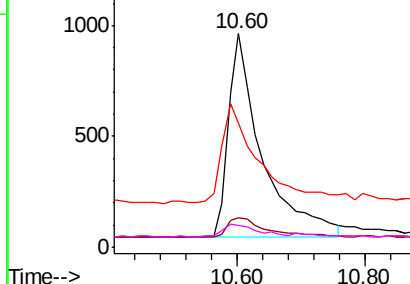

#8

Nitrobenzene-d5

Concen: 0.112 ng


RT: 9.04 min Scan# 530

Delta R.T. 0.08 min

Lab File: BE098861.D

Acq: 11 Mar 2019 13:39

Tgt Ion	Ratio	Lower	Upper
82	100		
128	243.0	123.8	185.8#
54	325.2	203.4	305.2#


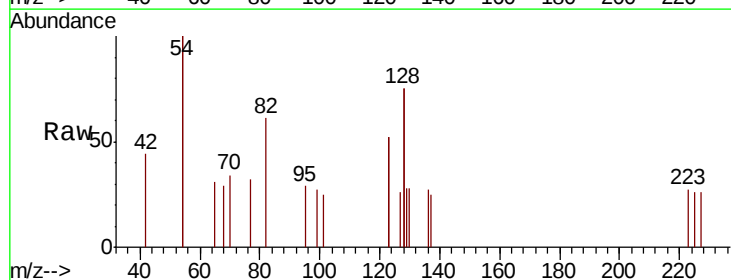


Abundance

Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0

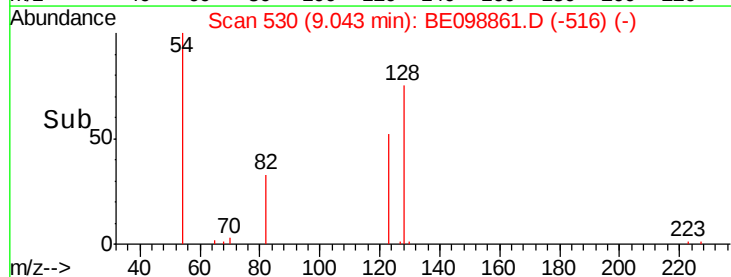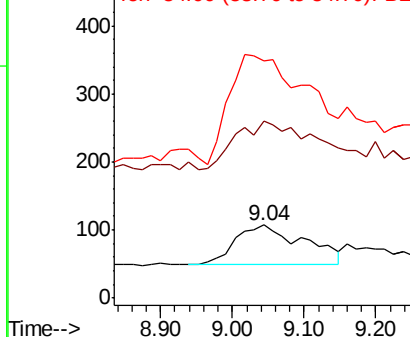







#11
 2-Methylnaphthalene-d10
 Concen: 0.164 ng
 RT: 12.22 min Scan# 765
 Delta R.T. 0.03 min
 Lab File: BE098861.D
 Acq: 11 Mar 2019 13:39

Instrument :
 BNA_E
 ClientSampleId :
 RE108D2-20190306DL

Tot Ion:152 Resp: 1017
 Ion Ratio Lower Upper
 152 100
 151 21.6 16.5 24.7




Manual Integrations
 APPROVED

Sohil
 3/12/2019 4:33:41 PM

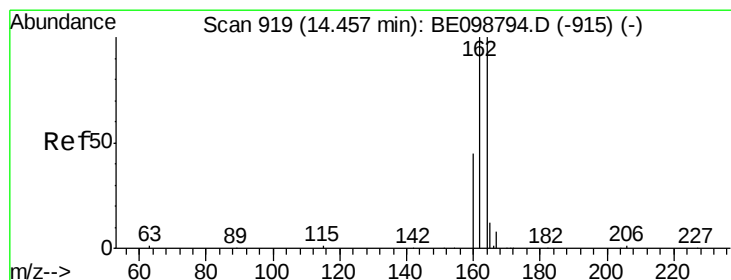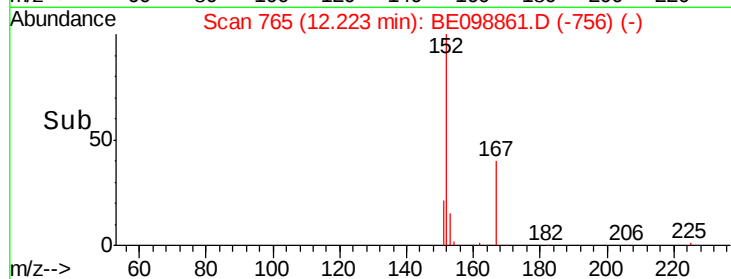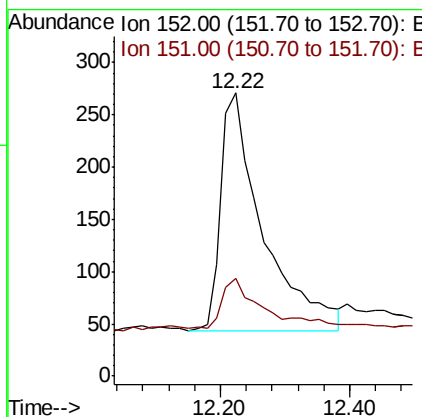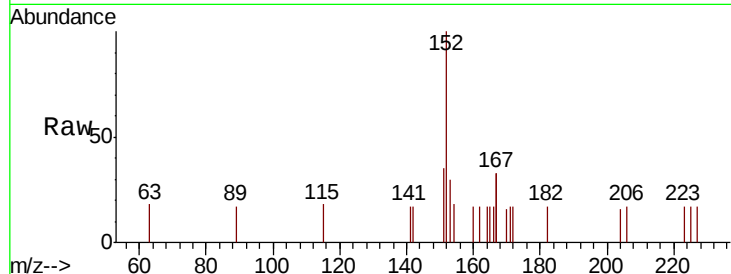

#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.46 min Scan# 920
 Delta R.T. -0.00 min
 Lab File: BE098861.D
 Acq: 11 Mar 2019 13:39

Tgt Ion:164 Resp: 2382
 Ion Ratio Lower Upper
 164 100
 162 104.1 80.2 120.2
 160 52.1 37.8 56.8

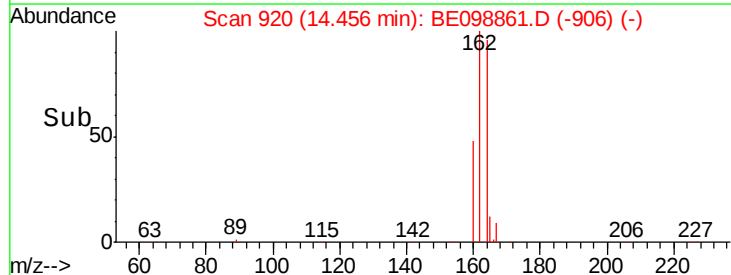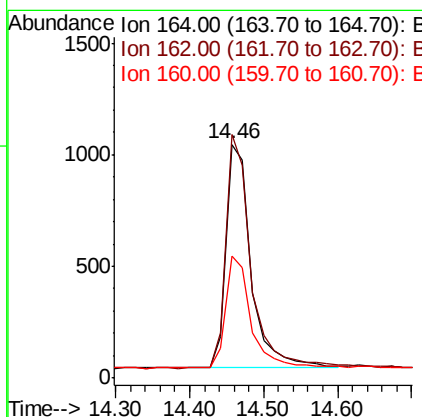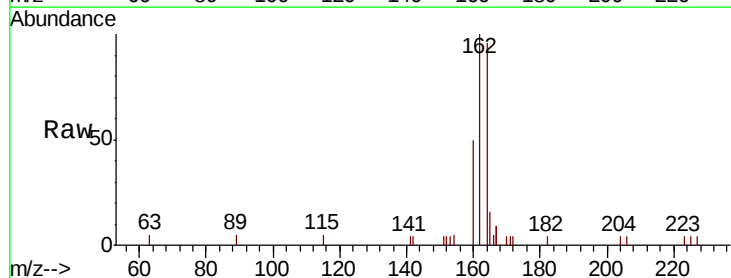




#14
 2,4,6-Tribromophenol
 Concen: 0.158 ng
 RT: 15.98 min Scan# 1028
 Delta R.T. 0.01 min
 Lab File: BE098861.D
 Acq: 11 Mar 2019 13:39

Instrument :
 BNA_E
 ClientSampleID :
 RE108D2-20190306DL




Tot Ion	Ratio	Lower	Upper
330	100		
332	83.2	77.6	116.4
141	44.7	31.0	46.4

Manual Integrations
 APPROVED

Sohil
 3/12/2019 4:33:41 PM

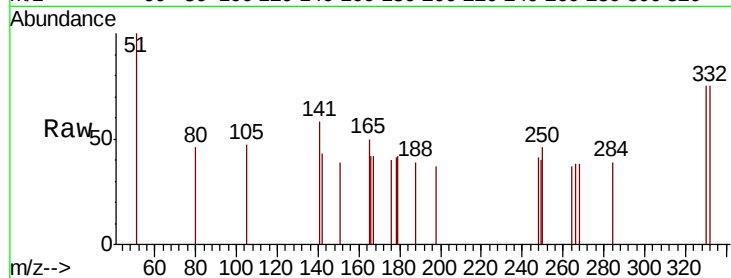


Abundance Ion 330.00 (329.70 to 330.70): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

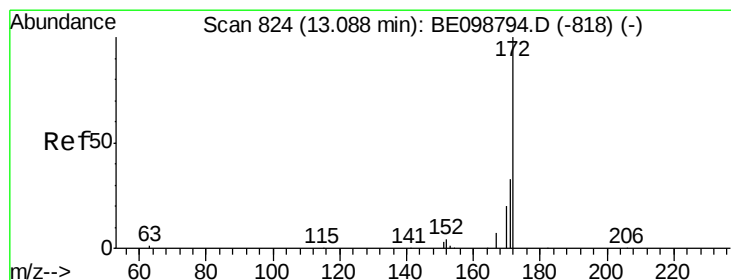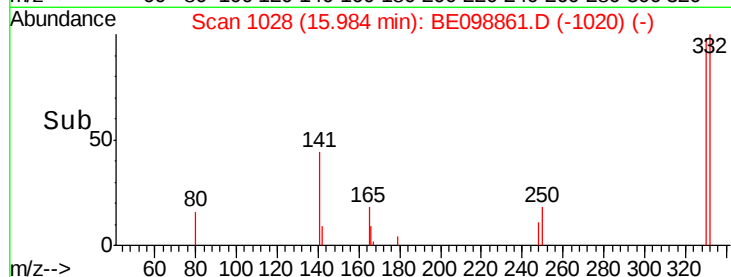
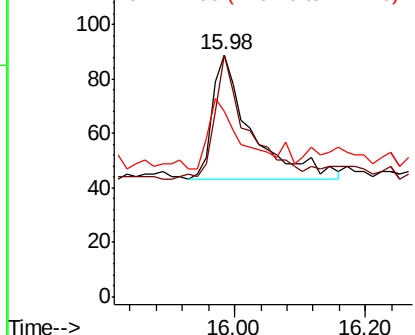


#15
 2-Fluorobiphenyl
 Concen: 0.187 ng
 RT: 13.10 min Scan# 826
 Delta R.T. 0.01 min
 Lab File: BE098861.D
 Acq: 11 Mar 2019 13:39

Tgt Ion	Ratio	Lower	Upper
172	100		
171	38.5	28.0	42.0
170	29.5	17.7	26.5

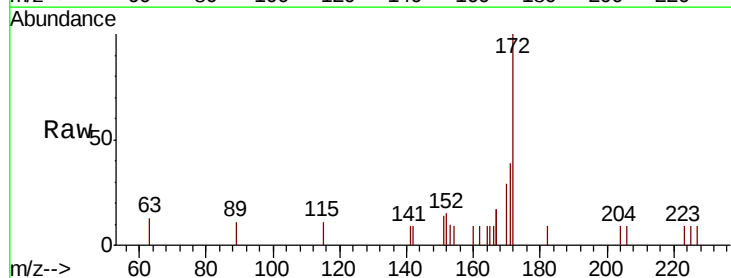

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

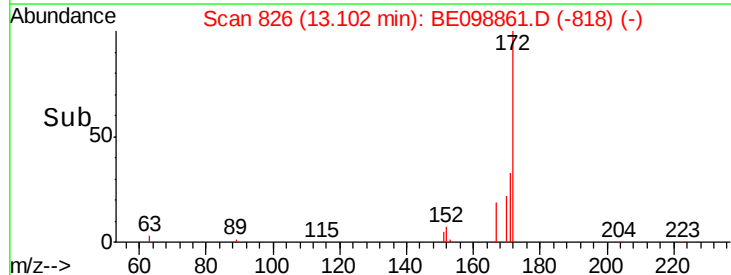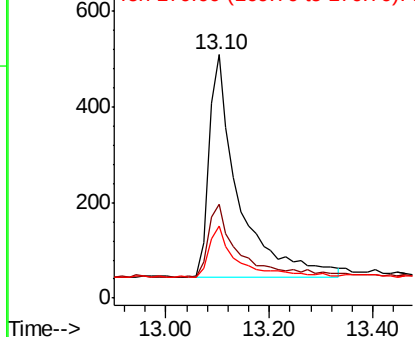







#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.22 min Scan# 1120
Delta R.T. -0.00 min
Lab File: BE098861.D
Acq: 11 Mar 2019 13:39

Instrument :
BNA_E
ClientSampleId :
RE108D2-20190306DL

Tot Ion	Ratio	Resp Lower	Upper
188	100		
94	0.0	0.0	0.0
80	10.3	6.3	9.5




Manual Integrations
APPROVED

Sohil
3/12/2019 4:33:41 PM

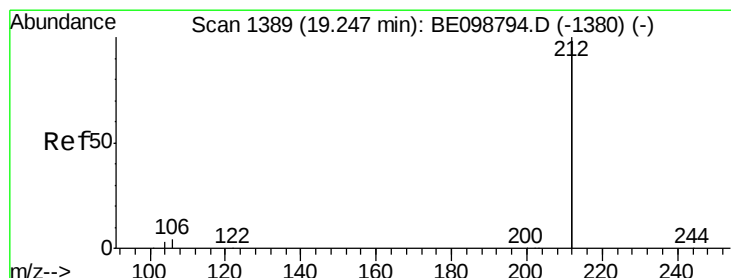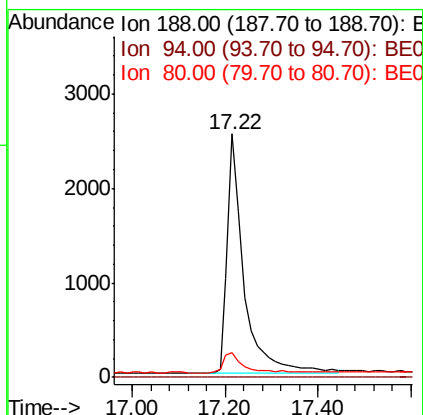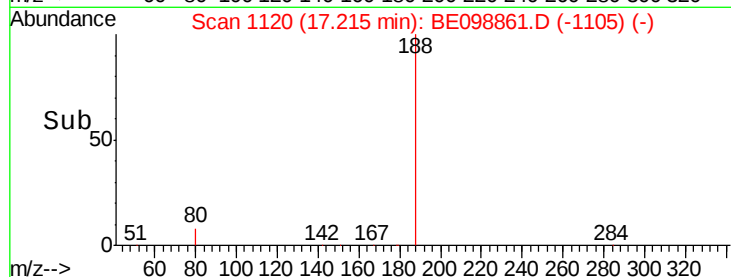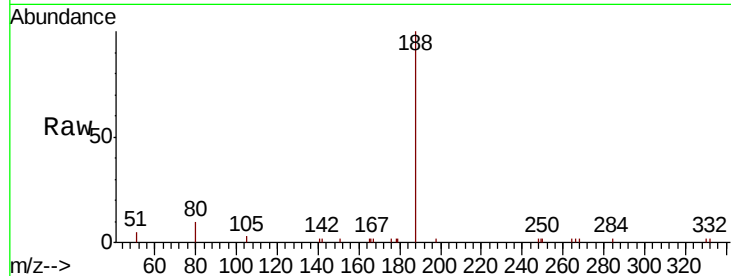

#25
Fluoranthene-d10
Concen: 0.166 ng
RT: 19.25 min Scan# 1390
Delta R.T. 0.00 min
Lab File: BE098861.D
Acq: 11 Mar 2019 13:39

Tgt Ion	Ratio	Resp Lower	Upper
212	100		
106	2.4	1.8	2.8
104	1.5	1.0	1.6

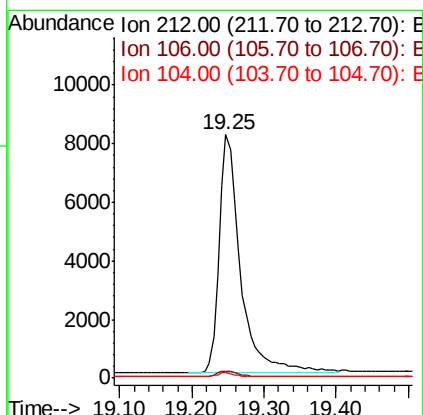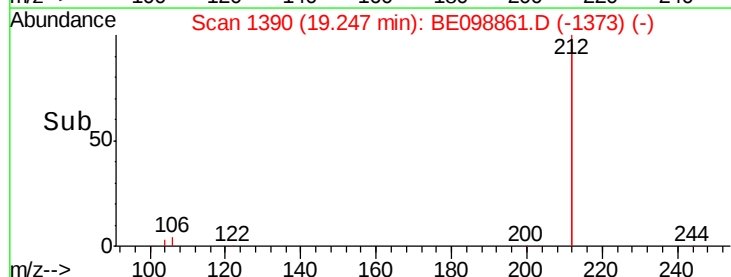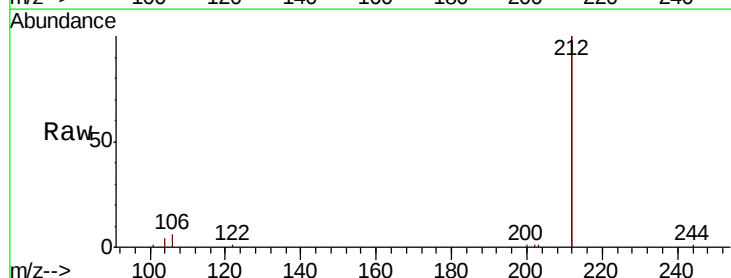







#27
 Chrysene-d12
 Concen: 0.400 ng
 RT: 21.40 min Scan# 1634
 Delta R.T. 0.00 min
 Lab File: BE098861.D
 Acq: 11 Mar 2019 13:39

Instrument :
 BNA_E
 ClientSampleId :
 RE108D2-20190306DL

Tot Ion	Ratio	Lower	Upper
240	100		
120	7.6	5.0	7.4#
236	27.7	22.7	34.1




Manual Integrations
 APPROVED



Sohil
 3/12/2019 4:33:41 PM

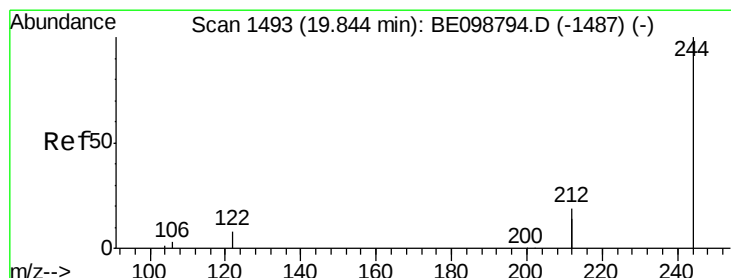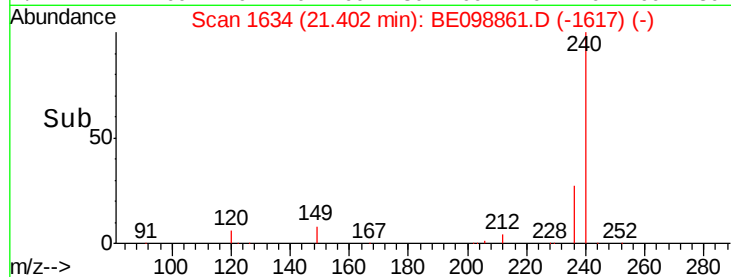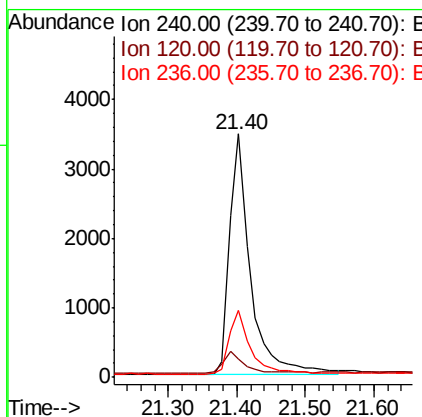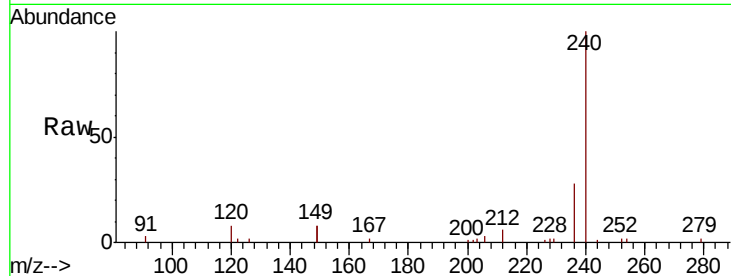

#29
 Terphenyl-d14
 Concen: 0.231 ng
 RT: 19.84 min Scan# 1494
 Delta R.T. 0.00 min
 Lab File: BE098861.D
 Acq: 11 Mar 2019 13:39

Tgt Ion	Ratio	Lower	Upper
244	100		
212	41.4	29.4	44.2
122	9.5	7.1	10.7

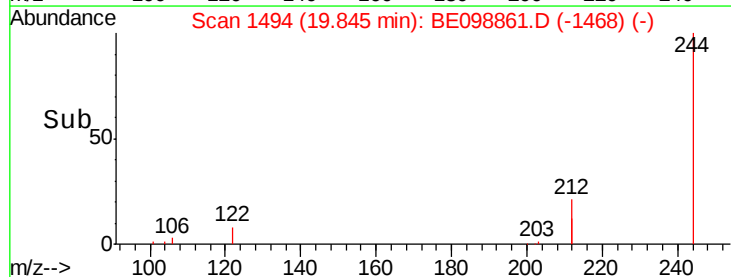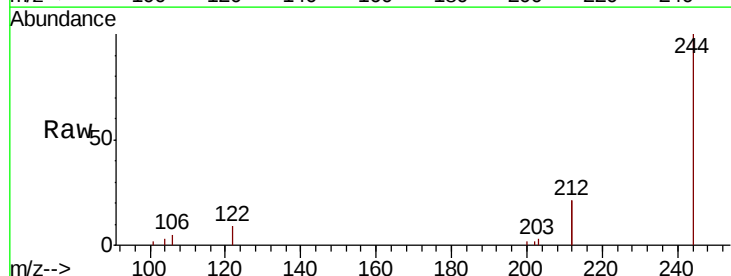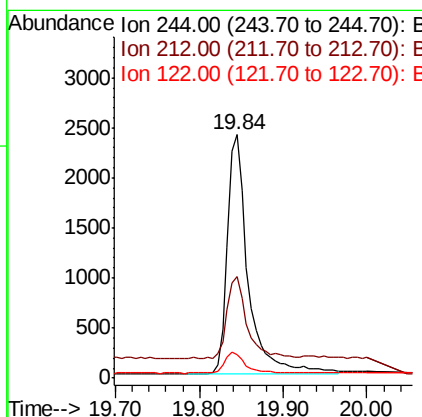

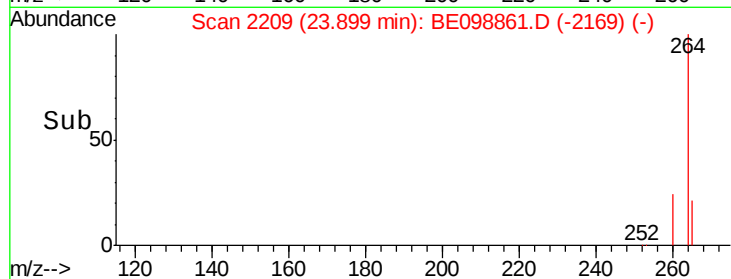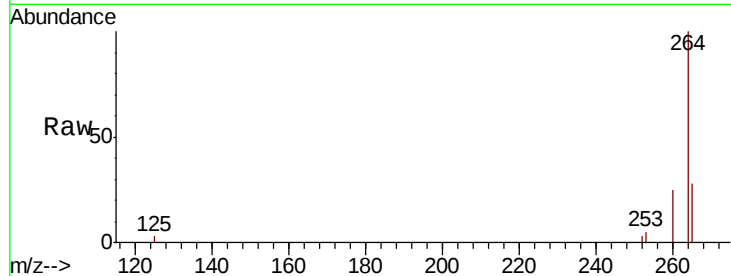

#34
 Pervlene-d12
 Concen: 0.400 ng
 RT: 23.90 min Scan# 2209
 Delta R.T. -0.01 min
 Lab File: BE098861.D
 Acq: 11 Mar 2019 13:39

Tot Ion:	264	Resp:	7083
Ion Ratio	Lower	Upper	
264	100		
260	25.4	21.2	31.8
265	27.6	24.6	36.8

Instrument :
 BNA_E
 ClientSampleId :
 RE108D2-20190306DL

Manual Integrations
 APPROVED

Sohil
 3/12/2019 4:33:41 PM

