

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE031119\
 Data File : BE098866.D
 Acq On : 11 Mar 2019 17:40
 Operator : JU/SJ
 Sample : K1839-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 RE109D2-20190307

Quant Time: Mar 12 07:29:03 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE030619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 06 15:33:24 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	815	0.40	ng	0.00
7) Naphthalene-d8	10.60	136	3247	0.40	ng	0.01
13) Acenaphthene-d10	14.46	164	2146	0.40	ng	0.00
19) Phenanthrene-d10	17.21	188	6123	0.40	ng	0.00
27) Chrysene-d12	21.40	240	6895	0.40	ng	0.00
34) Perylene-d12	23.91	264	4711	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.42	112	220	0.09	ng	0.04
5) Phenol-d6	6.97	99	274	0.08	ng	-0.01
8) Nitrobenzene-d5	9.00	82	796	0.23	ng	0.04
11) 2-Methylnaphthalene-d10	12.21	152	1704	0.28	ng	0.01
14) 2,4,6-Tribromophenol	15.97	330	316	0.29	ng	0.00
15) 2-Fluorobiphenyl	13.09	172	2880	0.32	ng	0.00
25) Fluoranthene-d10	19.25	212	25079	0.26	ng	0.00
29) Terphenyl-d14	19.84	244	6988	0.42	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.28	88	4360	3.371	ng	Qvalue 98
32) Bis(2-ethylhexyl)phthalate	21.29	149	4008	0.088	ng	# 100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE031119\
Data File : BE098866.D
Acq On : 11 Mar 2019 17:40
Operator : JU/SJ
Sample : K1839-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
RE109D2-20190307

Quant Time: Mar 12 07:29:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE030619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 06 15:33:24 2019
Response via : Initial Calibration

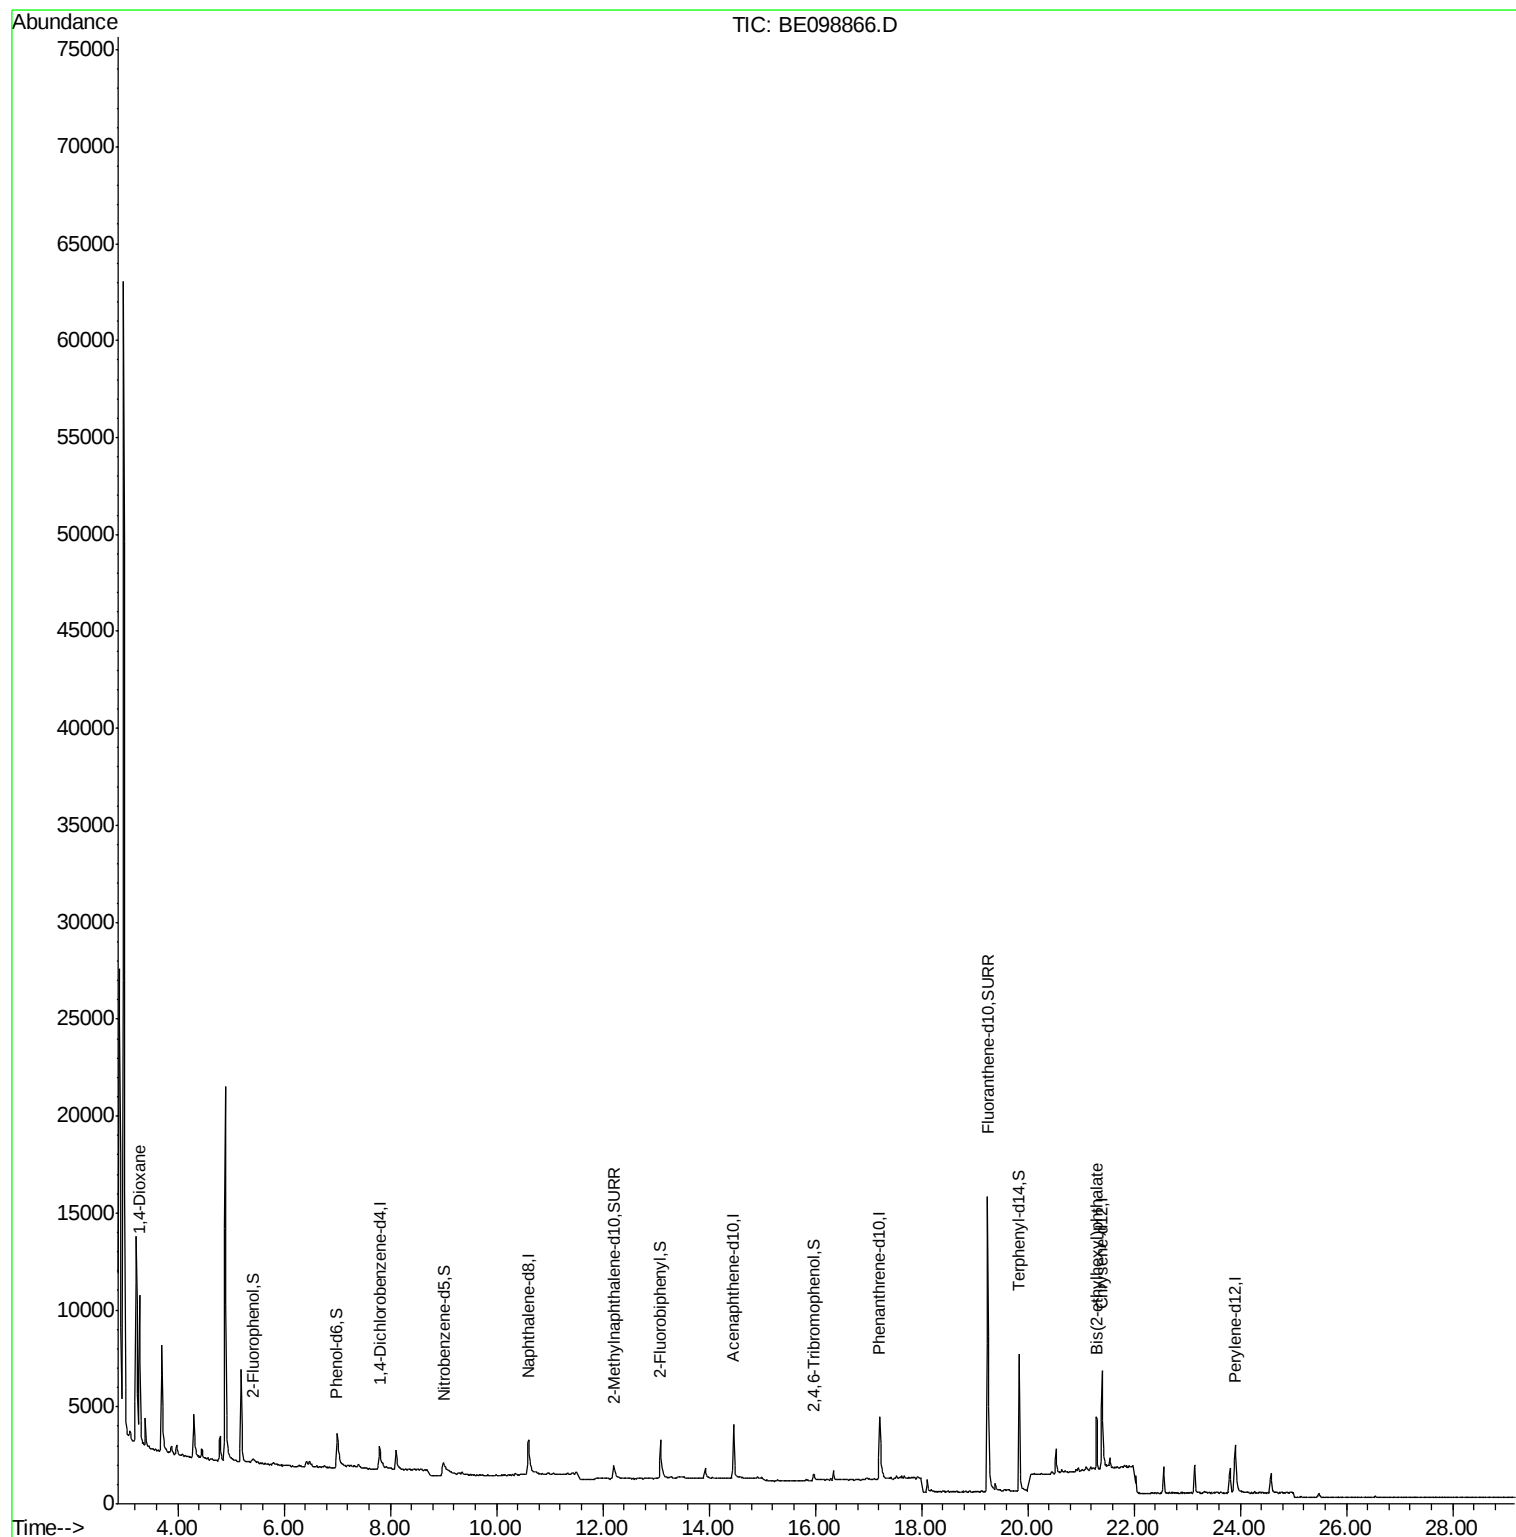




#1



1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.79 min Scan# 428
Delta R.T. 0.00 min
Lab File: BE098866.D
Acq: 11 Mar 2019 17:40

Instrument :
BNA_E
ClientSampleId :
RE109D2-20190307

Tot Ion:152 Resp: 815
Ion Ratio Lower Upper
152 100
150 156.3 122.5 183.7
115 79.1 57.4 86.2

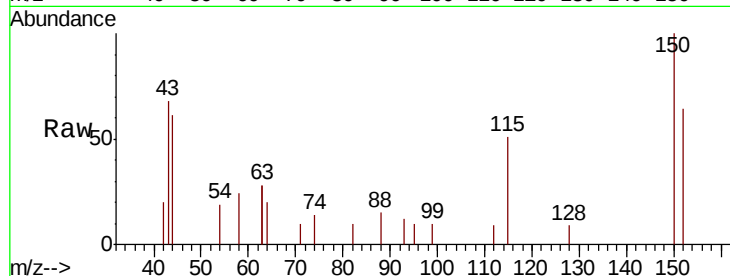


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

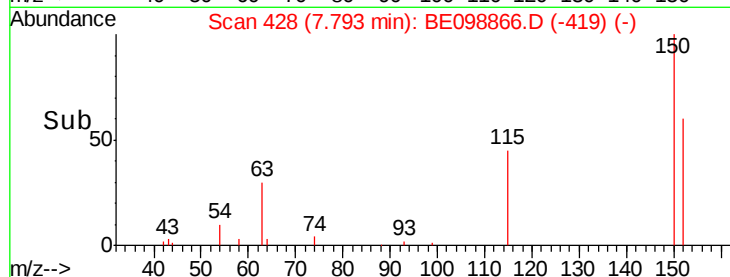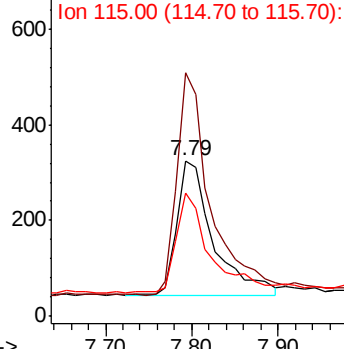



#2

1,4-Dioxane
Concen: 3.371 ng
RT: 3.28 min Scan# 36
Delta R.T. -0.01 min
Lab File: BE098866.D
Acq: 11 Mar 2019 17:40

Tgt Ion: 88 Resp: 4360
Ion Ratio Lower Upper
88 100
58 96.9 75.8 113.6
43 52.9 41.8 62.8

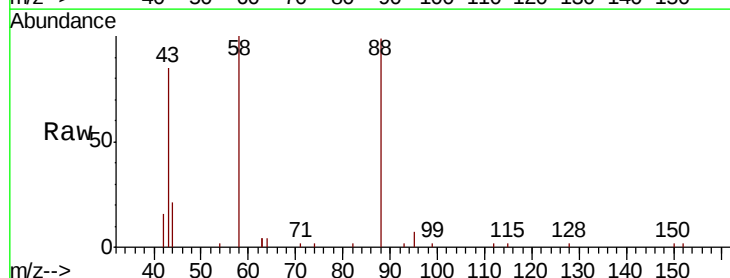

Abundance Ion 88.00 (87.70 to 88.70): BE0
Ion 58.00 (57.70 to 58.70): BE0
Ion 43.00 (42.70 to 43.70): BE0

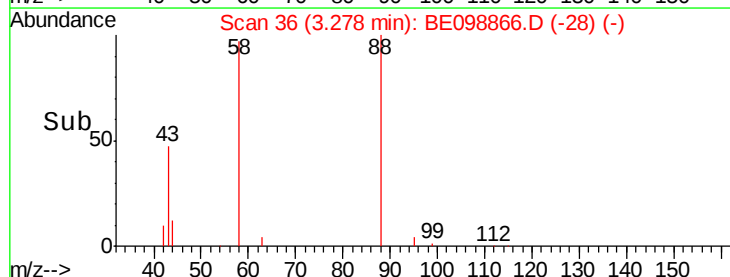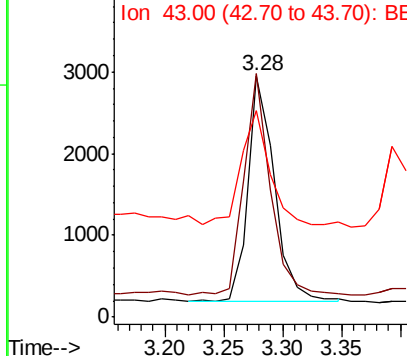



#4

2-Fluorophenol

Concen: 0.090 ng

RT: 5.42 min Scan# 222

Delta R.T. 0.04 min

Lab File: BE098866.D

Acq: 11 Mar 2019 17:40

Instrument :

BNA_E

ClientSampleId :

RE109D2-20190307


Tot Ion:112 Resp: 220

Ion Ratio Lower Upper

112 100

64 0.0 57.9 86.9#



63 160.9 158.3 237.5

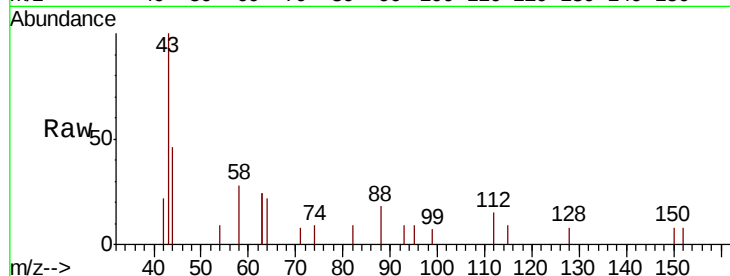

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

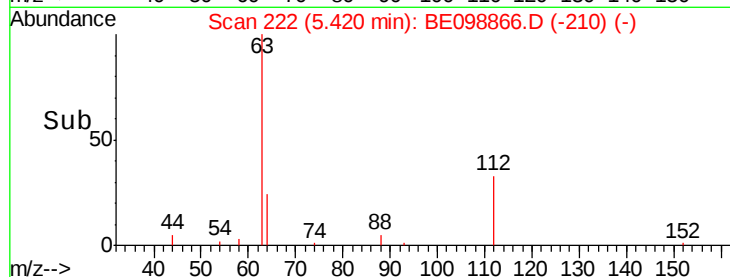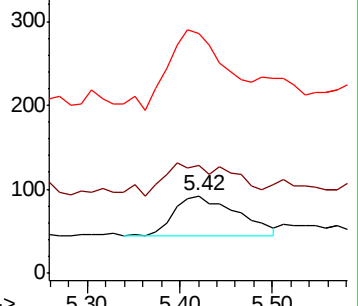

#5

Phenol-d6

Concen: 0.080 ng

RT: 6.97 min Scan# 357

Delta R.T. -0.01 min

Lab File: BE098866.D

Acq: 11 Mar 2019 17:40


Tgt Ion: 99 Resp: 274

Ion Ratio Lower Upper

99 100

42 80.3 24.2 36.2#



71 31.8 35.7 53.5#

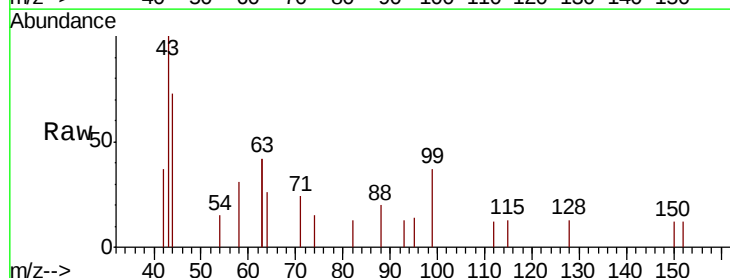

Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

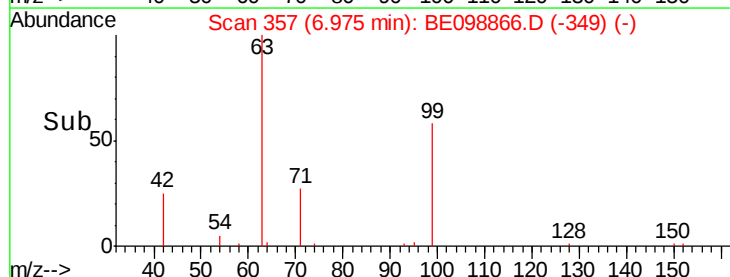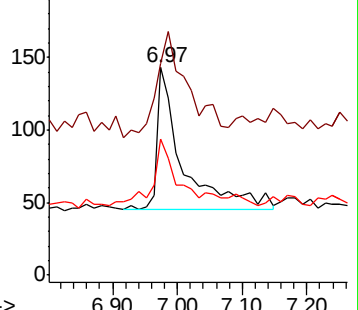



#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.60 min Scan# 649

Delta R.T. 0.01 min

Lab File: BE098866.D

Acq: 11 Mar 2019 17:40

Instrument :

BNA_E

ClientSampleId :

RE109D2-20190307

Tot Ion:136 Resp: 3247


Ion Ratio Lower Upper

136 100

137 16.1 11.4 17.0

54 57.4 39.3 58.9

68 9.7 6.7 10.1


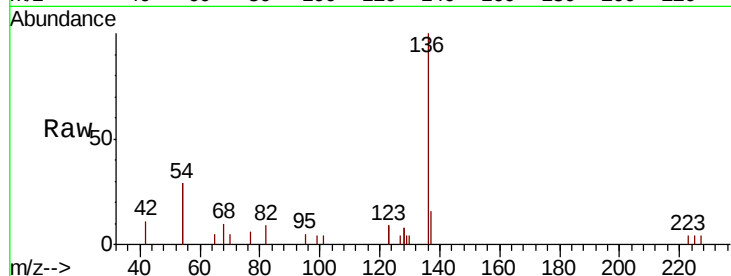


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

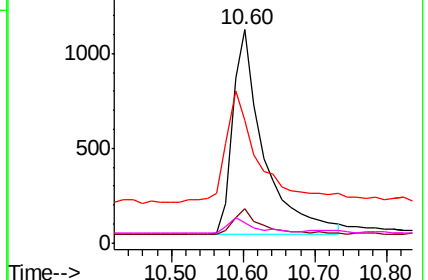

#8

Nitrobenzene-d5

Concen: 0.234 ng

RT: 9.00 min Scan# 526

Delta R.T. 0.04 min

Lab File: BE098866.D

Acq: 11 Mar 2019 17:40


Tgt Ion: 82 Resp: 796

Ion Ratio Lower Upper

82 100

128 187.8 123.8 185.8#



54 309.4 203.4 305.2#

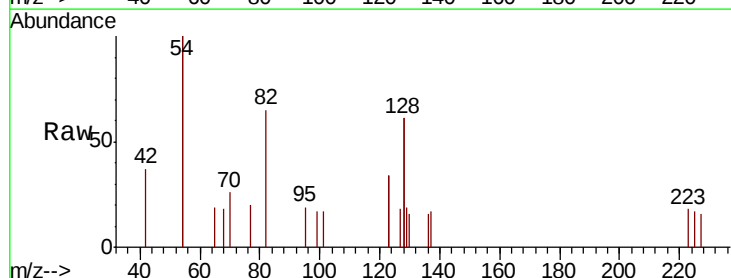

Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0


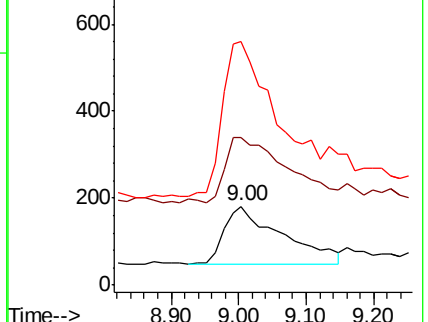





#11
2-Methylnaphthalene-d10
Concen: 0.284 ng
RT: 12.21 min Scan# 763
Delta R.T. 0.01 min
Lab File: BE098866.D
Acq: 11 Mar 2019 17:40




Instrument :
BNA_E
ClientSampleId :
RE109D2-20190307

Tot Ion:152 Resp: 1704
Ion Ratio Lower Upper
152 100
151 22.7 16.5 24.7

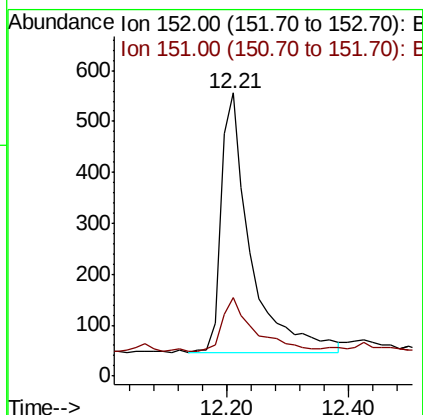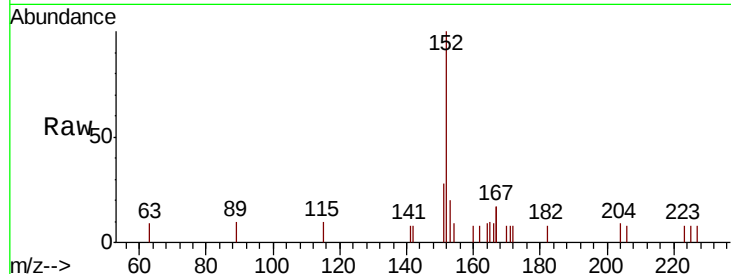

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.46 min Scan# 919
Delta R.T. 0.00 min
Lab File: BE098866.D
Acq: 11 Mar 2019 17:40

Tgt Ion:164 Resp: 2146
Ion Ratio Lower Upper
164 100
162 102.5 80.2 120.2
160 52.1 37.8 56.8

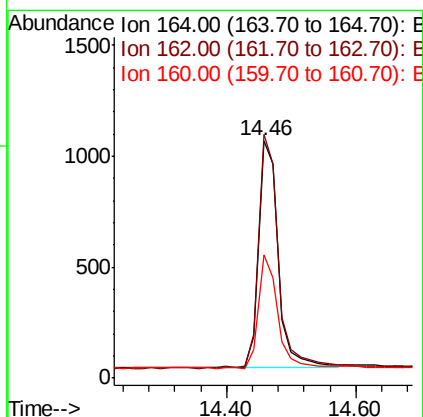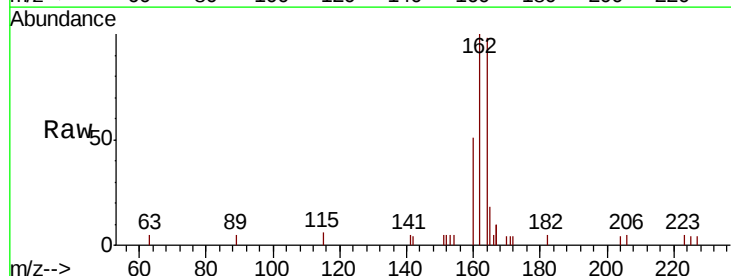







#14
 2,4,6-Tribromophenol
 Concen: 0.292 ng
 RT: 15.97 min Scan# 1026
 Delta R.T. -0.00 min
 Lab File: BE098866.D
 Acq: 11 Mar 2019 17:40

Instrument :
 BNA_E
 ClientSampleId :
 RE109D2-20190307

Tot Ion:330 Resp: 316
 Ion Ratio Lower Upper
 330 100
 332 97.8 77.6 116.4
 141 47.5 31.0 46.4#

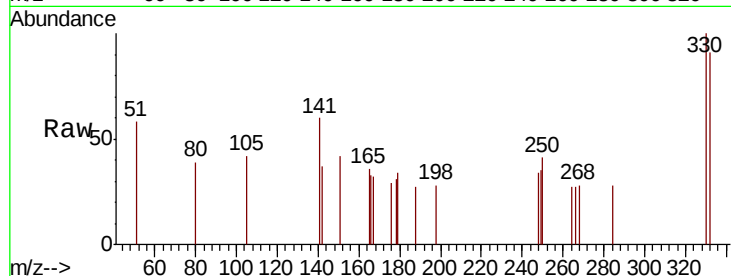


Abundance Ion 330.00 (329.70 to 330.70): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

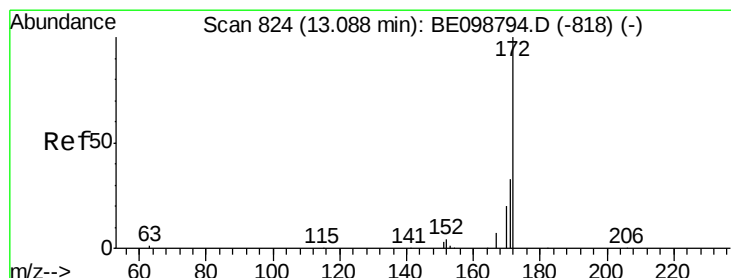
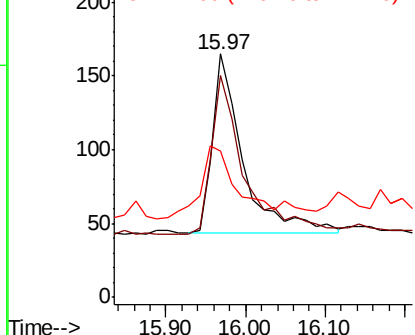


#15
 2-Fluorobiphenyl
 Concen: 0.324 ng
 RT: 13.09 min Scan# 824
 Delta R.T. 0.00 min
 Lab File: BE098866.D
 Acq: 11 Mar 2019 17:40

Tgt Ion:172 Resp: 2880
 Ion Ratio Lower Upper
 172 100
 171 36.9 28.0 42.0
 170 26.8 17.7 26.5#

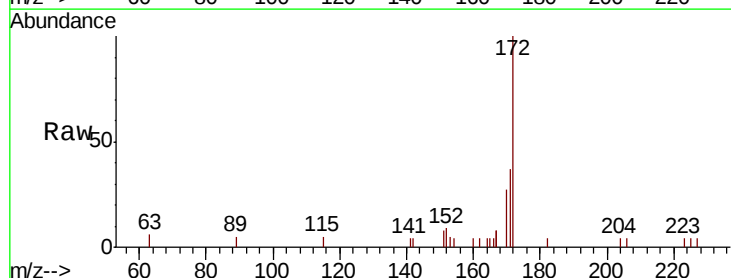

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

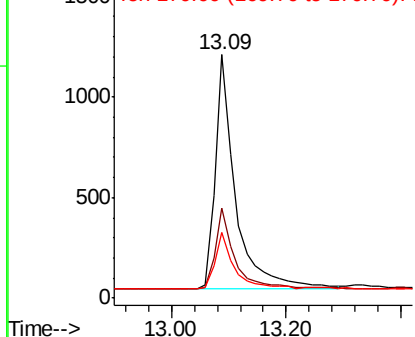



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.21 min Scan# 1119

Delta R.T. -0.00 min

Lab File: BE098866.D

Acq: 11 Mar 2019 17:40

Instrument :

BNA_E

ClientSampleId :

RE109D2-20190307


Tot Ion:188 Resp: 6123

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0




80 11.0 6.3 9.5#

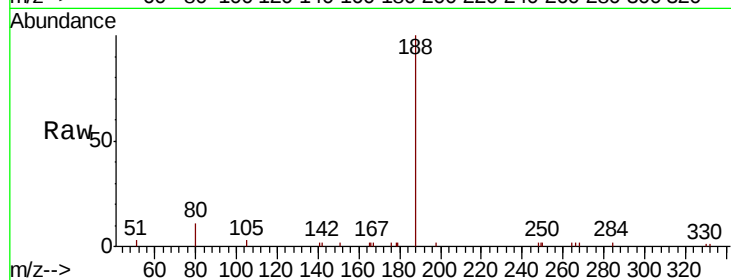

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

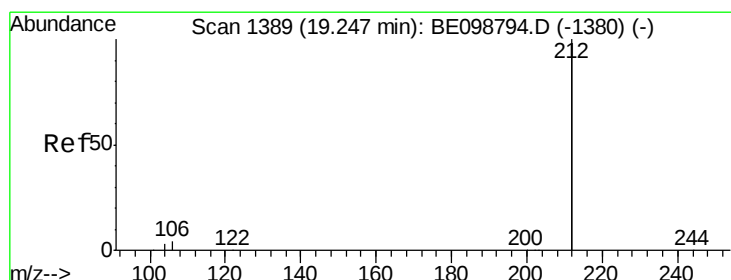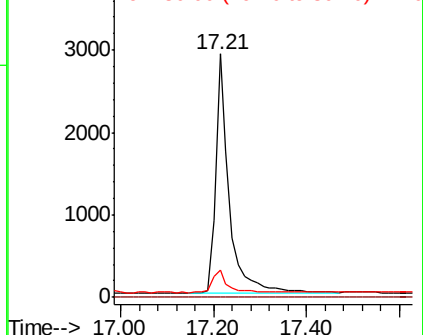

#25

Fluoranthene-d10

Concen: 0.257 ng

RT: 19.25 min Scan# 1389

Delta R.T. 0.00 min

Lab File: BE098866.D

Acq: 11 Mar 2019 17:40


Tgt Ion:212 Resp: 25079

Ion Ratio Lower Upper

212 100

106 2.3 1.8 2.8



104 1.4 1.0 1.6

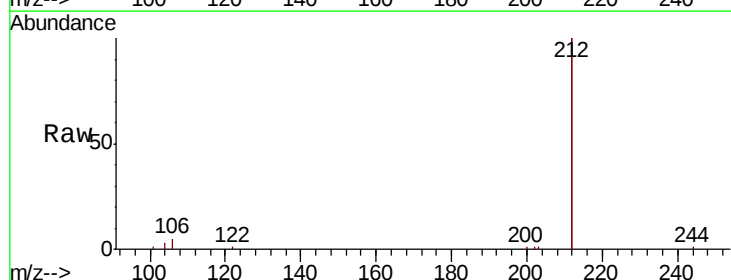

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

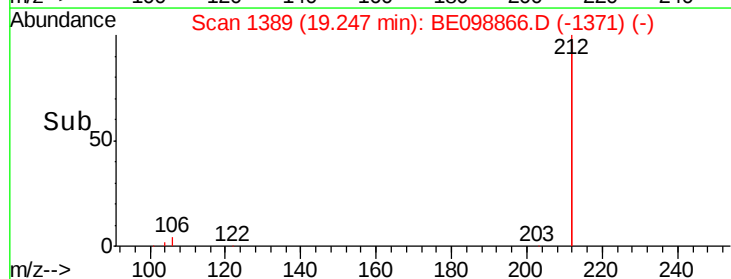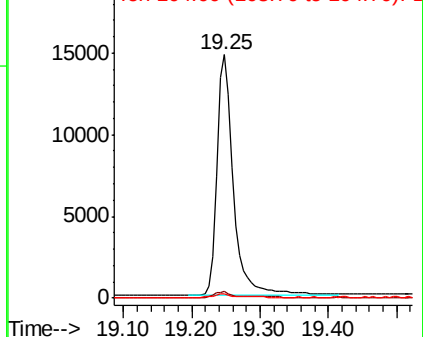







#27
 Chrysene-d12
 Concen: 0.400 ng
 RT: 21.40 min Scan# 1633
 Delta R.T. 0.00 min
 Lab File: BE098866.D
 Acq: 11 Mar 2019 17:40

Instrument :
 BNA_E
 ClientSampleId :
 RE109D2-20190307

Tot Ion:240 Resp: 6895
 Ion Ratio Lower Upper
 240 100
 120 7.5 5.0 7.4#
 236 28.3 22.7 34.1

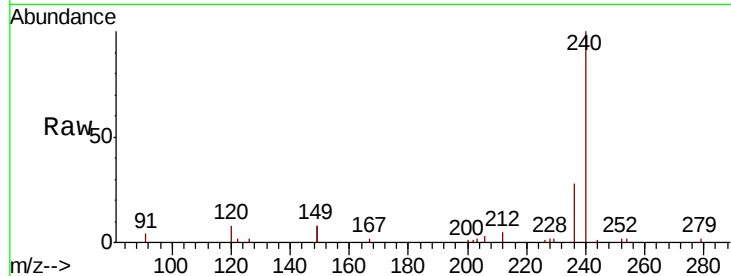


Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

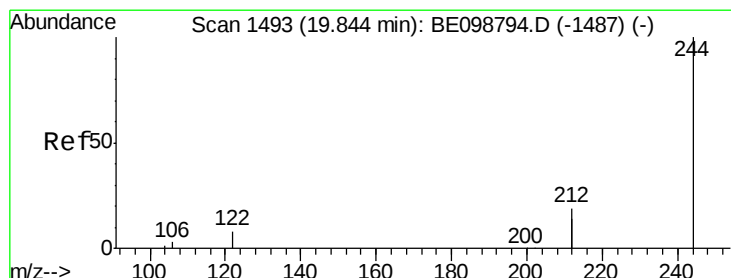
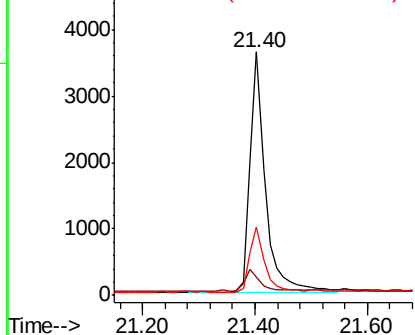


#29
 Terphenyl-d14
 Concen: 0.417 ng
 RT: 19.84 min Scan# 1492
 Delta R.T. -0.01 min
 Lab File: BE098866.D
 Acq: 11 Mar 2019 17:40

Tgt Ion:244 Resp: 6988
 Ion Ratio Lower Upper
 244 100
 212 38.7 29.4 44.2
 122 9.7 7.1 10.7

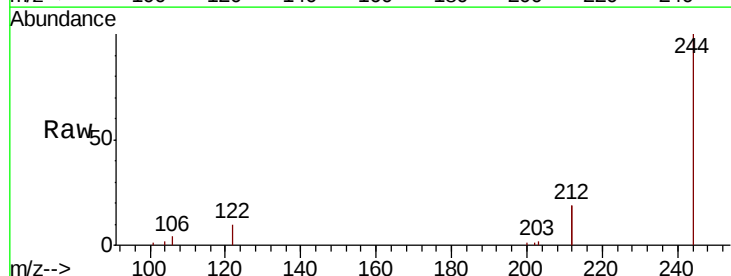

Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

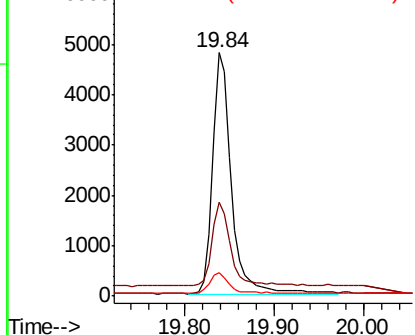



#32

Bis(2-ethylhexyl)phthalate

Concen: 0.088 ng

RT: 21.29 min Scan# 1624

Delta R.T. -0.01 min

Lab File: BE098866.D

Acq: 11 Mar 2019 17:40

Instrument :

BNA_E

ClientSampleId :

RE109D2-20190307


Tot Ion:149 Resp: 4008

Ion Ratio Lower Upper

149 100

167 6.7 5.4 8.0




279 1.9 1.0 1.4#

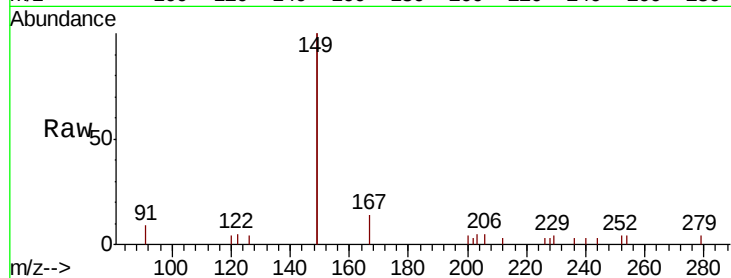

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

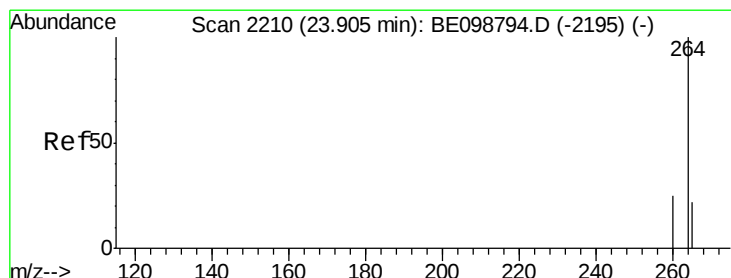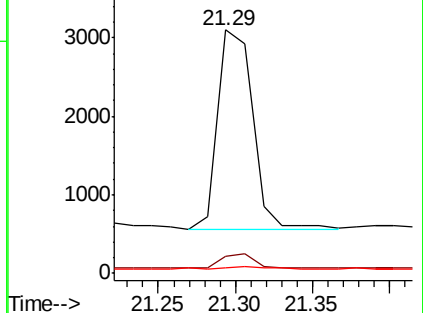

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.91 min Scan# 2210

Delta R.T. -0.00 min

Lab File: BE098866.D

Acq: 11 Mar 2019 17:40


Tgt Ion:264 Resp: 4711

Ion Ratio Lower Upper

264 100

260 25.7 21.2 31.8

265 31.1 24.6 36.8

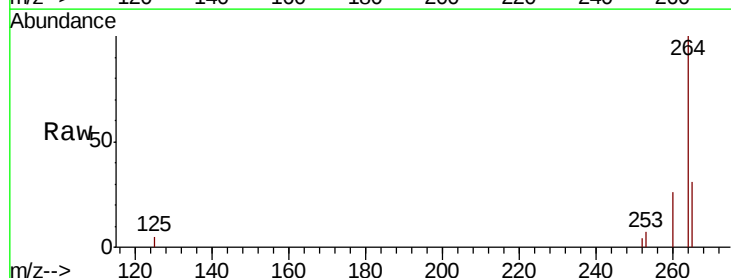

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

