


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE031119\
Data File : BE098856.D
Acq On : 11 Mar 2019 10:33
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE030619.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Mar 06 15:33:24 2019

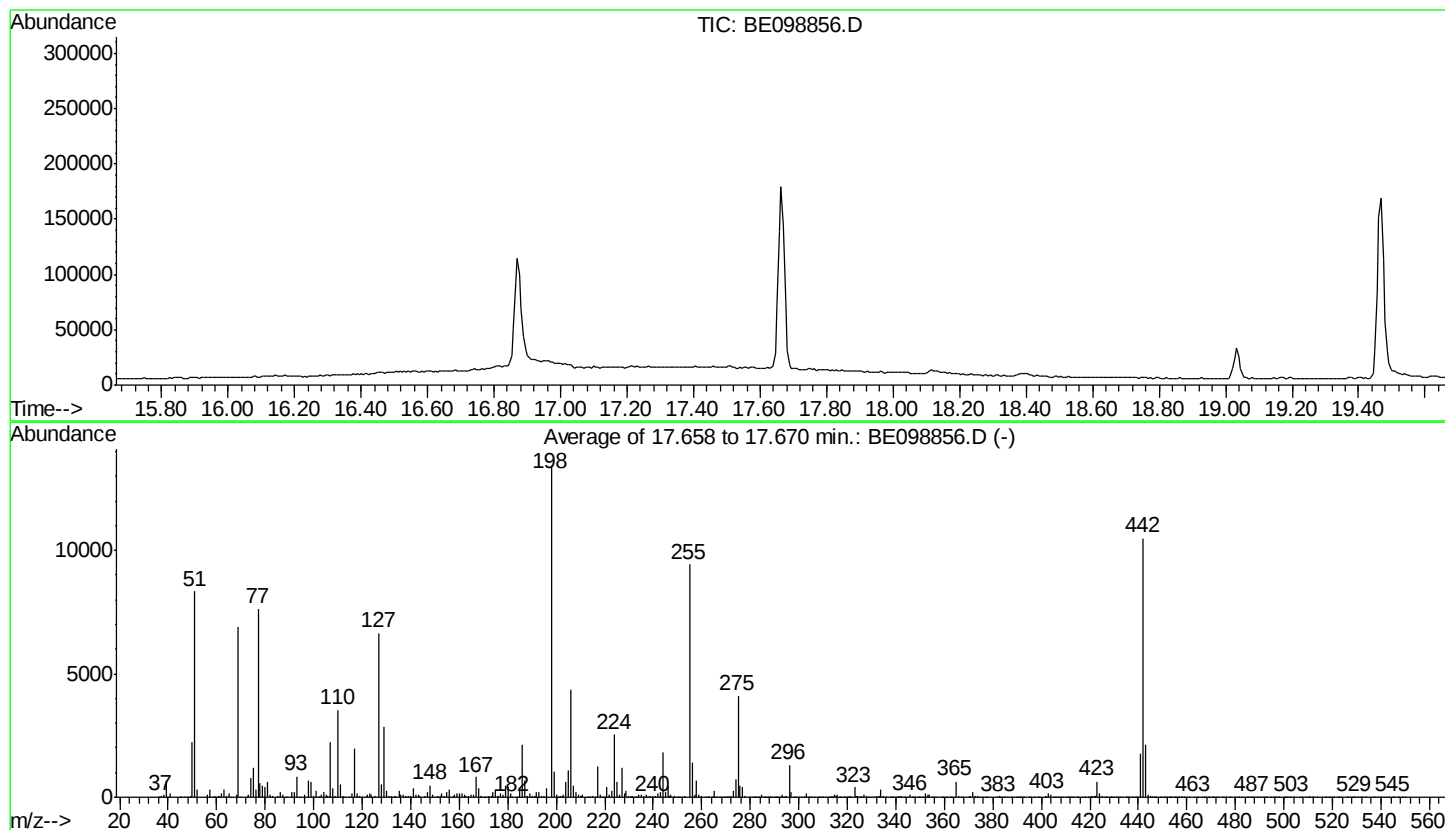

AutoFind: Scans 2565, 2566, 2567; Background Corrected with Scan 2559

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	62.1	8335	PASS
68	69	0.00	2	1.4	100	PASS
69	198	0.00	100	51.5	6923	PASS
70	69	0.00	2	0.2	15	PASS
127	198	10	80	49.6	6660	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	13430	PASS
199	198	5	9	7.7	1039	PASS
275	198	10	60	30.6	4105	PASS
365	198	1	100	4.8	643	PASS
441	198	0.01	100	13.3	1787	PASS
442	198	50	100	78.2	10497	PASS
443	442	15	24	20.2	2117	PASS