


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE031119\
 Data File : BE098873.D
 Acq On : 11 Mar 2019 23:15
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE030619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 06 15:33:24 2019

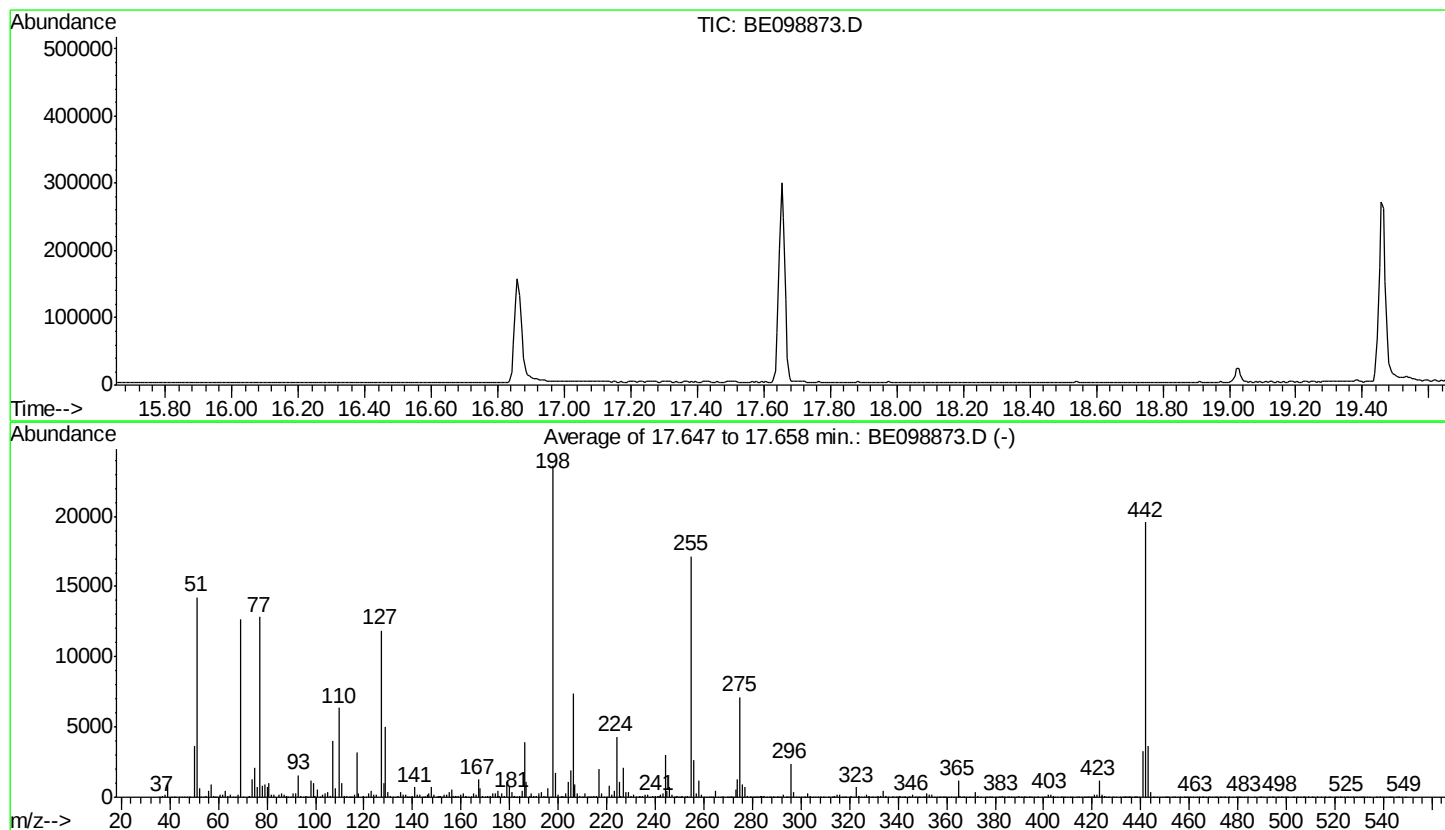

AutoFind: Scans 2563, 2564, 2565; Background Corrected with Scan 2555

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.4	14262	PASS
68	69	0.00	2	1.4	181	PASS
69	198	0.00	100	53.5	12631	PASS
70	69	0.00	2	0.4	46	PASS
127	198	10	80	50.3	11871	PASS
197	198	0.00	2	0.2	44	PASS
198	198	100	100	100.0	23613	PASS
199	198	5	9	7.5	1776	PASS
275	198	10	60	30.3	7153	PASS
365	198	1	100	5.0	1169	PASS
441	198	0.01	100	13.8	3252	PASS
442	198	50	100	82.9	19583	PASS
443	442	15	24	18.6	3638	PASS