
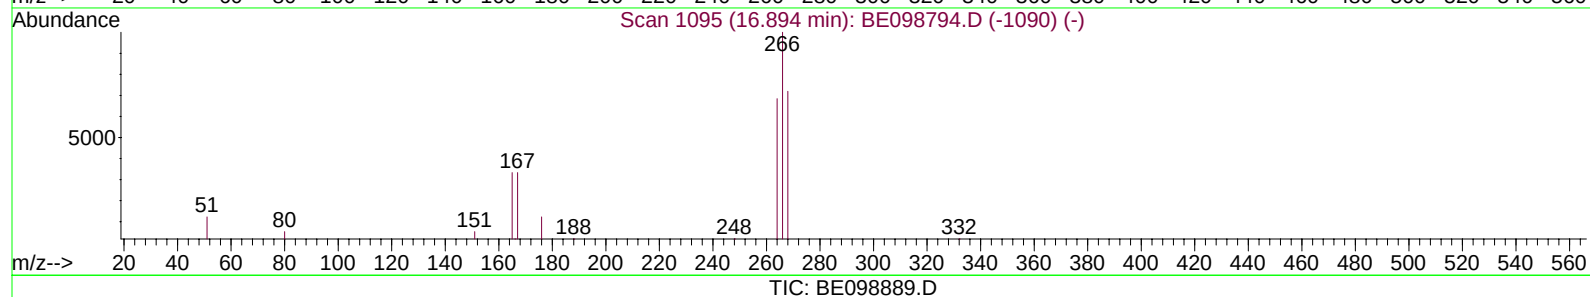
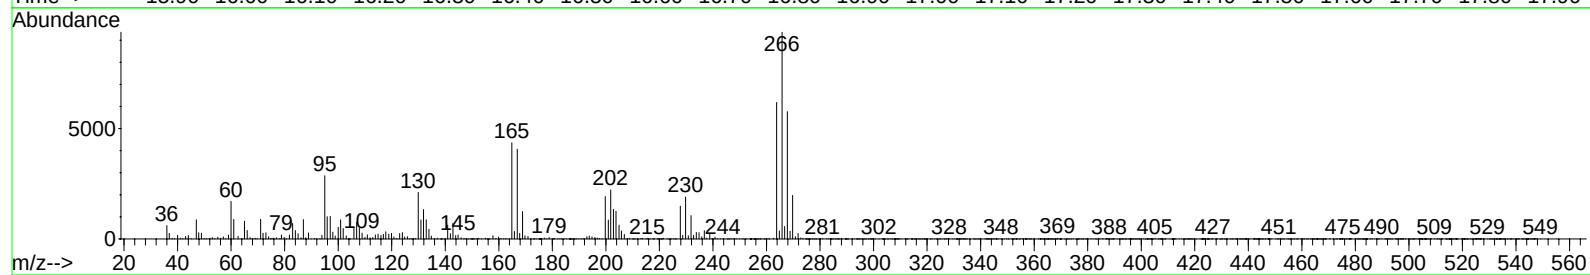


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE031219\
 Data File : BE098889.D
 Acq On : 12 Mar 2019 9:36
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 12 19:13:01 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE030619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 06 15:33:24 2019
 Response via : Initial Calibration

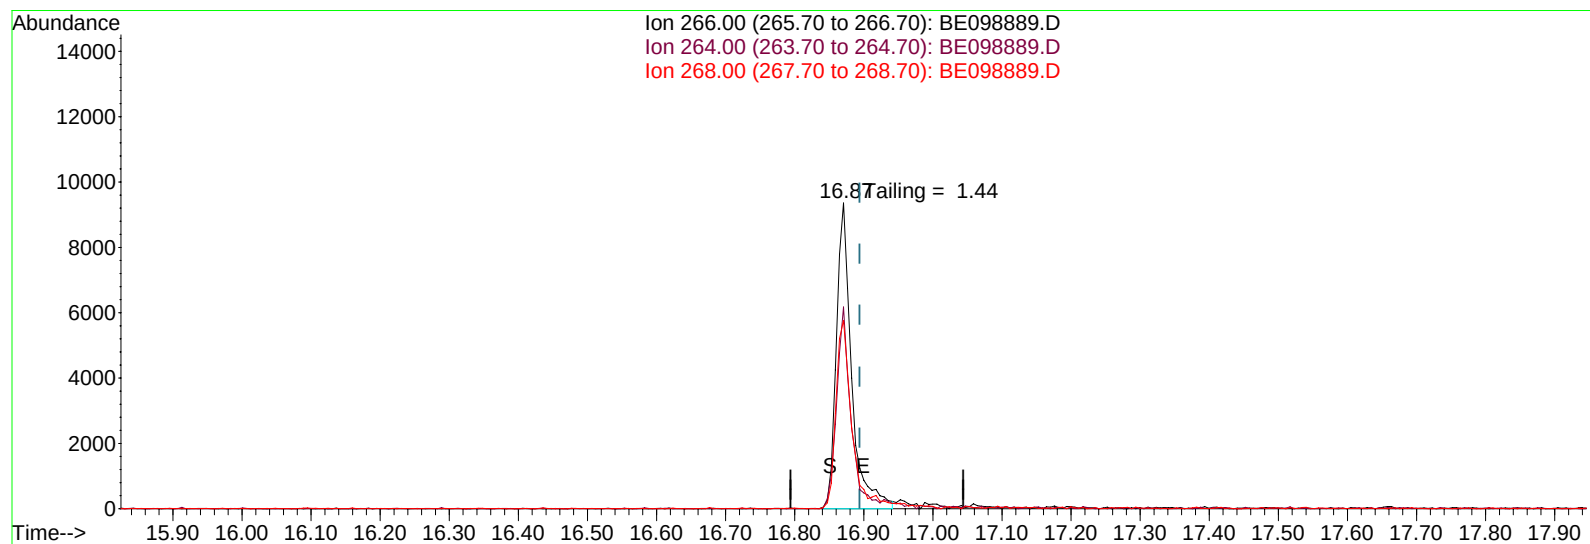

(22) Pentachlorophenol

16.871min (-0.023) 2196.31ng

response 14456

Ion	Exp%	Act%
266.00	100	100
264.00	83.30	66.00#
268.00	87.30	61.59#
0.00	0.00	0.00