


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE031219\
Data File : BE098889.D
Acq On : 12 Mar 2019 9:36
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE030619.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Mar 06 15:33:24 2019

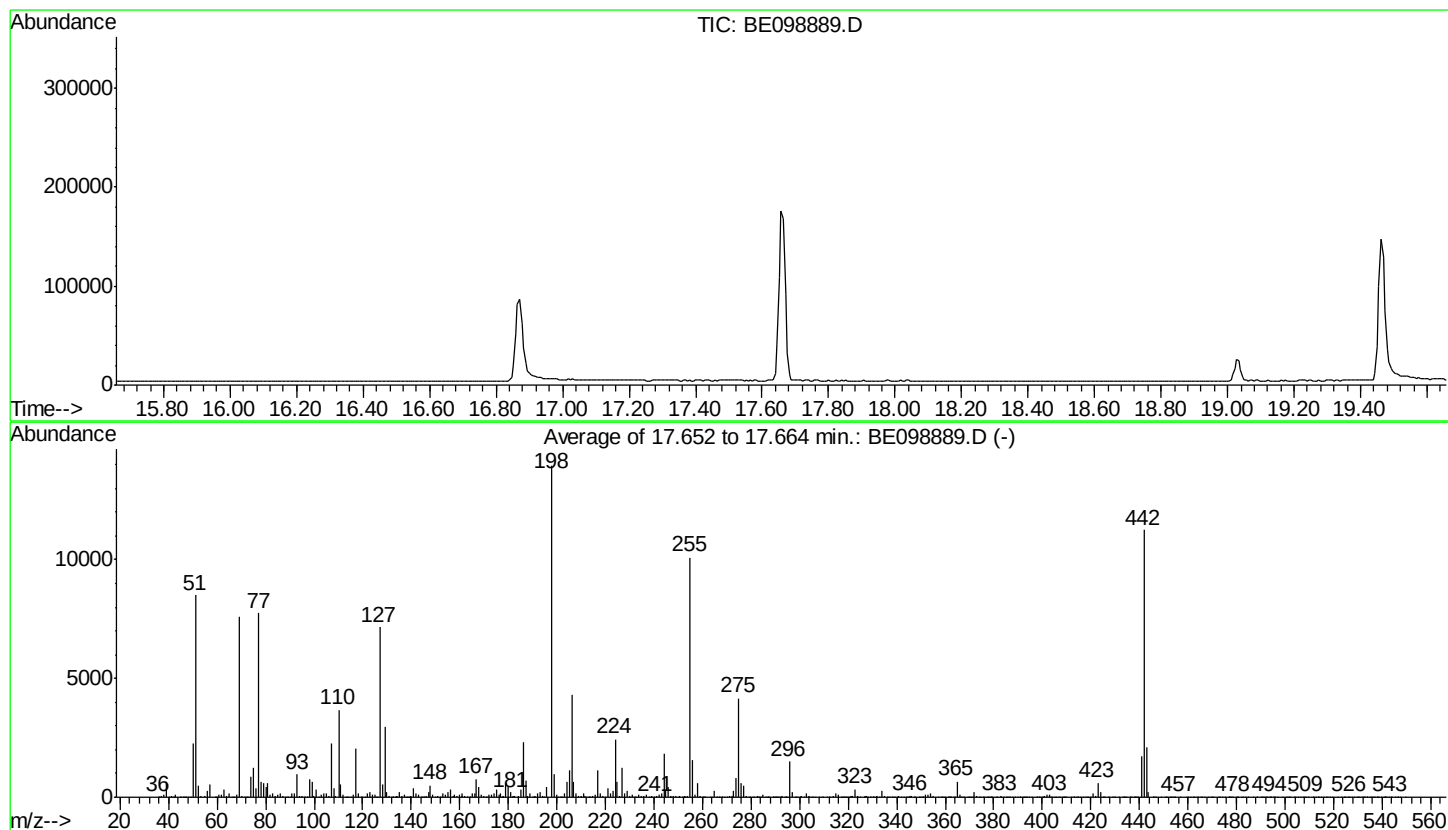

AutoFind: Scans 2564, 2565, 2566; Background Corrected with Scan 2557

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.8	8492	PASS
68	69	0.00	2	1.7	130	PASS
69	198	0.00	100	54.5	7604	PASS
70	69	0.00	2	0.5	35	PASS
127	198	10	80	51.3	7165	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	13959	PASS
199	198	5	9	6.8	945	PASS
275	198	10	60	29.9	4168	PASS
365	198	1	100	4.7	659	PASS
441	198	0.01	100	12.5	1743	PASS
442	198	50	100	80.6	11245	PASS
443	442	15	24	18.5	2079	PASS