
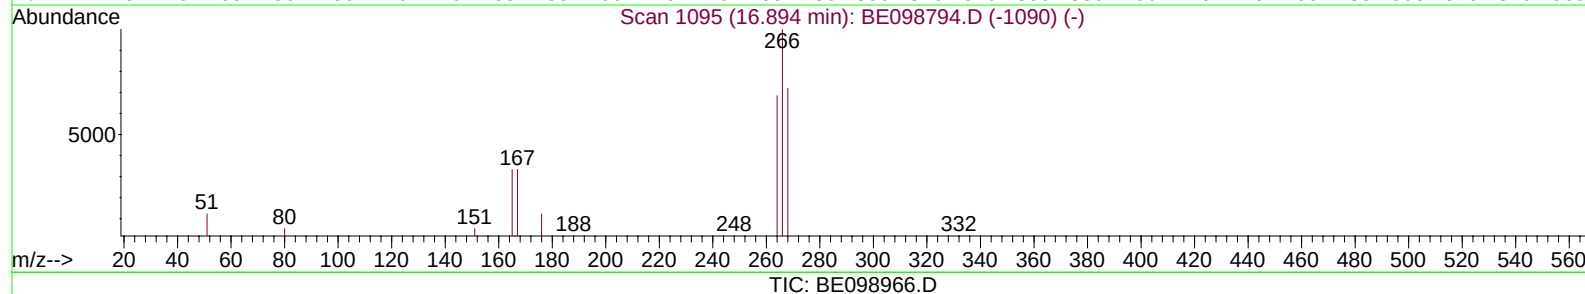
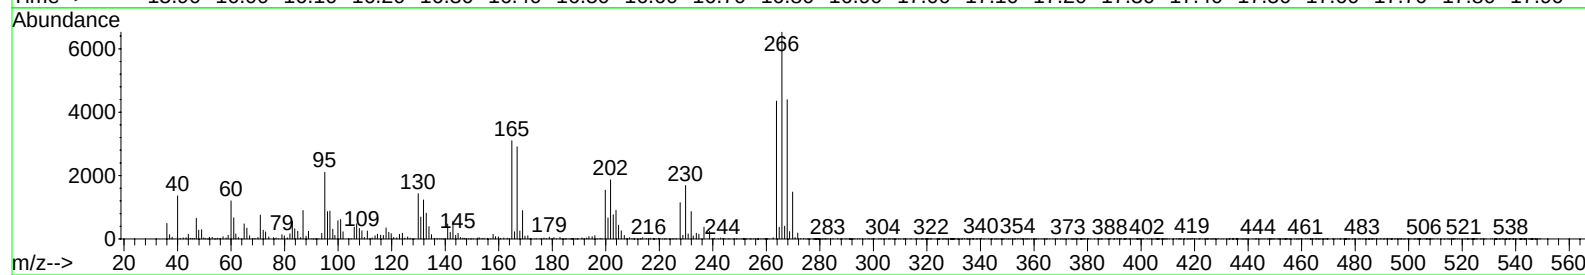


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE031519\
 Data File : BE098966.D
 Acq On : 15 Mar 2019 9:37
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 15 18:48:44 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE030619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 15 05:31:33 2019
 Response via : Initial Calibration

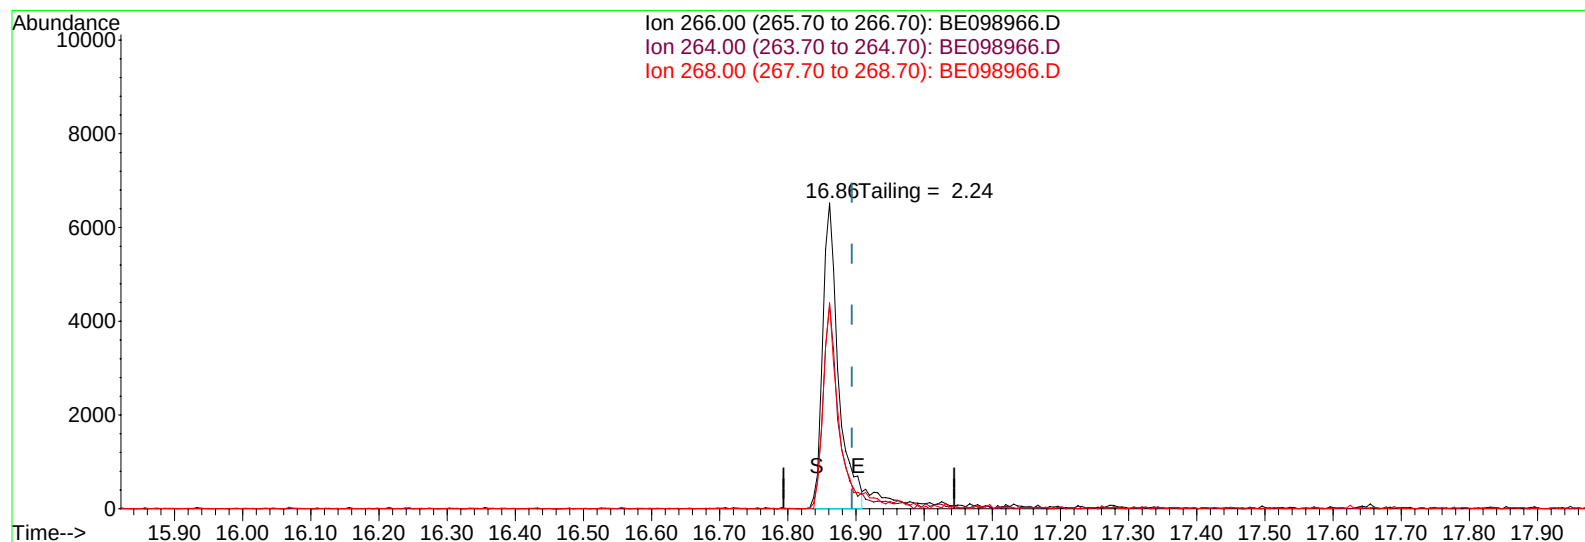

(22) Pentachlorophenol

16.861min (-0.033) 4744.91ng

response 11452

Ion	Exp%	Act%
266.00	100	100
264.00	83.30	66.69
268.00	87.30	70.89
0.00	0.00	0.00