

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE031519\
 Data File : BE098980.D
 Acq On : 15 Mar 2019 20:27
 Operator : JU/SJ
 Sample : K1912-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 M3-T3-OZ(POST)

Quant Time: Mar 16 01:09:58 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE030619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 15 05:31:33 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	904	0.40	ng	0.00
7) Naphthalene-d8	10.60	136	3622	0.40	ng	0.01
13) Acenaphthene-d10	14.46	164	2632	0.40	ng	0.00
19) Phenanthrene-d10	17.21	188	5939	0.40	ng	0.00
27) Chrysene-d12	21.40	240	7302	0.40	ng	0.00
34) Perylene-d12	23.91	264	6753	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.41	112	498	0.18	ng	0.03
5) Phenol-d6	7.00	99	330	0.09	ng	0.01
8) Nitrobenzene-d5	8.99	82	1400	0.37	ng	0.03
11) 2-Methylnaphthalene-d10	12.21	152	2623	0.39	ng	0.02
14) 2,4,6-Tribromophenol	15.97	330	386	0.29	ng	0.00
15) 2-Fluorobiphenyl	13.09	172	4493	0.41	ng	0.00
25) Fluoranthene-d10	19.25	212	38060	0.40	ng	0.00
29) Terphenyl-d14	19.84	244	7507	0.42	ng	0.00
Target Compounds						
32) Bis(2-ethylhexyl)phthalate	21.29	149	5851	0.121	ng	Qvalue # 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE031519\
Data File : BE098980.D
Acq On : 15 Mar 2019 20:27
Operator : JU/SJ
Sample : K1912-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
M3-T3-OZ(POST)

Quant Time: Mar 16 01:09:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE030619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 15 05:31:33 2019
Response via : Initial Calibration

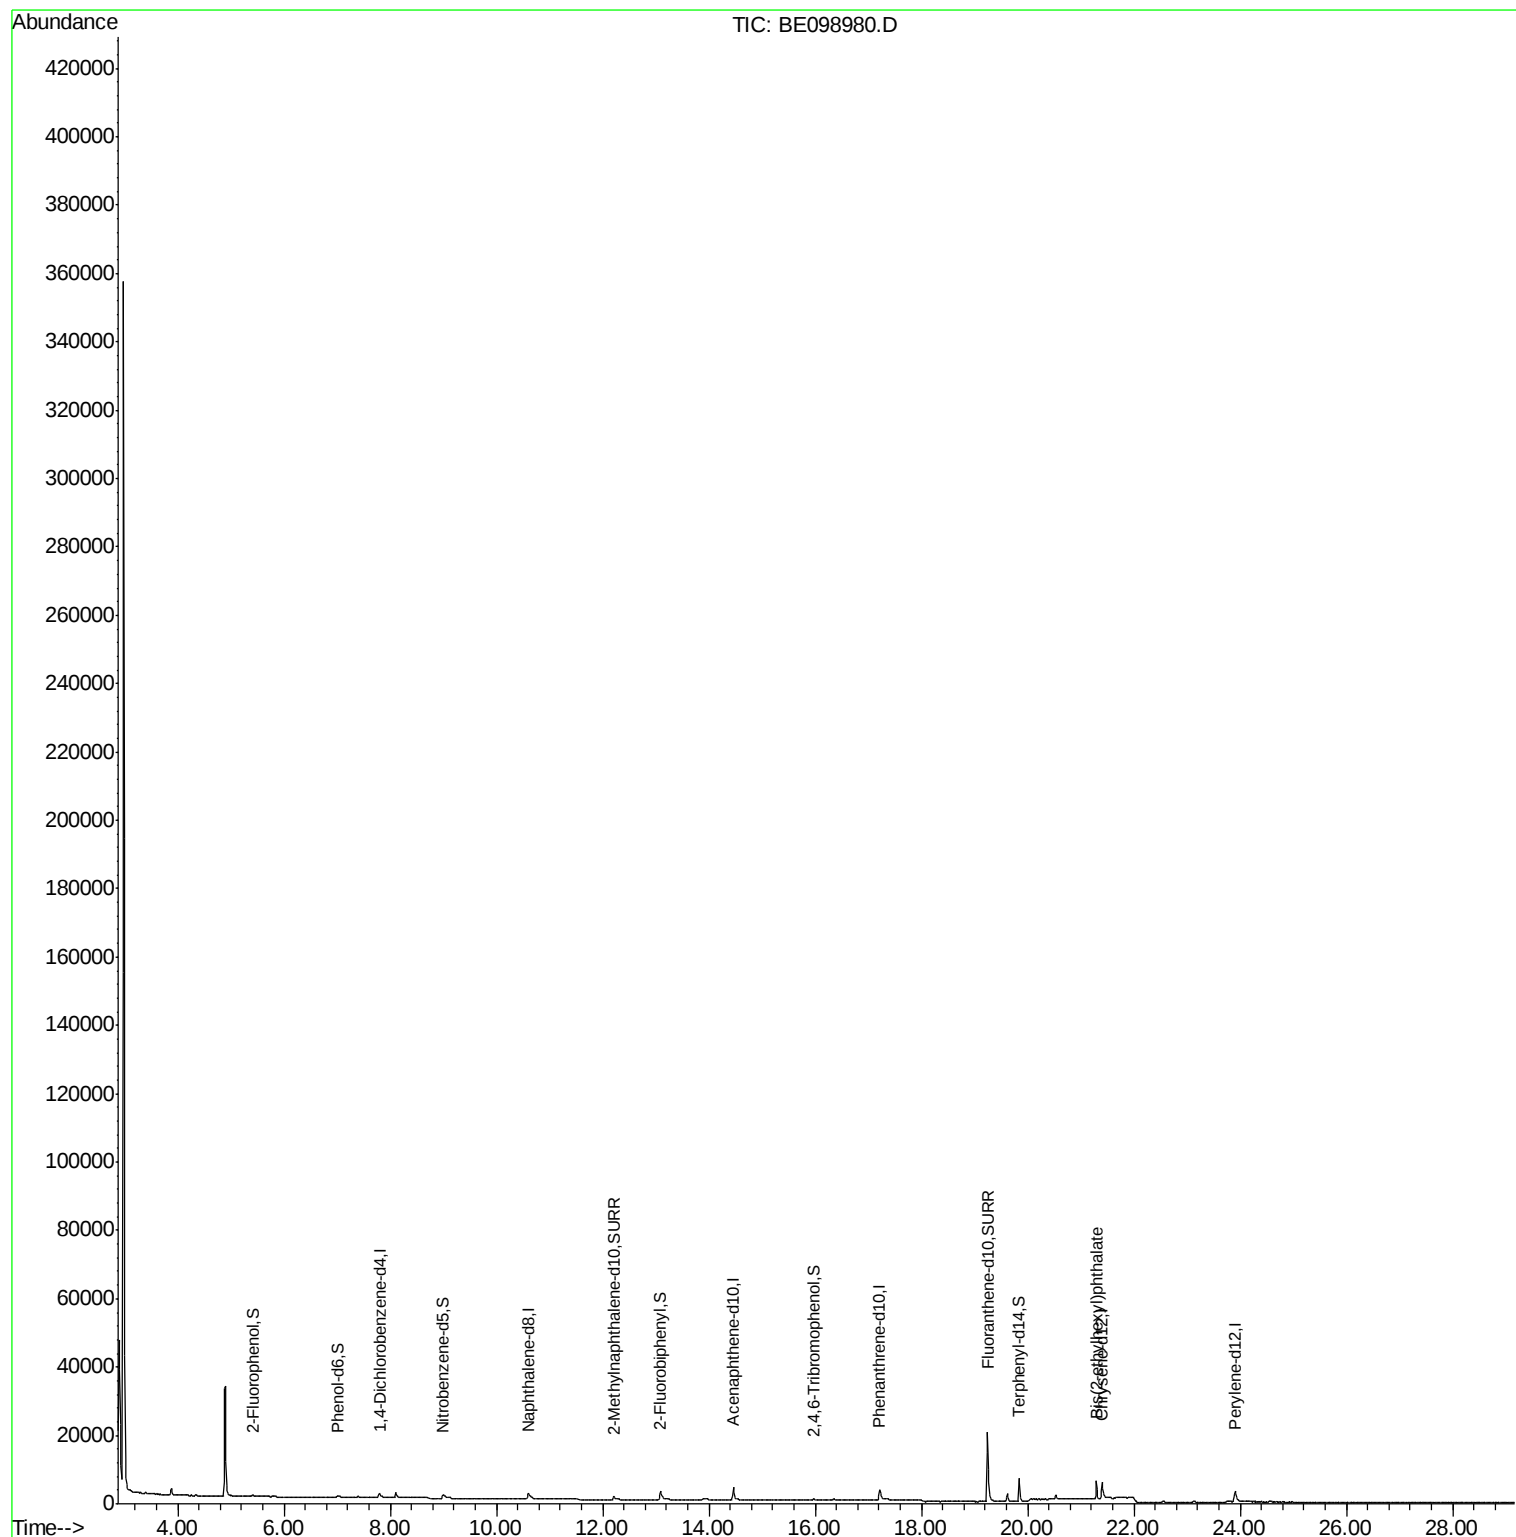







#1

1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.80 min Scan# 428
 Delta R.T. 0.00 min
 Lab File: BE098980.D
 Acq: 15 Mar 2019 20:27

Instrument :
 BNA_E
 ClientSampleId :
 M3-T3-OZ(POST)




Tot Ion:152 Resp: 904
 Ion Ratio Lower Upper
 152 100
 150 136.9 122.5 183.7
 115 67.3 57.4 86.2

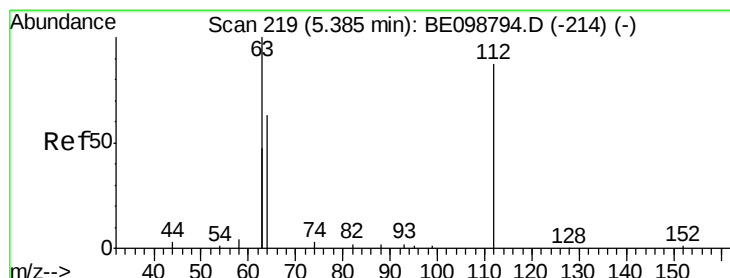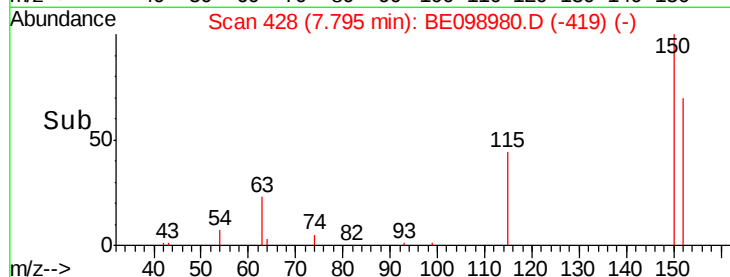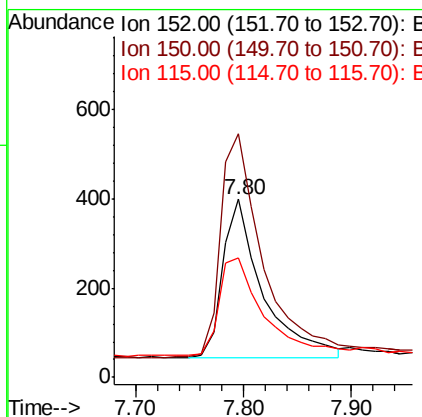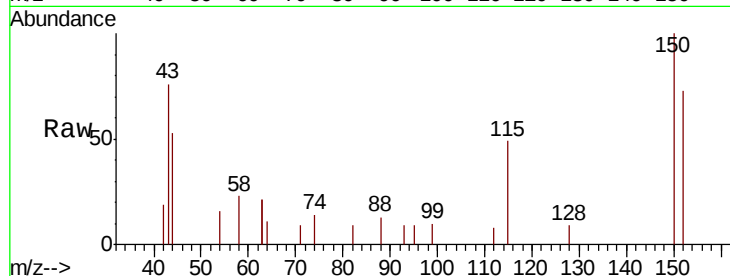


#4

2-Fluorophenol
 Concen: 0.184 ng
 RT: 5.41 min Scan# 221
 Delta R.T. 0.03 min
 Lab File: BE098980.D
 Acq: 15 Mar 2019 20:27

Tgt Ion:112 Resp: 498
 Ion Ratio Lower Upper
 112 100
 64 80.1 57.9 86.9
 63 150.6 158.3 237.5#

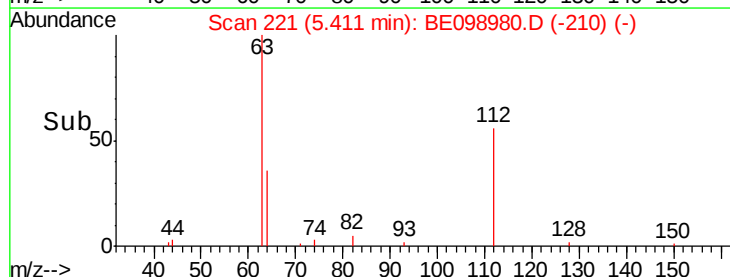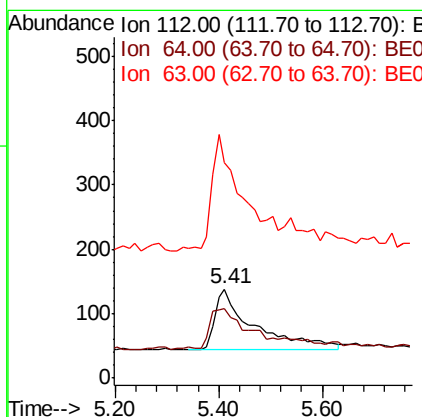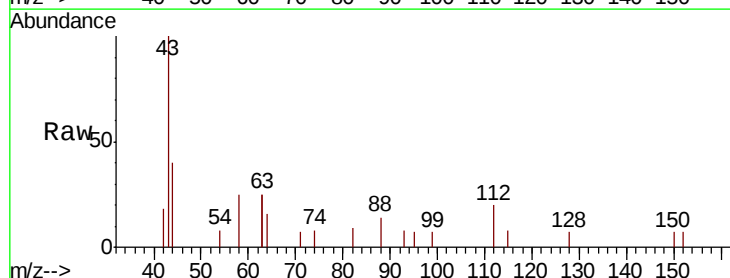

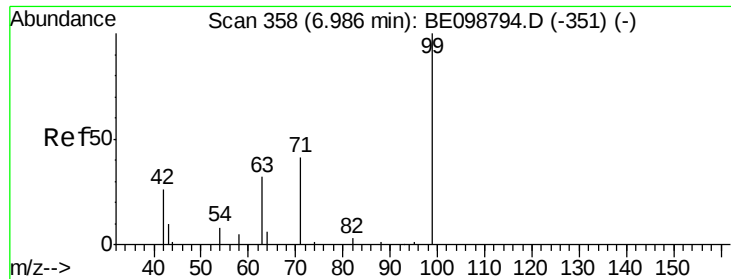

#5

Phenol-d6

Concen: 0.086 ng

RT: 7.00 min Scan# 359

Delta R.T. 0.01 min

Lab File: BE098980.D

Acq: 15 Mar 2019 20:27

Instrument :

BNA_E

ClientSampleId :

M3-T3-OZ(POST)


Tot Ion: 99 Resp: 330

Ion Ratio Lower Upper

99 100

42 58.5 24.2 36.2#

71 44.2 35.7 53.5



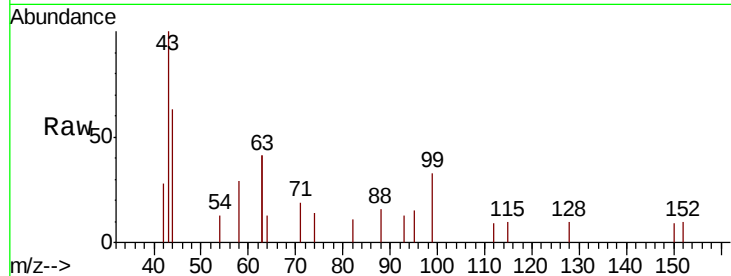


Abundance

Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

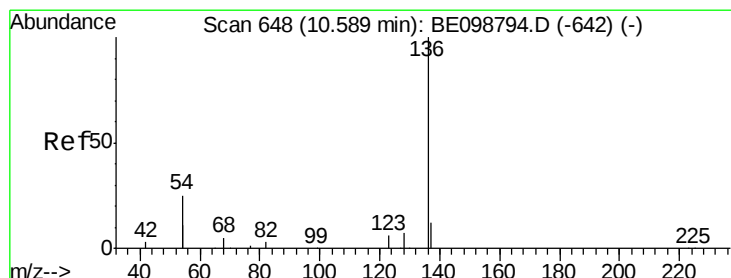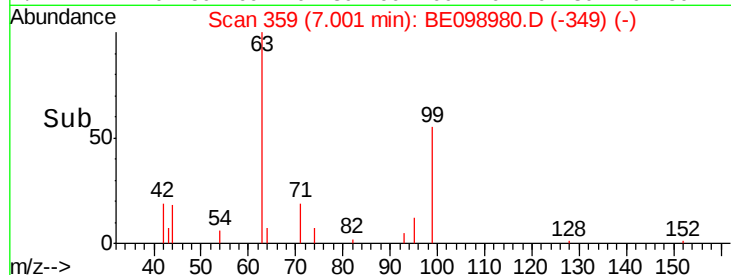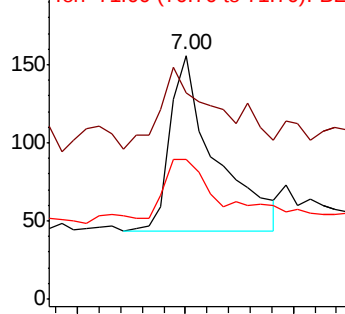

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.60 min Scan# 649

Delta R.T. 0.01 min

Lab File: BE098980.D

Acq: 15 Mar 2019 20:27

Tgt Ion: 136 Resp: 3622


Ion Ratio Lower Upper

136 100

137 15.1 11.4 17.0

54 60.4 39.3 58.9#

68 10.2 6.7 10.1#

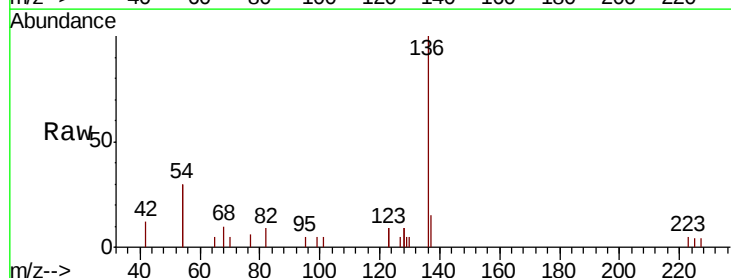



Abundance

Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

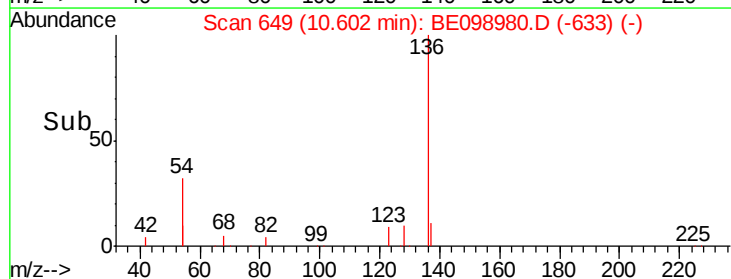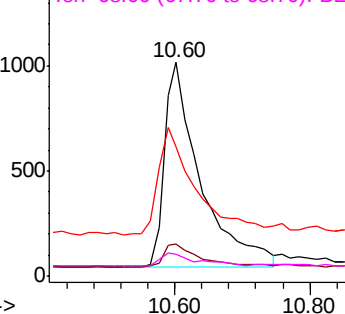







#8
 Nitrobenzene-d5
 Concen: 0.369 ng
 RT: 8.99 min Scan# 525
 Delta R.T. 0.03 min
 Lab File: BE098980.D
 Acq: 15 Mar 2019 20:27

Instrument :
 BNA_E
 ClientSampleId :
 M3-T3-OZ(POST)

Tot Ion	82	Resp	1400
Ion Ratio	Lower	Upper	
82	100		
128	161.4	123.8	185.8
54	303.9	203.4	305.2

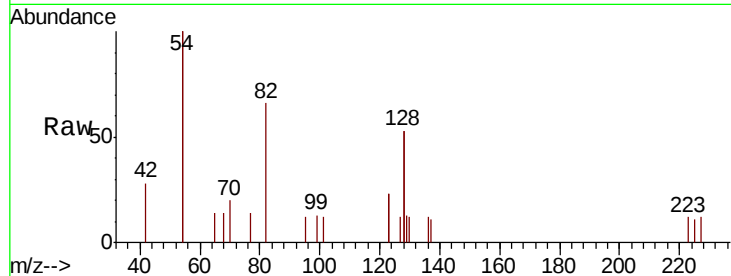


Abundance Ion 82.00 (81.70 to 82.70): BE0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BE0

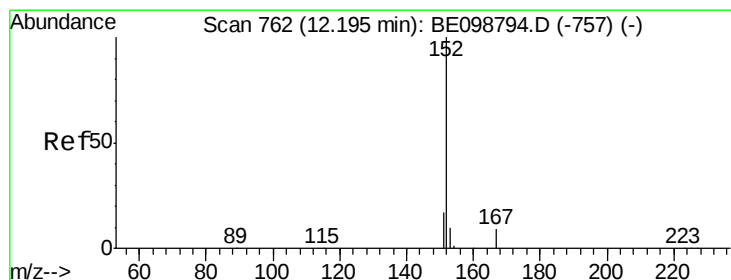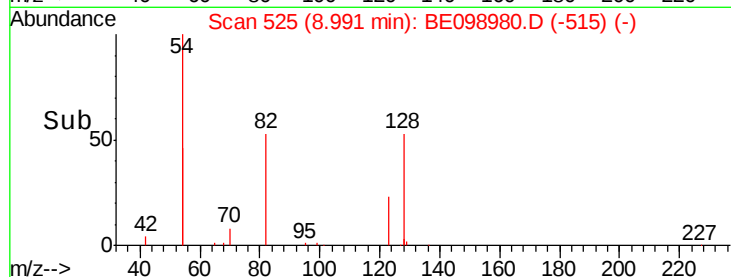
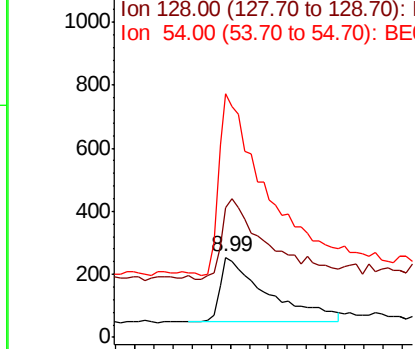



#11
 2-Methylnaphthalene-d10
 Concen: 0.392 ng
 RT: 12.21 min Scan# 763
 Delta R.T. 0.02 min
 Lab File: BE098980.D
 Acq: 15 Mar 2019 20:27

Tgt Ion	152	Resp	2623
Ion Ratio	Lower	Upper	
152	100		
151	19.4	16.5	24.7

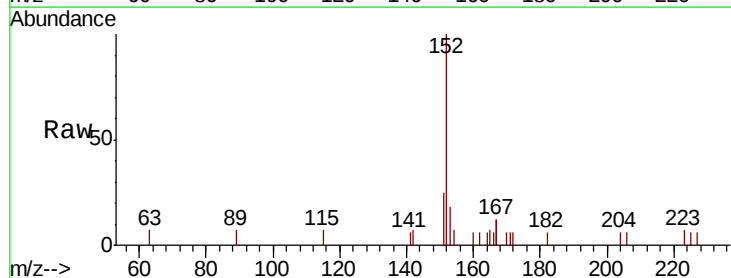

Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 151.00 (150.70 to 151.70): E

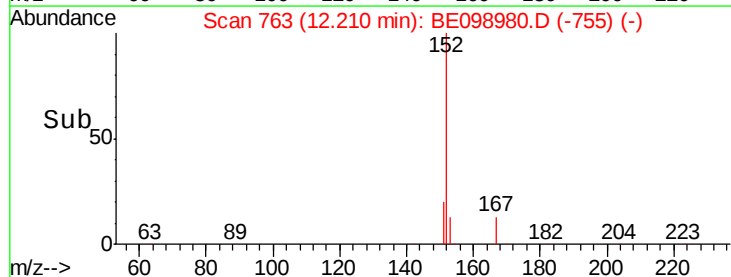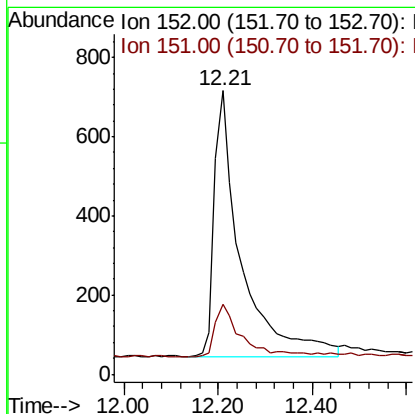


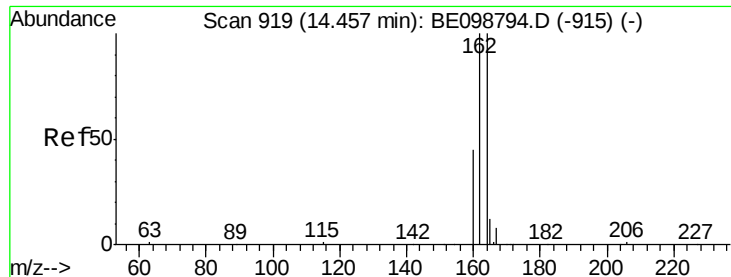




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.46 min Scan# 919
Delta R.T. 0.00 min
Lab File: BE098980.D
Acq: 15 Mar 2019 20:27

Instrument :
BNA_E
ClientSampleId :
M3-T3-OZ(POST)

Tot Ion:164 Resp: 2632
Ion Ratio Lower Upper
164 100
162 102.7 80.2 120.2
160 49.5 37.8 56.8

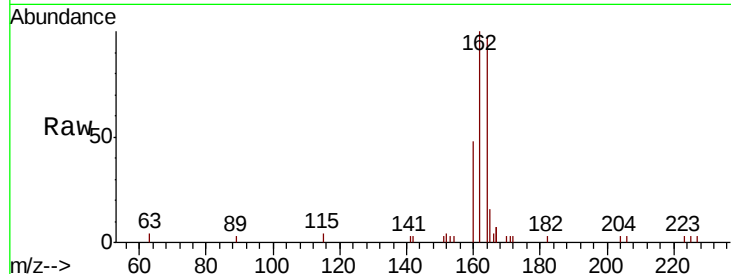


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

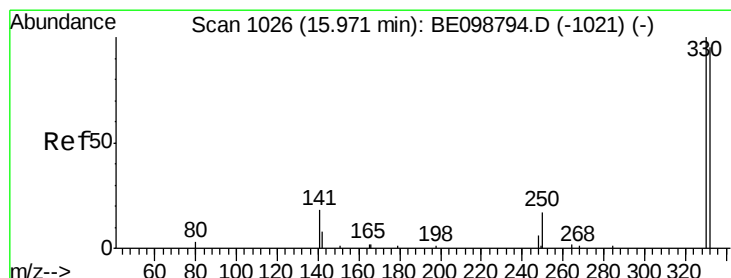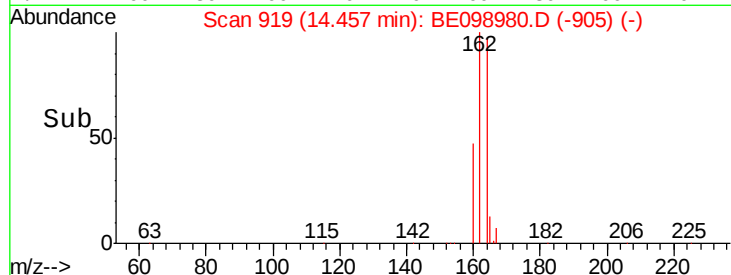
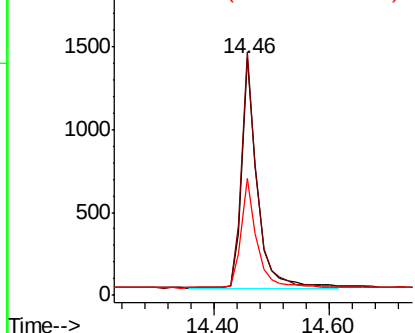



#14
2,4,6-Tribromophenol
Concen: 0.291 ng
RT: 15.97 min Scan# 1026
Delta R.T. -0.00 min
Lab File: BE098980.D
Acq: 15 Mar 2019 20:27

Tgt Ion:330 Resp: 386
Ion Ratio Lower Upper
330 100
332 100.8 77.6 116.4
141 48.2 31.0 46.4#

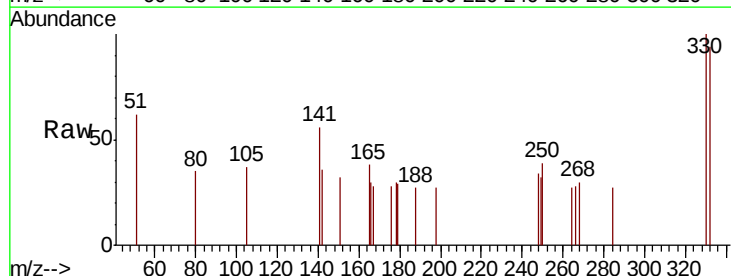

Abundance Ion 330.00 (329.70 to 330.70): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

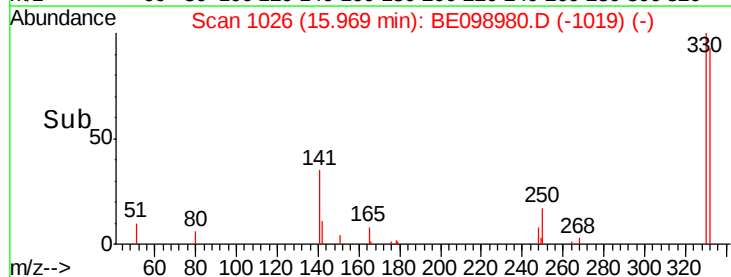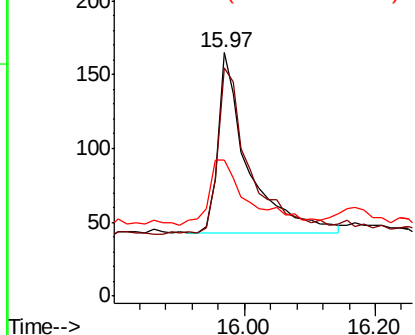


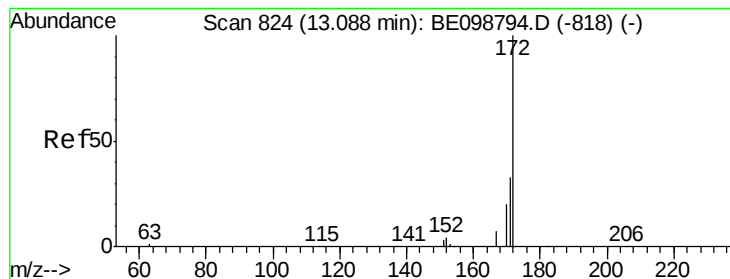




#15
2-Fluorobiphenyl
Concen: 0.412 ng
RT: 13.09 min Scan# 824
Delta R.T. 0.00 min
Lab File: BE098980.D
Acq: 15 Mar 2019 20:27

Instrument :
BNA_E
ClientSampleId :
M3-T3-OZ(POST)

Tot Ion:172 Resp: 4493
Ion Ratio Lower Upper
172 100
171 35.2 28.0 42.0
170 25.2 17.7 26.5

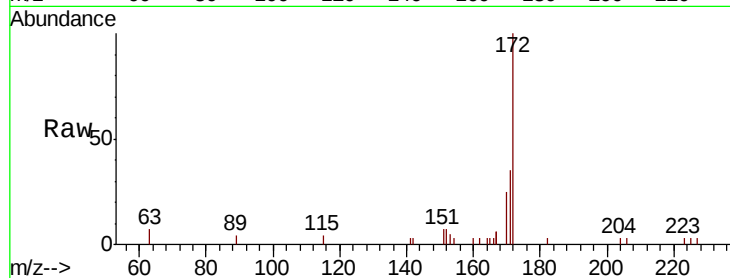


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

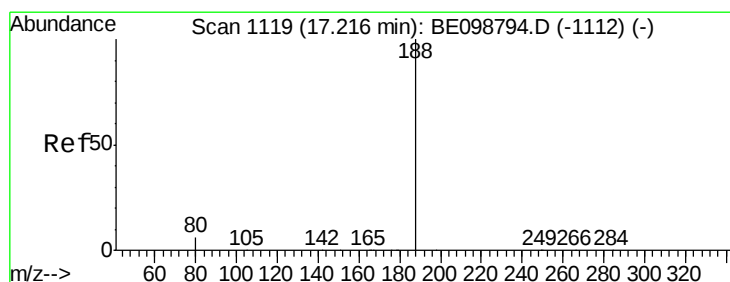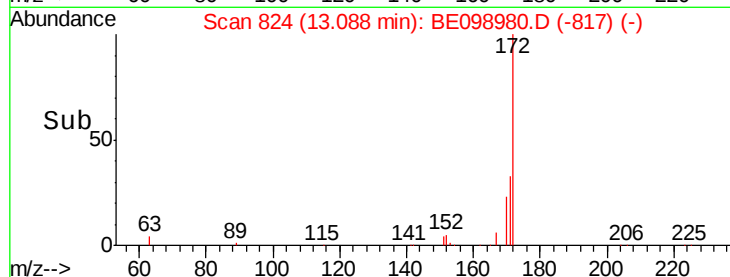
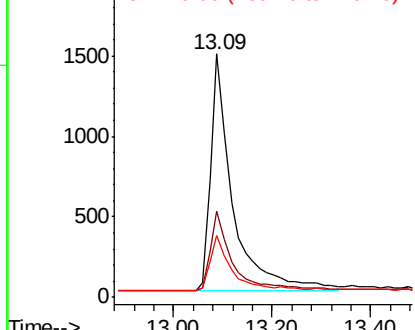



#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.21 min Scan# 1119
Delta R.T. -0.00 min
Lab File: BE098980.D
Acq: 15 Mar 2019 20:27

Tgt Ion:188 Resp: 5939
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 11.8 6.3 9.5#

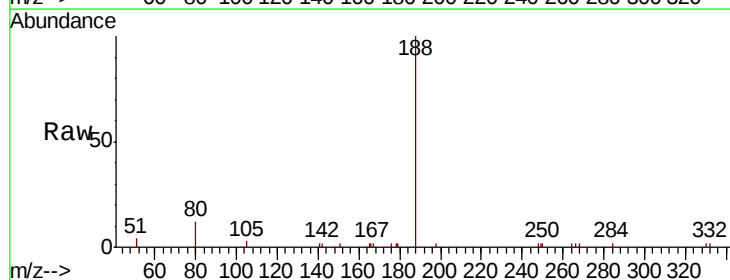

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BE0
Ion 80.00 (79.70 to 80.70): BE0



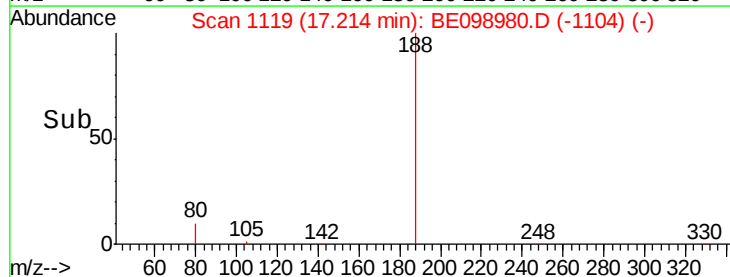
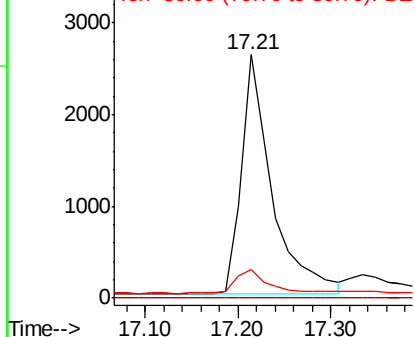


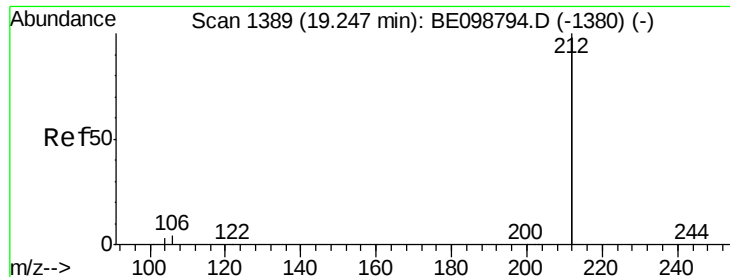

#25
 Fluoranthene-d10
 Concen: 0.401 ng
 RT: 19.25 min Scan# 1389
 Delta R.T. 0.00 min
 Lab File: BE098980.D
 Acq: 15 Mar 2019 20:27




Instrument :
 BNA_E
 ClientSampleId :
 M3-T3-OZ(POST)


Tot Ion:212 Resp: 38060
 Ion Ratio Lower Upper
 212 100
 106 2.3 1.8 2.8
 104 1.4 1.0 1.6

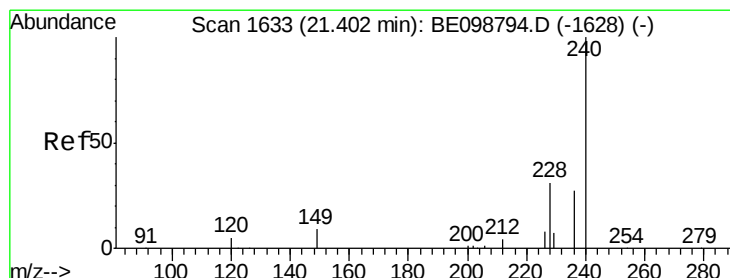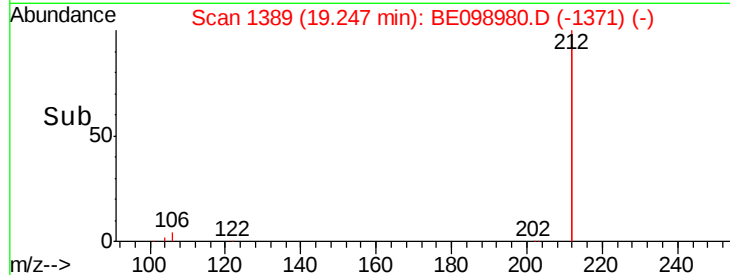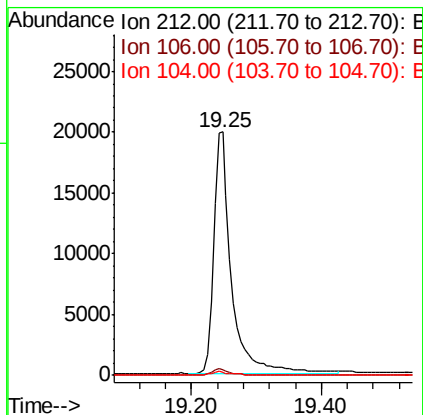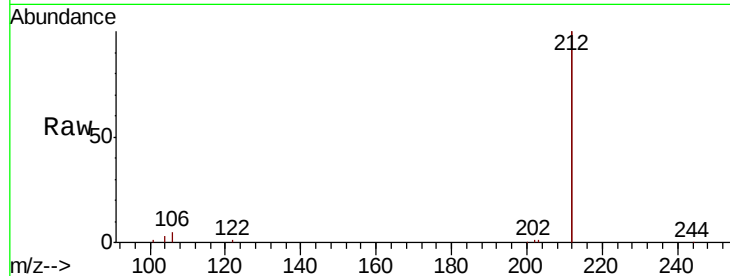

#27
 Chrysene-d12
 Concen: 0.400 ng
 RT: 21.40 min Scan# 1633
 Delta R.T. -0.00 min
 Lab File: BE098980.D
 Acq: 15 Mar 2019 20:27

Tgt Ion:240 Resp: 7302
 Ion Ratio Lower Upper
 240 100
 120 8.2 5.0 7.4#
 236 28.0 22.7 34.1

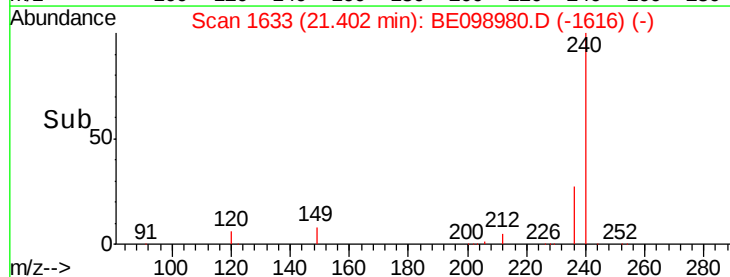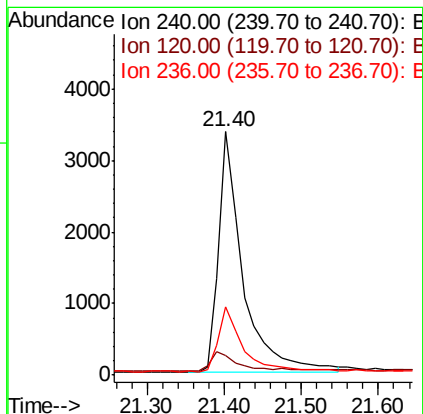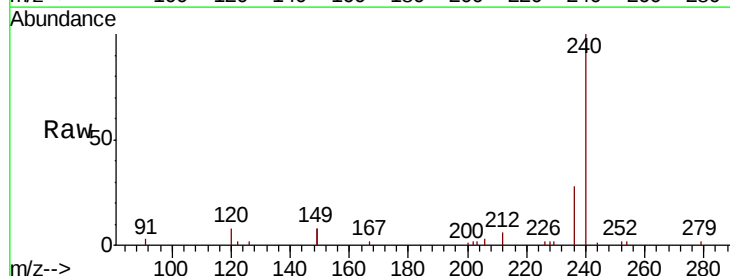

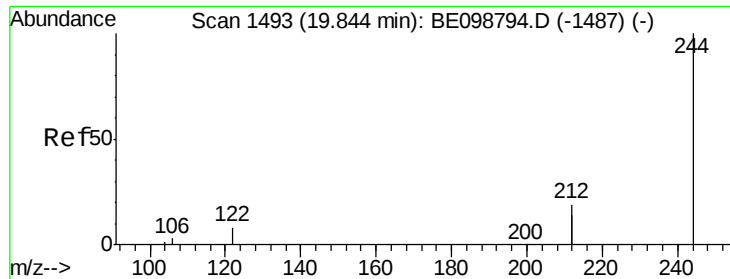

#29

Terphenyl-d14

Concen: 0.423 ng

RT: 19.84 min Scan# 1492

Delta R.T. -0.01 min

Lab File: BE098980.D

Acq: 15 Mar 2019 20:27

Instrument :

BNA_E

ClientSampleId :

M3-T3-OZ(POST)


Tot Ion:244 Resp: 7507

Ion Ratio Lower Upper

244 100

212 40.1 29.4 44.2




122 10.3 7.1 10.7

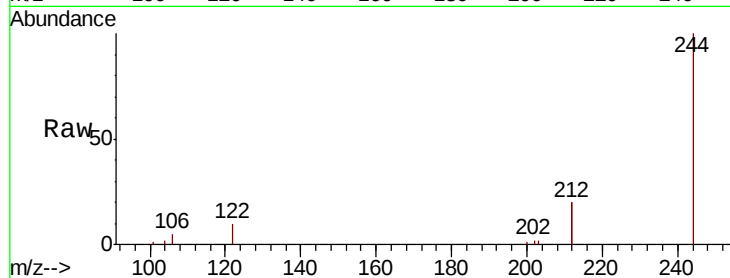

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

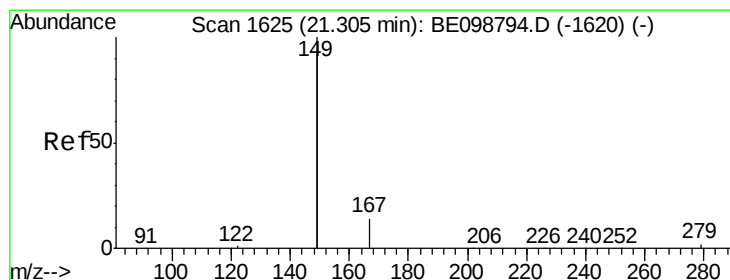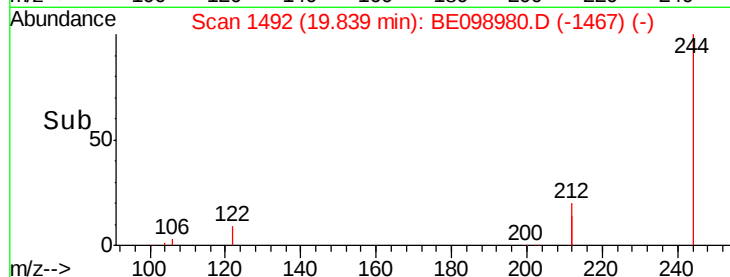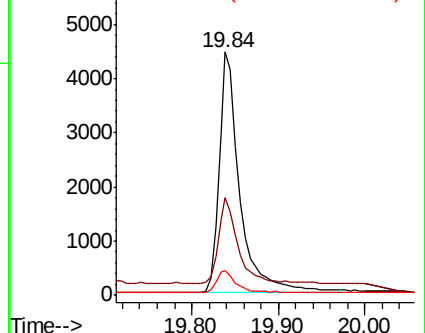

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.121 ng

RT: 21.29 min Scan# 1624

Delta R.T. -0.01 min

Lab File: BE098980.D

Acq: 15 Mar 2019 20:27


Tgt Ion:149 Resp: 5851

Ion Ratio Lower Upper

149 100

167 7.2 5.4 8.0



279 1.7 1.0 1.4#


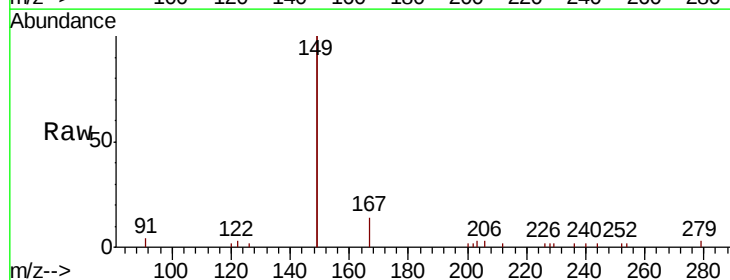


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

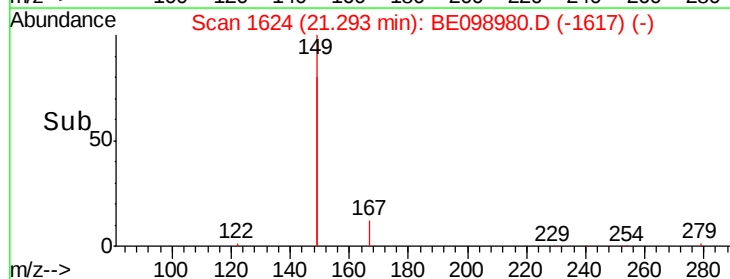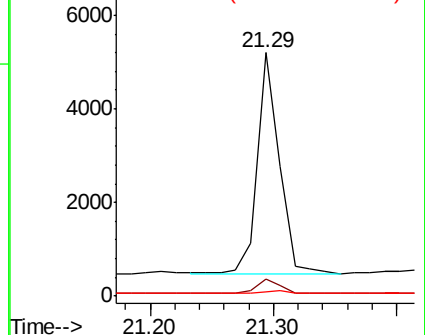

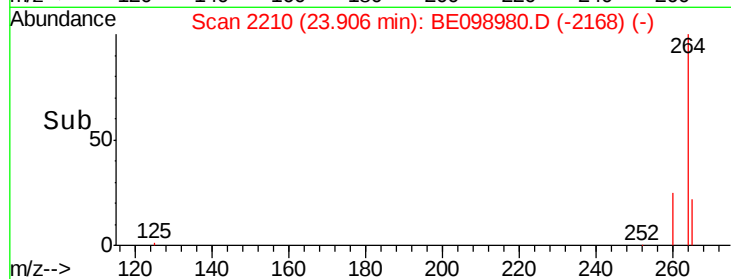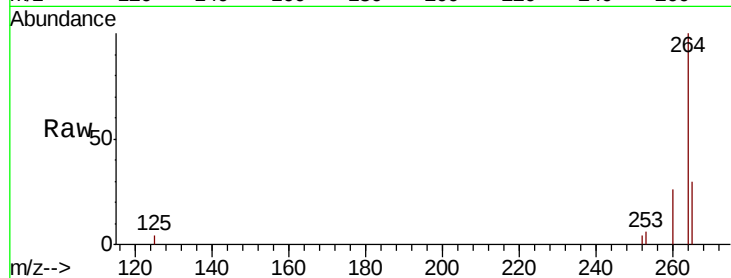

#34

Pervlone-d12

Concen: 0.400 ng

RT: 23.91 min Scan# 2210

Delta R.T. 0.00 min

Lab File: BE098980.D

Acq: 15 Mar 2019 20:27

Instrument :

BNA_E

ClientSampleId :

M3-T3-OZ(POST)

Tot Ion:264 Resp: 6753

Ion Ratio Lower Upper

264 100

260 26.4 21.2 31.8

265 30.1 24.6 36.8

