


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE031519\
 Data File : BE098966.D
 Acq On : 15 Mar 2019 9:37
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE030619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 15 05:31:33 2019

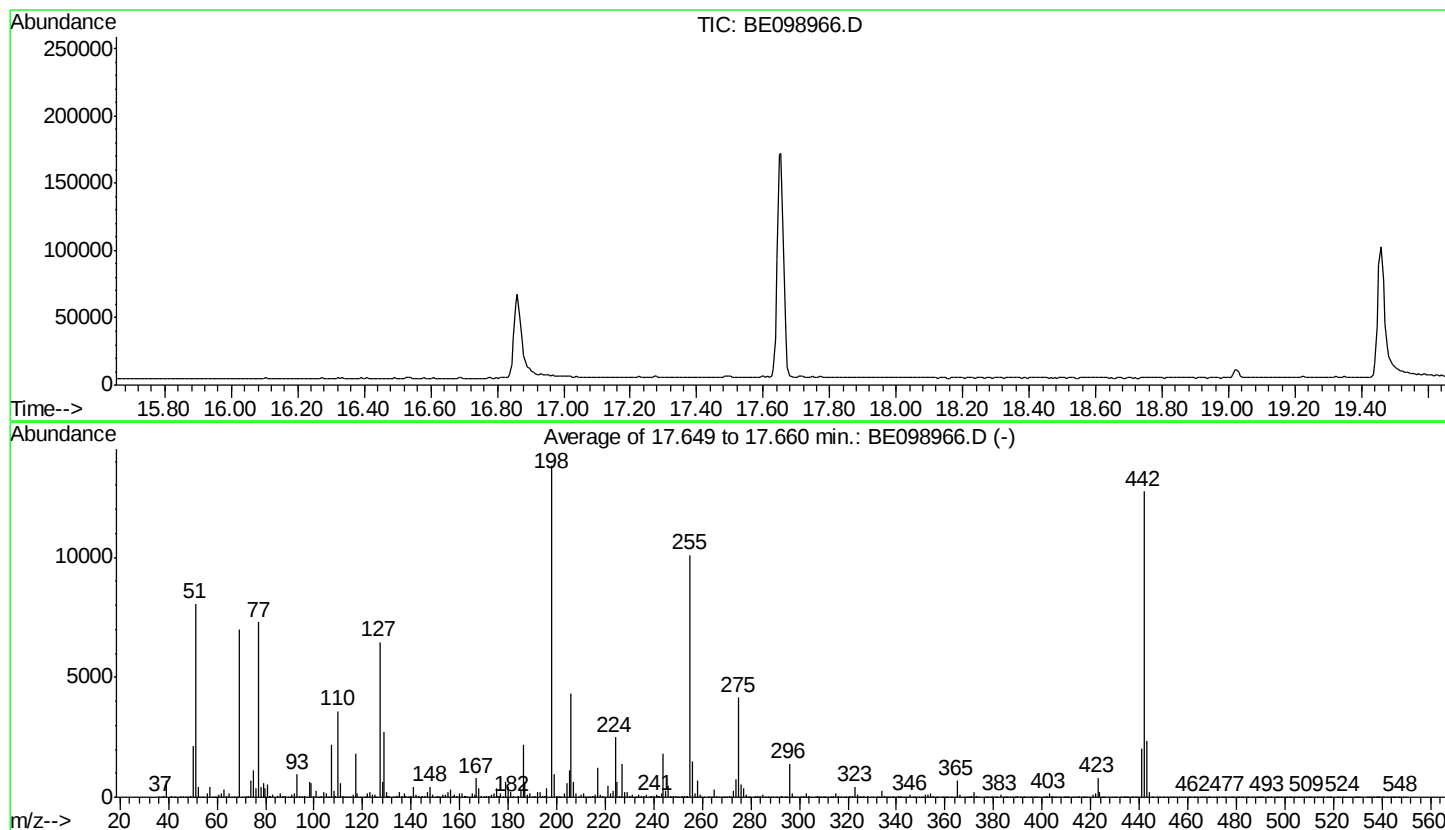

AutoFind: Scans 2563, 2564, 2565; Background Corrected with Scan 2555

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.3	8058	PASS
68	69	0.00	2	0.3	19	PASS
69	198	0.00	100	50.5	6981	PASS
70	69	0.00	2	0.1	6	PASS
127	198	10	80	46.8	6471	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	13814	PASS
199	198	5	9	6.9	959	PASS
275	198	10	60	29.9	4136	PASS
365	198	1	100	4.9	672	PASS
441	198	0.01	100	14.5	2003	PASS
442	198	50	100	92.1	12728	PASS
443	442	15	24	18.6	2367	PASS