


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE031519\
 Data File : BE098982.D
 Acq On : 15 Mar 2019 22:20
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE030619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 15 05:31:33 2019

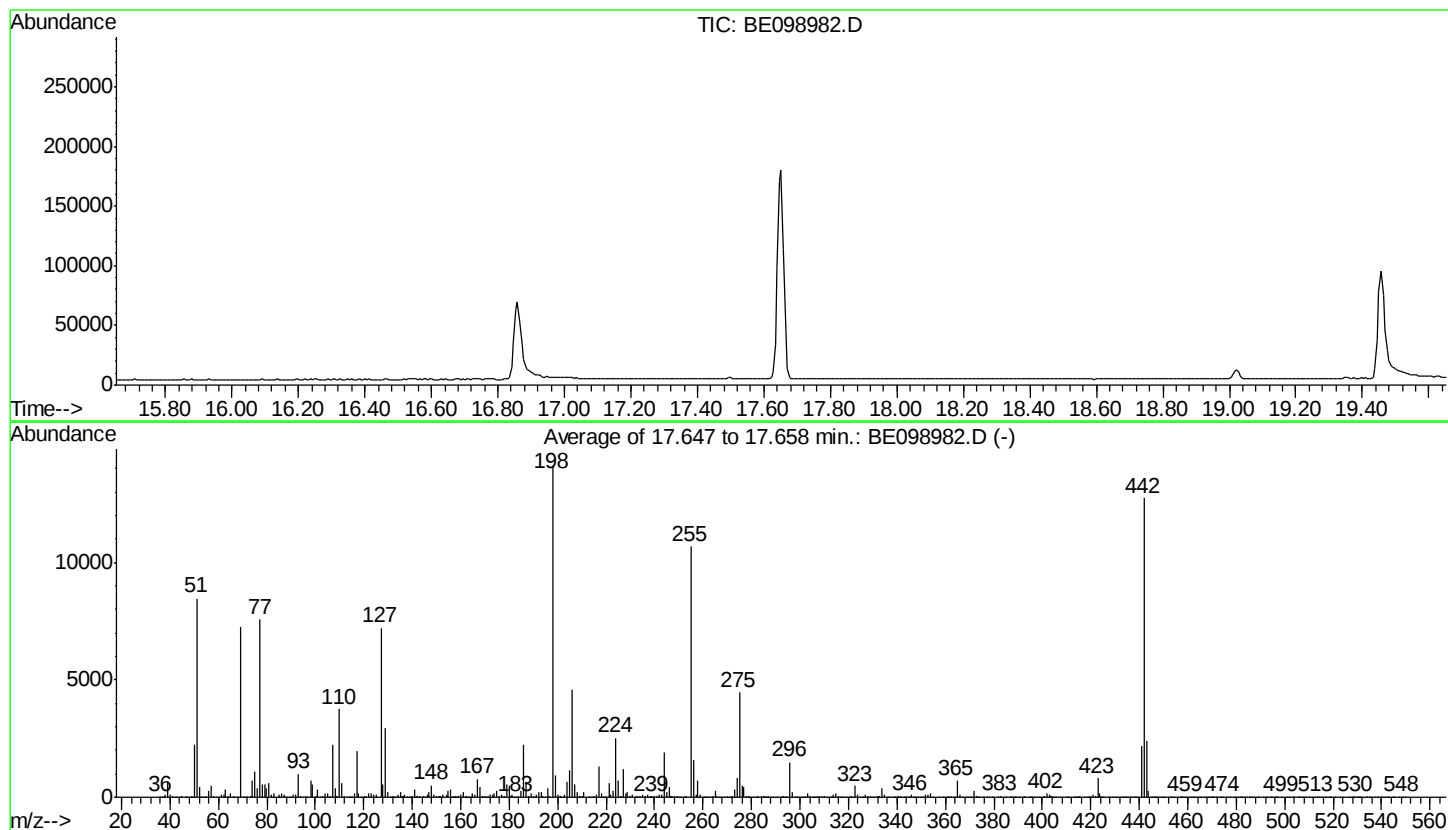

AutoFind: Scans 2563, 2564, 2565; Background Corrected with Scan 2556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.0	8468	PASS
68	69	0.00	2	0.0	2	PASS
69	198	0.00	100	51.3	7246	PASS
70	69	0.00	2	0.2	15	PASS
127	198	10	80	51.1	7212	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	14122	PASS
199	198	5	9	6.7	953	PASS
275	198	10	60	31.6	4458	PASS
365	198	1	100	5.0	703	PASS
441	198	0.01	100	15.4	2180	PASS
442	198	50	100	90.2	12737	PASS
443	442	15	24	18.8	2400	PASS