

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE031819\
 Data File : BE099017.D
 Acq On : 19 Mar 2019 1:47
 Operator : JU/SJ
 Sample : K1937-18
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 BPS1-TT-MW202S-20190314

Quant Time: Mar 19 02:56:32 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE030619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 15 05:31:33 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	738	0.40	ng	0.00
7) Naphthalene-d8	10.60	136	3632	0.40	ng	0.01
13) Acenaphthene-d10	14.46	164	2557	0.40	ng	0.00
19) Phenanthrene-d10	17.22	188	6553	0.40	ng	0.00
27) Chrysene-d12	21.40	240	7002	0.40	ng	0.00
34) Perylene-d12	23.89	264	6621	0.40	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.42	112	404	0.18	ng	0.03
5) Phenol-d6	7.02	99	326	0.10	ng	0.03
8) Nitrobenzene-d5	9.00	82	1067	0.28	ng	0.04
11) 2-Methylnaphthalene-d10	12.19	152	2500	0.37	ng	0.00
14) 2,4,6-Tribromophenol	15.97	330	436	0.34	ng	0.00
15) 2-Fluorobiphenyl	13.09	172	4307	0.41	ng	0.00
25) Fluoranthene-d10	19.24	212	36470	0.35	ng	0.00
29) Terphenyl-d14	19.83	244	6876	0.40	ng	-0.01
Target Compounds						
22) Pentachlorophenol	16.92	266	23	0.280	ng	98
32) Bis(2-ethylhexyl)phthalate	21.29	149	1548	0.033	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE031819\
Data File : BE099017.D
Acq On : 19 Mar 2019 1:47
Operator : JU/SJ
Sample : K1937-18
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BPS1-TT-MW202S-20190314

Quant Time: Mar 19 02:56:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE030619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 15 05:31:33 2019
Response via : Initial Calibration

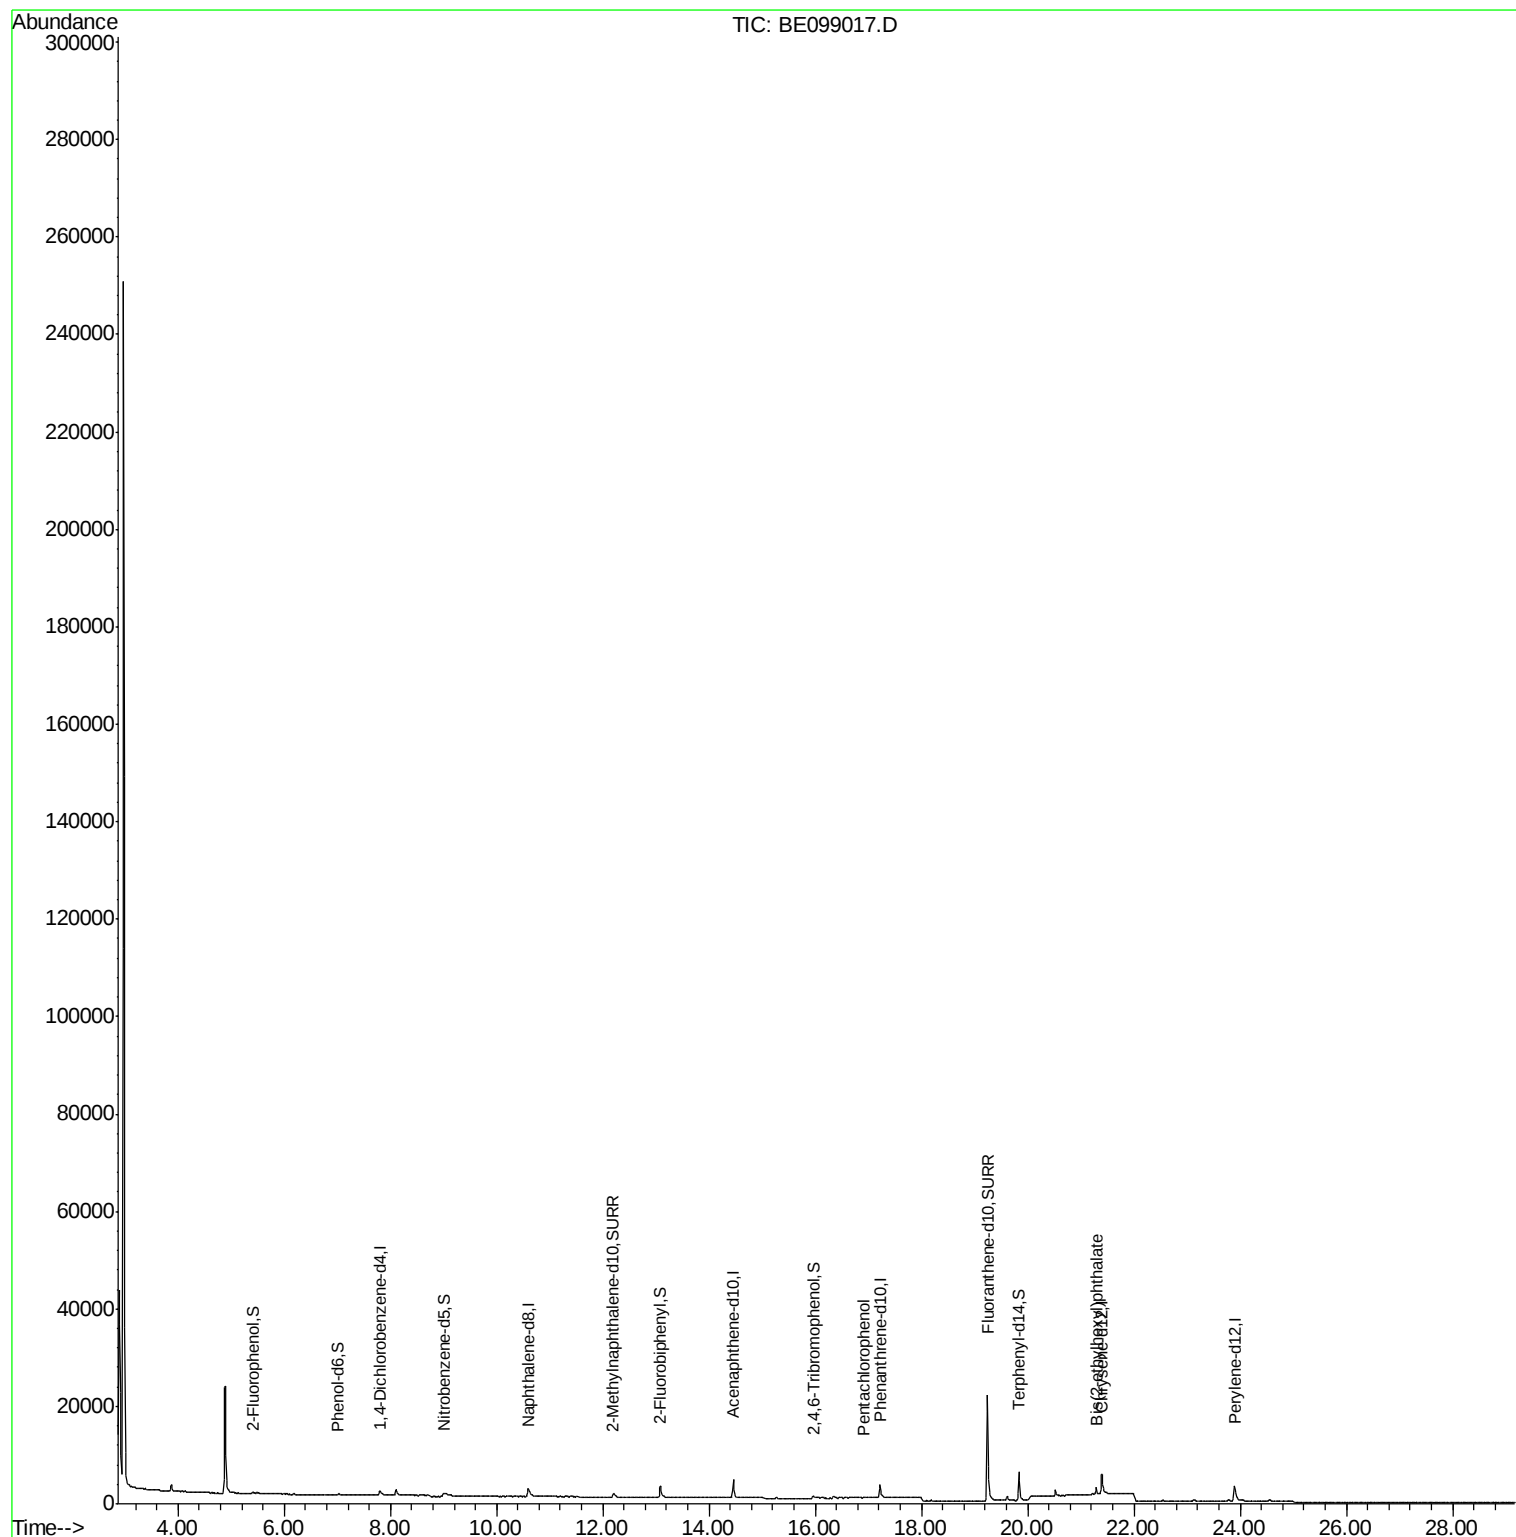




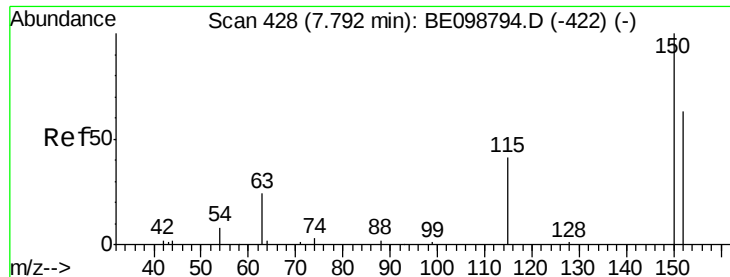


#1

1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.79 min Scan# 428
Delta R.T. -0.00 min
Lab File: BE099017.D
Acq: 19 Mar 2019 1:47

Instrument :
BNA_E
ClientSampleId :
BPS1-TT-MW202S-20190314




Tgt Ion:152 Resp: 738
Ion Ratio Lower Upper
152 100
150 150.4 122.5 183.7
115 76.7 57.4 86.2

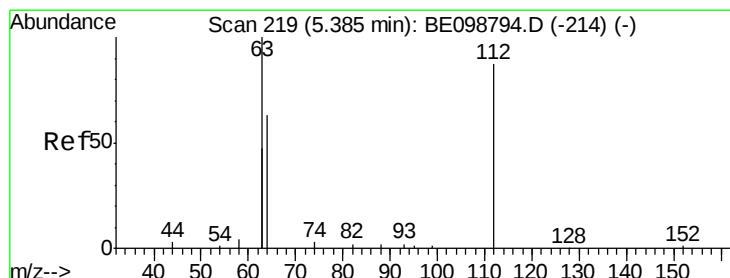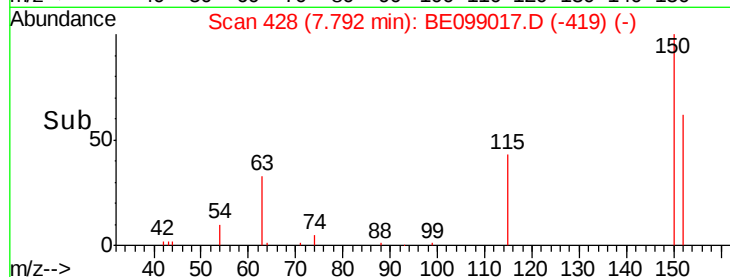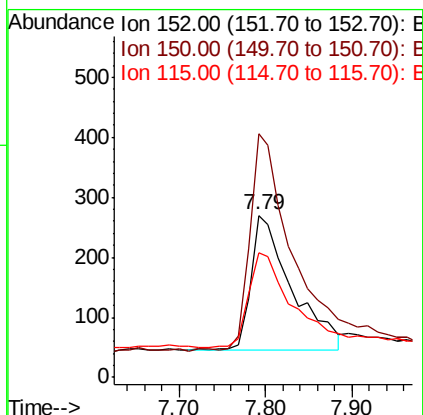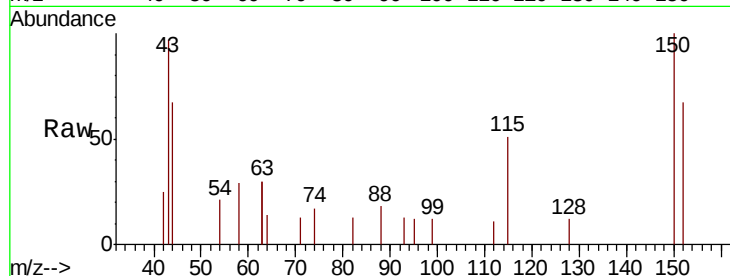


#4

2-Fluorophenol
Concen: 0.183 ng
RT: 5.42 min Scan# 222
Delta R.T. 0.03 min
Lab File: BE099017.D
Acq: 19 Mar 2019 1:47

Tgt Ion:112 Resp: 404
Ion Ratio Lower Upper
112 100
64 66.6 57.9 86.9
63 157.7 158.3 237.5#

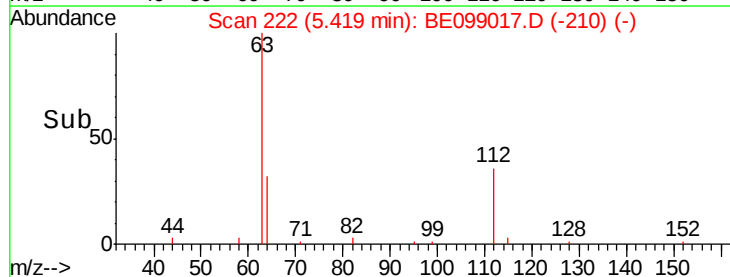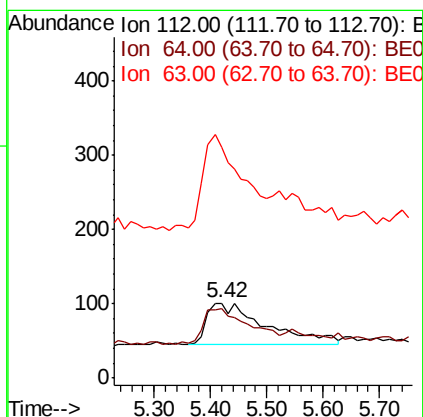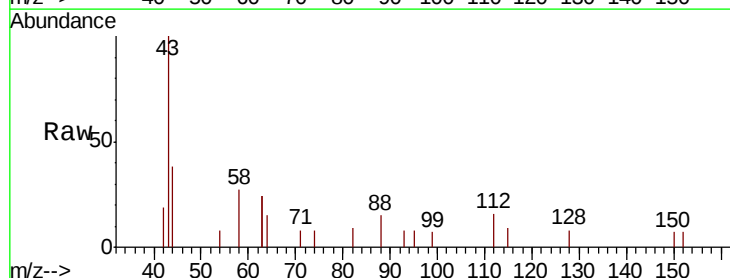

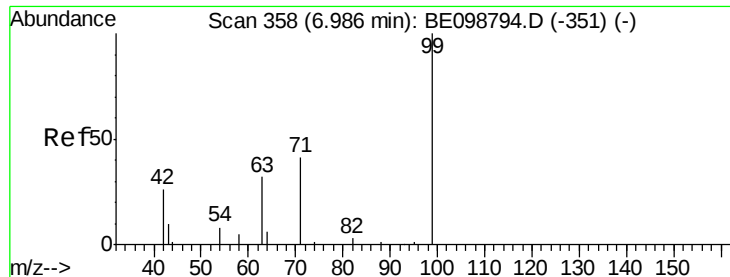

#5

Phenol-d6

Concen: 0.105 ng

RT: 7.02 min Scan# 361

Delta R.T. 0.03 min

Lab File: BE099017.D

Acq: 19 Mar 2019 1:47

Instrument :

BNA_E

ClientSampleId :

BPS1-TT-MW202S-20190314


Tgt Ion: 99 Resp: 326

Ion Ratio Lower Upper

99 100

42 0.0 24.2 36.2#




71 0.0 35.7 53.5#

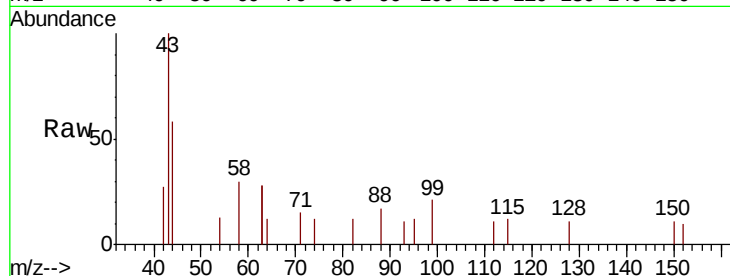

Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

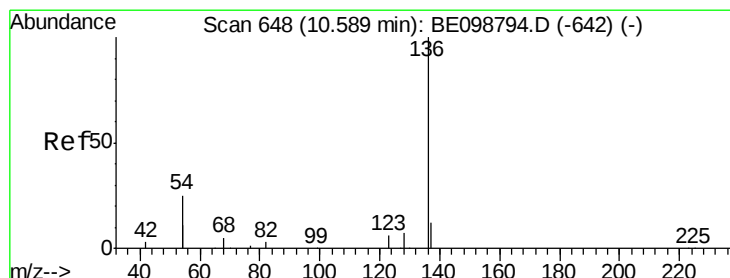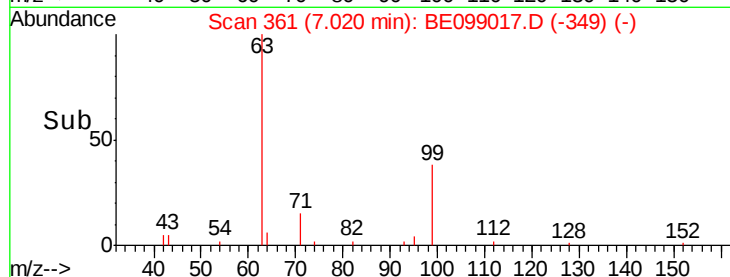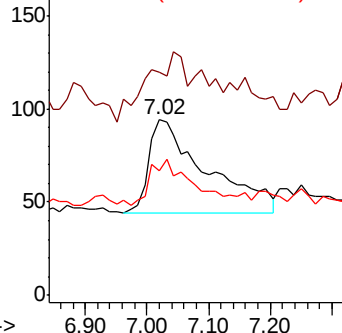

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.60 min Scan# 650

Delta R.T. 0.01 min

Lab File: BE099017.D

Acq: 19 Mar 2019 1:47

Tgt Ion: 136 Resp: 3632


Ion Ratio Lower Upper

136 100

137 14.7 11.4 17.0

54 61.4 39.3 58.9#

68 9.8 6.7 10.1


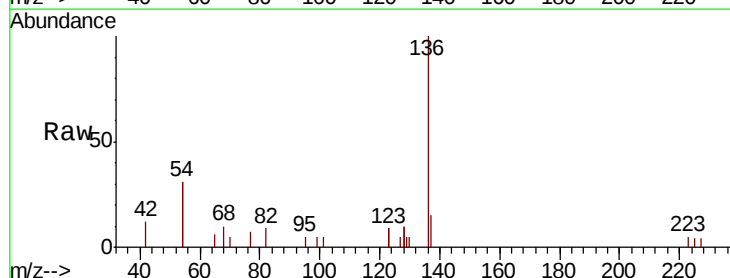



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0



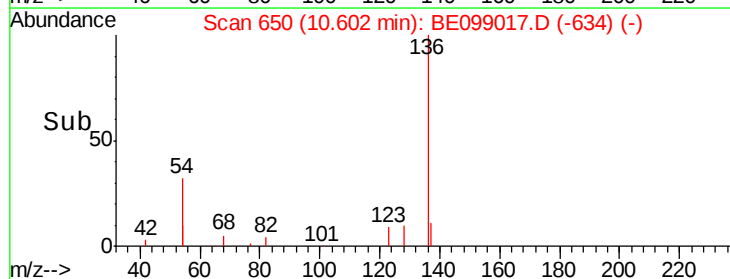
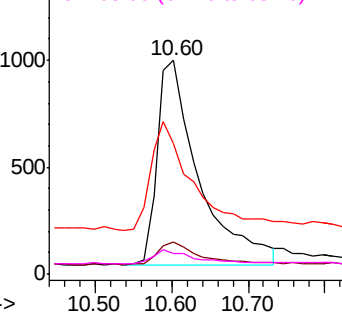




#8
 Nitrobenzene-d5
 Concen: 0.280 ng
 RT: 9.00 min Scan# 527
 Delta R.T. 0.04 min
 Lab File: BE099017.D
 Acq: 19 Mar 2019 1:47




Instrument :
 BNA_E
 ClientSampleId :
 BPS1-TT-MW202S-20190314


Tgt Ion: 82 Resp: 1067
 Ion Ratio Lower Upper
 82 100
 128 189.8 123.8 185.8#
 54 312.2 203.4 305.2#

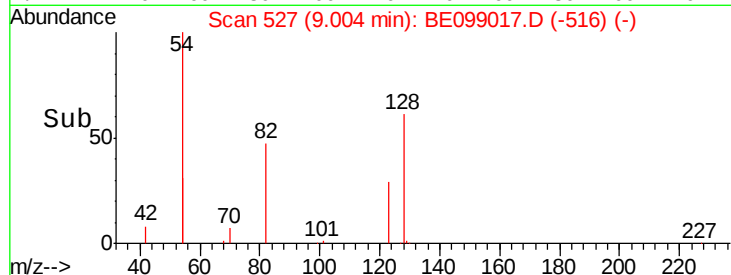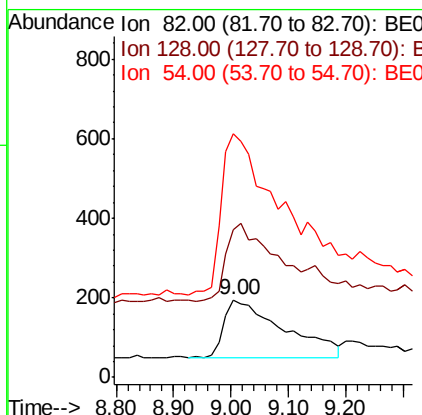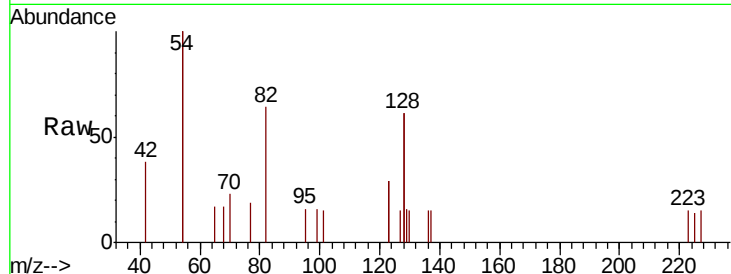

#11
 2-Methylnaphthalene-d10
 Concen: 0.372 ng
 RT: 12.19 min Scan# 763
 Delta R.T. 0.00 min
 Lab File: BE099017.D
 Acq: 19 Mar 2019 1:47

Tgt Ion: 152 Resp: 2500
 Ion Ratio Lower Upper
 152 100
 151 18.7 16.5 24.7



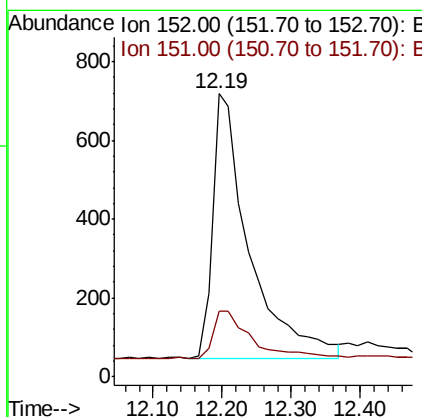
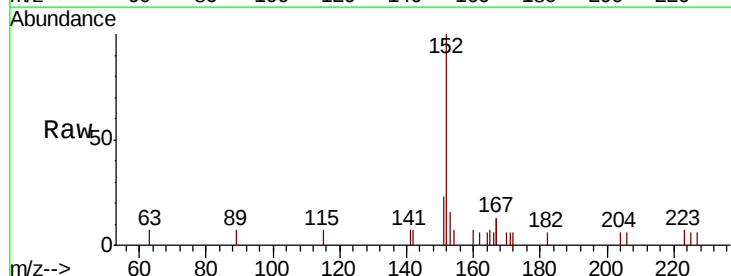




#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.46 min Scan# 920
 Delta R.T. 0.00 min
 Lab File: BE099017.D
 Acq: 19 Mar 2019 1:47




Instrument :
 BNA_E
 ClientSampleId :
 BPS1-TT-MW202S-20190314


Tgt Ion:164 Resp: 2557
 Ion Ratio Lower Upper
 164 100
 162 105.1 80.2 120.2
 160 49.5 37.8 56.8

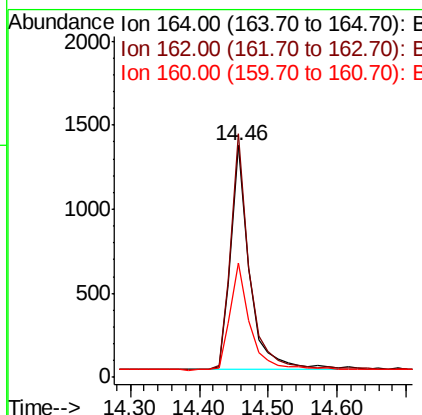

#14
 2,4,6-Tribromophenol
 Concen: 0.338 ng
 RT: 15.97 min Scan# 1027
 Delta R.T. -0.00 min
 Lab File: BE099017.D
 Acq: 19 Mar 2019 1:47

Tgt Ion:330 Resp: 436
 Ion Ratio Lower Upper
 330 100
 332 99.8 77.6 116.4
 141 46.8 31.0 46.4#

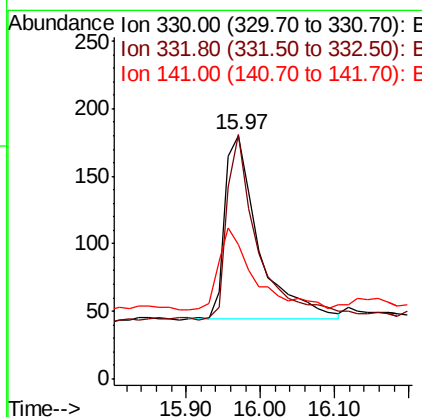

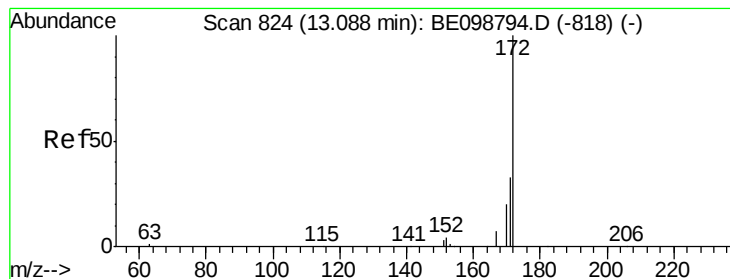

#15

2-Fluorobiphenyl

Concen: 0.407 ng

RT: 13.09 min Scan# 825

Delta R.T. 0.00 min

Lab File: BE099017.D

Acq: 19 Mar 2019 1:47

Instrument :

BNA_E

ClientSampleId :

BPS1-TT-MW202S-20190314


Tgt Ion:172 Resp: 4307

Ion Ratio Lower Upper

172 100

171 33.3 28.0 42.0




170 23.4 17.7 26.5

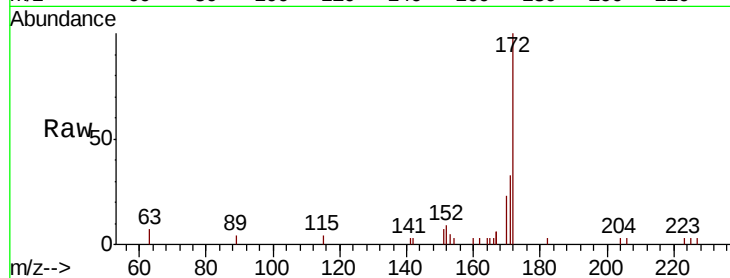

Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

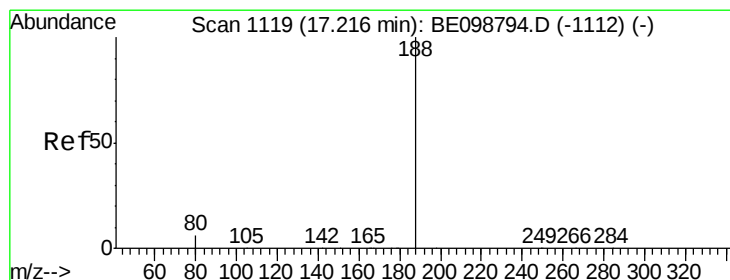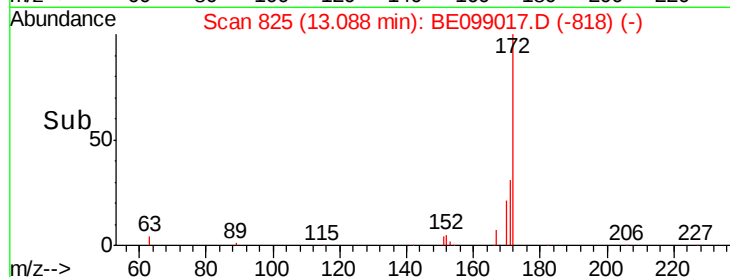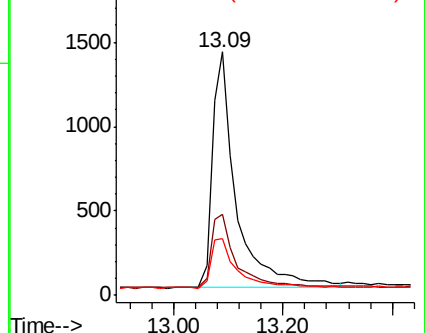

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.22 min Scan# 1120

Delta R.T. -0.00 min

Lab File: BE099017.D

Acq: 19 Mar 2019 1:47


Tgt Ion:188 Resp: 6553

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0



80 9.6 6.3 9.5#

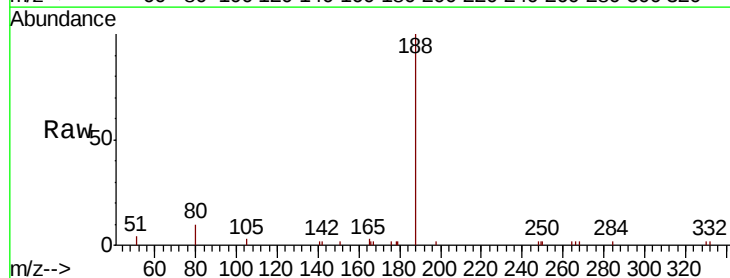


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

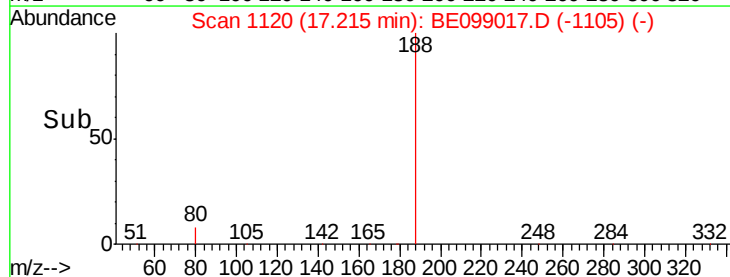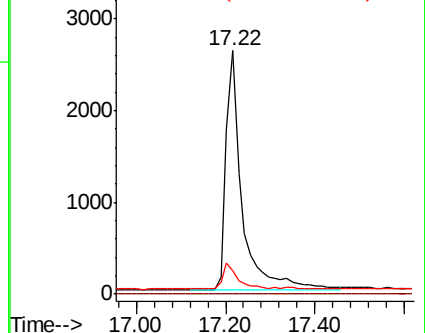



#22

Pentachlorophenol

Concen: 0.280 ng

RT: 16.92 min Scan# 1098

Delta R.T. 0.03 min

Lab File: BE099017.D

Acq: 19 Mar 2019 1:47

Instrument :

BNA_E

ClientSampleId :

BPS1-TT-MW202S-20190314


Tgt Ion: 266 Resp: 23

Ion Ratio Lower Upper

266 100

264 83.0 66.6 100.0




268 90.6 69.8 104.8

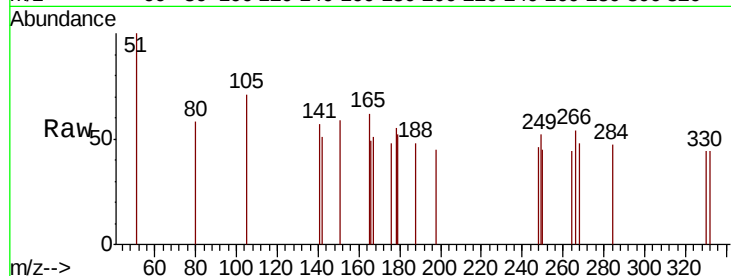

Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

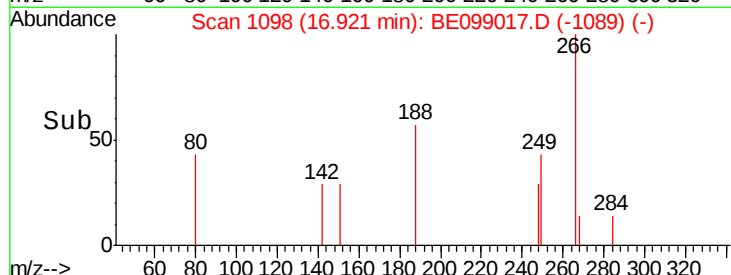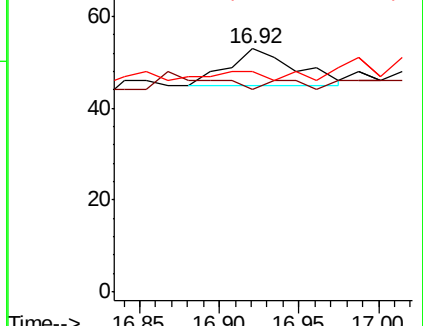

#25

Fluoranthene-d10

Concen: 0.349 ng

RT: 19.24 min Scan# 1389

Delta R.T. -0.01 min

Lab File: BE099017.D

Acq: 19 Mar 2019 1:47


Tgt Ion: 212 Resp: 36470

Ion Ratio Lower Upper

212 100

106 2.4 1.8 2.8



104 1.5 1.0 1.6




Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

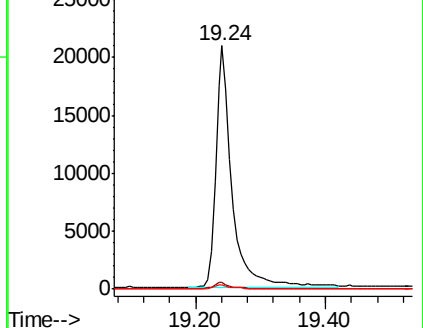







#27
 Chrysene-d12
 Concen: 0.400 ng
 RT: 21.40 min Scan# 1634
 Delta R.T. 0.00 min
 Lab File: BE099017.D
 Acq: 19 Mar 2019 1:47

Instrument :
 BNA_E
 ClientSampleId :
 BPS1-TT-MW202S-20190314

Tgt Ion:240 Resp: 7002
 Ion Ratio Lower Upper
 240 100
 120 7.6 5.0 7.4#
 236 28.0 22.7 34.1




Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E


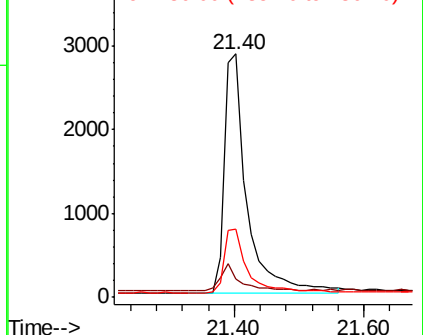



#29
 Terphenyl-d14
 Concen: 0.404 ng
 RT: 19.83 min Scan# 1492
 Delta R.T. -0.01 min
 Lab File: BE099017.D
 Acq: 19 Mar 2019 1:47

Tgt Ion:244 Resp: 6876
 Ion Ratio Lower Upper
 244 100
 212 39.6 29.4 44.2
 122 11.4 7.1 10.7#



Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E




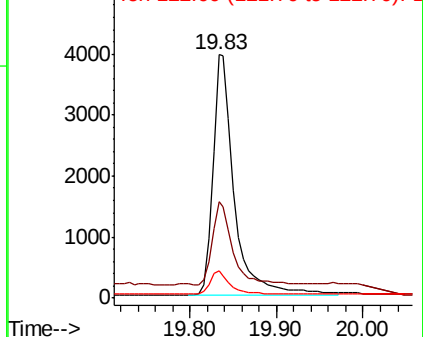




#32
 Bis(2-ethylhexyl)phthalate
 Concen: 0.033 ng
 RT: 21.29 min Scan# 1625
 Delta R.T. -0.01 min
 Lab File: BE099017.D
 Acq: 19 Mar 2019 1:47

Instrument :
 BNA_E
 ClientSampleId :
 BPS1-TT-MW202S-20190314

Tgt Ion:149 Resp: 1548
 Ion Ratio Lower Upper
 149 100
 167 6.4 5.4 8.0
 279 1.4 1.0 1.4

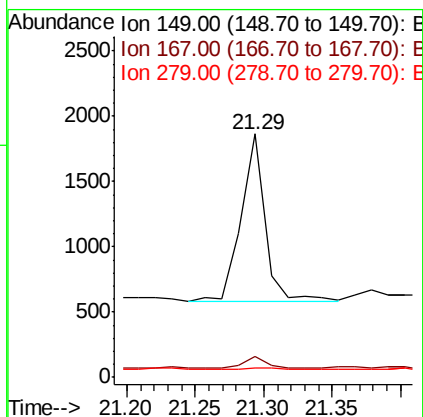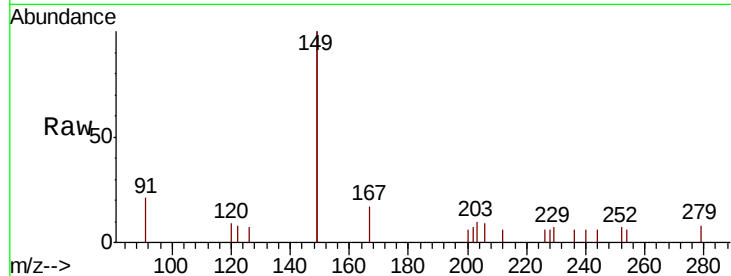

#34
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.89 min Scan# 2207
 Delta R.T. -0.01 min
 Lab File: BE099017.D
 Acq: 19 Mar 2019 1:47

Tgt Ion:264 Resp: 6621
 Ion Ratio Lower Upper
 264 100
 260 24.9 21.2 31.8
 265 28.6 24.6 36.8

