


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE031819\
 Data File : BE098993.D
 Acq On : 18 Mar 2019 10:22
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE030619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 15 05:31:33 2019

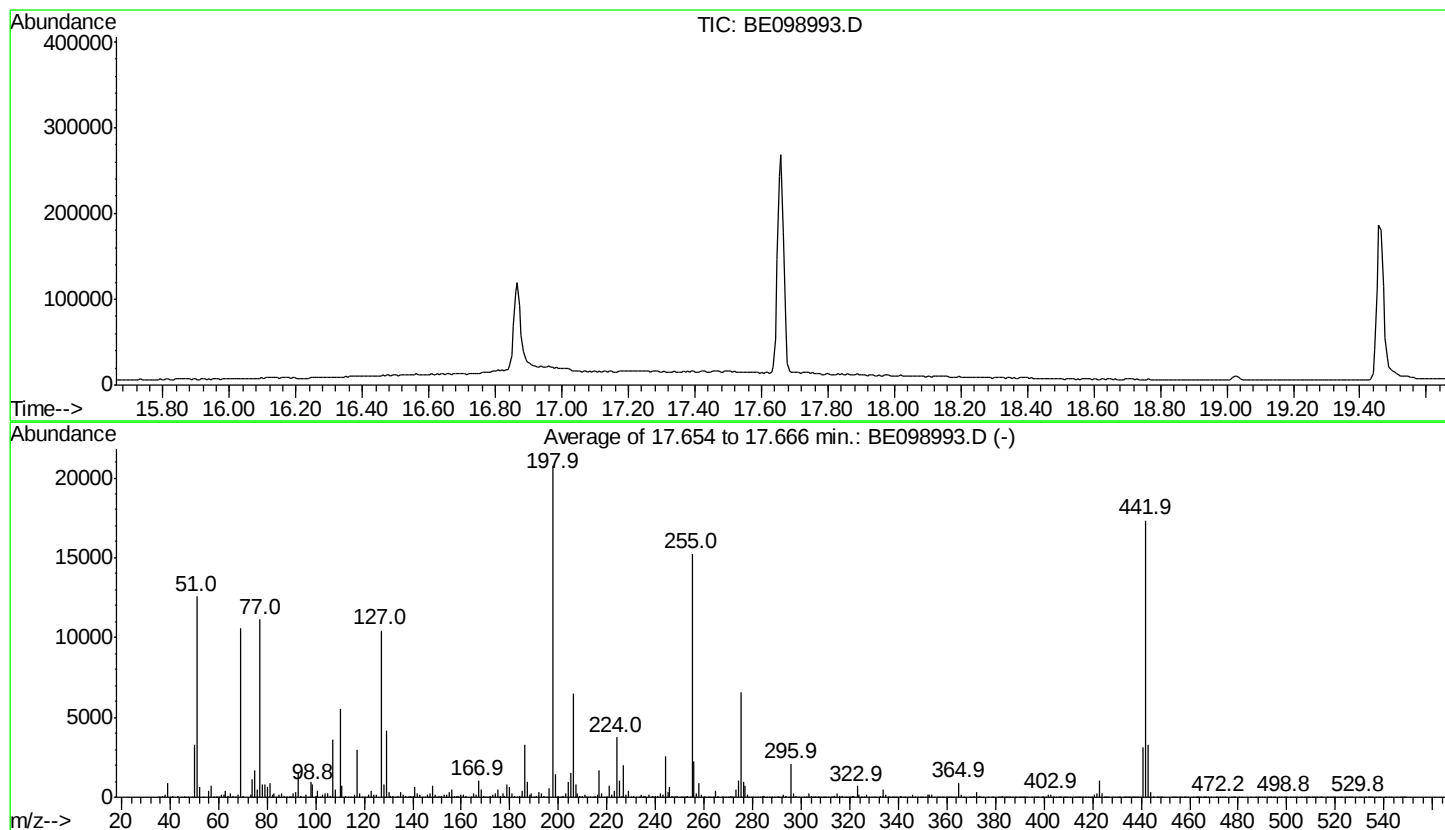

AutoFind: Scans 2564, 2565, 2566; Background Corrected with Scan 2556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.5	12568	PASS
68	69	0.00	2	1.2	130	PASS
69	198	0.00	100	50.9	10568	PASS
70	69	0.00	2	0.8	83	PASS
127	198	10	80	50.2	10425	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	20767	PASS
199	198	5	9	7.1	1476	PASS
275	198	10	60	31.6	6563	PASS
365	198	1	100	4.3	902	PASS
441	198	0.01	100	15.1	3130	PASS
442	198	50	100	83.5	17346	PASS
443	442	15	24	19.1	3315	PASS