

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE032019\
 Data File : BE099071.D
 Acq On : 20 Mar 2019 16:31
 Operator : JU/SJ
 Sample : K1985-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 BP-EB03-20190317

Quant Time: Mar 20 17:53:19 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE030619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 15 05:31:33 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	647	0.40	ng	0.00
7) Naphthalene-d8	10.59	136	3313	0.40	ng	0.00
13) Acenaphthene-d10	14.46	164	2350	0.40	ng	0.00
19) Phenanthrene-d10	17.22	188	5572	0.40	ng	0.00
27) Chrysene-d12	21.40	240	6297	0.40	ng	0.00
34) Perylene-d12	23.90	264	5444	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.43	112	119	0.06	ng	0.05
5) Phenol-d6	7.09	99	67	0.02	ng	0.11
8) Nitrobenzene-d5	9.02	82	497	0.14	ng	0.05
11) 2-Methylnaphthalene-d10	12.21	152	1245	0.20	ng	0.01
14) 2,4,6-Tribromophenol	15.98	330	181	0.15	ng	0.01
15) 2-Fluorobiphenyl	13.10	172	2127	0.22	ng	0.01
25) Fluoranthene-d10	19.25	212	17002	0.19	ng	0.00
29) Terphenyl-d14	19.84	244	3055	0.20	ng	0.00
Target Compounds						Qvalue
32) Bis(2-ethylhexyl)phthalate	21.29	149	2108	0.050	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE032019\
Data File : BE099071.D
Acq On : 20 Mar 2019 16:31
Operator : JU/SJ
Sample : K1985-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-EB03-20190317

Quant Time: Mar 20 17:53:19 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE030619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 15 05:31:33 2019
Response via : Initial Calibration




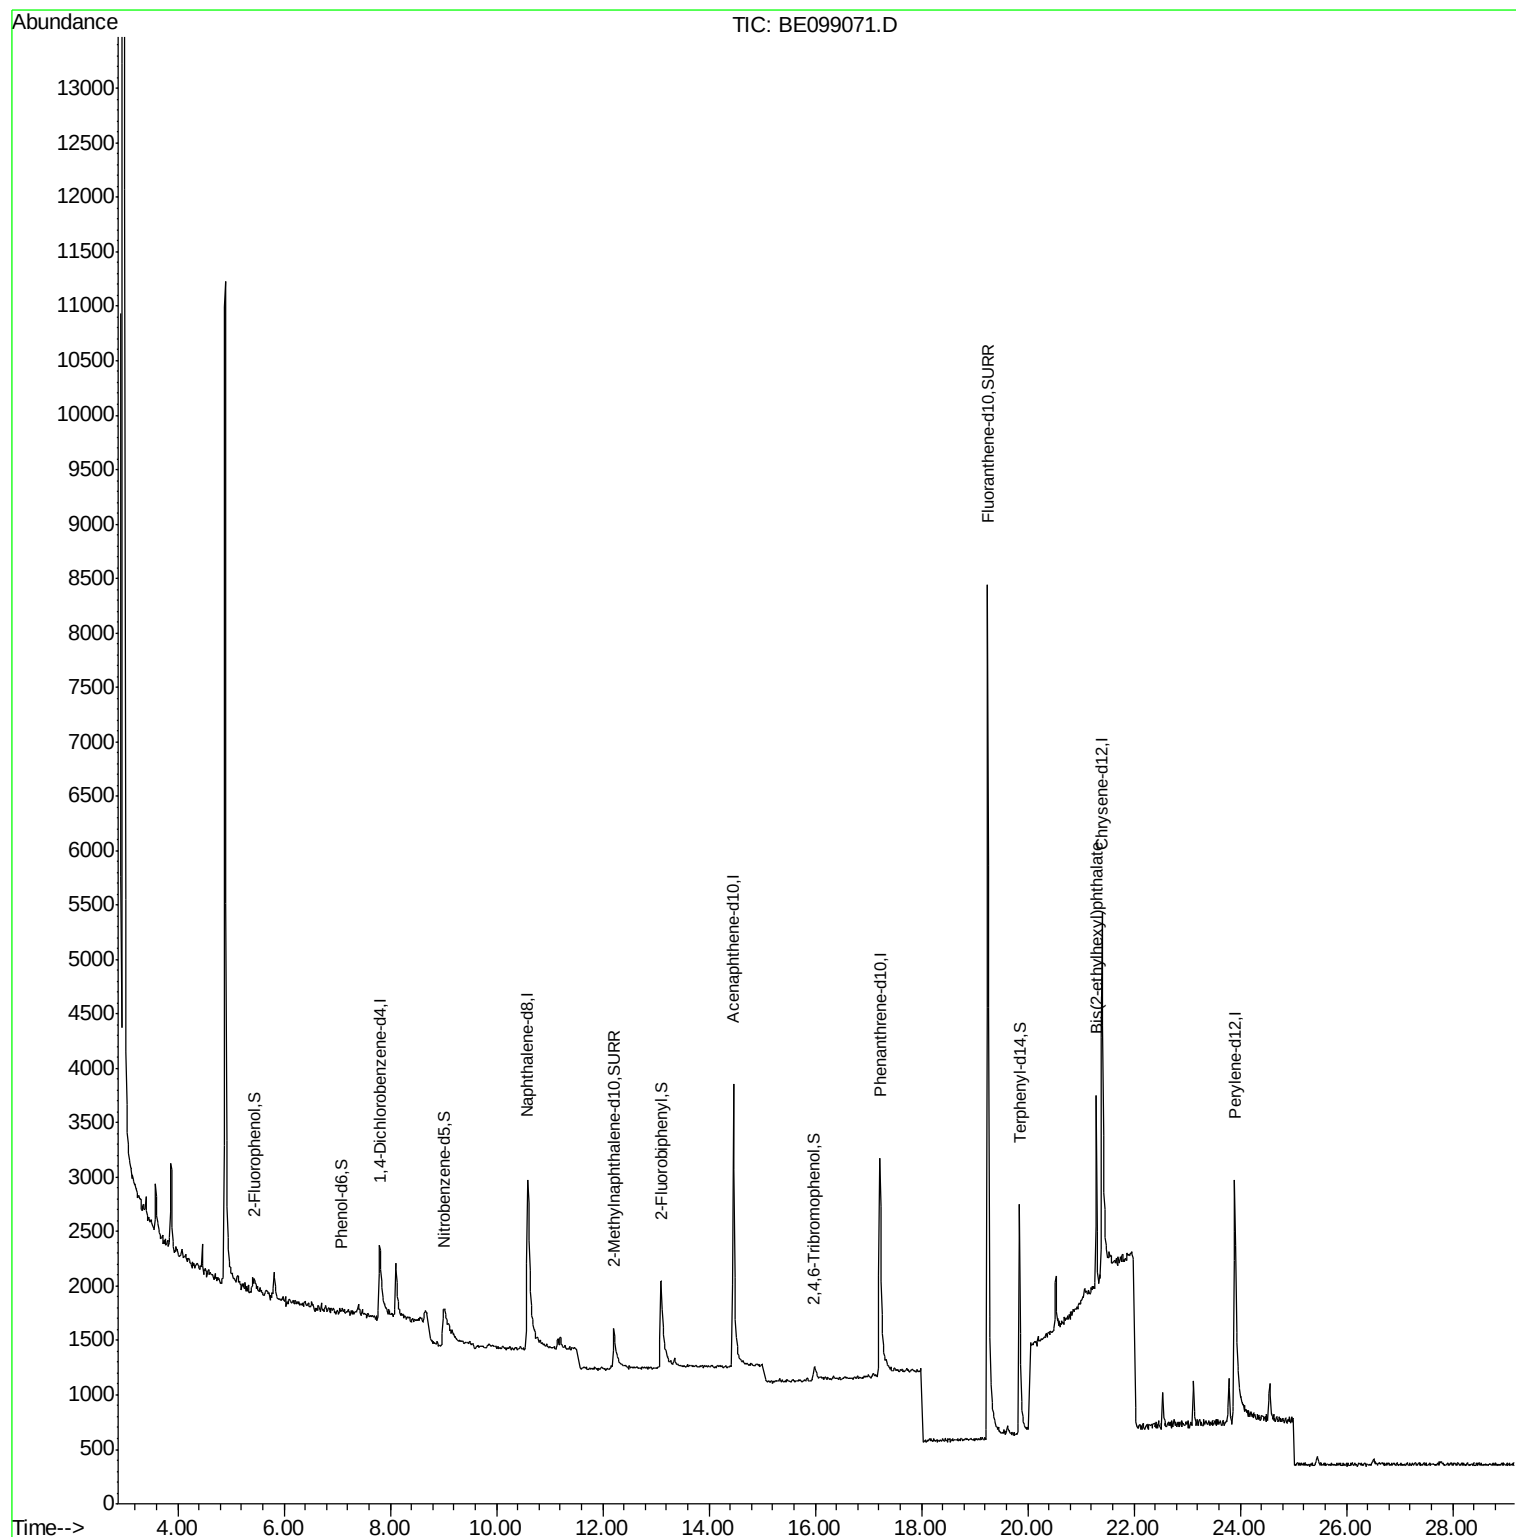


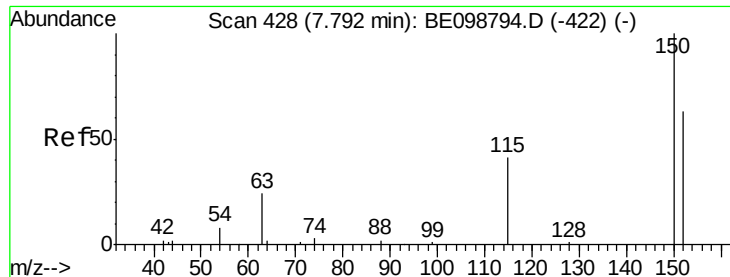

#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.80 min Scan# 428
 Delta R.T. 0.00 min
 Lab File: BE099071.D
 Acq: 20 Mar 2019 16:31




Instrument :
 BNA_E
 ClientSampleId :
 BP-EB03-20190317


Tot Ion:152 Resp: 647
 Ion Ratio Lower Upper
 152 100
 150 151.6 122.5 183.7
 115 82.9 57.4 86.2

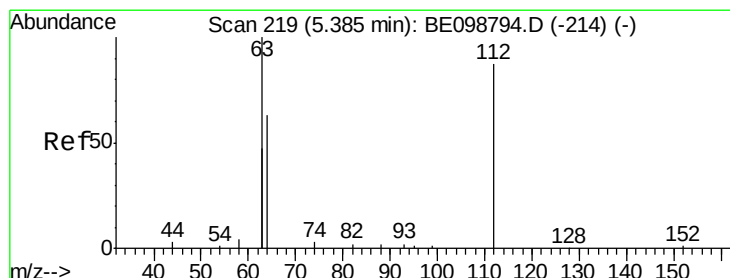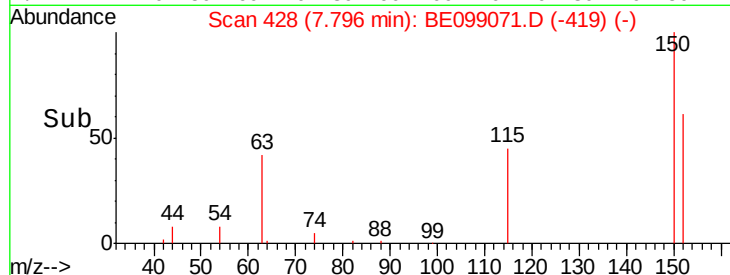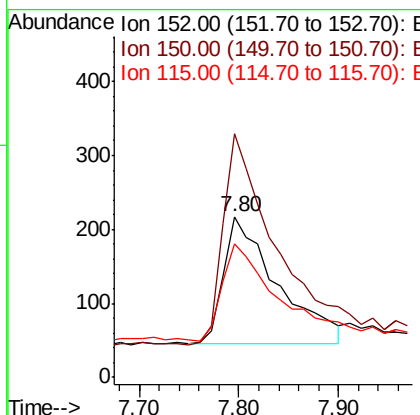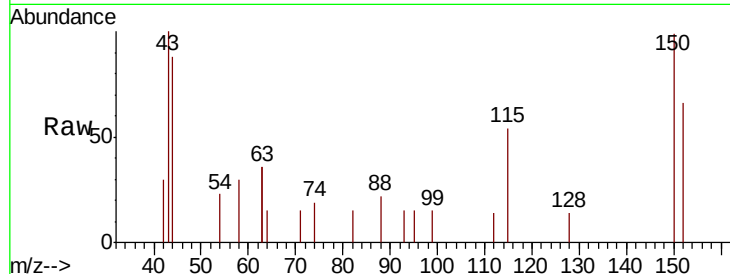

#4
 2-Fluorophenol
 Concen: 0.062 ng
 RT: 5.43 min Scan# 223
 Delta R.T. 0.05 min
 Lab File: BE099071.D
 Acq: 20 Mar 2019 16:31

Tgt Ion:112 Resp: 119
 Ion Ratio Lower Upper
 112 100
 64 95.0 57.9 86.9#
 63 230.3 158.3 237.5

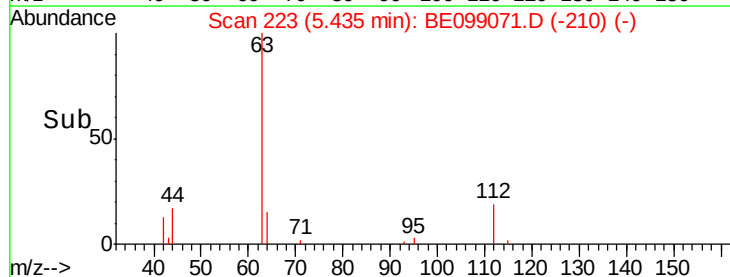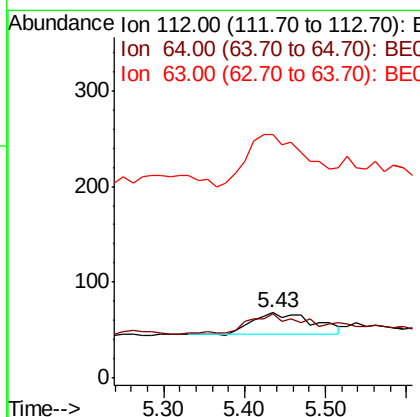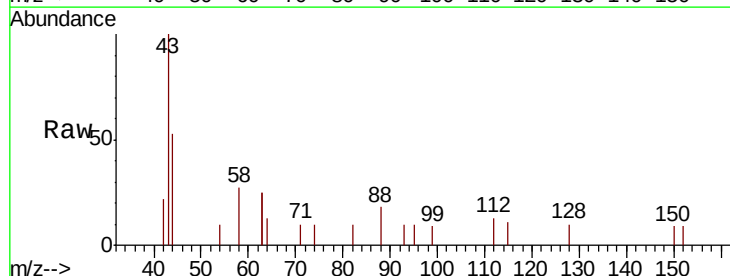

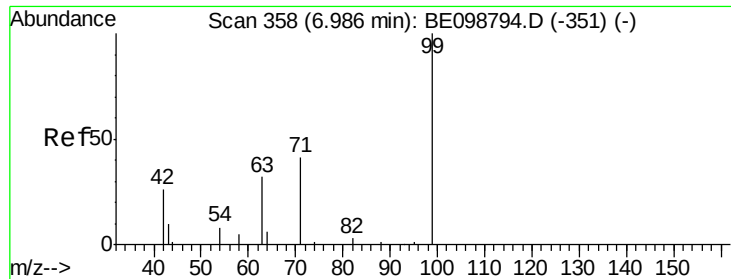

#5

Phenol-d6

Concen: 0.025 ng

RT: 7.09 min Scan# 367

Delta R.T. 0.11 min

Lab File: BE099071.D

Acq: 20 Mar 2019 16:31

Instrument :

BNA_E

ClientSampleId :

BP-EB03-20190317


Tot Ion: 99 Resp: 67

Ion Ratio Lower Upper

99 100

42 0.0 24.2 36.2#


71 0.0 35.7 53.5#

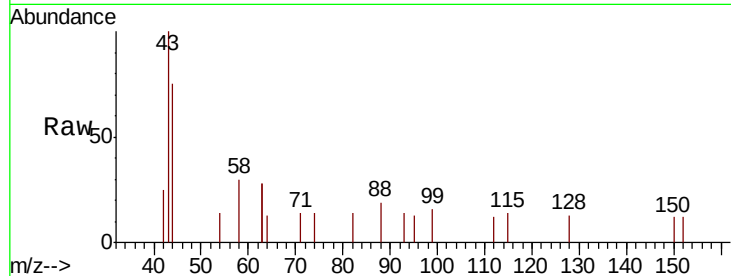



Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

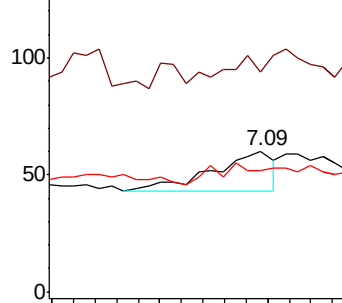

Time--> 6.90 7.00 7.10

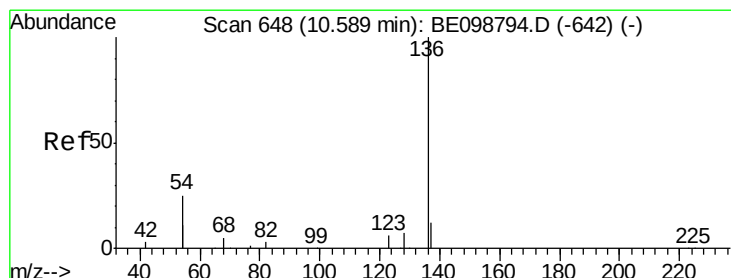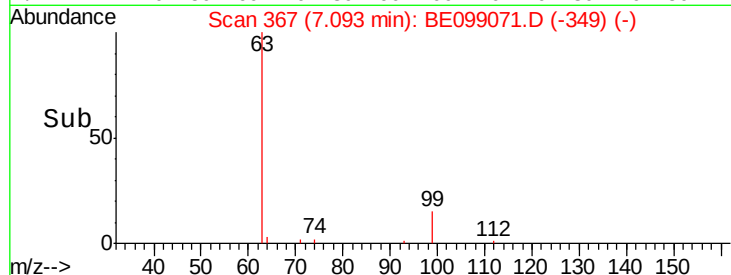

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.59 min Scan# 648

Delta R.T. -0.00 min

Lab File: BE099071.D

Acq: 20 Mar 2019 16:31

Tgt Ion: 136 Resp: 3313


Ion Ratio Lower Upper

136 100

137 15.0 11.4 17.0

54 76.4 39.3 58.9#

68 11.8 6.7 10.1#

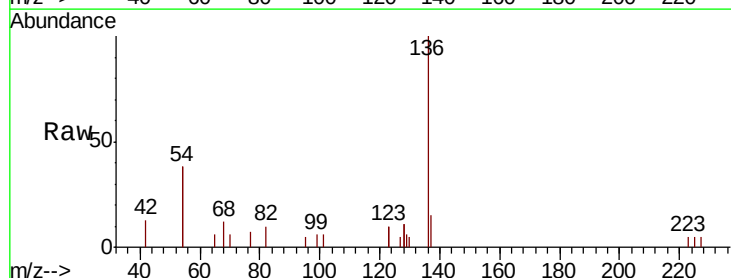


Abundance Ion 136.00 (135.70 to 136.70): E


Ion 137.00 (136.70 to 137.70): E


Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

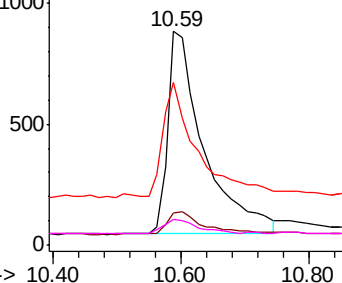

Time--> 10.40 10.60 10.80

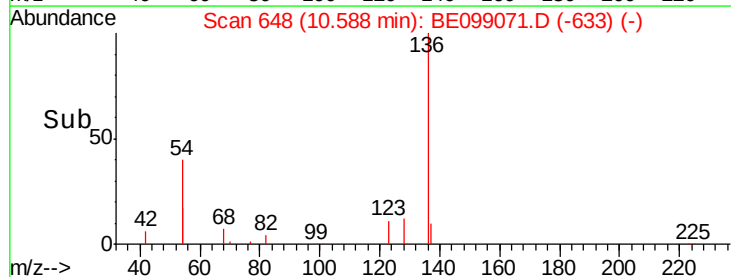


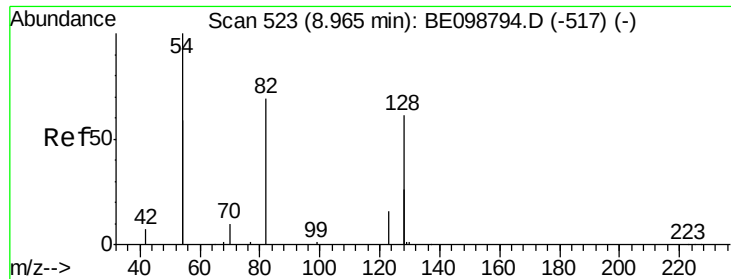




#8
 Nitrobenzene-d5
 Concen: 0.143 ng
 RT: 9.02 min Scan# 527
 Delta R.T. 0.05 min
 Lab File: BE099071.D
 Acq: 20 Mar 2019 16:31

Instrument :
 BNA_E
 ClientSampleId :
 BP-EB03-20190317

Tot Ion	82	Resp	497
Ion	Ratio	Lower	Upper
82	100		
128	233.9	123.8	185.8#
54	311.9	203.4	305.2#

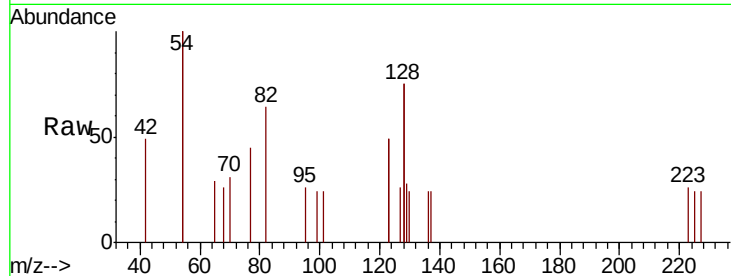


Abundance Ion 82.00 (81.70 to 82.70): BE0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BE0

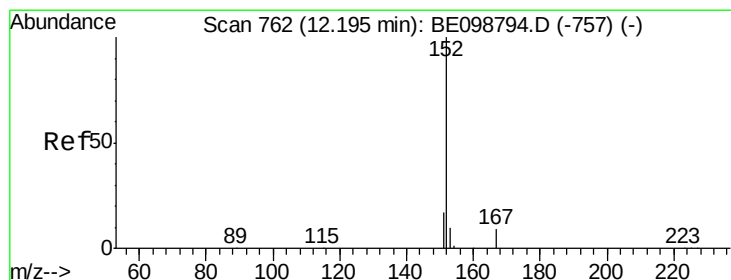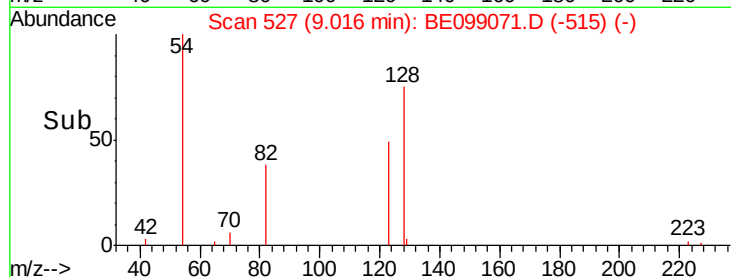
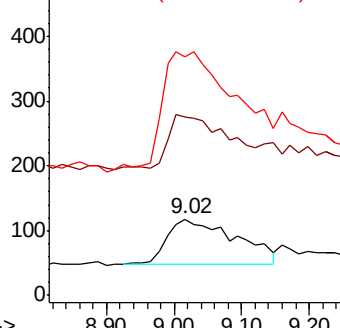



#11
 2-Methylnaphthalene-d10
 Concen: 0.203 ng
 RT: 12.21 min Scan# 763
 Delta R.T. 0.01 min
 Lab File: BE099071.D
 Acq: 20 Mar 2019 16:31

Tgt Ion	152	Resp	1245
Ion	Ratio	Lower	Upper
152	100		
151	21.3	16.5	24.7

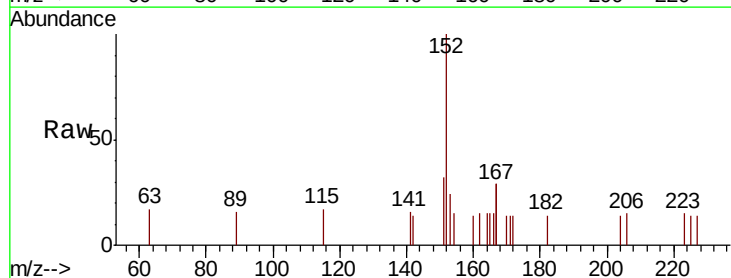

Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 151.00 (150.70 to 151.70): E

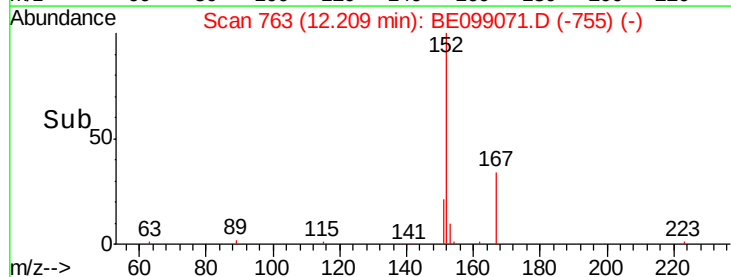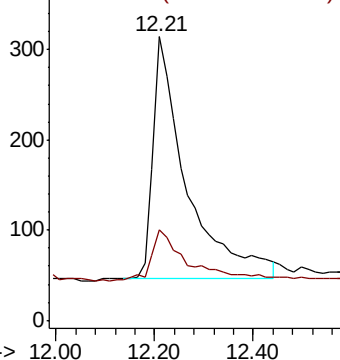


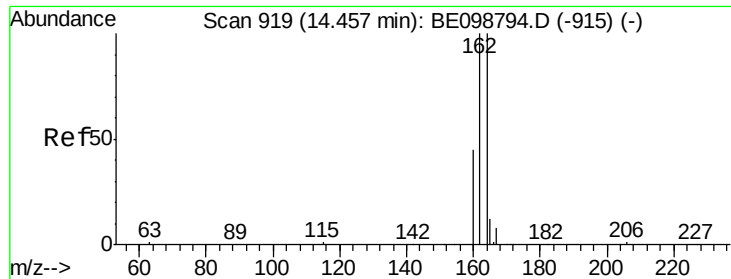




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.46 min Scan# 919
Delta R.T. 0.00 min
Lab File: BE099071.D
Acq: 20 Mar 2019 16:31

Instrument :
BNA_E
ClientSampleId :
BP-EB03-20190317

Tot Ion:164 Resp: 2350
Ion Ratio Lower Upper
164 100
162 102.8 80.2 120.2
160 51.4 37.8 56.8

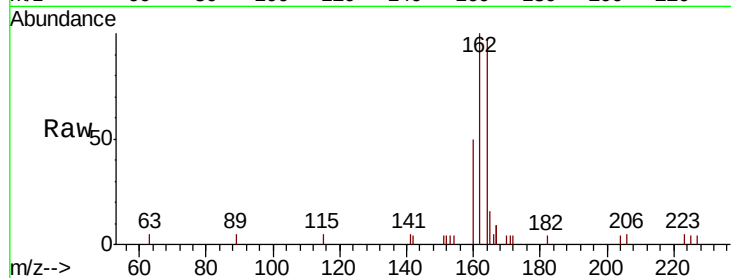


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

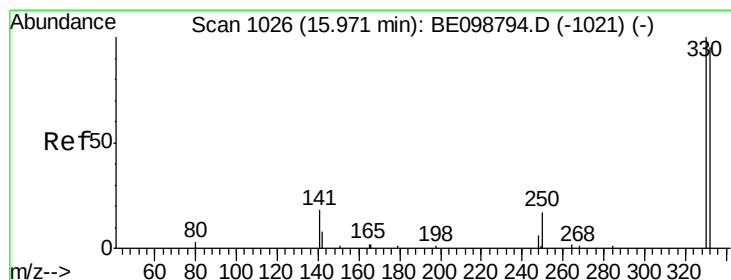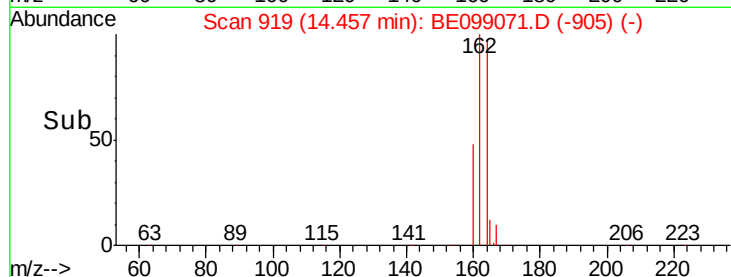
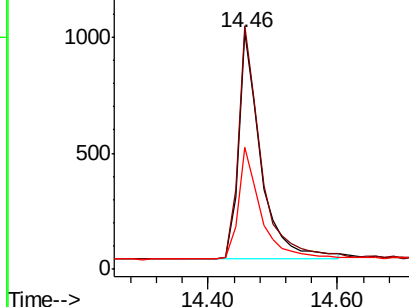



#14
2,4,6-Tribromophenol
Concen: 0.153 ng
RT: 15.98 min Scan# 1027
Delta R.T. 0.01 min
Lab File: BE099071.D
Acq: 20 Mar 2019 16:31

Tgt Ion:330 Resp: 181
Ion Ratio Lower Upper
330 100
332 92.3 77.6 116.4
141 45.9 31.0 46.4

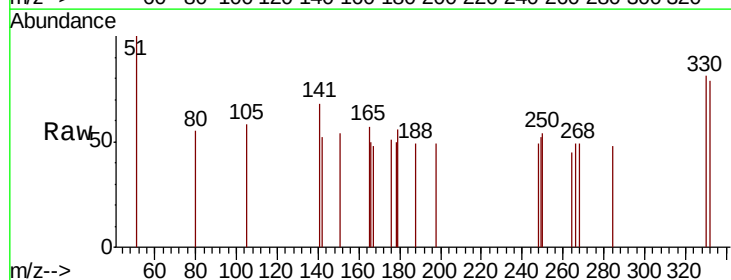

Abundance Ion 330.00 (329.70 to 330.70): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

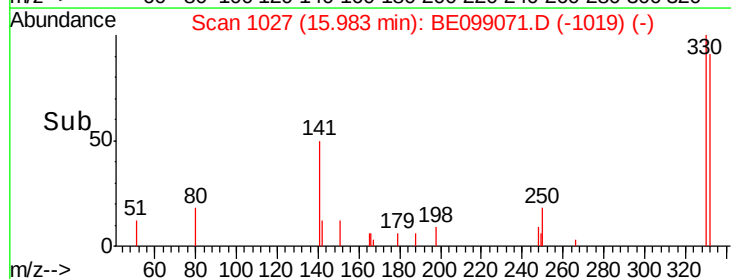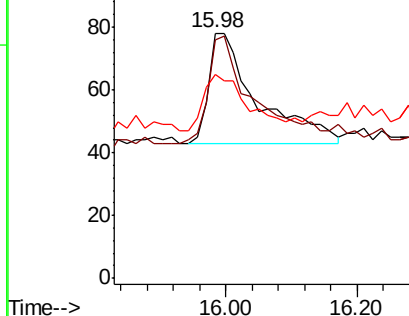


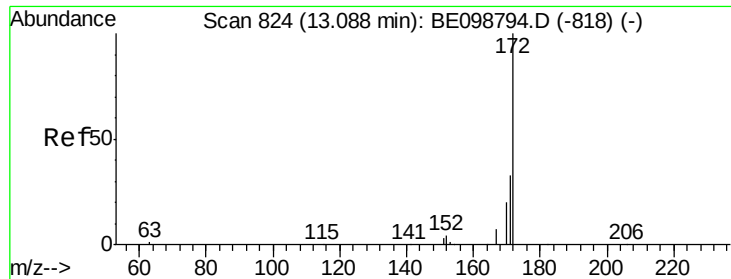




#15
2-Fluorobiphenyl
Concen: 0.219 ng
RT: 13.10 min Scan# 825
Delta R.T. 0.01 min
Lab File: BE099071.D
Acq: 20 Mar 2019 16:31

Instrument :
BNA_E
ClientSampleId :
BP-EB03-20190317

Tot Ion:172 Resp: 2127
Ion Ratio Lower Upper
172 100
171 38.2 28.0 42.0
170 27.6 17.7 26.5#

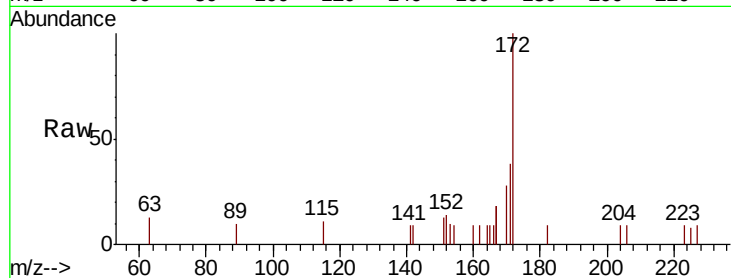


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

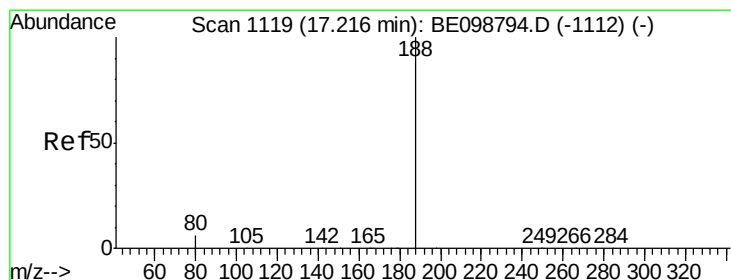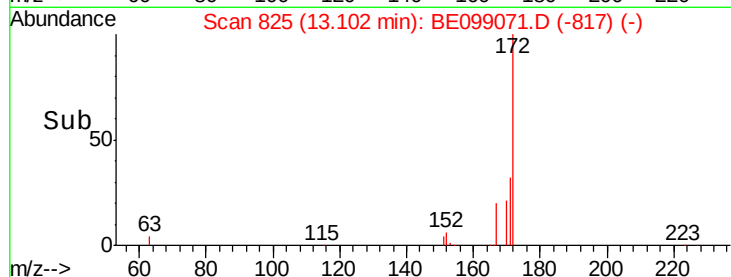
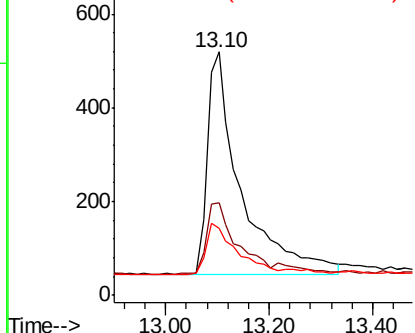



#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.22 min Scan# 1119
Delta R.T. -0.00 min
Lab File: BE099071.D
Acq: 20 Mar 2019 16:31

Tgt Ion:188 Resp: 5572
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 12.8 6.3 9.5#

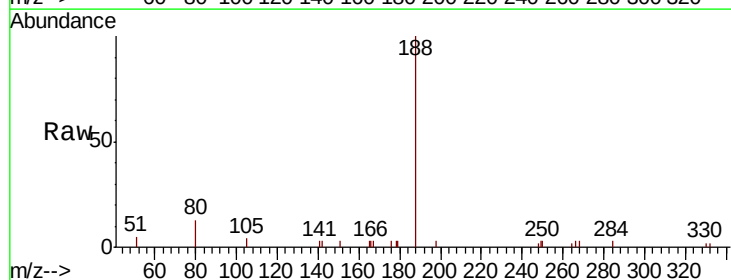

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BE0
Ion 80.00 (79.70 to 80.70): BE0



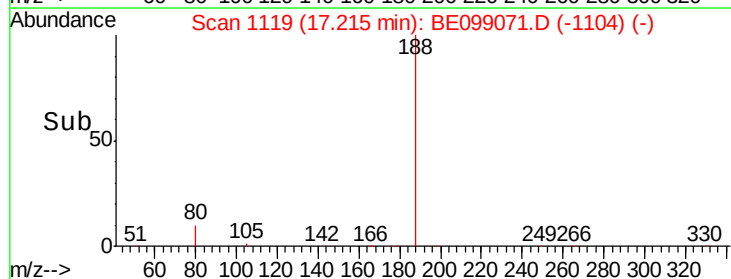
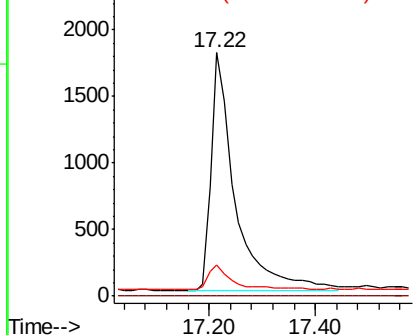


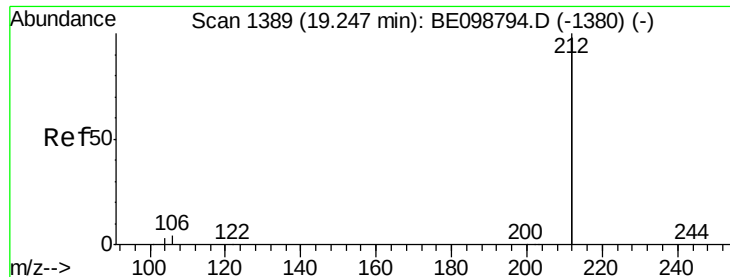

#25
 Fluoranthene-d10
 Concen: 0.191 ng
 RT: 19.25 min Scan# 1389
 Delta R.T. -0.00 min
 Lab File: BE099071.D
 Acq: 20 Mar 2019 16:31




Instrument :
 BNA_E
 ClientSampleId :
 BP-EB03-20190317


Tot Ion:212 Resp: 17002
 Ion Ratio Lower Upper
 212 100
 106 2.4 1.8 2.8
 104 1.2 1.0 1.6

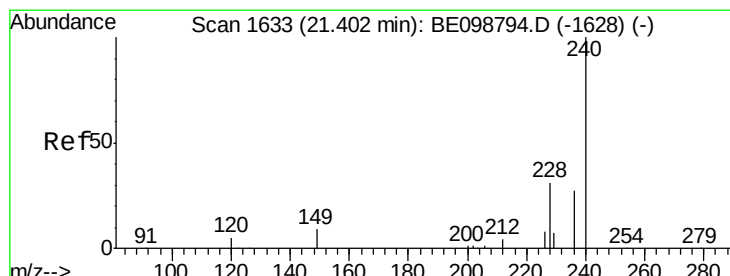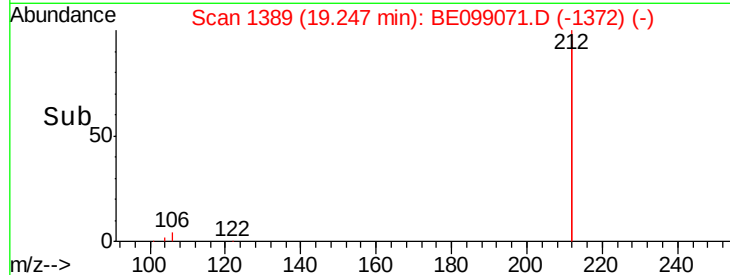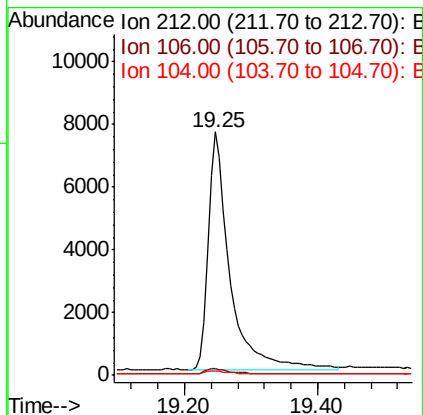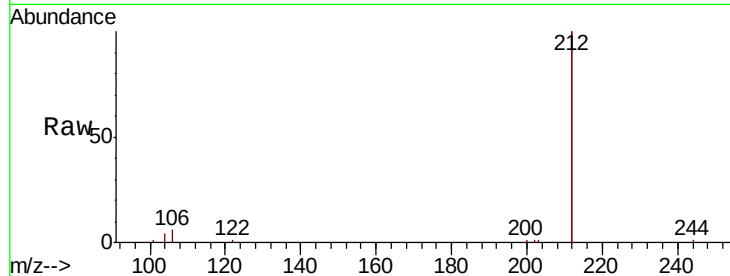

#27
 Chrysene-d12
 Concen: 0.400 ng
 RT: 21.40 min Scan# 1633
 Delta R.T. -0.00 min
 Lab File: BE099071.D
 Acq: 20 Mar 2019 16:31

Tgt Ion:240 Resp: 6297
 Ion Ratio Lower Upper
 240 100
 120 9.9 5.0 7.4#
 236 29.7 22.7 34.1

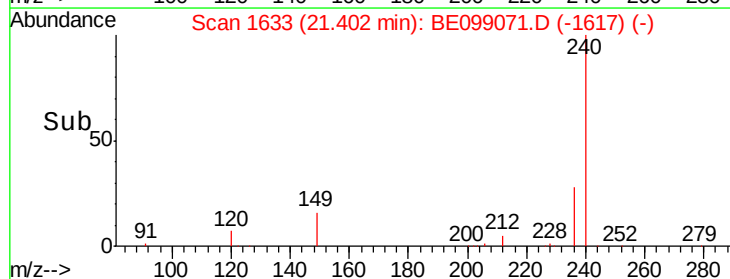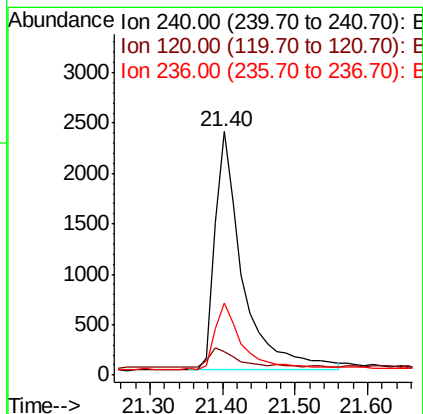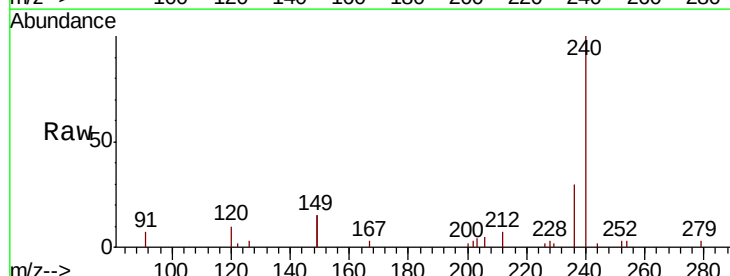

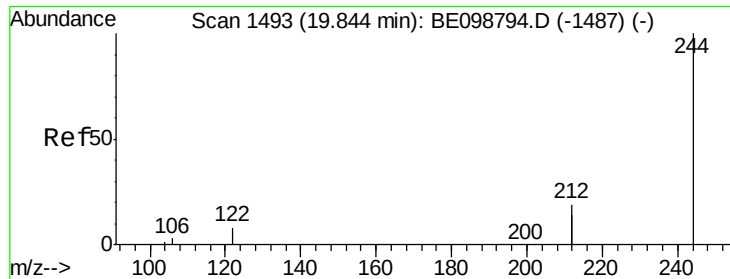

#29

Terphenyl-d14

Concen: 0.200 ng

RT: 19.84 min Scan# 1493

Delta R.T. -0.00 min

Lab File: BE099071.D

Acq: 20 Mar 2019 16:31

Instrument :

BNA_E

ClientSampleId :

BP-EB03-20190317


Tot Ion:244 Resp: 3055

Ion Ratio Lower Upper

244 100

212 46.0 29.4 44.2#




122 11.6 7.1 10.7#

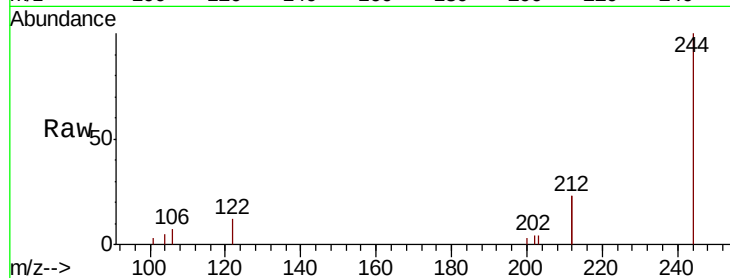

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

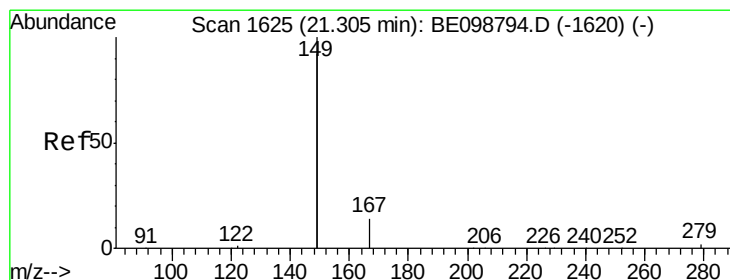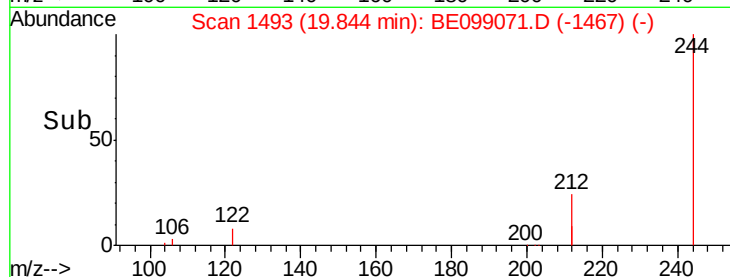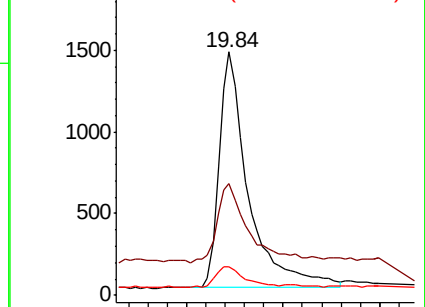

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.050 ng

RT: 21.29 min Scan# 1624

Delta R.T. -0.01 min

Lab File: BE099071.D

Acq: 20 Mar 2019 16:31


Tgt Ion:149 Resp: 2108

Ion Ratio Lower Upper

149 100

167 6.9 5.4 8.0



279 1.3 1.0 1.4



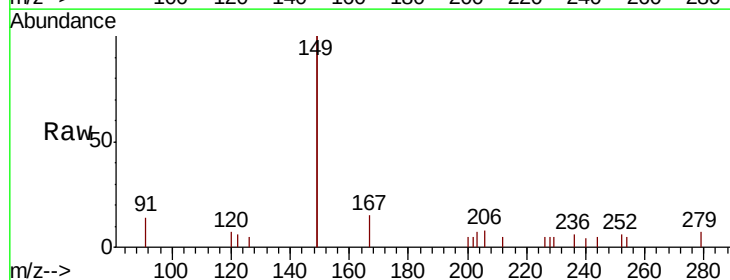


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

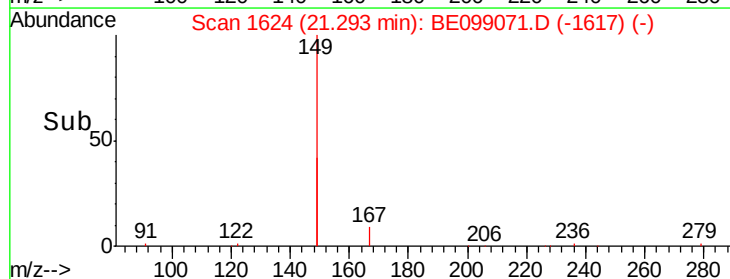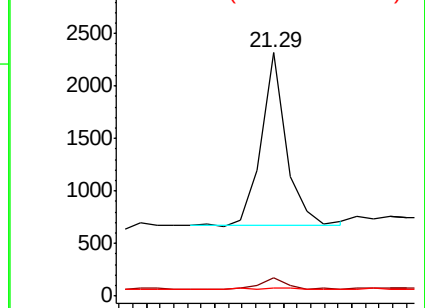

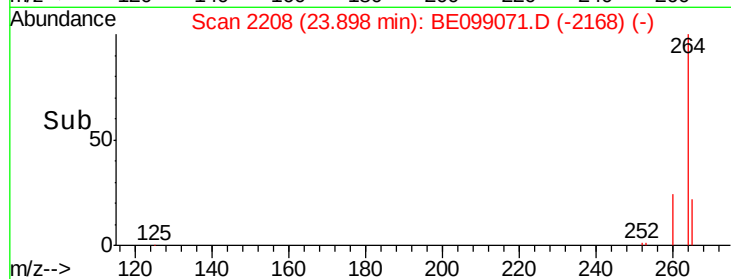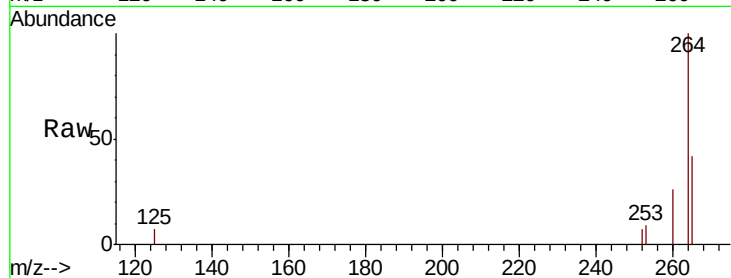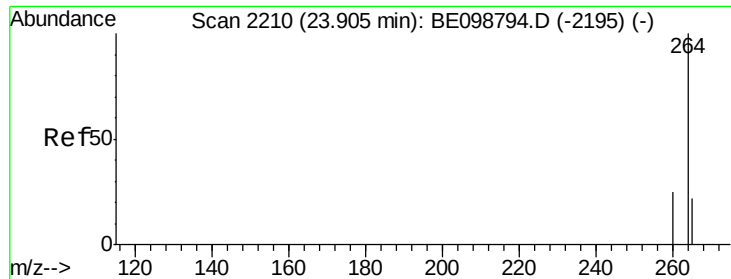

#34
 Pervlene-d12
 Concen: 0.400 ng
 RT: 23.90 min Scan# 2208
 Delta R.T. -0.01 min
 Lab File: BE099071.D
 Acq: 20 Mar 2019 16:31

Instrument :
 BNA_E
 ClientSampleId :
 BP-EB03-20190317

Tot Ion:264 Resp: 5444
 Ion Ratio Lower Upper
 264 100
 260 26.4 21.2 31.8
 265 41.8 24.6 36.8#

