


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE032019\
 Data File : BE099066.D
 Acq On : 20 Mar 2019 11:30
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE030619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 15 05:31:33 2019

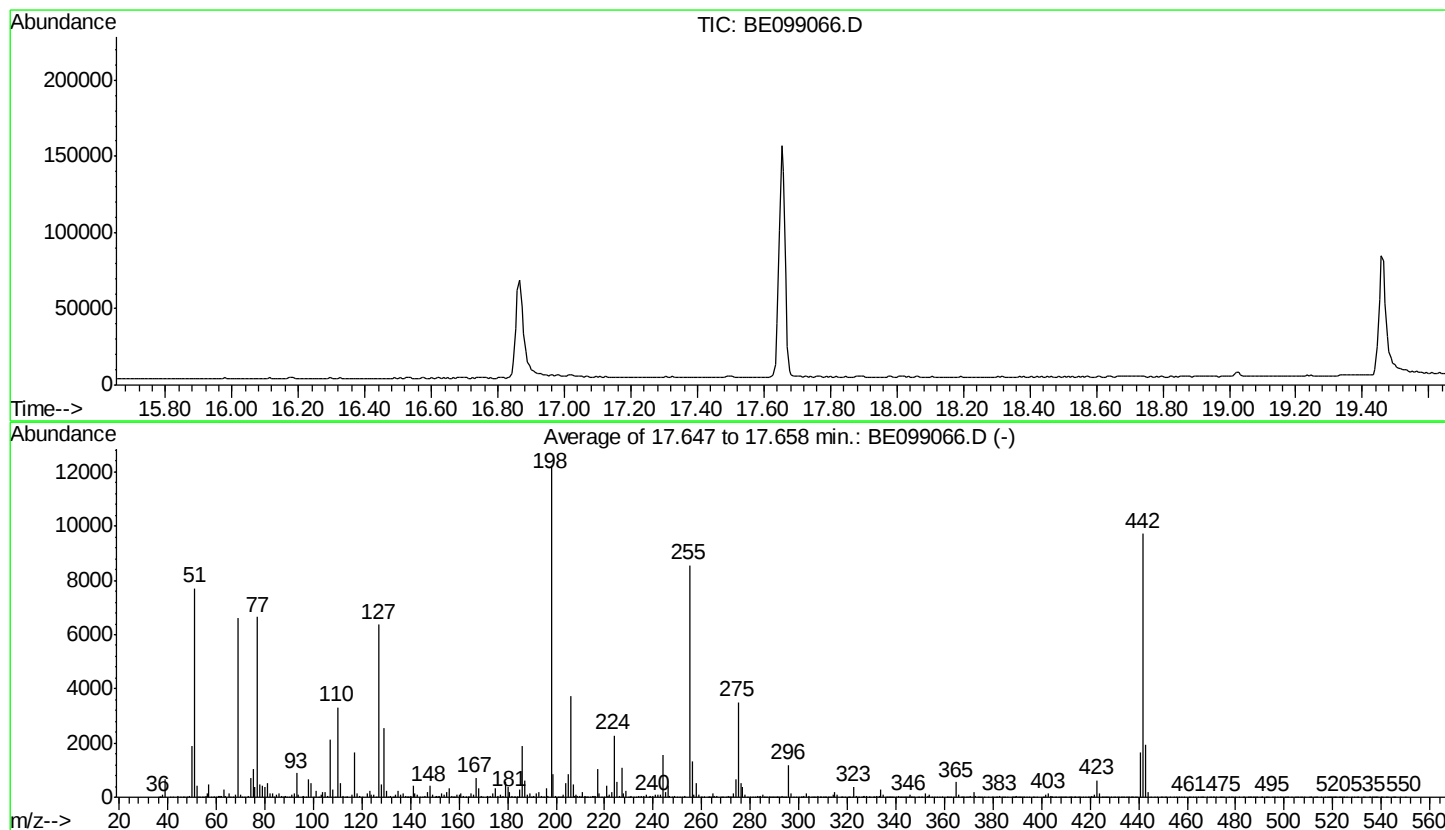

AutoFind: Scans 2563, 2564, 2565; Background Corrected with Scan 2556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	63.1	7714	PASS
68	69	0.00	2	1.2	80	PASS
69	198	0.00	100	53.9	6596	PASS
70	69	0.00	2	1.3	86	PASS
127	198	10	80	51.9	6355	PASS
197	198	0.00	2	0.3	38	PASS
198	198	100	100	100.0	12234	PASS
199	198	5	9	7.0	859	PASS
275	198	10	60	28.7	3510	PASS
365	198	1	100	4.6	564	PASS
441	198	0.01	100	13.4	1635	PASS
442	198	50	100	79.4	9709	PASS
443	442	15	24	20.1	1953	PASS