


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE032219\
 Data File : BE099074.D
 Acq On : 22 Mar 2019 10:05
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE032219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 23 04:40:11 2019

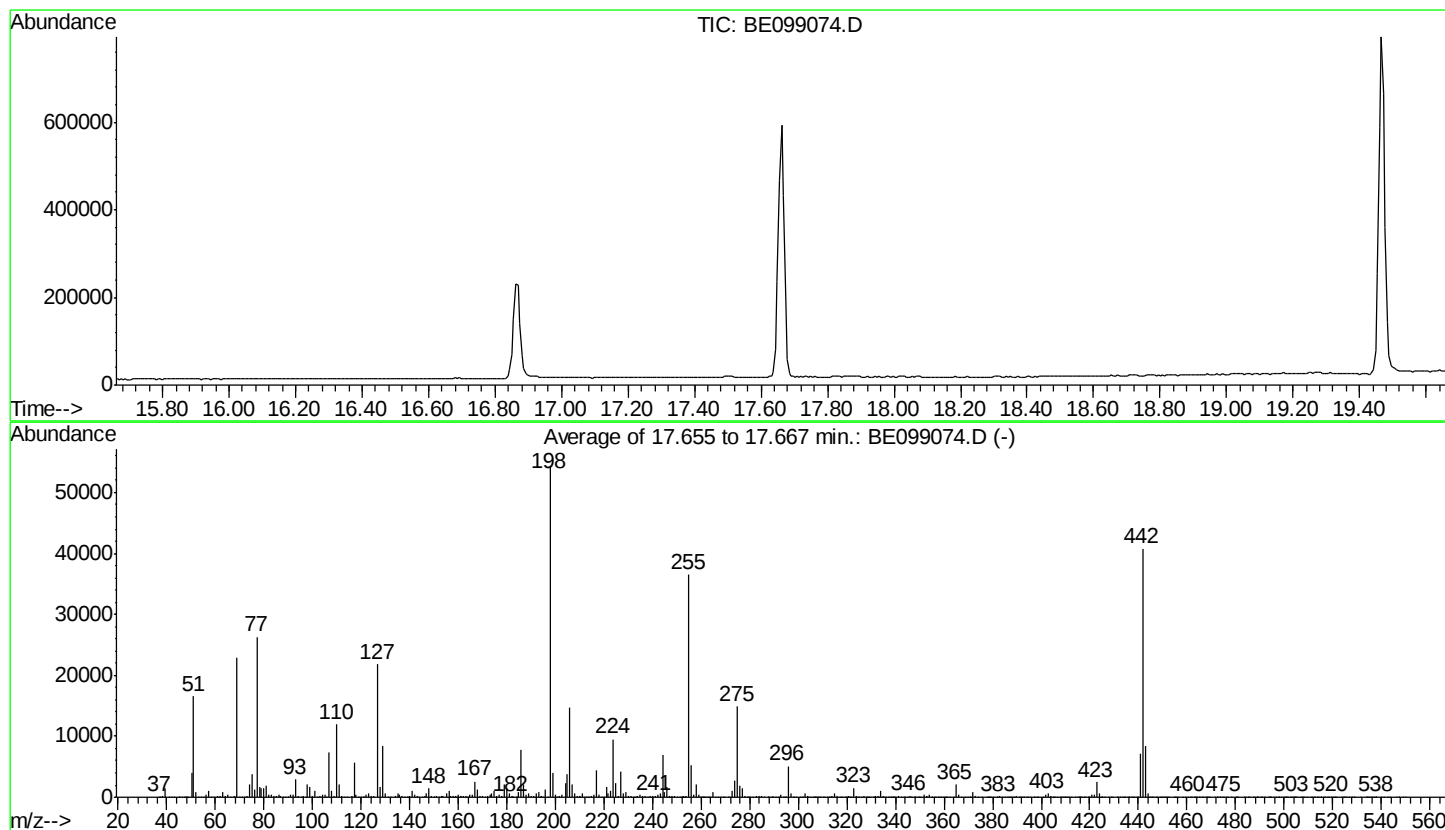

AutoFind: Scans 2564, 2565, 2566; Background Corrected with Scan 2555

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.4	16527	PASS
68	69	0.00	2	0.9	211	PASS
69	198	0.00	100	42.2	22964	PASS
70	69	0.00	2	0.5	105	PASS
127	198	10	80	40.0	21782	PASS
197	198	0.00	2	0.2	98	PASS
198	198	100	100	100.0	54400	PASS
199	198	5	9	7.2	3932	PASS
275	198	10	60	27.2	14815	PASS
365	198	1	100	3.8	2070	PASS
441	198	0.01	100	13.1	7149	PASS
442	198	50	100	75.1	40846	PASS
443	442	15	24	20.8	8498	PASS