


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE032219\
Data File : BE099083.D
Acq On : 22 Mar 2019 16:51
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE032219.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Mar 23 04:40:11 2019

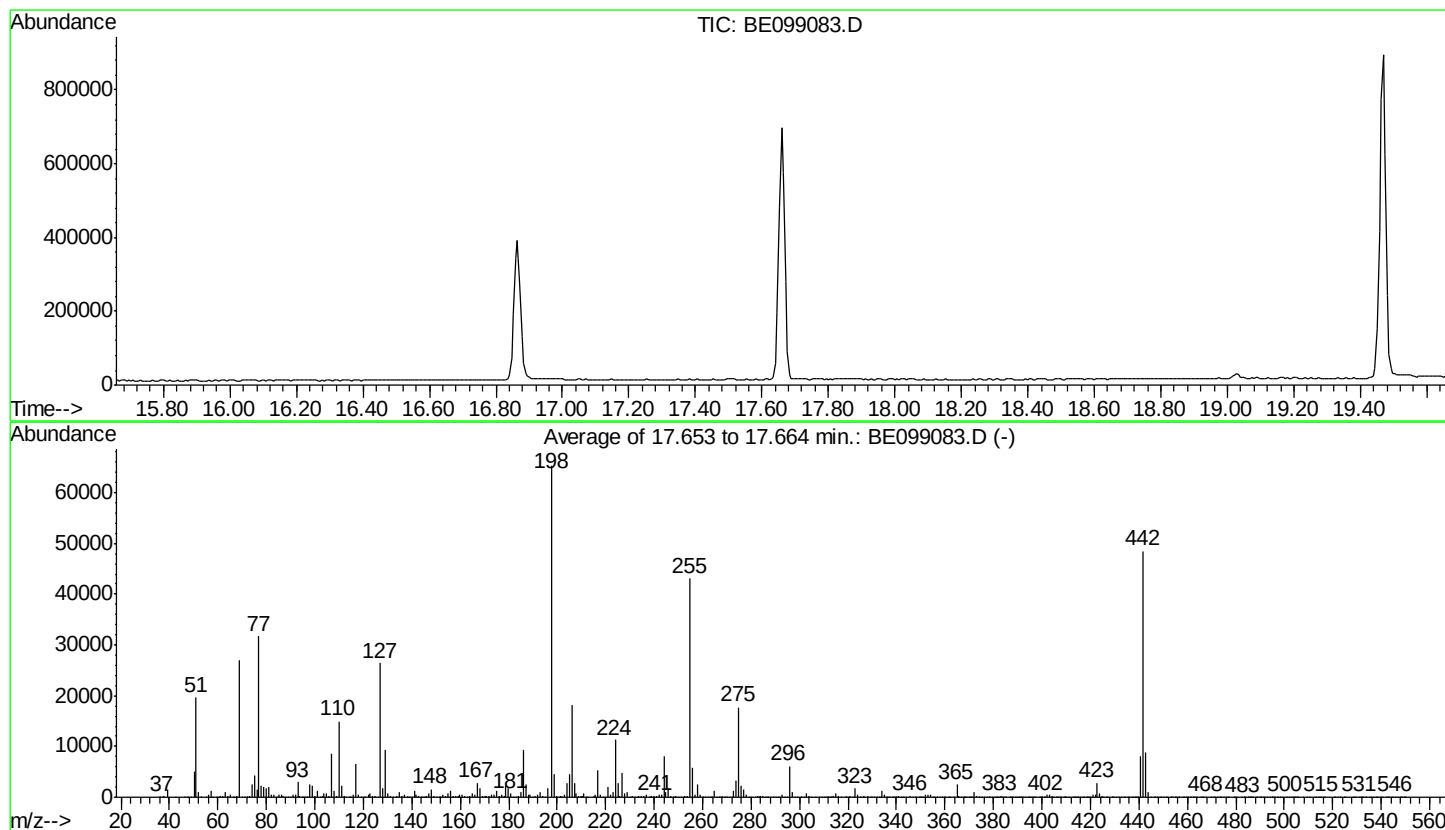

AutoFind: Scans 2564, 2565, 2566; Background Corrected with Scan 2556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.9	19548	PASS
68	69	0.00	2	1.1	295	PASS
69	198	0.00	100	41.4	27056	PASS
70	69	0.00	2	0.4	99	PASS
127	198	10	80	40.4	26394	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	65312	PASS
199	198	5	9	6.9	4531	PASS
275	198	10	60	27.1	17703	PASS
365	198	1	100	3.7	2440	PASS
441	198	0.01	100	12.3	8049	PASS
442	198	50	100	74.3	48498	PASS
443	442	15	24	18.3	8853	PASS