


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE032319\
 Data File : BE099102.D
 Acq On : 23 Mar 2019 8:17
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE032219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 23 04:40:11 2019

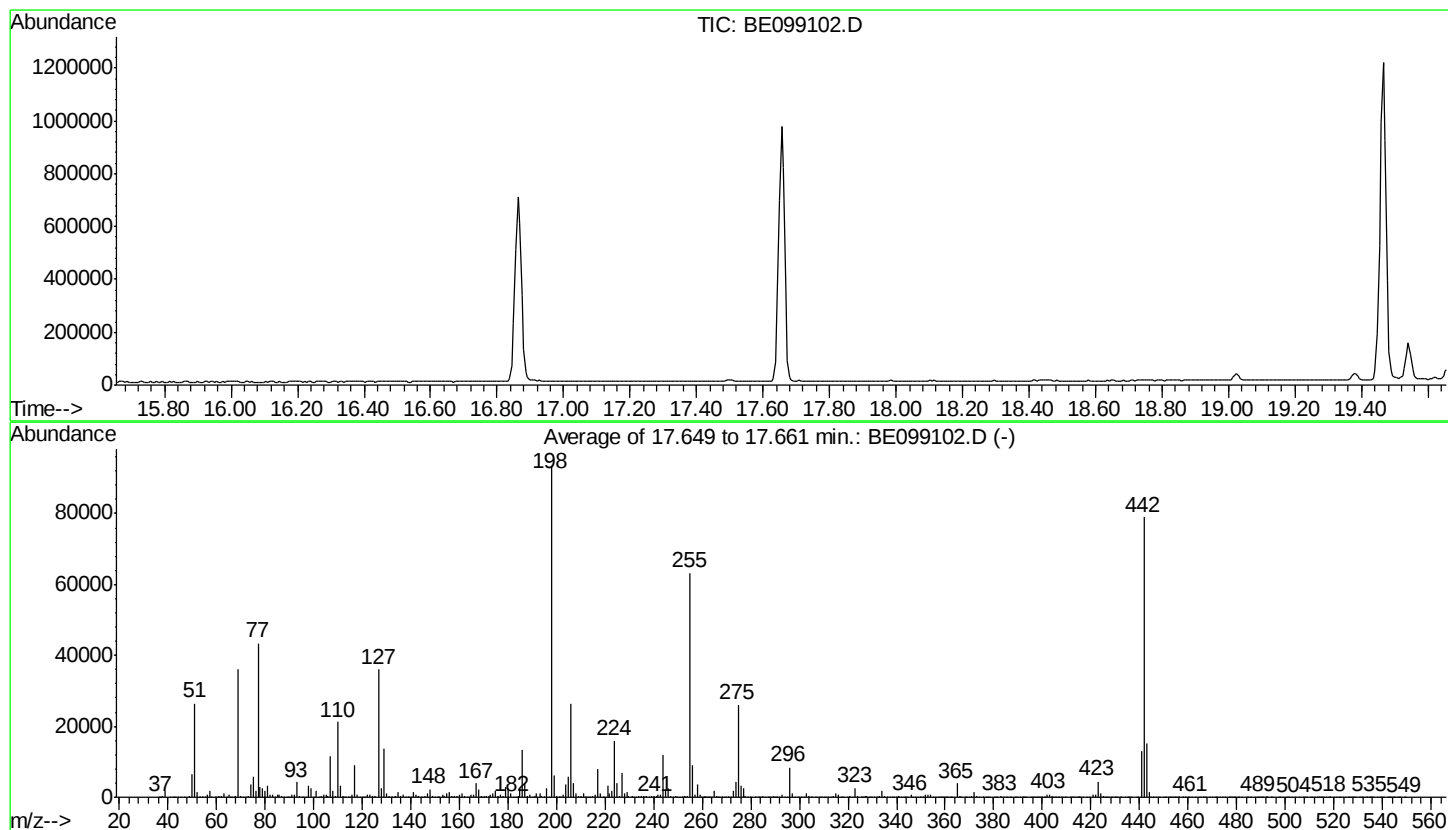

AutoFind: Scans 2563, 2564, 2565; Background Corrected with Scan 2556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.4	26543	PASS
68	69	0.00	2	1.0	359	PASS
69	198	0.00	100	38.8	36264	PASS
70	69	0.00	2	0.6	221	PASS
127	198	10	80	38.5	35999	PASS
197	198	0.00	2	0.1	134	PASS
198	198	100	100	100.0	93522	PASS
199	198	5	9	6.7	6253	PASS
275	198	10	60	27.9	26115	PASS
365	198	1	100	4.2	3883	PASS
441	198	0.01	100	14.0	13133	PASS
442	198	50	100	84.5	78980	PASS
443	442	15	24	19.4	15329	PASS