


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE032319\
 Data File : BE099121.D
 Acq On : 23 Mar 2019 21:25
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE032219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 23 04:40:11 2019

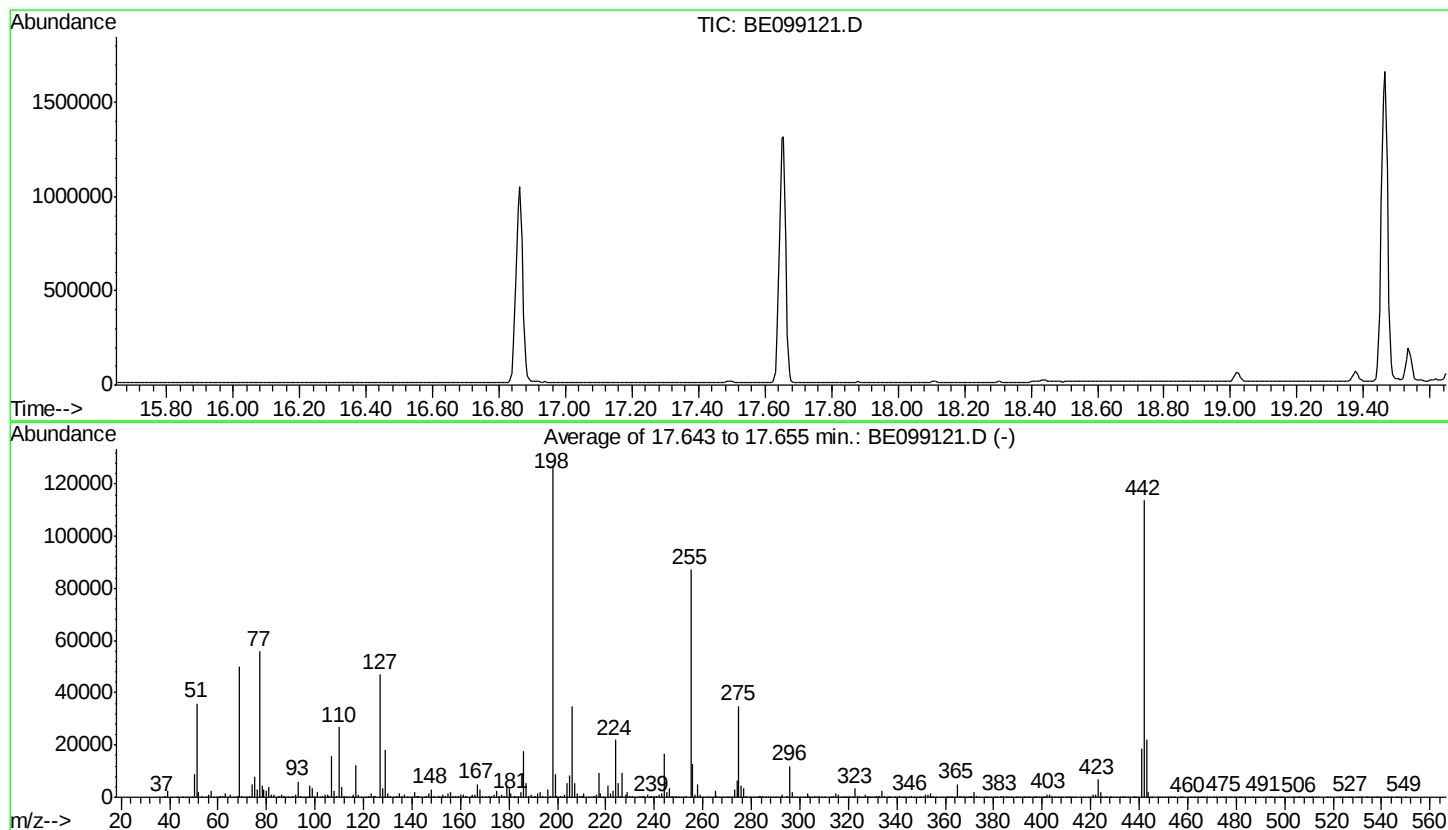

AutoFind: Scans 2562, 2563, 2564; Background Corrected with Scan 2554

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.2	35810	PASS
68	69	0.00	2	1.4	676	PASS
69	198	0.00	100	39.3	49936	PASS
70	69	0.00	2	0.6	282	PASS
127	198	10	80	37.0	47061	PASS
197	198	0.00	2	0.3	387	PASS
198	198	100	100	100.0	127048	PASS
199	198	5	9	6.8	8616	PASS
275	198	10	60	27.5	34888	PASS
365	198	1	100	4.0	5118	PASS
441	198	0.01	100	14.6	18532	PASS
442	198	50	100	89.5	113733	PASS
443	442	15	24	19.5	22187	PASS