


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE032519\
 Data File : BE099174.D
 Acq On : 25 Mar 2019 8:37
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE032519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 26 07:02:06 2019

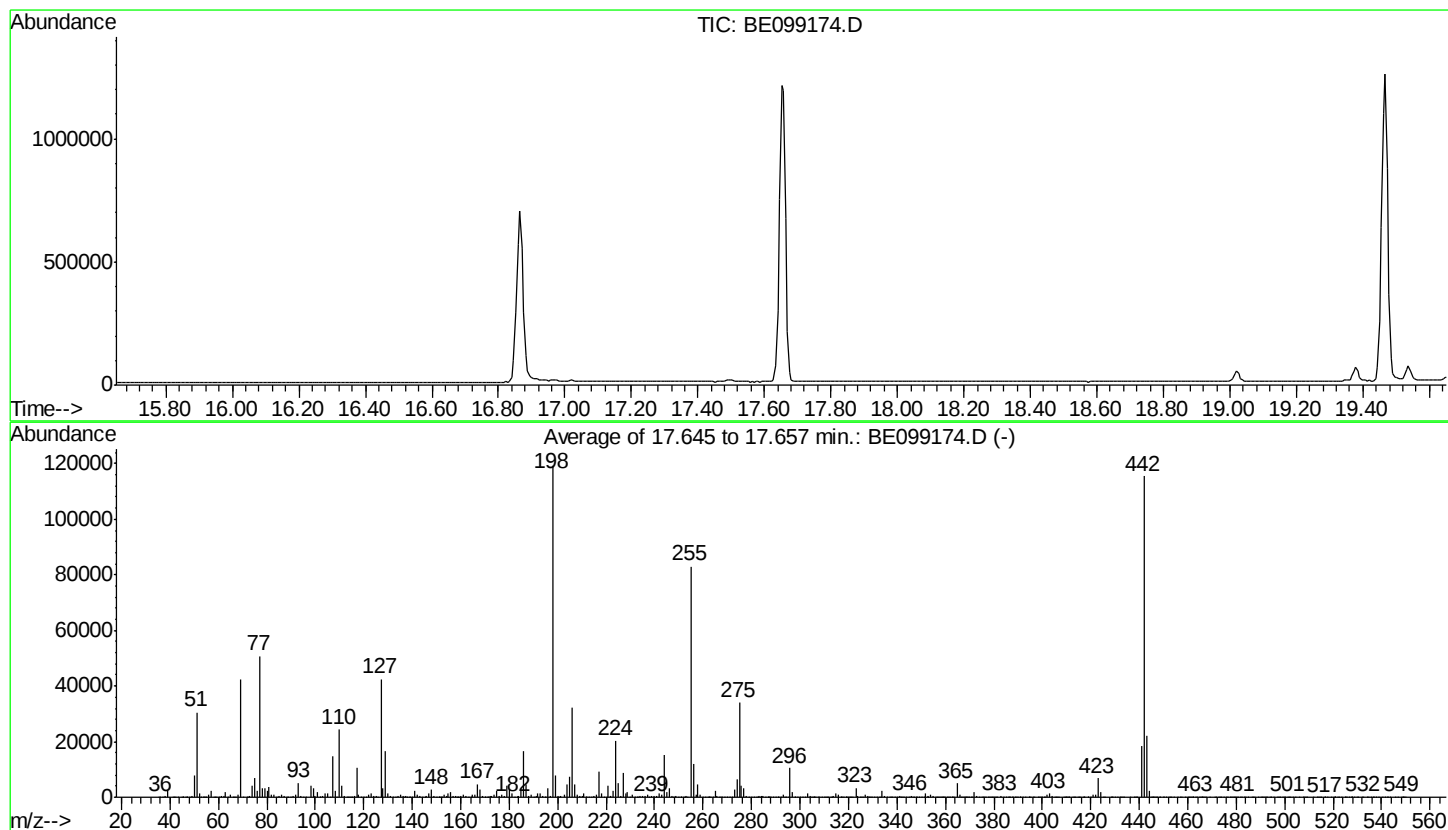

AutoFind: Scans 2563, 2564, 2565; Background Corrected with Scan 2556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.5	30450	PASS
68	69	0.00	2	1.8	748	PASS
69	198	0.00	100	35.6	42495	PASS
70	69	0.00	2	0.4	178	PASS
127	198	10	80	35.5	42400	PASS
197	198	0.00	2	0.4	437	PASS
198	198	100	100	100.0	119269	PASS
199	198	5	9	6.4	7690	PASS
275	198	10	60	28.6	34068	PASS
365	198	1	100	4.2	5001	PASS
441	198	0.01	100	15.6	18649	PASS
442	198	50	100	96.7	115352	PASS
443	442	15	24	19.3	22252	PASS