


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE032519\
 Data File : BE099184.D
 Acq On : 25 Mar 2019 17:43
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE032519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 26 07:02:06 2019

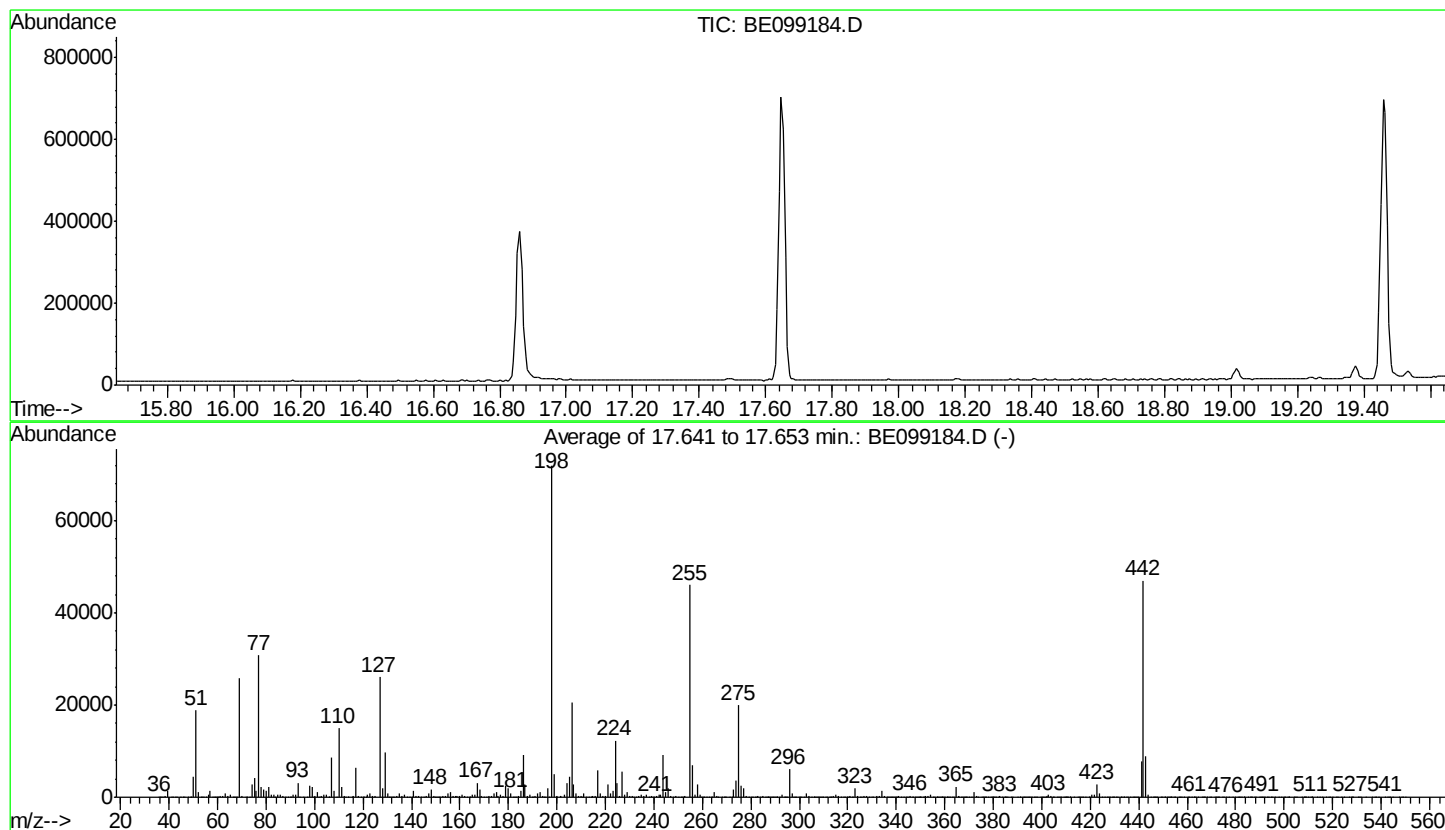

AutoFind: Scans 2562, 2563, 2564; Background Corrected with Scan 2549

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.2	18821	PASS
68	69	0.00	2	0.4	106	PASS
69	198	0.00	100	36.1	25946	PASS
70	69	0.00	2	0.6	161	PASS
127	198	10	80	36.2	26002	PASS
197	198	0.00	2	0.1	48	PASS
198	198	100	100	100.0	71919	PASS
199	198	5	9	7.1	5138	PASS
275	198	10	60	27.6	19870	PASS
365	198	1	100	3.2	2295	PASS
441	198	0.01	100	11.0	7906	PASS
442	198	50	100	65.4	47061	PASS
443	442	15	24	18.9	8907	PASS