


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE032519\
Data File : BE099203.D
Acq On : 26 Mar 2019 6:14
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE032519.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Mar 26 07:02:06 2019

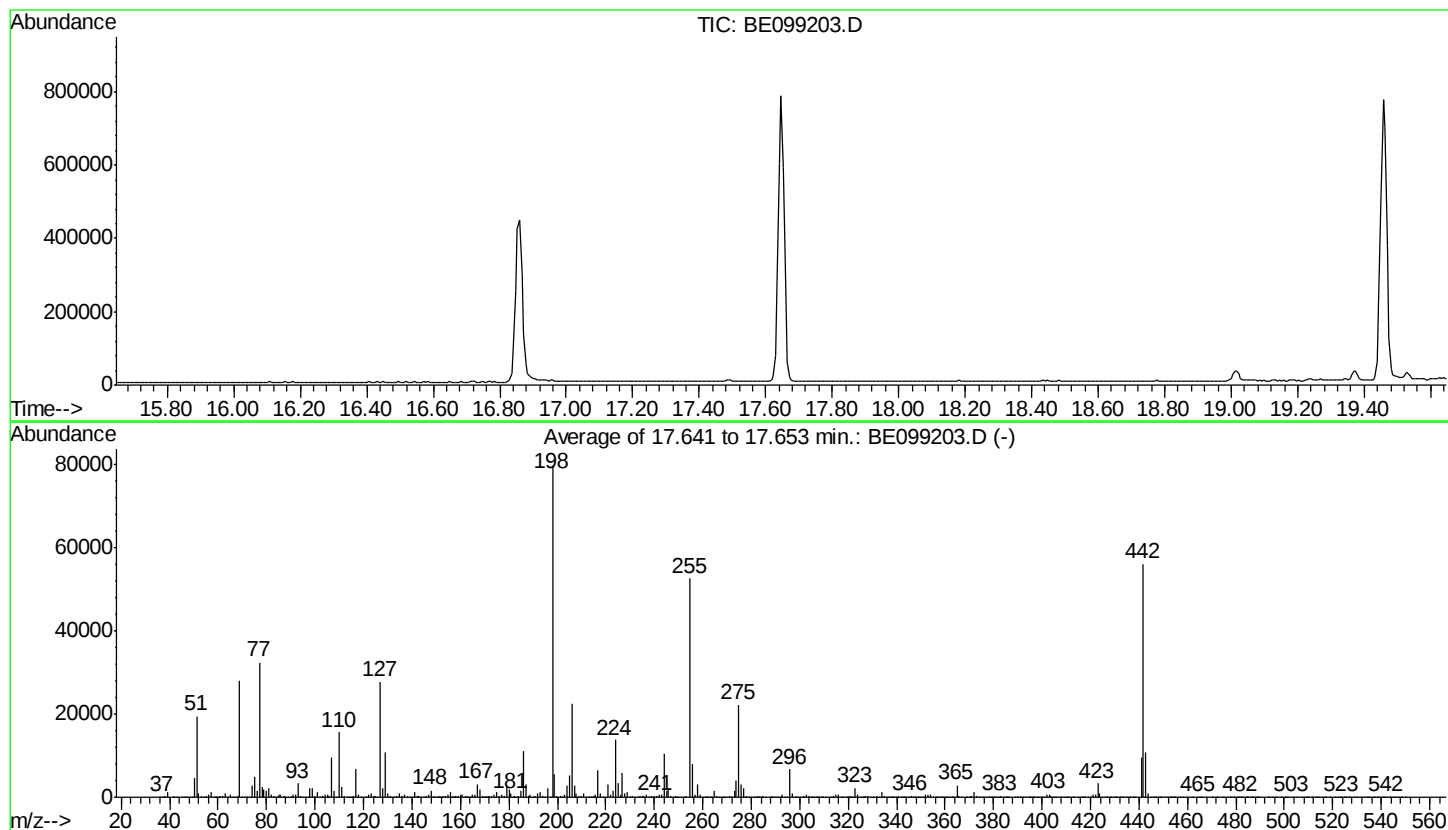

AutoFind: Scans 2562, 2563, 2564; Background Corrected with Scan 2553

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.4	19460	PASS
68	69	0.00	2	0.8	221	PASS
69	198	0.00	100	35.0	27924	PASS
70	69	0.00	2	0.5	151	PASS
127	198	10	80	34.8	27753	PASS
197	198	0.00	2	0.2	128	PASS
198	198	100	100	100.0	79744	PASS
199	198	5	9	7.1	5625	PASS
275	198	10	60	27.9	22287	PASS
365	198	1	100	3.6	2894	PASS
441	198	0.01	100	12.1	9612	PASS
442	198	50	100	70.4	56140	PASS
443	442	15	24	19.5	10927	PASS