

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE032619\
 Data File : BE099221.D
 Acq On : 26 Mar 2019 18:48
 Operator : JU/SJ
 Sample : K2020-03
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 KY038PS035-190318

Quant Time: Mar 27 08:51:02 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE032519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 26 07:02:06 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	3352	0.40	ng	-0.01
7) Naphthalene-d8	10.63	136	14282	0.40	ng	0.00
13) Acenaphthene-d10	14.47	164	11192	0.40	ng	-0.01
19) Phenanthrene-d10	17.20	188	32593	0.40	ng	-0.01
27) Chrysene-d12	21.38	240	36127	0.40	ng	-0.01
34) Perylene-d12	23.89	264	32935	0.40	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Fluorophenol	5.41	112	1654	0.17	ng	0.00
5) Phenol-d6	6.99	99	1321	0.09	ng	0.00
8) Nitrobenzene-d5	8.99	82	4581	0.39	ng	0.00
11) 2-Methylnaphthalene-d10	12.22	152	10127	0.37	ng	0.00
14) 2,4,6-Tribromophenol	15.96	330	1601	0.48	ng	0.00
15) 2-Fluorobiphenyl	13.10	172	17019	0.37	ng	0.00
25) Fluoranthene-d10	19.24	212	148223	0.38	ng	0.00
29) Terphenyl-d14	19.83	244	29209	0.37	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) n-Nitrosodimethylamine	3.64	42	206	0.083	ng	# 1
22) Pentachlorophenol	16.85	266	34	0.250	ng	# 67
32) Bis(2-ethylhexyl)phthalate	21.29	149	4349	0.031	ng	# 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE032619\
Data File : BE099221.D
Acq On : 26 Mar 2019 18:48
Operator : JU/SJ
Sample : K2020-03
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
KY038PS035-190318

Quant Time: Mar 27 08:51:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE032519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 26 07:02:06 2019
Response via : Initial Calibration

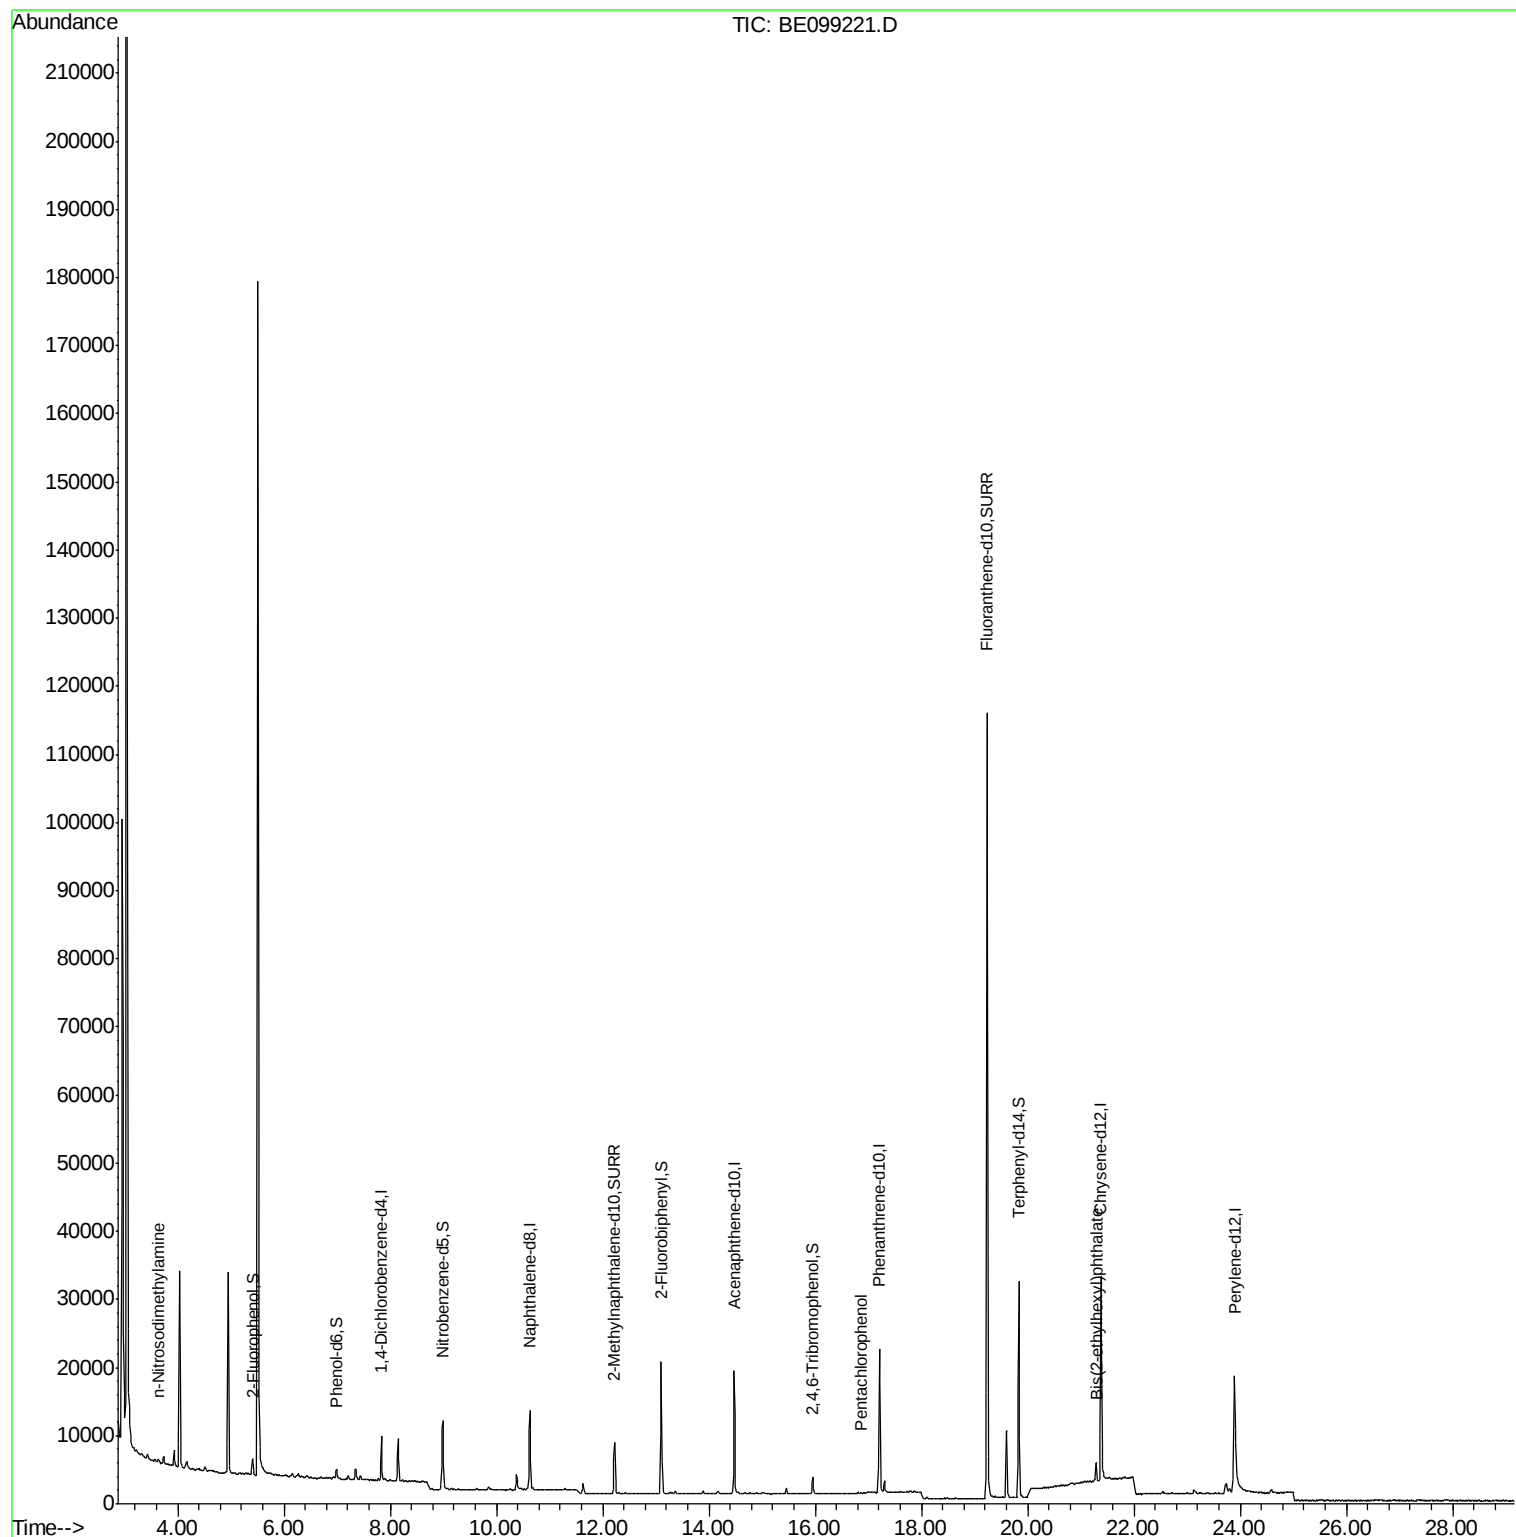



#1

1,4-Dichlorobenzene-d4

Concen: 0.400 ng

RT: 7.83 min Scan# 431

Delta R.T. -0.01 min

Lab File: BE099221.D

Acq: 26 Mar 2019 18:48

Instrument :

BNA_E

ClientSampleId :

KY038PS035-190318


Tgt Ion:152 Resp: 3352

Ion Ratio Lower Upper

152 100

150 141.9 112.8 169.2




115 67.4 45.1 67.7

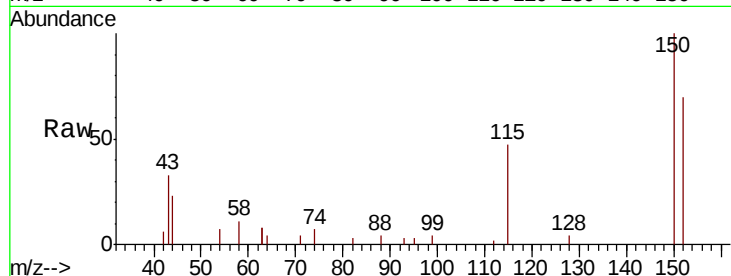

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

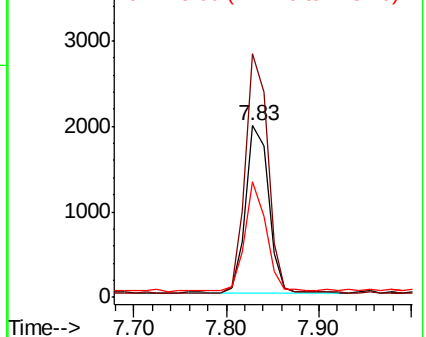

#3

n-Nitrosodimethylamine

Concen: 0.083 ng

RT: 3.64 min Scan# 67

Delta R.T. -0.04 min

Lab File: BE099221.D

Acq: 26 Mar 2019 18:48


Tgt Ion: 42 Resp: 206

Ion Ratio Lower Upper

42 100

74 23.8 138.6 207.8#



44 0.0 15.0 22.6#




Abundance Ion 42.00 (41.70 to 42.70): BE0

Ion 74.00 (73.70 to 74.70): BE0

Ion 44.00 (43.70 to 44.70): BE0

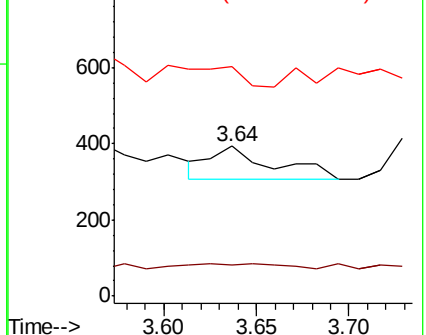

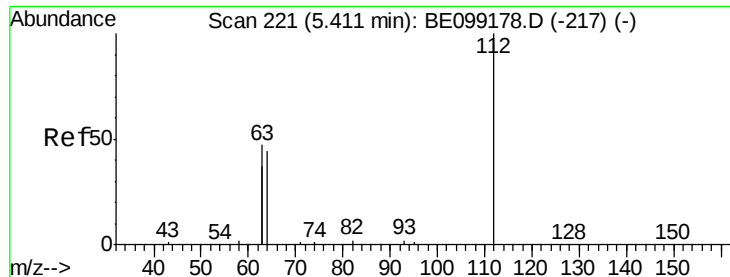

#4

2-Fluorophenol

Concen: 0.165 ng

RT: 5.41 min Scan# 221

Delta R.T. -0.00 min

Lab File: BE099221.D

Acq: 26 Mar 2019 18:48

Instrument :

BNA_E

ClientSampleId :

KY038PS035-190318


Tgt Ion: 112 Resp: 1654

Ion Ratio Lower Upper

112 100

64 56.5 46.2 69.2




63 111.2 89.9 134.9

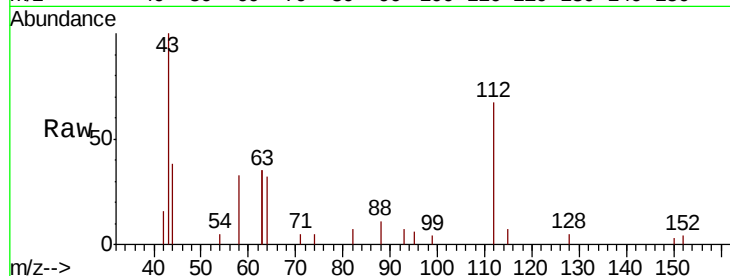

Abundance Ion 112.00 (111.70 to 112.70): BE099221.D (-217) (-)

Ion 64.00 (63.70 to 64.70): BE099221.D (-217) (-)

Ion 63.00 (62.70 to 63.70): BE099221.D (-217) (-)

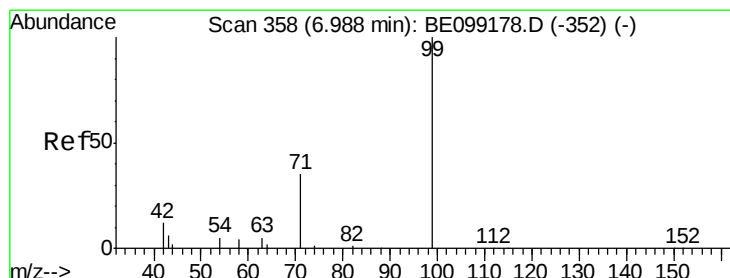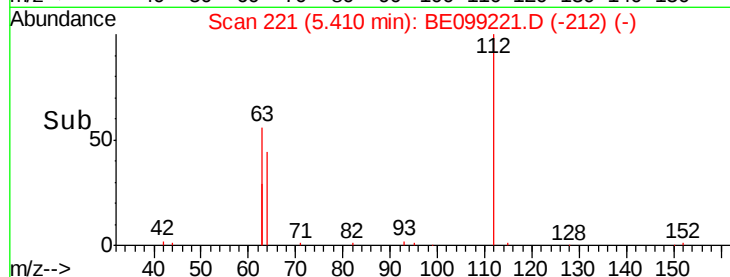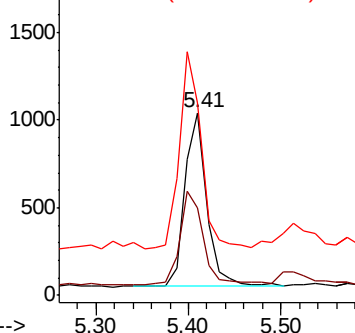

#5

Phenol-d6

Concen: 0.086 ng

RT: 6.99 min Scan# 358

Delta R.T. -0.00 min

Lab File: BE099221.D

Acq: 26 Mar 2019 18:48


Tgt Ion: 99 Resp: 1321

Ion Ratio Lower Upper

99 100

42 21.4 12.4 18.6#



71 43.8 28.4 42.6#

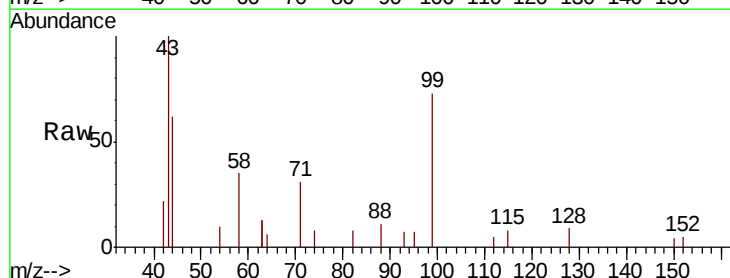


Abundance Ion 99.00 (98.70 to 99.70): BE099221.D (-352) (-)

Ion 42.00 (41.70 to 42.70): BE099221.D (-352) (-)

Ion 71.00 (70.70 to 71.70): BE099221.D (-352) (-)

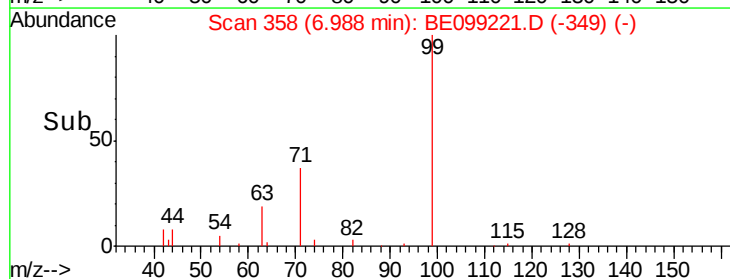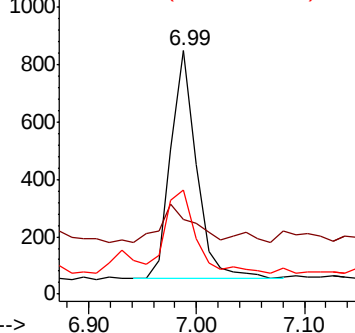

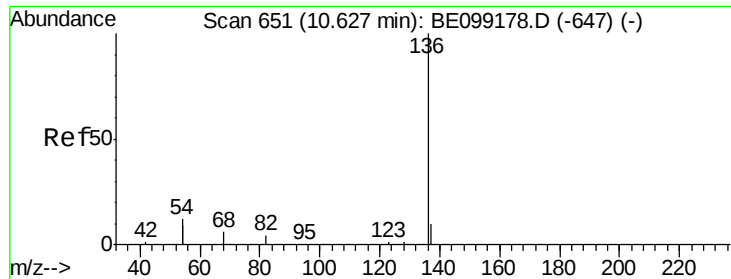

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.63 min Scan# 651

Delta R.T. 0.00 min

Lab File: BE099221.D

Acq: 26 Mar 2019 18:48

Instrument :

BNA_E

ClientSampleId :

KY038PS035-190318

Tgt Ion:136 Resp: 14282


Ion Ratio Lower Upper

136 100

137 11.5 8.7 13.1

54 20.0 18.7 28.1

68 5.5 5.2 7.8



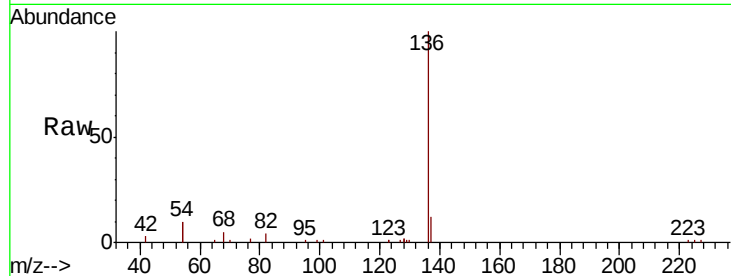


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

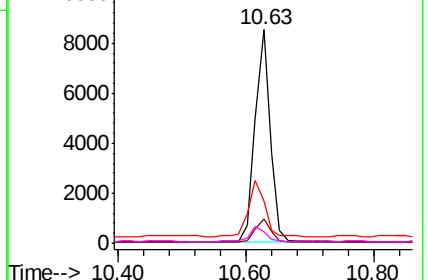

#8

Nitrobenzene-d5

Concen: 0.393 ng

RT: 8.99 min Scan# 525

Delta R.T. 0.00 min

Lab File: BE099221.D

Acq: 26 Mar 2019 18:48


Tgt Ion: 82 Resp: 4581

Ion Ratio Lower Upper

82 100

128 166.2 107.5 161.3#



54 130.1 106.3 159.5




Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0



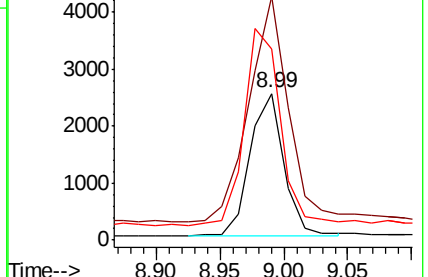



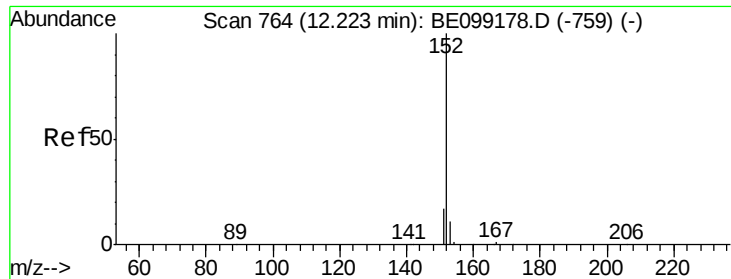

#11
 2-Methylnaphthalene-d10
 Concen: 0.368 ng
 RT: 12.22 min Scan# 764
 Delta R.T. 0.00 min
 Lab File: BE099221.D
 Acq: 26 Mar 2019 18:48




Instrument :
 BNA_E
 ClientSampleId :
 KY038PS035-190318


Tgt Ion:152 Resp: 10127
 Ion Ratio Lower Upper
 152 100
 151 18.7 15.0 22.6

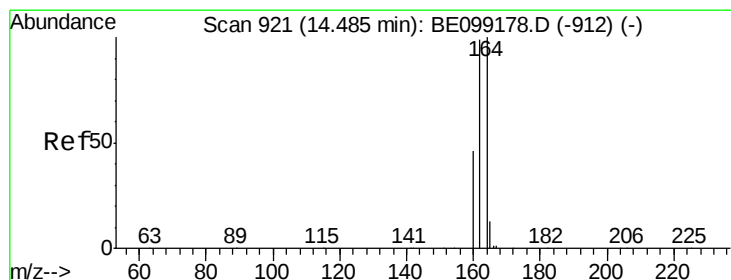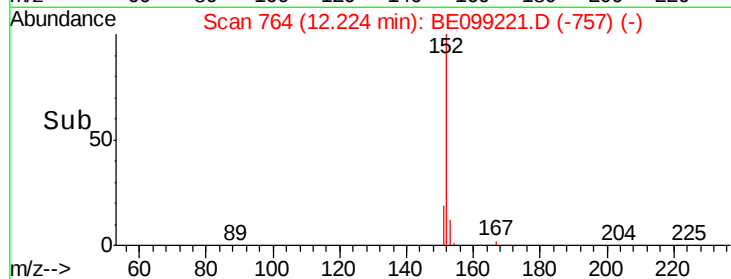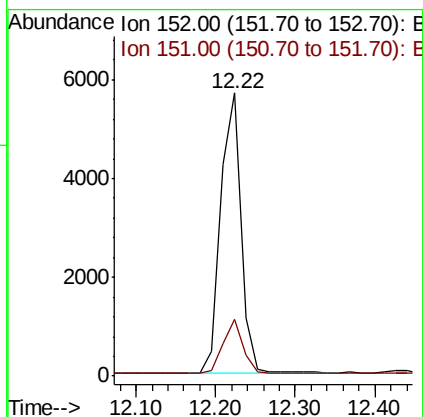

#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.47 min Scan# 920
 Delta R.T. -0.01 min
 Lab File: BE099221.D
 Acq: 26 Mar 2019 18:48

Tgt Ion:164 Resp: 11192
 Ion Ratio Lower Upper
 164 100
 162 100.9 79.2 118.8
 160 48.3 36.7 55.1

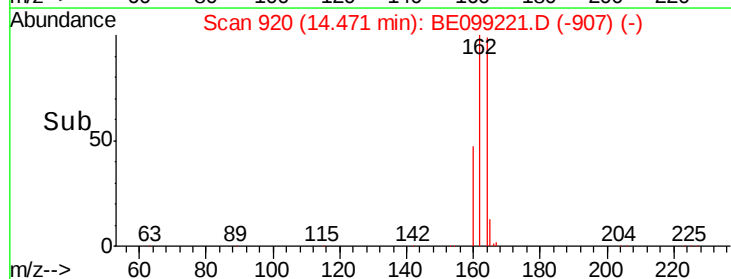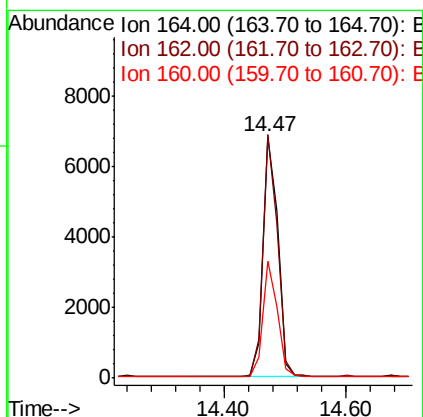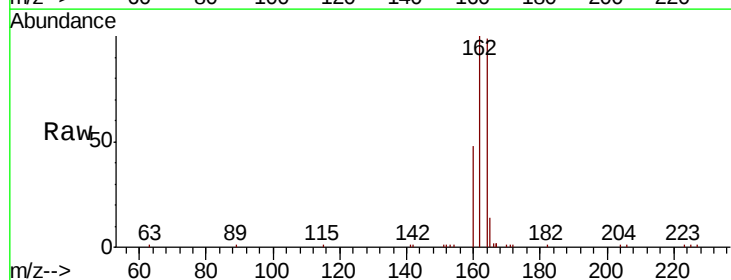


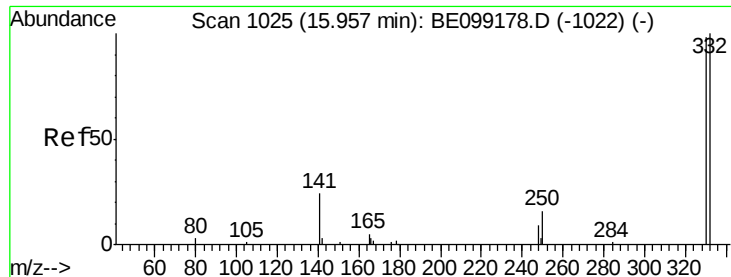




#14
 2,4,6-Tribromophenol
 Concen: 0.480 ng
 RT: 15.96 min Scan# 1025
 Delta R.T. 0.00 min
 Lab File: BE099221.D
 Acq: 26 Mar 2019 18:48

Instrument :
 BNA_E
 ClientSampleId :
 KY038PS035-190318

Tgt Ion:330 Resp: 1601
 Ion Ratio Lower Upper
 330 100
 332 97.0 71.3 106.9
 141 31.4 21.7 32.5

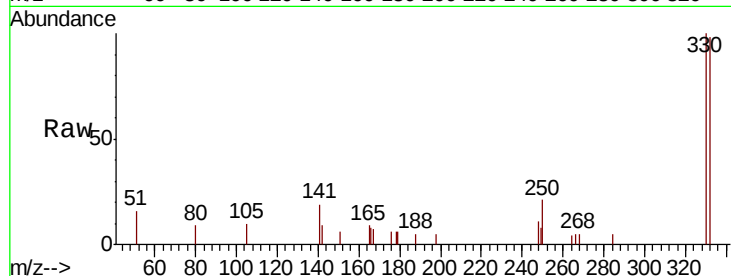


Abundance Ion 330.00 (329.70 to 330.70): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

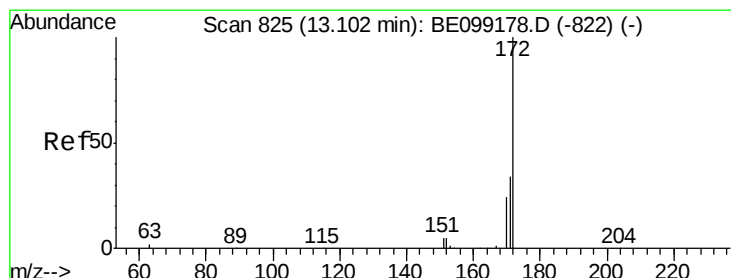
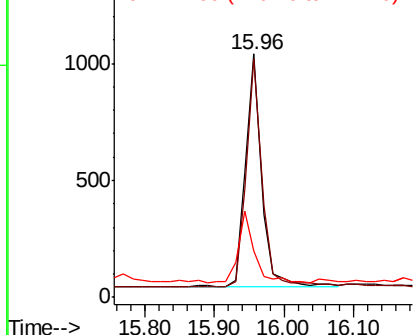



#15
 2-Fluorobiphenyl
 Concen: 0.373 ng
 RT: 13.10 min Scan# 825
 Delta R.T. 0.00 min
 Lab File: BE099221.D
 Acq: 26 Mar 2019 18:48

Tgt Ion:172 Resp: 17019
 Ion Ratio Lower Upper
 172 100
 171 34.2 27.4 41.0
 170 24.0 19.1 28.7



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

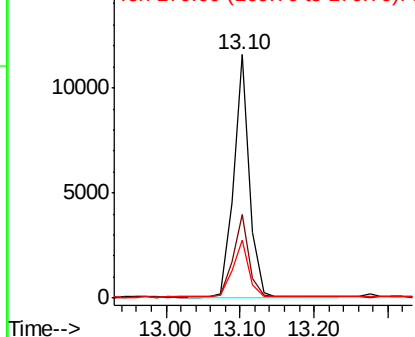

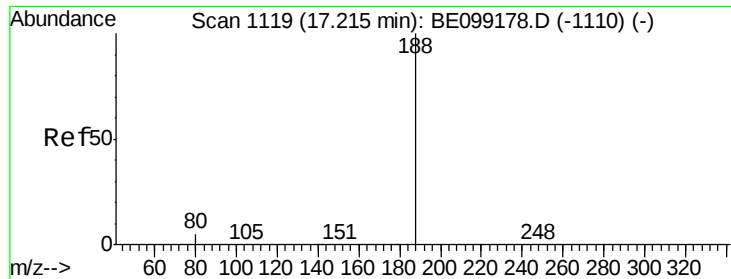

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.20 min Scan# 1118

Delta R.T. -0.01 min

Lab File: BE099221.D

Acq: 26 Mar 2019 18:48

Instrument :

BNA_E

ClientSampleId :

KY038PS035-190318


Tgt Ion:188 Resp: 32593

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0




80 10.4 4.5 6.7#



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

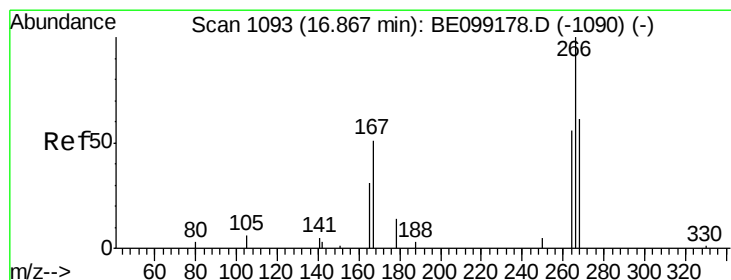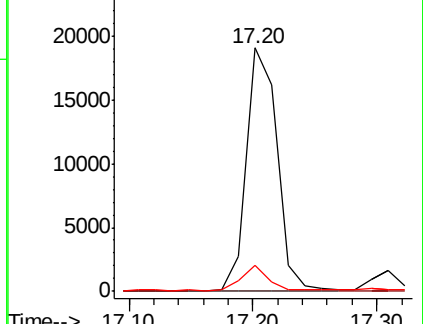

#22

Pentachlorophenol

Concen: 0.250 ng

RT: 16.85 min Scan# 1092

Delta R.T. -0.01 min

Lab File: BE099221.D

Acq: 26 Mar 2019 18:48


Tgt Ion:266 Resp: 34

Ion Ratio Lower Upper

266 100

264 91.7 54.4 81.6#



268 108.3 61.3 91.9#

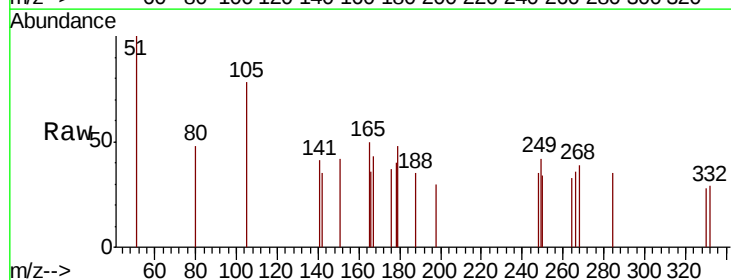


Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

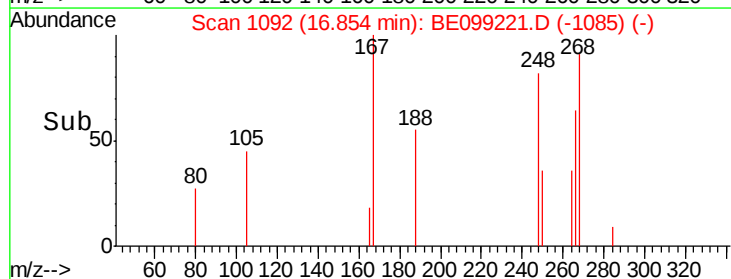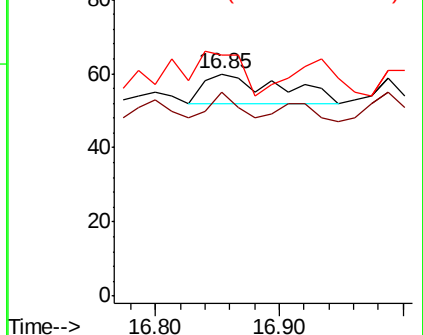



#25

Fluoranthene-d10

Concen: 0.375 ng

RT: 19.24 min Scan# 1387

Delta R.T. -0.01 min

Lab File: BE099221.D

Acq: 26 Mar 2019 18:48

Instrument :

BNA_E

ClientSampleId :

KY038PS035-190318


Tgt Ion: 212 Resp: 148223

Ion Ratio Lower Upper

212 100

106 2.3 1.8 2.8




104 1.3 1.1 1.7

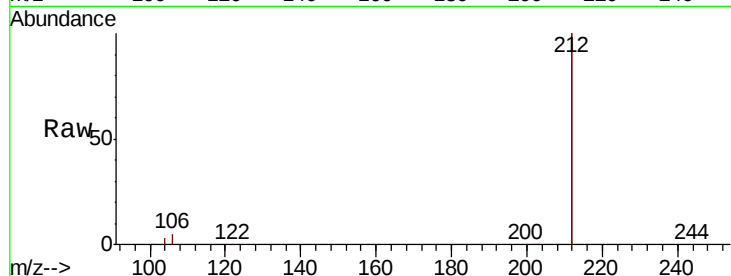

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

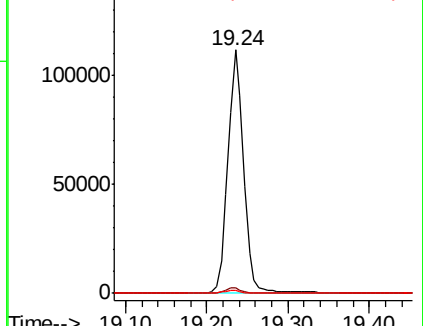

#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.38 min Scan# 1631

Delta R.T. -0.01 min

Lab File: BE099221.D

Acq: 26 Mar 2019 18:48


Tgt Ion: 240 Resp: 36127

Ion Ratio Lower Upper

240 100

120 8.6 2.6 3.8#



236 28.0 20.9 31.3




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

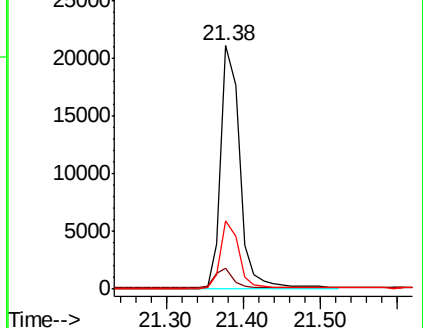



#29

Terphenyl-d14

Concen: 0.372 ng

RT: 19.83 min Scan# 1491

Delta R.T. -0.00 min

Lab File: BE099221.D

Acq: 26 Mar 2019 18:48

Instrument :

BNA_E

ClientSampleId :

KY038PS035-190318


Tgt Ion:244 Resp: 29209

Ion Ratio Lower Upper

244 100

212 28.7 22.7 34.1




122 6.6 5.8 8.6

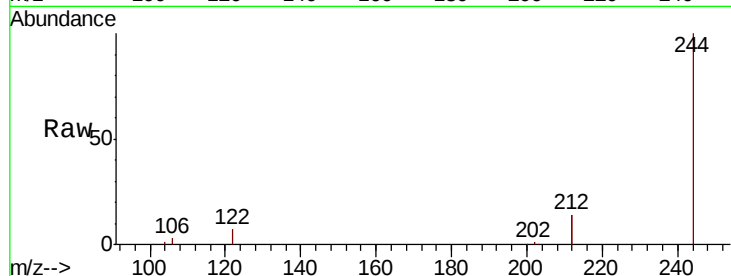

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

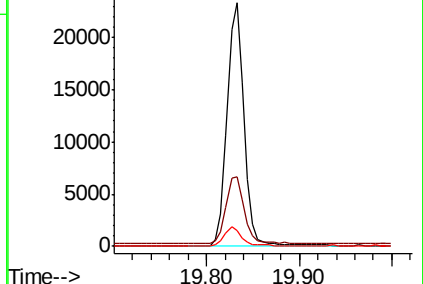

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.031 ng

RT: 21.29 min Scan# 1624

Delta R.T. -0.00 min

Lab File: BE099221.D

Acq: 26 Mar 2019 18:48


Tgt Ion:149 Resp: 4349

Ion Ratio Lower Upper

149 100

167 8.6 5.9 8.9



279 3.2 1.0 1.6#






Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

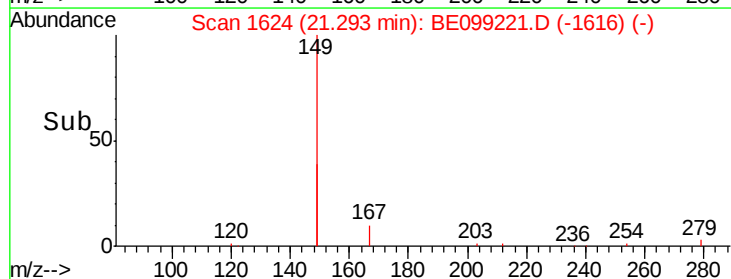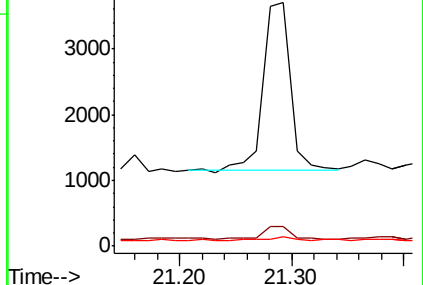

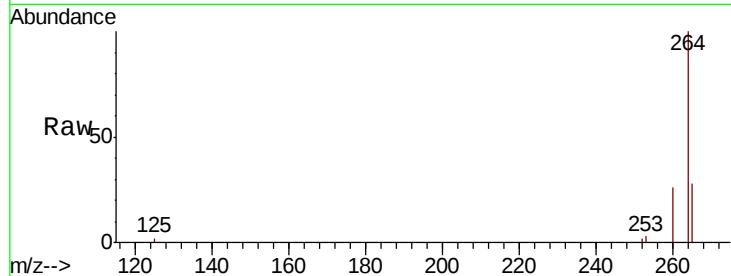

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.89 min Scan# 2207

Delta R.T. 0.00 min

Lab File: BE099221.D

Acq: 26 Mar 2019 18:48

Instrument :

BNA_E

ClientSampleId :

KY038PS035-190318

Tgt Ion:264 Resp: 32935

Ion Ratio Lower Upper

264 100

260 25.9 18.2 27.2

265 28.1 21.8 32.8

