

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE032619\
 Data File : BE099240.D
 Acq On : 27 Mar 2019 8:41
 Operator : JU/SJ
 Sample : K2064-09RE
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Mar 27 14:15:08 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE032519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 26 07:02:06 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	4545	0.40	ng	-0.01
7) Naphthalene-d8	10.63	136	20232	0.40	ng	0.00
13) Acenaphthene-d10	14.47	164	15975	0.40	ng	-0.01
19) Phenanthrene-d10	17.20	188	44671	0.40	ng	-0.01
27) Chrysene-d12	21.38	240	49254	0.40	ng	-0.01
34) Perylene-d12	23.89	264	39490	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.41	112	2261	0.17	ng	0.00
5) Phenol-d6	6.99	99	2019	0.10	ng	0.00
8) Nitrobenzene-d5	8.98	82	6012	0.36	ng	-0.01
11) 2-Methylnaphthalene-d10	12.21	152	15038	0.39	ng	-0.01
14) 2,4,6-Tribromophenol	15.96	330	1900	0.44	ng	0.00
15) 2-Fluorobiphenyl	13.10	172	24474	0.38	ng	0.00
25) Fluoranthene-d10	19.24	212	217324	0.40	ng	0.00
29) Terphenyl-d14	19.83	244	36253	0.34	ng	0.00
Target Compounds						
3) n-Nitrosodimethylamine	3.67	42	108	0.032	ng	# 1
22) Pentachlorophenol	16.87	266	54	0.252	ng	# 71
32) Bis(2-ethylhexyl)phthalate	21.28	149	6738	0.035	ng	# 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE032619\
Data File : BE099240.D
Acq On : 27 Mar 2019 8:41
Operator : JU/SJ
Sample : K2064-09RE
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Mar 27 14:15:08 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE032519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 26 07:02:06 2019
Response via : Initial Calibration

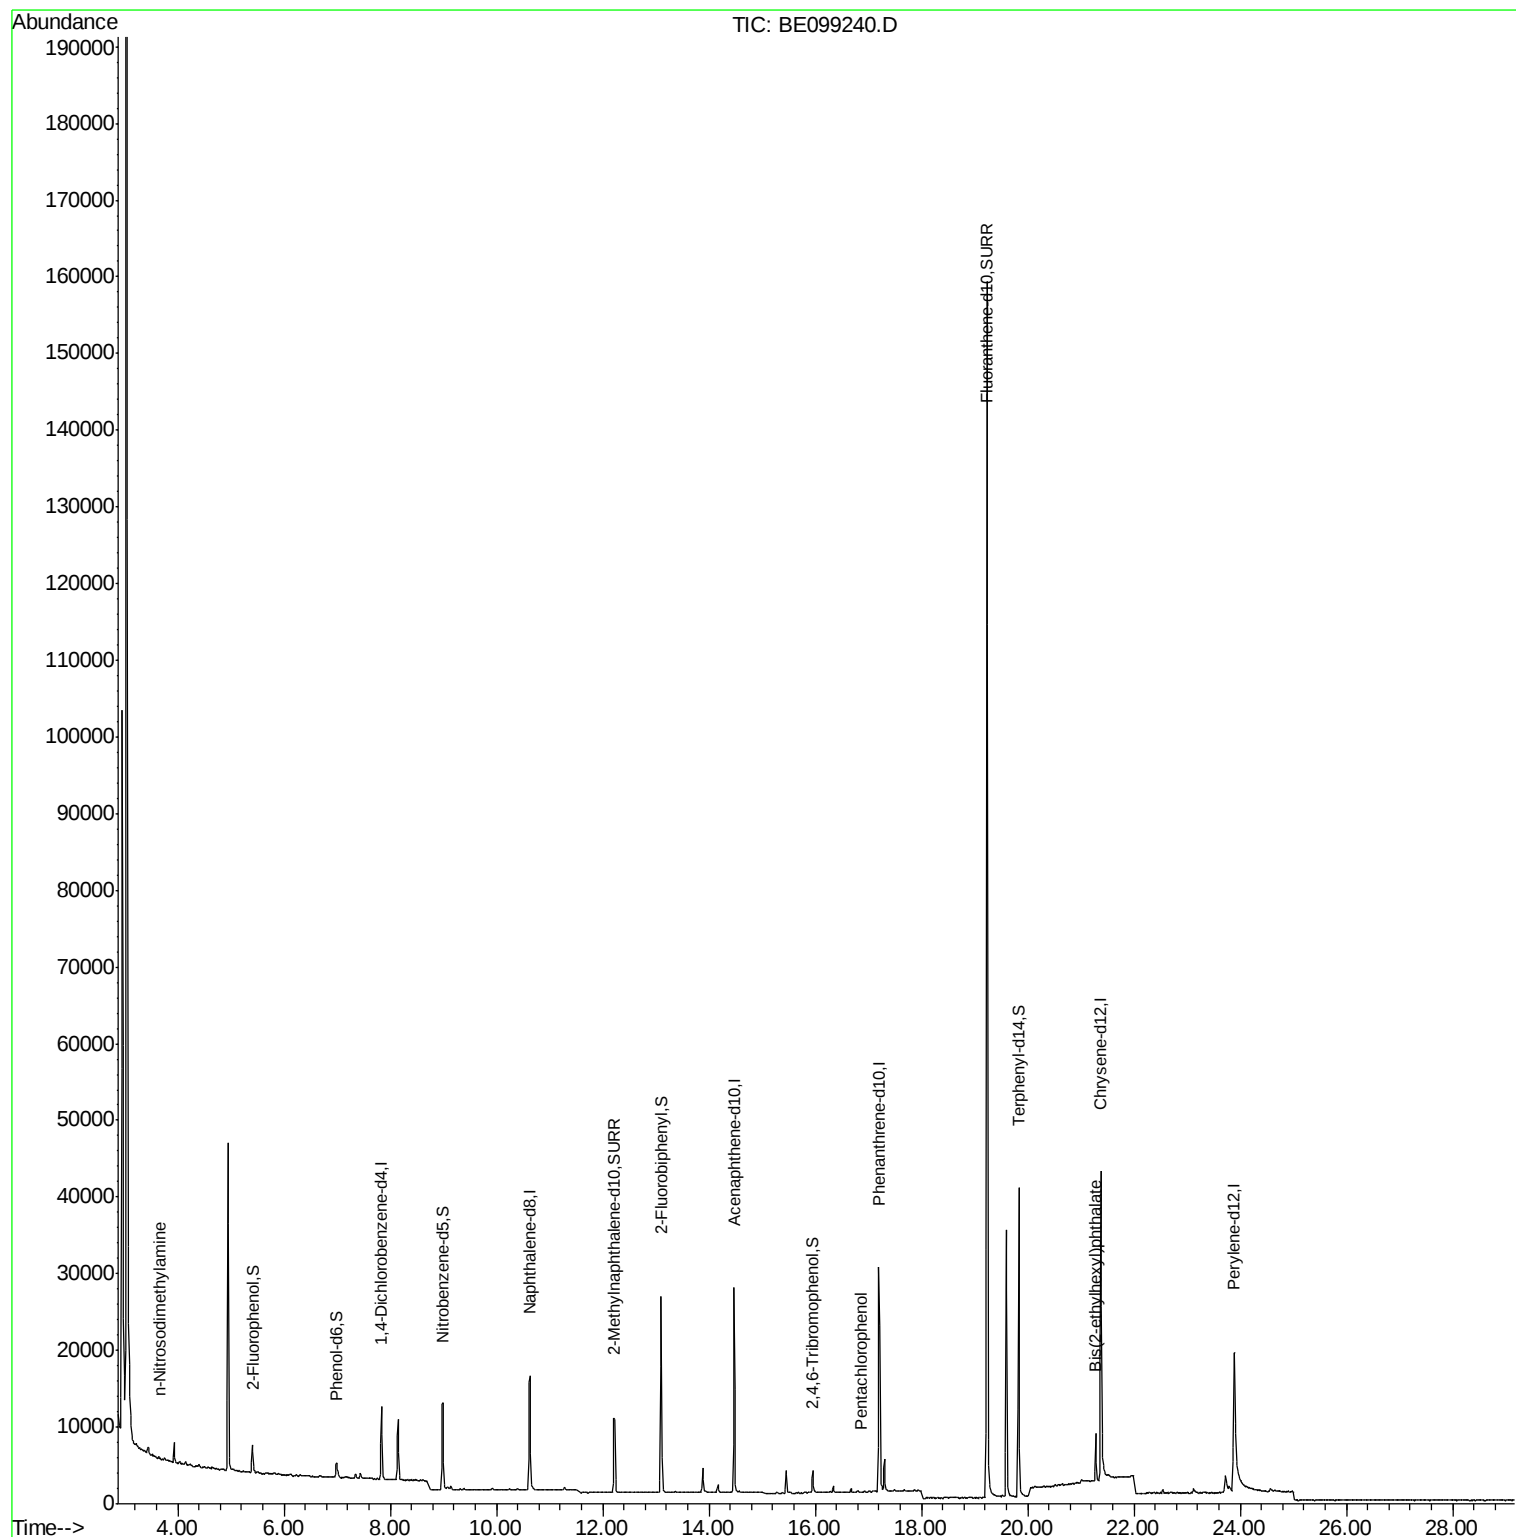




#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.83 min Scan# 431
Delta R.T. -0.01 min
Lab File: BE099240.D
Acq: 27 Mar 2019 8:41

Instrument :
BNA_E
ClientSampled :

Tot Ion:152 Resp: 4545
Ion Ratio Lower Upper
152 100
150 143.6 112.8 169.2
115 62.6 45.1 67.7

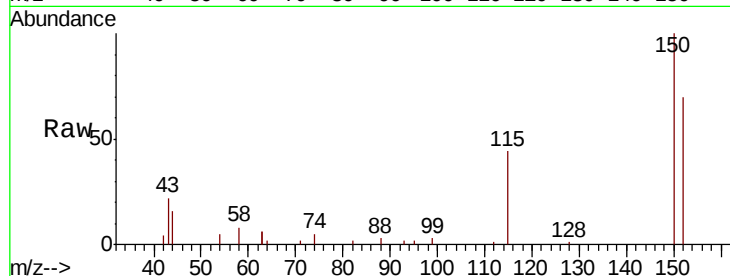


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

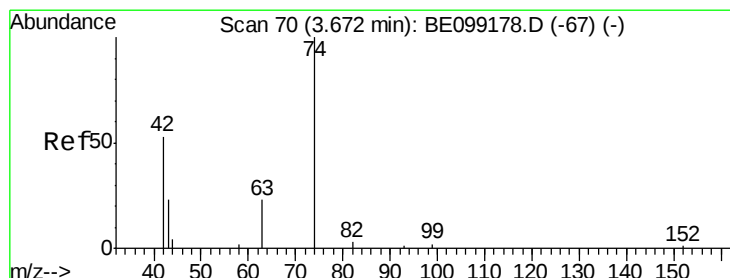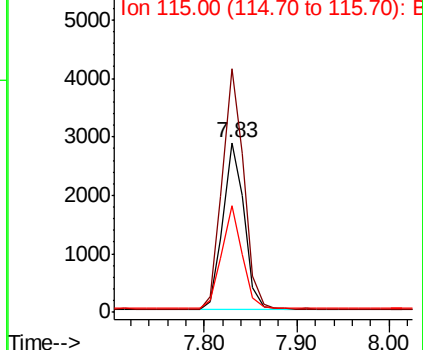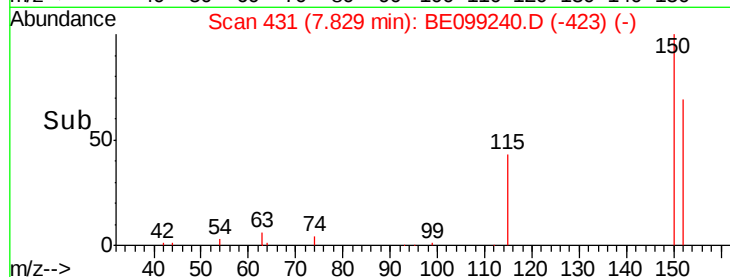



#3


n-Nitrosodimethylamine
Concen: 0.032 ng
RT: 3.67 min Scan# 70
Delta R.T. 0.00 min
Lab File: BE099240.D
Acq: 27 Mar 2019 8:41

Tgt Ion: 42 Resp: 108
Ion Ratio Lower Upper
42 100
74 13.9 138.6 207.8#
44 25.9 15.0 22.6#

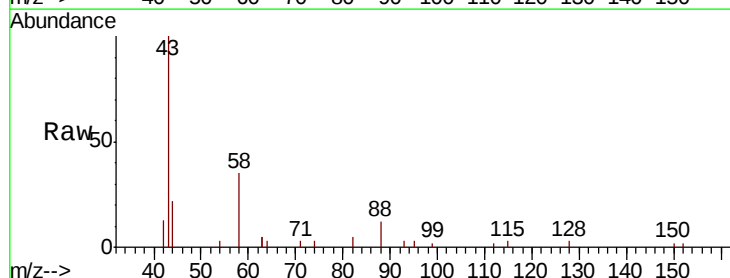

Abundance Ion 42.00 (41.70 to 42.70): BE0
Ion 74.00 (73.70 to 74.70): BE0
Ion 44.00 (43.70 to 44.70): BE0

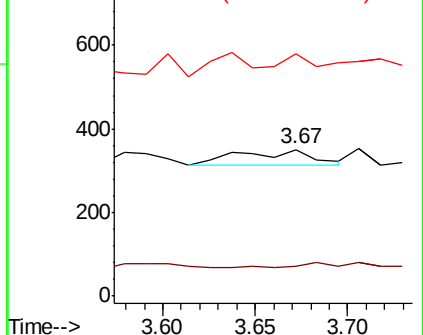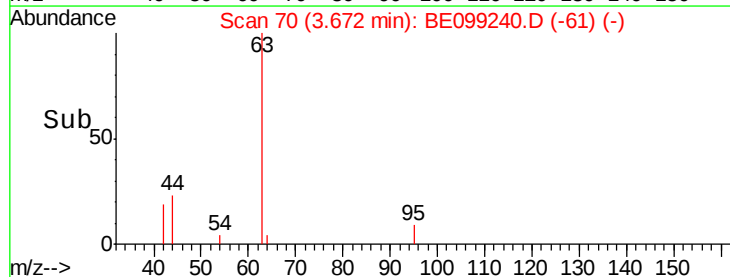

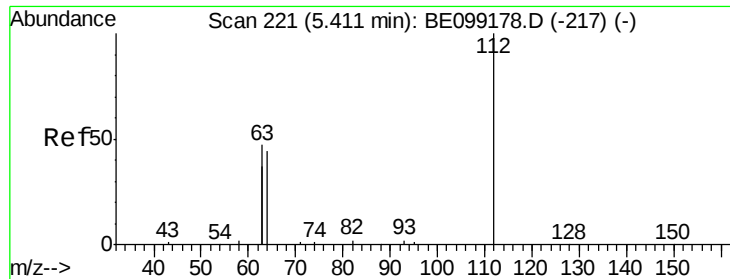

#4

2-Fluorophenol

Concen: 0.167 ng

RT: 5.41 min Scan# 221

Delta R.T. 0.00 min

Lab File: BE099240.D

Acq: 27 Mar 2019 8:41

Instrument :

BNA_E

ClientSampleId :


Tot Ion: 112 Resp: 2261

Ion Ratio Lower Upper

112 100

64 53.3 46.2 69.2




63 111.3 89.9 134.9

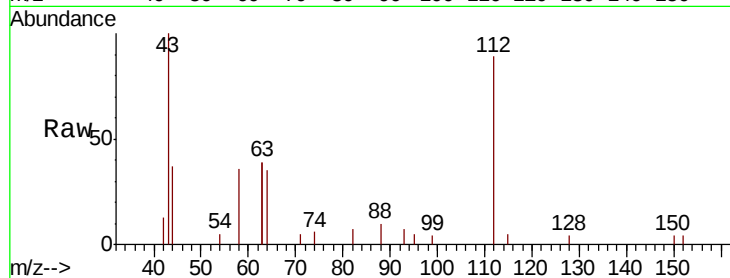

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

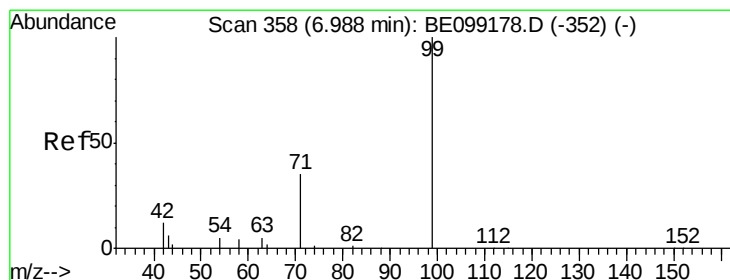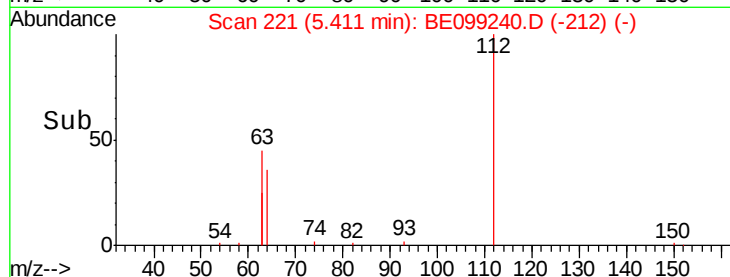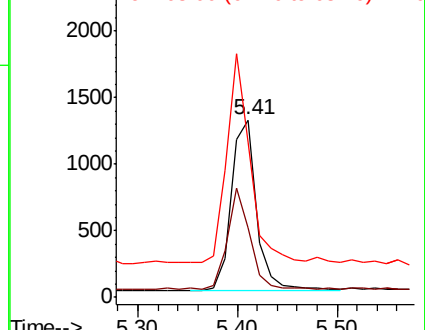

#5

Phenol-d6

Concen: 0.097 ng

RT: 6.99 min Scan# 358

Delta R.T. 0.00 min

Lab File: BE099240.D

Acq: 27 Mar 2019 8:41


Tgt Ion: 99 Resp: 2019

Ion Ratio Lower Upper

99 100

42 21.1 12.4 18.6#



71 38.2 28.4 42.6

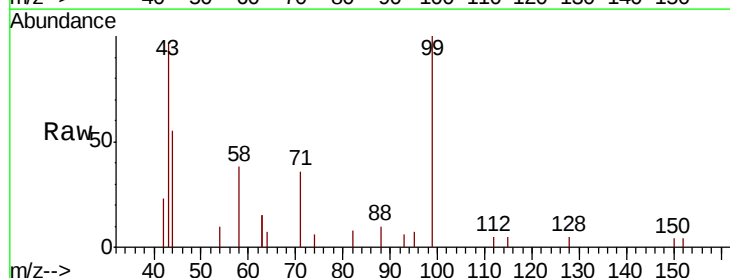


Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

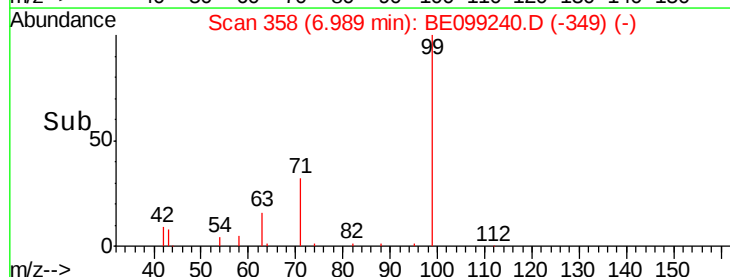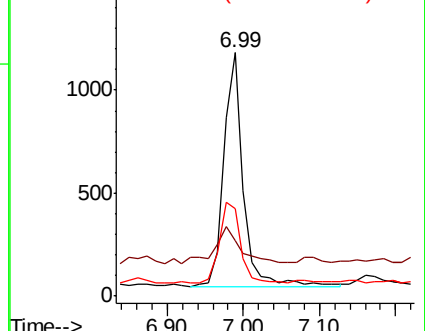

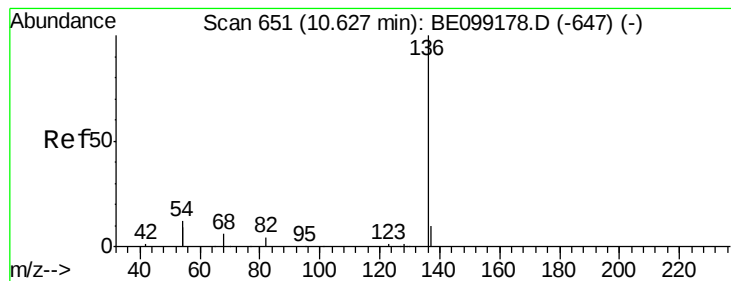

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.63 min Scan# 651

Delta R.T. 0.00 min

Lab File: BE099240.D

Acq: 27 Mar 2019 8:41

Instrument :

BNA_E

ClientSampleId :

Tot Ion:136 Resp: 20232


Ion Ratio Lower Upper

136 100

137 10.3 8.7 13.1

54 16.2 18.7 28.1#

68 4.6 5.2 7.8#

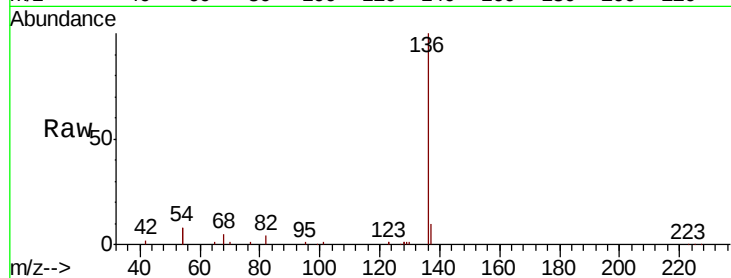




Abundance

Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

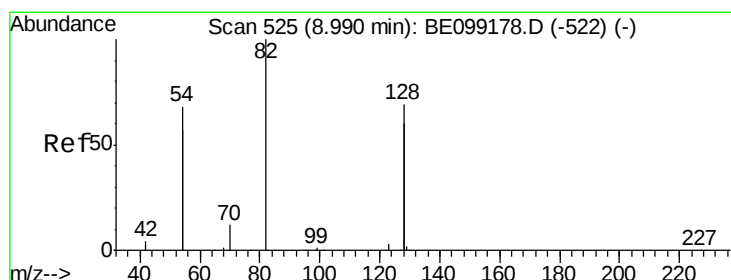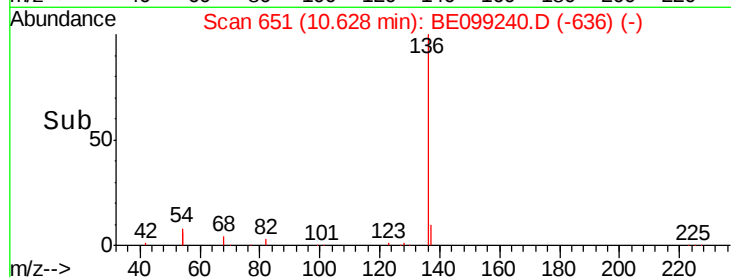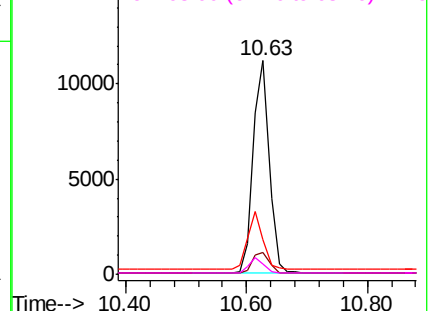

#8

Nitrobenzene-d5

Concen: 0.364 ng

RT: 8.98 min Scan# 524

Delta R.T. -0.01 min

Lab File: BE099240.D

Acq: 27 Mar 2019 8:41


Tgt Ion: 82 Resp: 6012

Ion Ratio Lower Upper

82 100

128 106.8 107.5 161.3#

54 164.2 106.3 159.5#


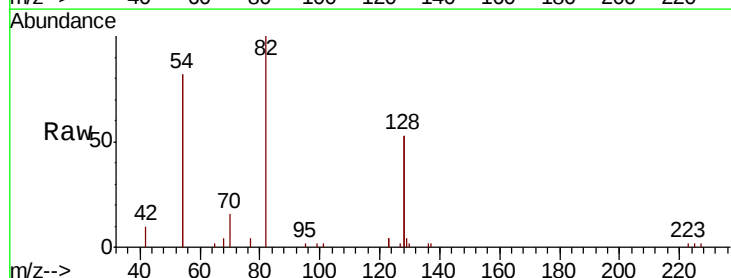



Abundance

Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0

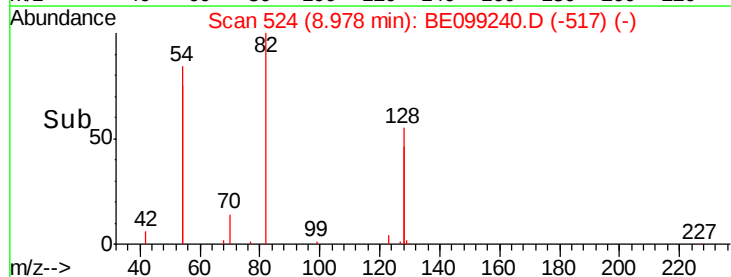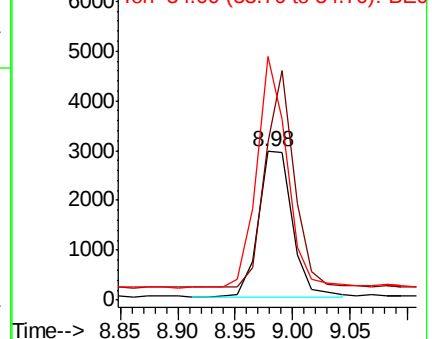

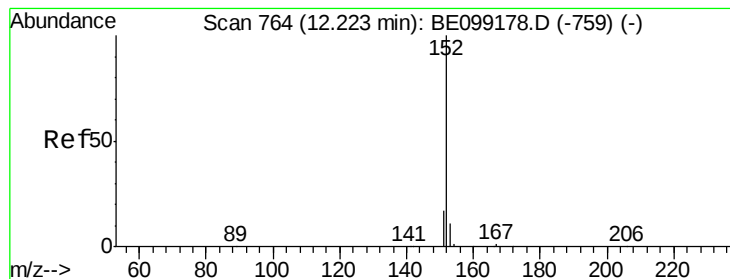

#11

2-Methylnaphthalene-d10

Concen: 0.386 ng

RT: 12.21 min Scan# 763

Delta R.T. -0.01 min

Lab File: BE099240.D

Acq: 27 Mar 2019 8:41

Instrument :

BNA_E





ClientSampleId :

Tot Ion:152 Resp: 15038

Ion Ratio Lower Upper

152 100

151 19.6 15.0 22.6

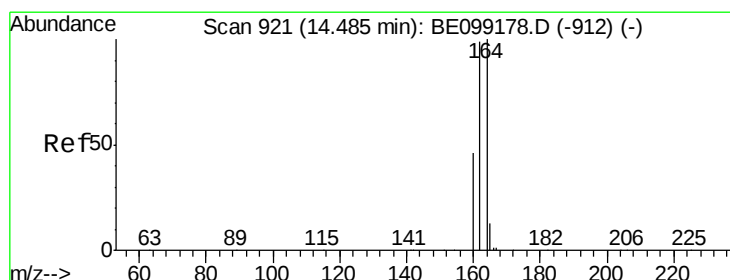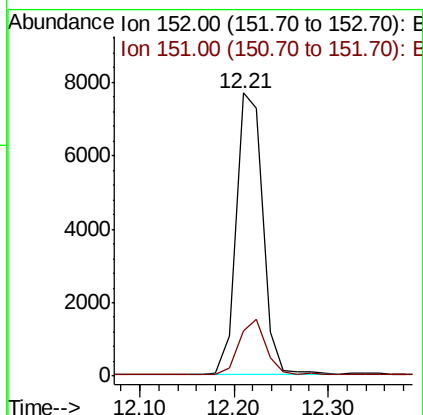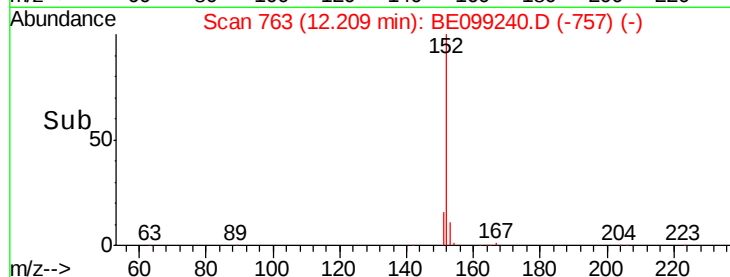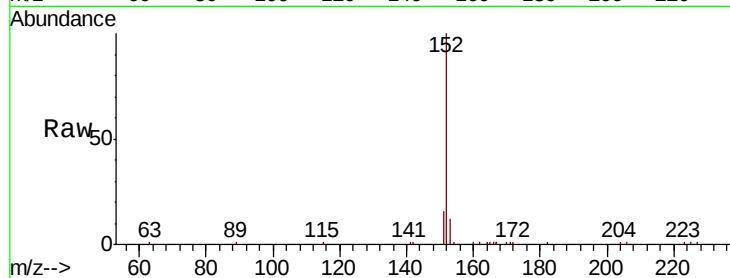

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.47 min Scan# 920

Delta R.T. -0.01 min

Lab File: BE099240.D

Acq: 27 Mar 2019 8:41




Tgt Ion:164 Resp: 15975


Ion Ratio Lower Upper

164 100

162 96.9 79.2 118.8

160 46.4 36.7 55.1

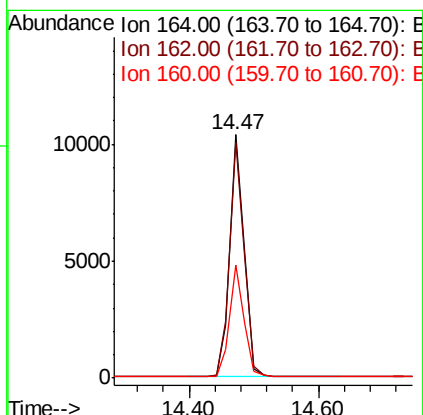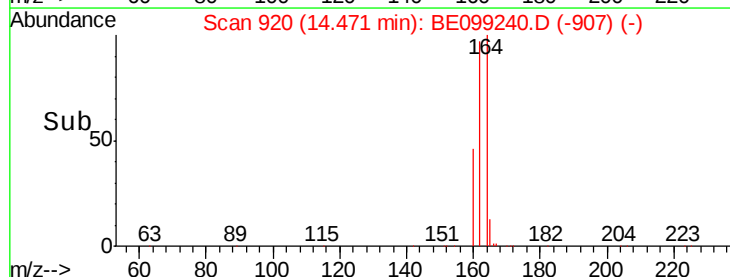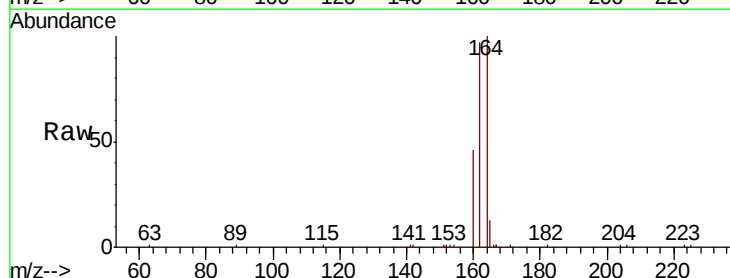


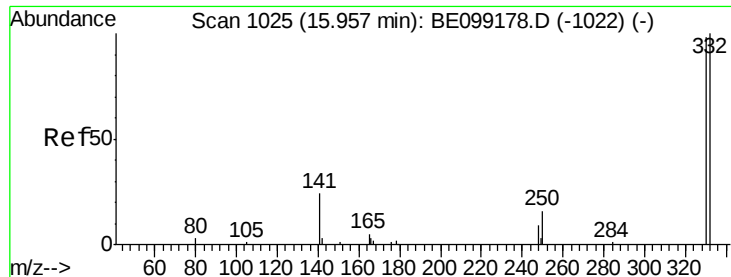




#14
 2,4,6-Tribromophenol
 Concen: 0.438 ng
 RT: 15.96 min Scan# 1025
 Delta R.T. -0.00 min
 Lab File: BE099240.D
 Acq: 27 Mar 2019 8:41

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion:330 Resp: 1900
 Ion Ratio Lower Upper
 330 100
 332 100.3 71.3 106.9
 141 30.8 21.7 32.5

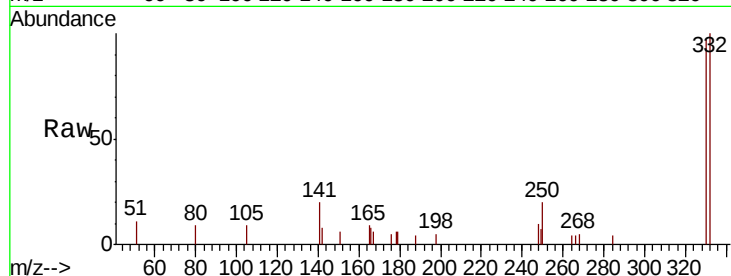


Abundance Ion 330.00 (329.70 to 330.70): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

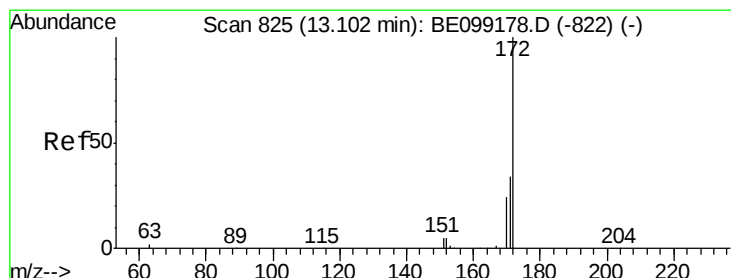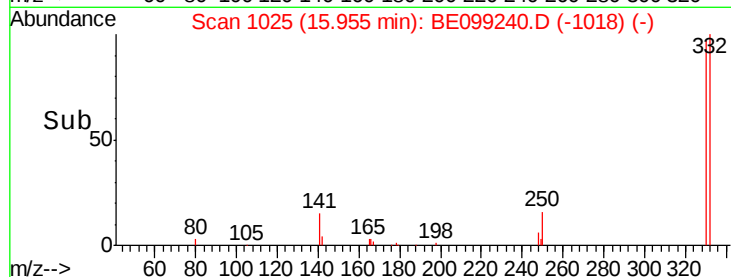
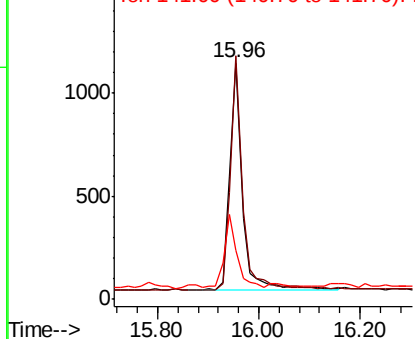



#15
 2-Fluorobiphenyl
 Concen: 0.376 ng
 RT: 13.10 min Scan# 825
 Delta R.T. 0.00 min
 Lab File: BE099240.D
 Acq: 27 Mar 2019 8:41

Tgt Ion:172 Resp: 24474
 Ion Ratio Lower Upper
 172 100
 171 34.5 27.4 41.0
 170 22.2 19.1 28.7

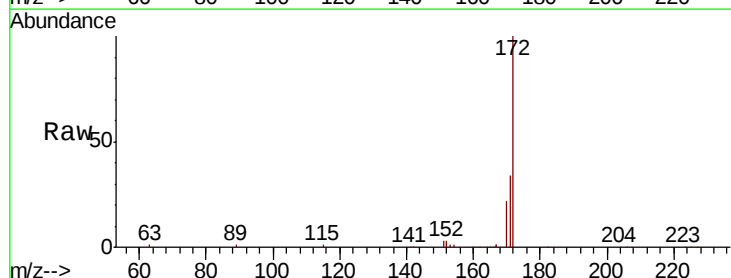

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

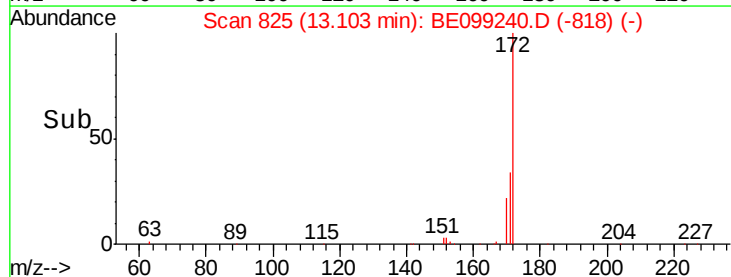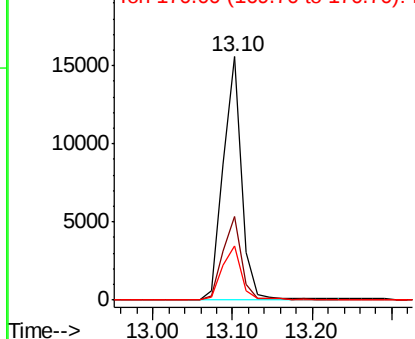

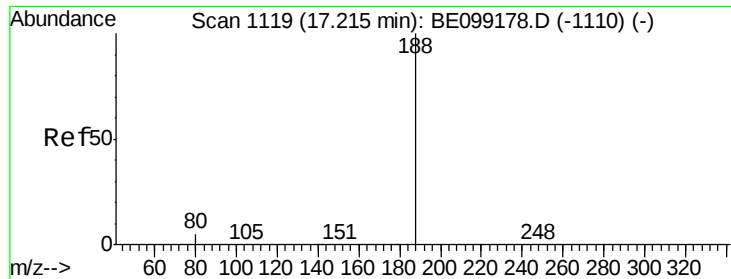

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.20 min Scan# 1118

Delta R.T. -0.01 min

Lab File: BE099240.D

Acq: 27 Mar 2019 8:41

Instrument :

BNA_E

ClientSampleId :


Tot Ion:188 Resp: 44671

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0




80 10.3 4.5 6.7#

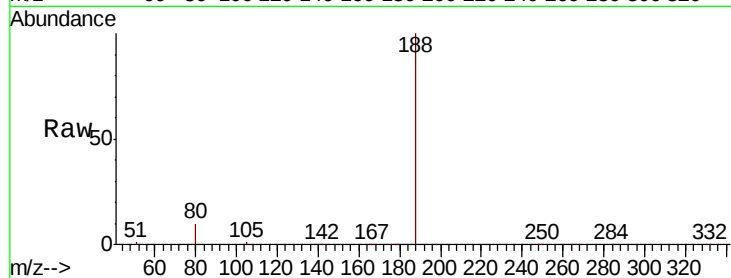

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

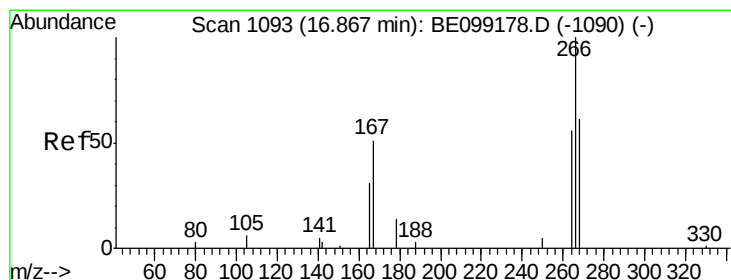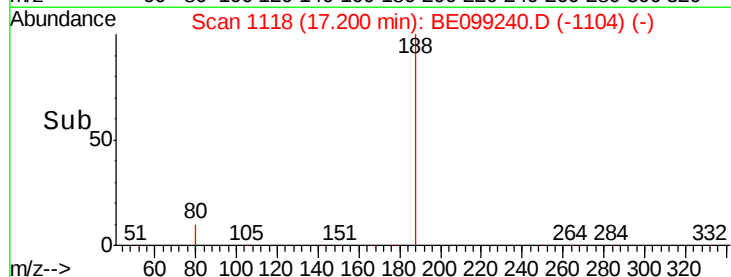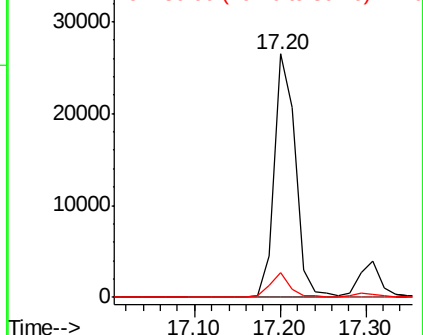

#22

Pentachlorophenol

Concen: 0.252 ng

RT: 16.87 min Scan# 1093

Delta R.T. -0.00 min

Lab File: BE099240.D

Acq: 27 Mar 2019 8:41


Tgt Ion:266 Resp: 54

Ion Ratio Lower Upper

266 100

264 86.2 54.4 81.6#



268 106.2 61.3 91.9#

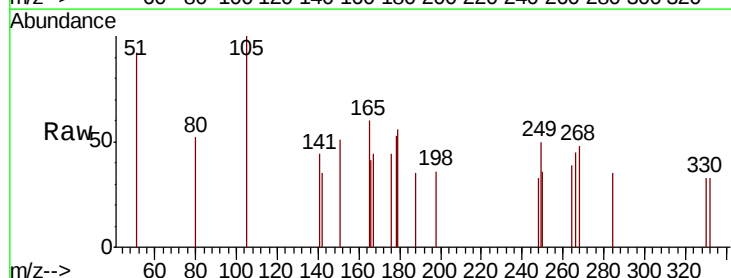


Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

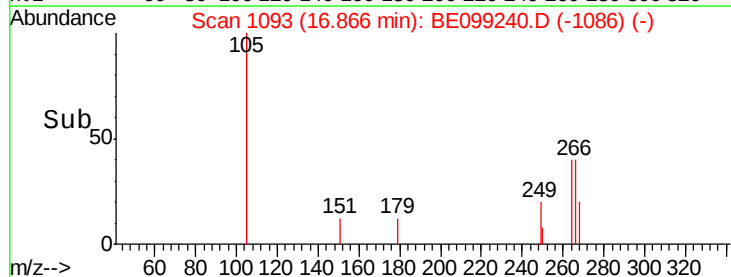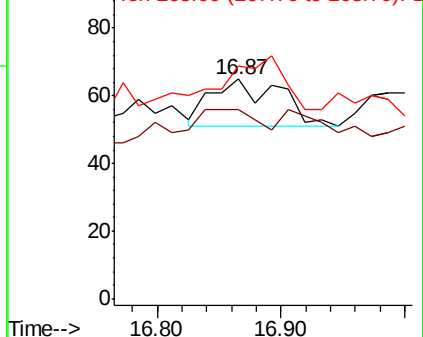

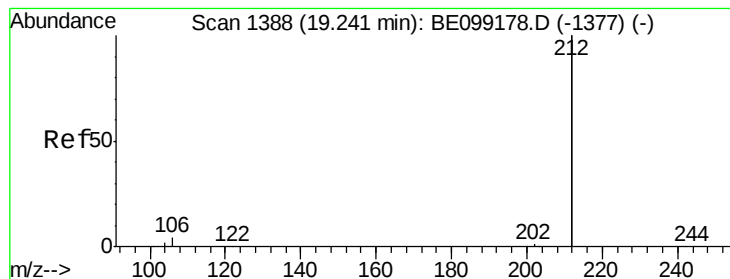

#25

Fluoranthene-d10

Concen: 0.402 ng

RT: 19.24 min Scan# 1387

Delta R.T. -0.01 min

Lab File: BE099240.D

Acq: 27 Mar 2019 8:41

Instrument :

BNA_E

ClientSampleId :


Tot Ion:212 Resp: 217324

Ion Ratio Lower Upper

212 100

106 2.2 1.8 2.8




104 1.3 1.1 1.7

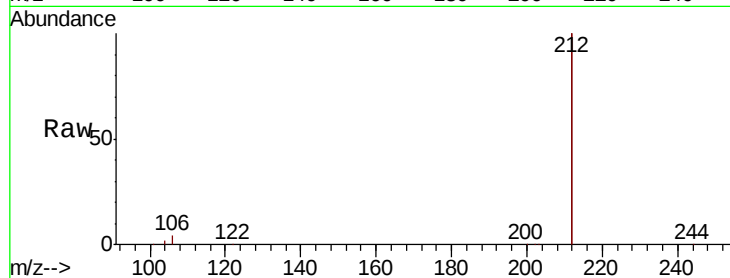

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

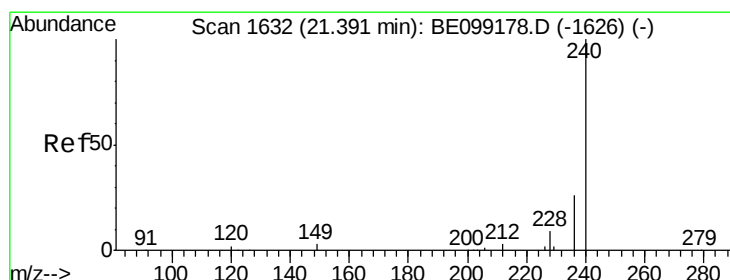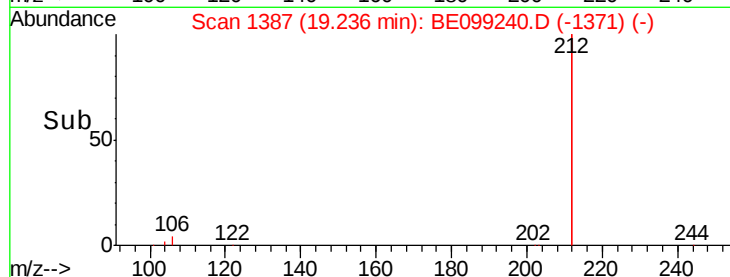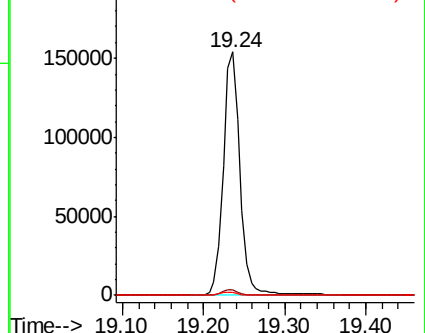

#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.38 min Scan# 1631

Delta R.T. -0.01 min

Lab File: BE099240.D

Acq: 27 Mar 2019 8:41


Tgt Ion:240 Resp: 49254

Ion Ratio Lower Upper

240 100

120 6.4 2.6 3.8#



236 27.7 20.9 31.3

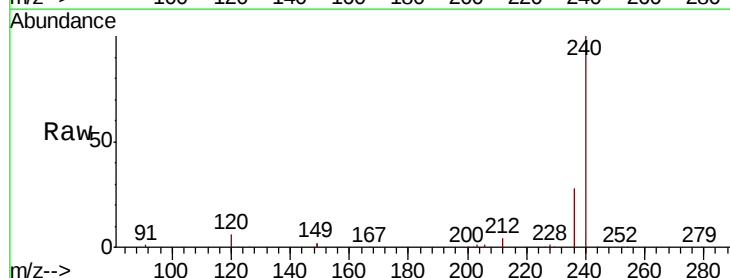


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

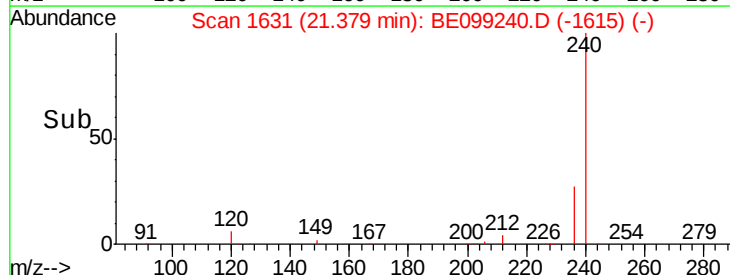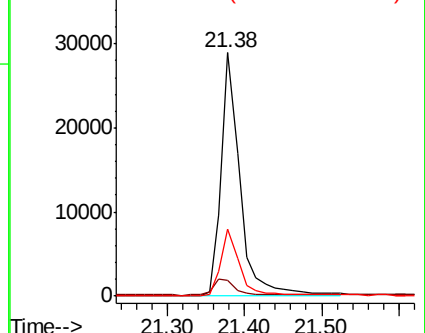

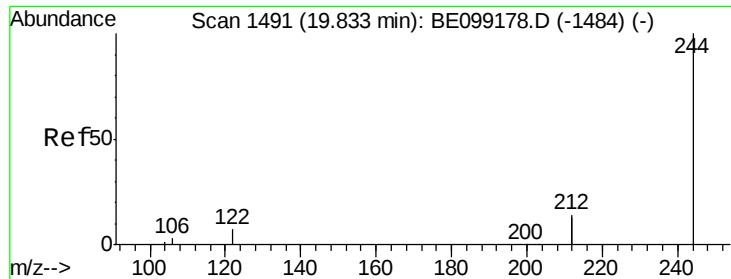

#29

Terphenyl-d14

Concen: 0.338 ng

RT: 19.83 min Scan# 1490

Delta R.T. -0.01 min

Lab File: BE099240.D

Acq: 27 Mar 2019 8:41

Instrument :

BNA_E

ClientSampleId :


Tot Ion:244 Resp: 36253

Ion Ratio Lower Upper

244 100

212 31.2 22.7 34.1




122 7.8 5.8 8.6

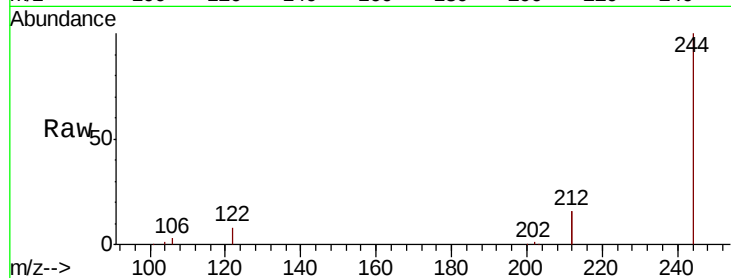

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

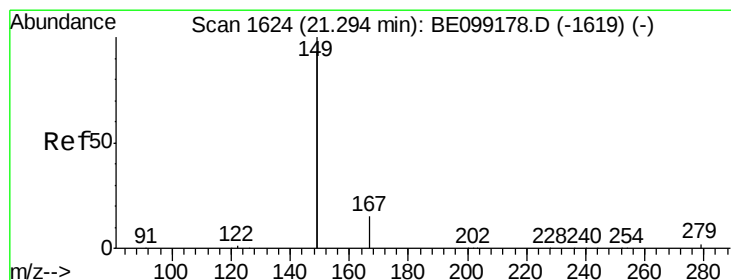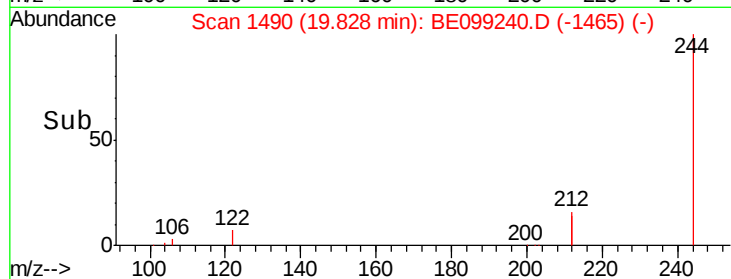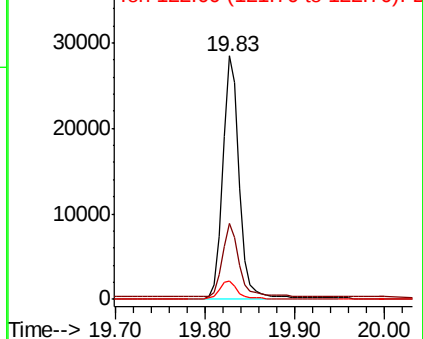

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.035 ng

RT: 21.28 min Scan# 1623

Delta R.T. -0.01 min

Lab File: BE099240.D

Acq: 27 Mar 2019 8:41


Tgt Ion:149 Resp: 6738

Ion Ratio Lower Upper

149 100

167 7.3 5.9 8.9



279 2.2 1.0 1.6#



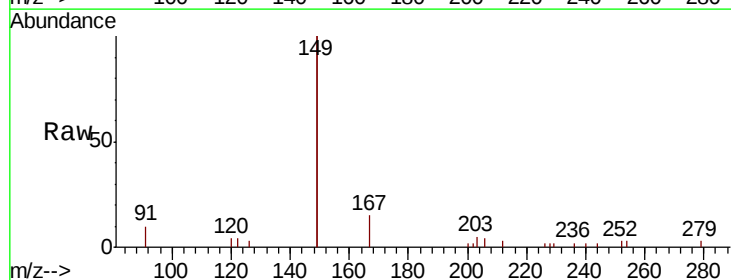


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

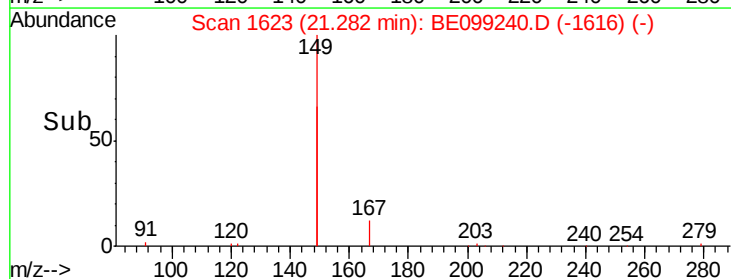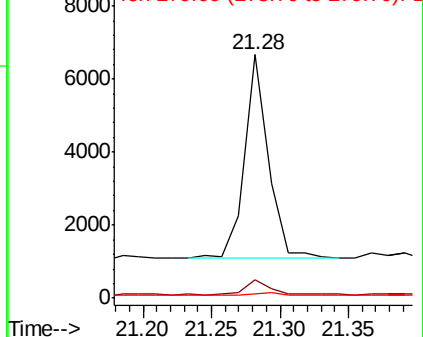

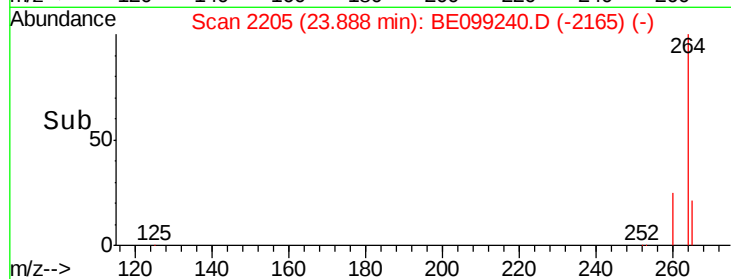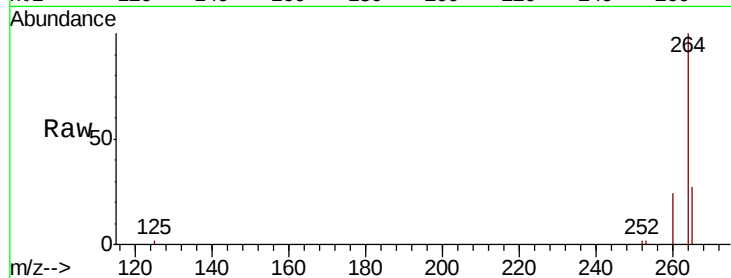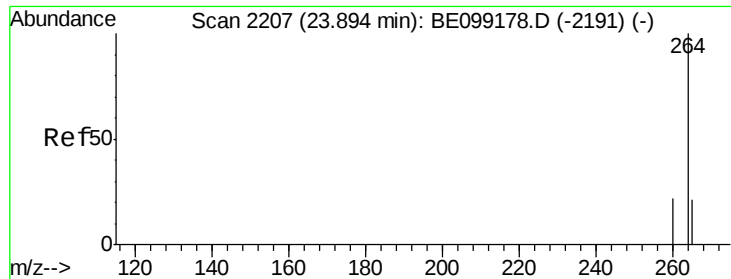

#34
Pervlene-d12
Concen: 0.400 ng
RT: 23.89 min Scan# 2205
Delta R.T. -0.01 min
Lab File: BE099240.D
Acq: 27 Mar 2019 8:41

Instrument :
BNA_E
ClientSampleId :

Tot Ion:264 Resp: 39490
Ion Ratio Lower Upper
264 100
260 24.4 18.2 27.2
265 27.2 21.8 32.8

