

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE032619\
 Data File : BE099235.D
 Acq On : 27 Mar 2019 3:40
 Operator : JU/SJ
 Sample : K2064-07
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 P006-TW001-01

Quant Time: Mar 27 09:23:41 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE032519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 26 07:02:06 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	3769	0.40	ng	0.00
7) Naphthalene-d8	10.63	136	16656	0.40	ng	0.00
13) Acenaphthene-d10	14.47	164	12981	0.40	ng	-0.01
19) Phenanthrene-d10	17.20	188	38150	0.40	ng	-0.01
27) Chrysene-d12	21.38	240	41724	0.40	ng	-0.01
34) Perylene-d12	23.89	264	34361	0.40	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Fluorophenol	5.41	112	2100	0.19	ng	0.00
5) Phenol-d6	6.99	99	1819	0.11	ng	0.00
8) Nitrobenzene-d5	8.99	82	5437	0.40	ng	0.00
11) 2-Methylnaphthalene-d10	12.22	152	14391	0.45	ng	0.00
14) 2,4,6-Tribromophenol	15.96	330	1725	0.46	ng	0.00
15) 2-Fluorobiphenyl	13.10	172	23616	0.45	ng	0.00
25) Fluoranthene-d10	19.24	212	207090	0.45	ng	0.00
29) Terphenyl-d14	19.83	244	34611	0.38	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
32) Bis(2-ethylhexyl)phthalate	21.28	149	3819	0.023	ng	# 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE032619\
Data File : BE099235.D
Acq On : 27 Mar 2019 3:40
Operator : JU/SJ
Sample : K2064-07
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
P006-TW001-01

Quant Time: Mar 27 09:23:41 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE032519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 26 07:02:06 2019
Response via : Initial Calibration

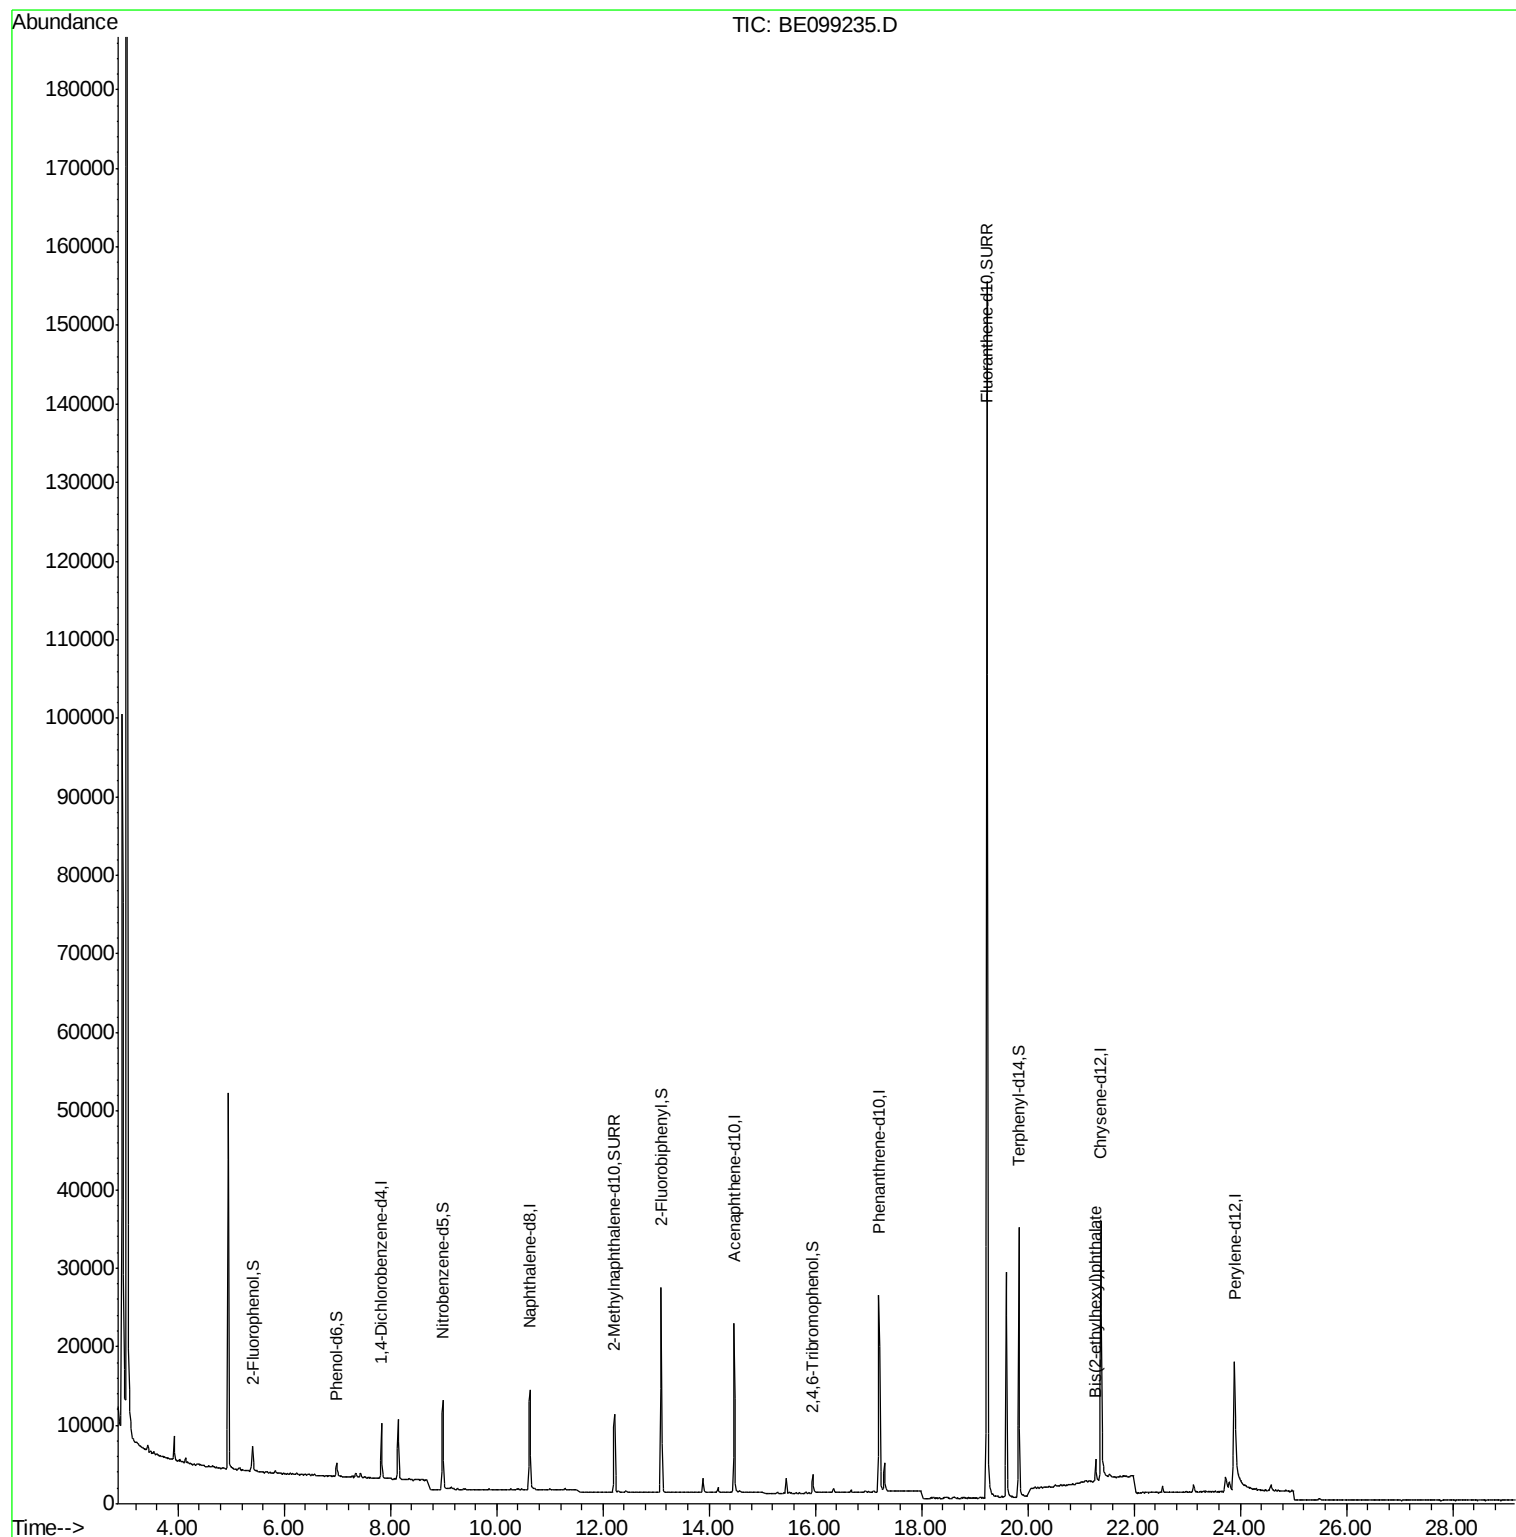

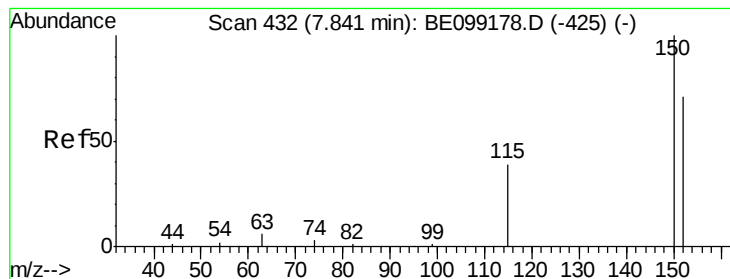

#1

1,4-Dichlorobenzene-d4

Concen: 0.400 ng

RT: 7.84 min Scan# 432

Delta R.T. -0.00 min

Lab File: BE099235.D

Acq: 27 Mar 2019 3:40

Instrument :

BNA_E

ClientSampleId :

P006-TW001-01


Tgt Ion:152 Resp: 3769

Ion Ratio Lower Upper

152 100

150 137.6 112.8 169.2




115 55.7 45.1 67.7



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

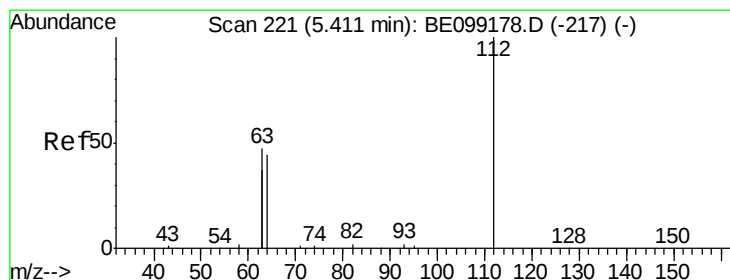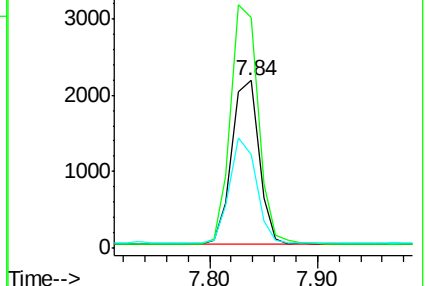

#4

2-Fluorophenol

Concen: 0.187 ng

RT: 5.41 min Scan# 221

Delta R.T. -0.00 min

Lab File: BE099235.D

Acq: 27 Mar 2019 3:40


Tgt Ion:112 Resp: 2100

Ion Ratio Lower Upper

112 100

64 54.6 46.2 69.2



63 125.4 89.9 134.9




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

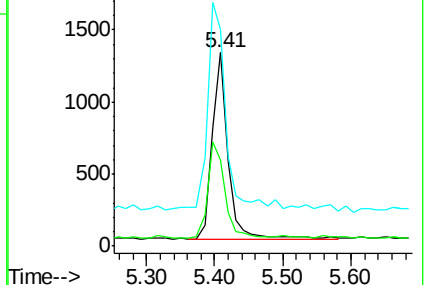



#5

Phenol-d6

Concen: 0.106 ng

RT: 6.99 min Scan# 358

Delta R.T. -0.00 min

Lab File: BE099235.D

Acq: 27 Mar 2019 3:40

Instrument :

BNA_E

ClientSampleId :

P006-TW001-01


Tgt Ion: 99 Resp: 1819

Ion Ratio Lower Upper

99 100

42 20.1 12.4 18.6#




71 40.4 28.4 42.6

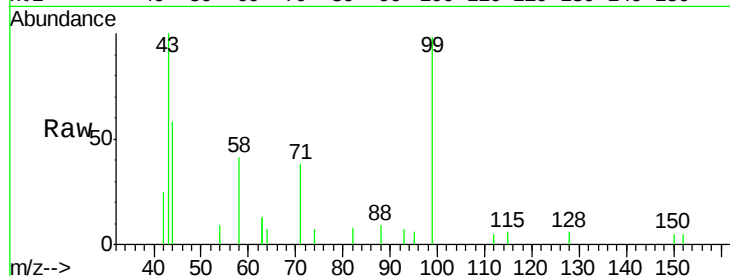

Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

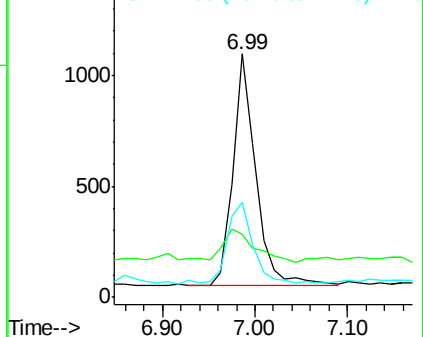

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.63 min Scan# 651

Delta R.T. 0.00 min

Lab File: BE099235.D

Acq: 27 Mar 2019 3:40

Tgt Ion: 136 Resp: 16656


Ion Ratio Lower Upper

136 100

137 11.1 8.7 13.1

54 18.1 18.7 28.1#

68 4.8 5.2 7.8#






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

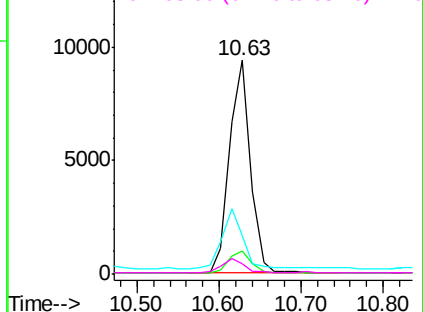

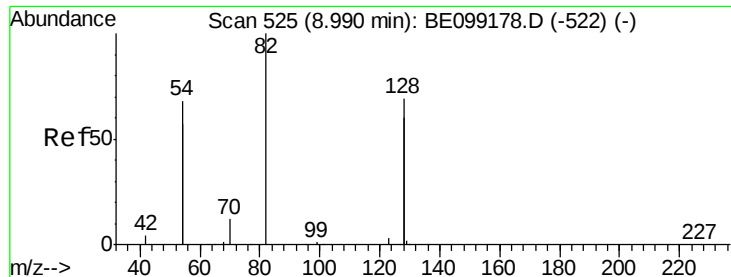

#8

Nitrobenzene-d5

Concen: 0.400 ng

RT: 8.99 min Scan# 525

Delta R.T. 0.00 min

Lab File: BE099235.D

Acq: 27 Mar 2019 3:40

Instrument :

BNA_E

ClientSampleId :

P006-TW001-01


Tgt Ion: 82 Resp: 5437

Ion Ratio Lower Upper

82 100

128 158.0 107.5 161.3




54 129.9 106.3 159.5

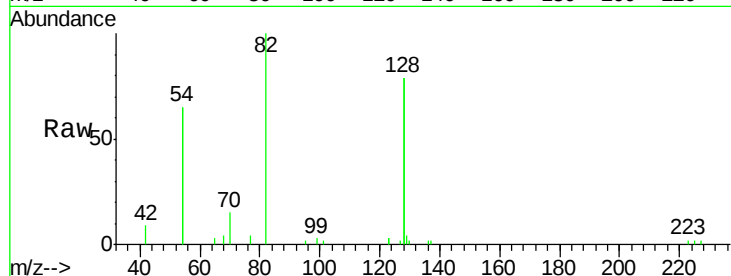

Abundance Ion 82.00 (81.70 to 82.70): BE099235.D (-517) (-)

Ion 128.00 (127.70 to 128.70): BE099235.D (-517) (-)

Ion 54.00 (53.70 to 54.70): BE099235.D (-517) (-)

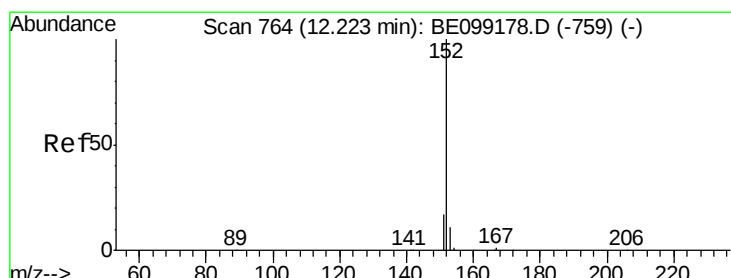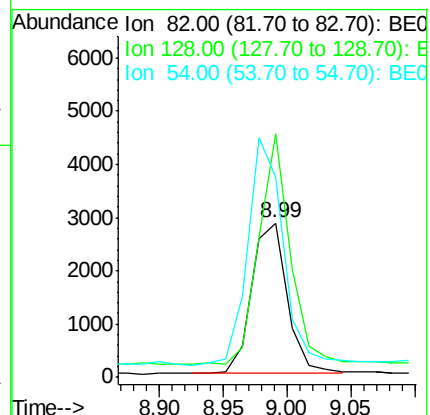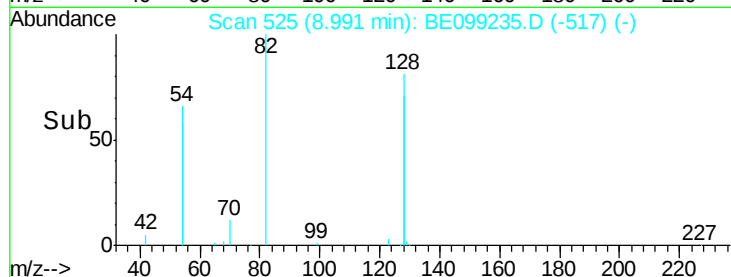

#11

2-Methylnaphthalene-d10

Concen: 0.448 ng

RT: 12.22 min Scan# 764

Delta R.T. 0.00 min

Lab File: BE099235.D


Acq: 27 Mar 2019 3:40

Tgt Ion: 152 Resp: 14391

Ion Ratio Lower Upper



152 100


151 19.2 15.0 22.6

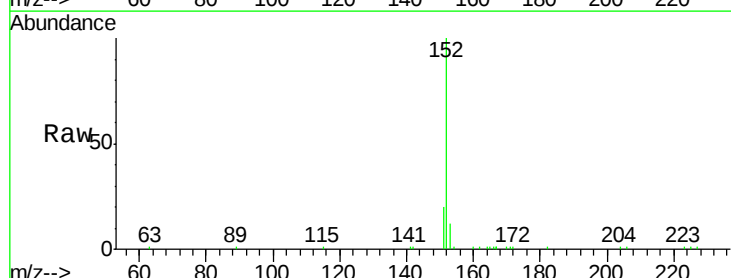

Abundance Ion 152.00 (151.70 to 152.70): BE099235.D (-757) (-)

Ion 151.00 (150.70 to 151.70): BE099235.D (-757) (-)

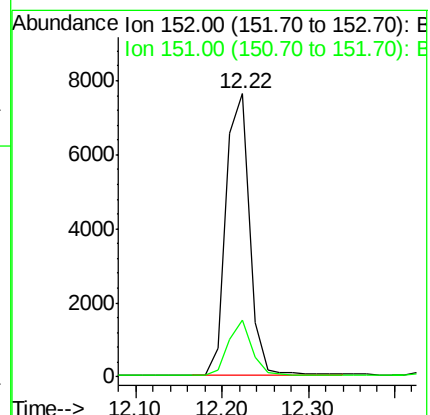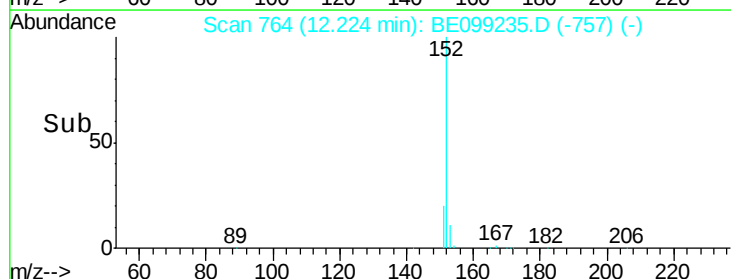

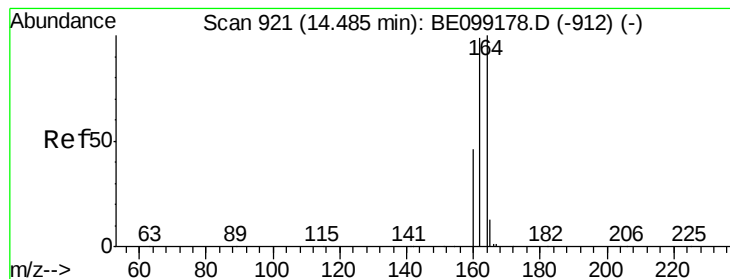

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.47 min Scan# 920

Delta R.T. -0.01 min

Lab File: BE099235.D

Acq: 27 Mar 2019 3:40

Instrument :

BNA_E

ClientSampleId :

P006-TW001-01


Tgt Ion:164 Resp: 12981

Ion Ratio Lower Upper

164 100

162 99.4 79.2 118.8




160 46.8 36.7 55.1



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

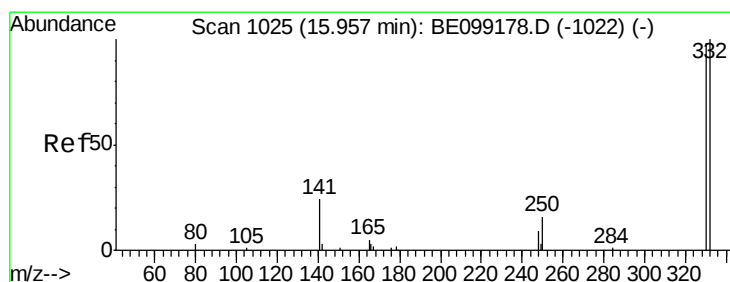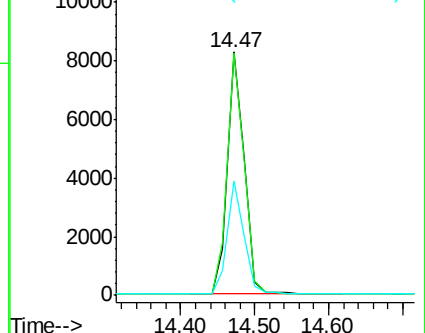

#14

2,4,6-Tribromophenol

Concen: 0.462 ng

RT: 15.96 min Scan# 1025

Delta R.T. -0.00 min

Lab File: BE099235.D

Acq: 27 Mar 2019 3:40


Tgt Ion:330 Resp: 1725

Ion Ratio Lower Upper

330 100

332 94.3 71.3 106.9



141 30.4 21.7 32.5




Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

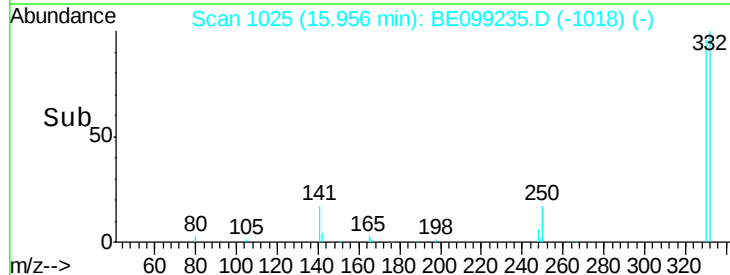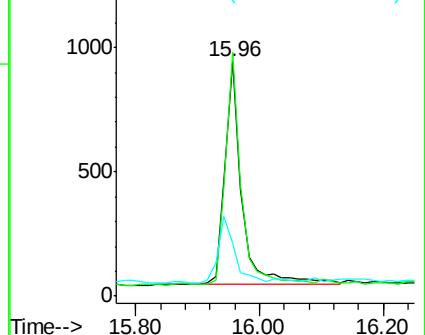

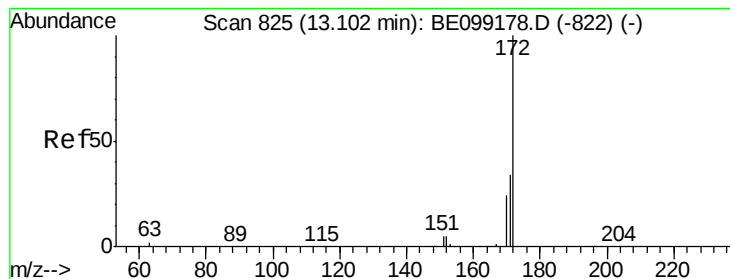

#15

2-Fluorobiphenyl

Concen: 0.446 ng

RT: 13.10 min Scan# 825

Delta R.T. 0.00 min

Lab File: BE099235.D

Acq: 27 Mar 2019 3:40

Instrument :

BNA_E

ClientSampleId :

P006-TW001-01


Tgt Ion:172 Resp: 23616

Ion Ratio Lower Upper

172 100

171 33.0 27.4 41.0




170 22.4 19.1 28.7



Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

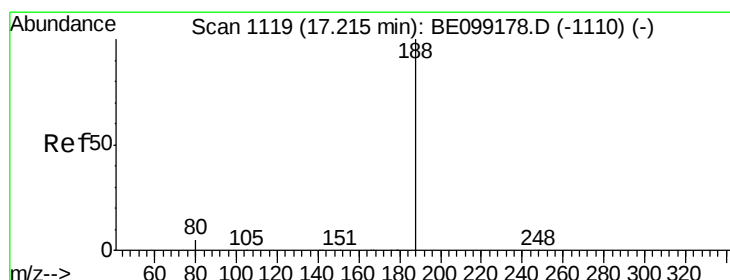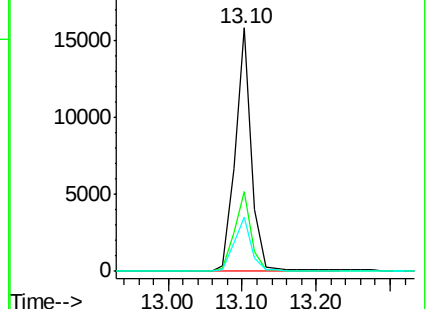

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.20 min Scan# 1118

Delta R.T. -0.01 min

Lab File: BE099235.D

Acq: 27 Mar 2019 3:40


Tgt Ion:188 Resp: 38150

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0



80 10.2 4.5 6.7#




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

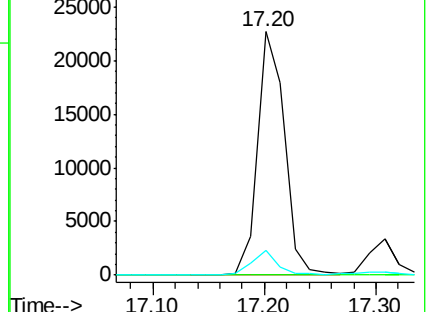

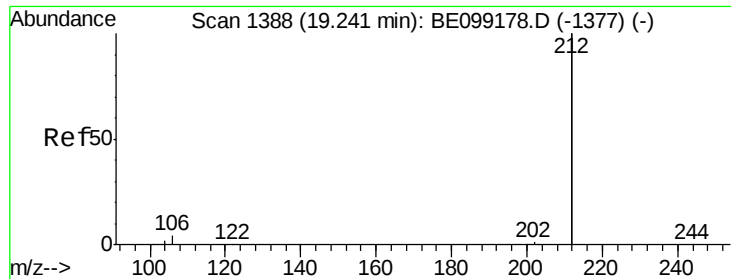

#25

Fluoranthene-d10

Concen: 0.448 ng

RT: 19.24 min Scan# 1387

Delta R.T. -0.01 min

Lab File: BE099235.D

Acq: 27 Mar 2019 3:40

Instrument :

BNA_E

ClientSampleId :

P006-TW001-01


Tgt Ion:212 Resp: 207090

Ion Ratio Lower Upper

212 100

106 2.3 1.8 2.8




104 1.3 1.1 1.7

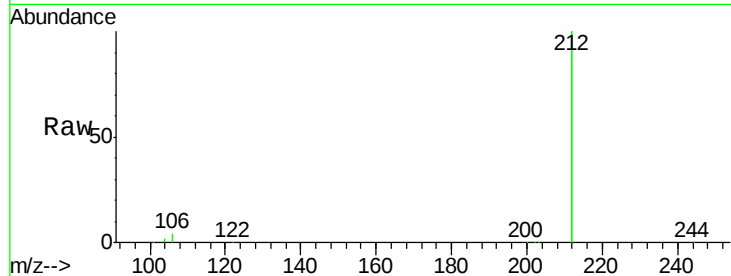

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

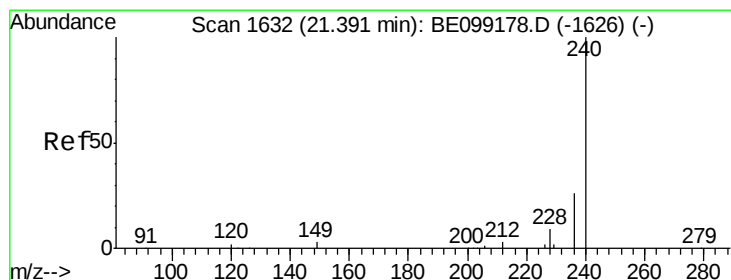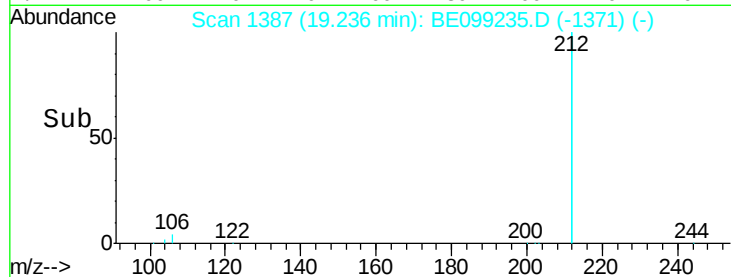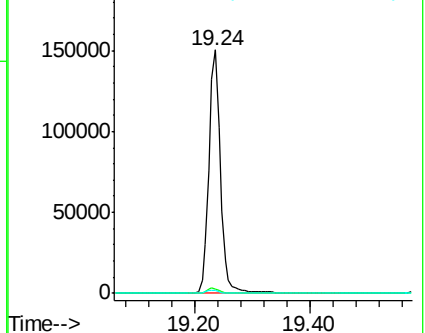

#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.38 min Scan# 1631

Delta R.T. -0.01 min

Lab File: BE099235.D

Acq: 27 Mar 2019 3:40


Tgt Ion:240 Resp: 41724

Ion Ratio Lower Upper

240 100

120 7.5 2.6 3.8#



236 27.1 20.9 31.3

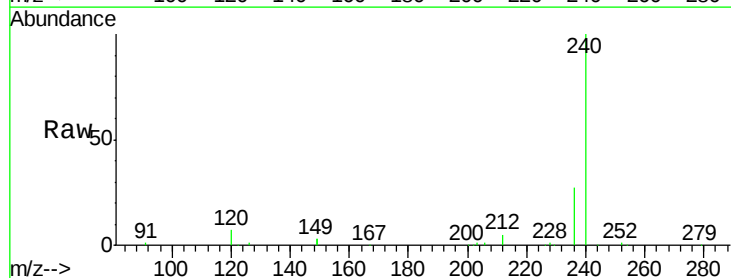


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

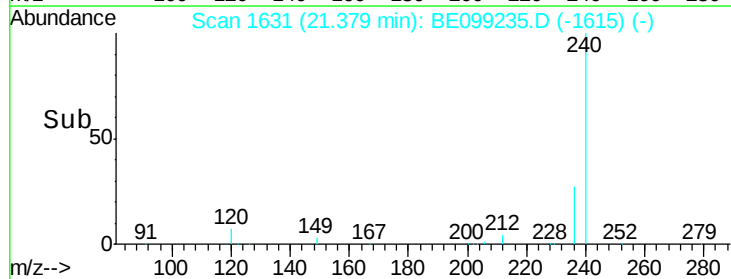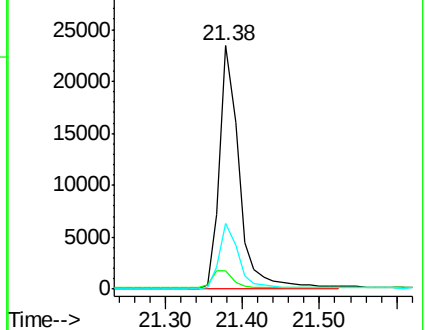



#29

Terphenyl-d14

Concen: 0.381 ng

RT: 19.83 min Scan# 1491

Delta R.T. 0.00 min

Lab File: BE099235.D

Acq: 27 Mar 2019 3:40

Instrument :

BNA_E

ClientSampleId :

P006-TW001-01


Tgt Ion:244 Resp: 34611

Ion Ratio Lower Upper

244 100

212 28.7 22.7 34.1




122 6.5 5.8 8.6

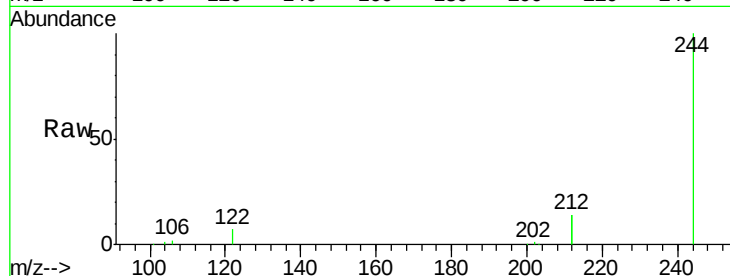

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

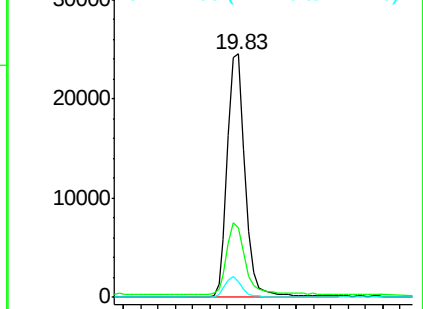

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.023 ng

RT: 21.28 min Scan# 1623

Delta R.T. -0.01 min

Lab File: BE099235.D

Acq: 27 Mar 2019 3:40


Tgt Ion:149 Resp: 3819

Ion Ratio Lower Upper

149 100

167 7.4 5.9 8.9



279 2.0 1.0 1.6#






Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

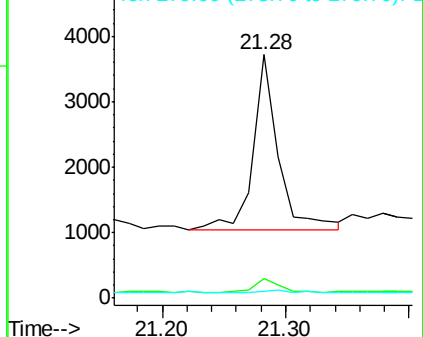

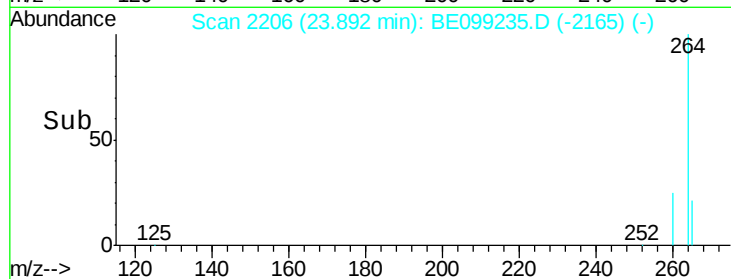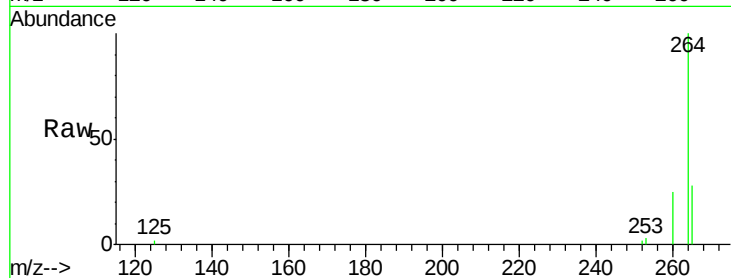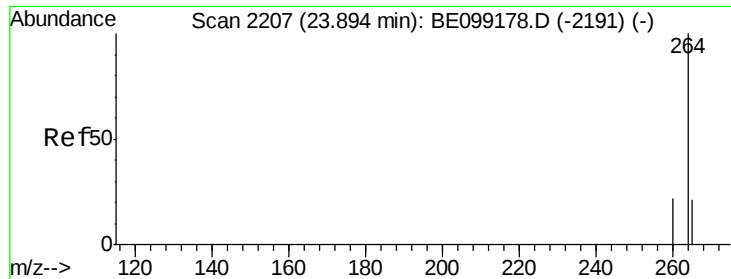

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.89 min Scan# 2206

Delta R.T. -0.00 min

Lab File: BE099235.D

Acq: 27 Mar 2019 3:40

Instrument :

BNA_E

ClientSampleId :

P006-TW001-01

Tgt Ion: 264 Resp: 34361

Ion Ratio Lower Upper

264 100

260 24.8 18.2 27.2

265 28.2 21.8 32.8

